

# INTERNATIONAL STANDARD

# NORME INTERNATIONALE

GROUP SAFETY PUBLICATION  
PUBLICATION GROUPEE DE SÉCURITÉ

**Safety requirements for electrical equipment for measurement, control and laboratory use –  
Part 2-101: Particular requirements for in vitro diagnostic (IVD) medical equipment**

**Règles de sécurité pour appareils électriques de mesurage, de régulation et de laboratoire –  
Partie 2-101: Exigences particulières pour les appareils médicaux de diagnostic in vitro (DIV)**



**THIS PUBLICATION IS COPYRIGHT PROTECTED**  
**Copyright © 2015 IEC, Geneva, Switzerland**

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either IEC or IEC's member National Committee in the country of the requester. If you have any questions about IEC copyright or have an enquiry about obtaining additional rights to this publication, please contact the address below or your local IEC member National Committee for further information.

Droits de reproduction réservés. Sauf indication contraire, aucune partie de cette publication ne peut être reproduite ni utilisée sous quelque forme que ce soit et par aucun procédé, électronique ou mécanique, y compris la photocopie et les microfilms, sans l'accord écrit de l'IEC ou du Comité national de l'IEC du pays du demandeur. Si vous avez des questions sur le copyright de l'IEC ou si vous désirez obtenir des droits supplémentaires sur cette publication, utilisez les coordonnées ci-après ou contactez le Comité national de l'IEC de votre pays de résidence.

IEC Central Office  
3, rue de Varembe  
CH-1211 Geneva 20  
Switzerland

Tel.: +41 22 919 02 11  
Fax: +41 22 919 03 00  
[info@iec.ch](mailto:info@iec.ch)  
[www.iec.ch](http://www.iec.ch)

#### About the IEC

The International Electrotechnical Commission (IEC) is the leading global organization that prepares and publishes International Standards for all electrical, electronic and related technologies.

#### About IEC publications

The technical content of IEC publications is kept under constant review by the IEC. Please make sure that you have the latest edition, a corrigenda or an amendment might have been published.

#### IEC Catalogue - [webstore.iec.ch/catalogue](http://webstore.iec.ch/catalogue)

The stand-alone application for consulting the entire bibliographical information on IEC International Standards, Technical Specifications, Technical Reports and other documents. Available for PC, Mac OS, Android Tablets and iPad.

#### IEC publications search - [www.iec.ch/searchpub](http://www.iec.ch/searchpub)

The advanced search enables to find IEC publications by a variety of criteria (reference number, text, technical committee,...). It also gives information on projects, replaced and withdrawn publications.

#### IEC Just Published - [webstore.iec.ch/justpublished](http://webstore.iec.ch/justpublished)

Stay up to date on all new IEC publications. Just Published details all new publications released. Available online and also once a month by email.

#### Electropedia - [www.electropedia.org](http://www.electropedia.org)

The world's leading online dictionary of electronic and electrical terms containing more than 30 000 terms and definitions in English and French, with equivalent terms in 15 additional languages. Also known as the International Electrotechnical Vocabulary (IEV) online.

#### IEC Glossary - [std.iec.ch/glossary](http://std.iec.ch/glossary)

More than 60 000 electrotechnical terminology entries in English and French extracted from the Terms and Definitions clause of IEC publications issued since 2002. Some entries have been collected from earlier publications of IEC TC 37, 77, 86 and CISPR.

#### IEC Customer Service Centre - [webstore.iec.ch/csc](http://webstore.iec.ch/csc)

If you wish to give us your feedback on this publication or need further assistance, please contact the Customer Service Centre: [csc@iec.ch](mailto:csc@iec.ch).

#### A propos de l'IEC

La Commission Electrotechnique Internationale (IEC) est la première organisation mondiale qui élabore et publie des Normes internationales pour tout ce qui a trait à l'électricité, à l'électronique et aux technologies apparentées.

#### A propos des publications IEC

Le contenu technique des publications IEC est constamment revu. Veuillez vous assurer que vous possédez l'édition la plus récente, un corrigendum ou amendement peut avoir été publié.

#### Catalogue IEC - [webstore.iec.ch/catalogue](http://webstore.iec.ch/catalogue)

Application autonome pour consulter tous les renseignements bibliographiques sur les Normes internationales, Spécifications techniques, Rapports techniques et autres documents de l'IEC. Disponible pour PC, Mac OS, tablettes Android et iPad.

#### Recherche de publications IEC - [www.iec.ch/searchpub](http://www.iec.ch/searchpub)

La recherche avancée permet de trouver des publications IEC en utilisant différents critères (numéro de référence, texte, comité d'études,...). Elle donne aussi des informations sur les projets et les publications remplacées ou retirées.

#### IEC Just Published - [webstore.iec.ch/justpublished](http://webstore.iec.ch/justpublished)

Restez informé sur les nouvelles publications IEC. Just Published détaille les nouvelles publications parues. Disponible en ligne et aussi une fois par mois par email.

#### Electropedia - [www.electropedia.org](http://www.electropedia.org)

Le premier dictionnaire en ligne de termes électroniques et électriques. Il contient plus de 30 000 termes et définitions en anglais et en français, ainsi que les termes équivalents dans 15 langues additionnelles. Egalement appelé Vocabulaire Electrotechnique International (IEV) en ligne.

#### Glossaire IEC - [std.iec.ch/glossary](http://std.iec.ch/glossary)

Plus de 60 000 entrées terminologiques électrotechniques, en anglais et en français, extraites des articles Termes et Définitions des publications IEC parues depuis 2002. Plus certaines entrées antérieures extraites des publications des CE 37, 77, 86 et CISPR de l'IEC.

#### Service Clients - [webstore.iec.ch/csc](http://webstore.iec.ch/csc)

Si vous désirez nous donner des commentaires sur cette publication ou si vous avez des questions contactez-nous: [csc@iec.ch](mailto:csc@iec.ch).

# INTERNATIONAL STANDARD

## NORME INTERNATIONALE

GROUP SAFETY PUBLICATION  
PUBLICATION GROUPEE DE SÉCURITÉ

**Safety requirements for electrical equipment for measurement, control and laboratory use –  
Part 2-101: Particular requirements for in vitro diagnostic (IVD) medical equipment**

**Règles de sécurité pour appareils électriques de mesurage, de régulation et de laboratoire –  
Partie 2-101: Exigences particulières pour les appareils médicaux de diagnostic in vitro (DIV)**

INTERNATIONAL  
ELECTROTECHNICAL  
COMMISSION

COMMISSION  
ELECTROTECHNIQUE  
INTERNATIONALE


ICS 11.040.55, 19.080

ISBN 978-2-8322-2206-5

**Warning! Make sure that you obtained this publication from an authorized distributor.  
Attention! Veuillez vous assurer que vous avez obtenu cette publication via un distributeur agréé.**

## CONTENTS

FOREWORD.....	3
1 Scope and object.....	6
2 Normative references.....	7
3 Terms and definitions .....	7
4 Tests.....	7
5 Marking and documentation .....	8
6 Protection against electric shock.....	12
7 Protection against mechanical HAZARDS.....	12
8 Resistance to mechanical stresses.....	14
9 Protection against the spread of fire.....	14
10 Equipment temperature limits and resistance to heat.....	14
11 Protection against HAZARDS from fluids.....	14
12 Protection against radiation, including laser sources, and against sonic and ultrasonic pressure .....	14
13 Protection against liberated gases and substances, explosion and implosion .....	15
14 Components and subassemblies.....	15
15 Protection by interlocks.....	15
16 HAZARDS resulting from application.....	15
17 RISK assessment .....	16
Annexes .....	16
Annex L (informative) Index of defined terms.....	17
Bibliography .....	18
Table 1 – Symbols.....	8

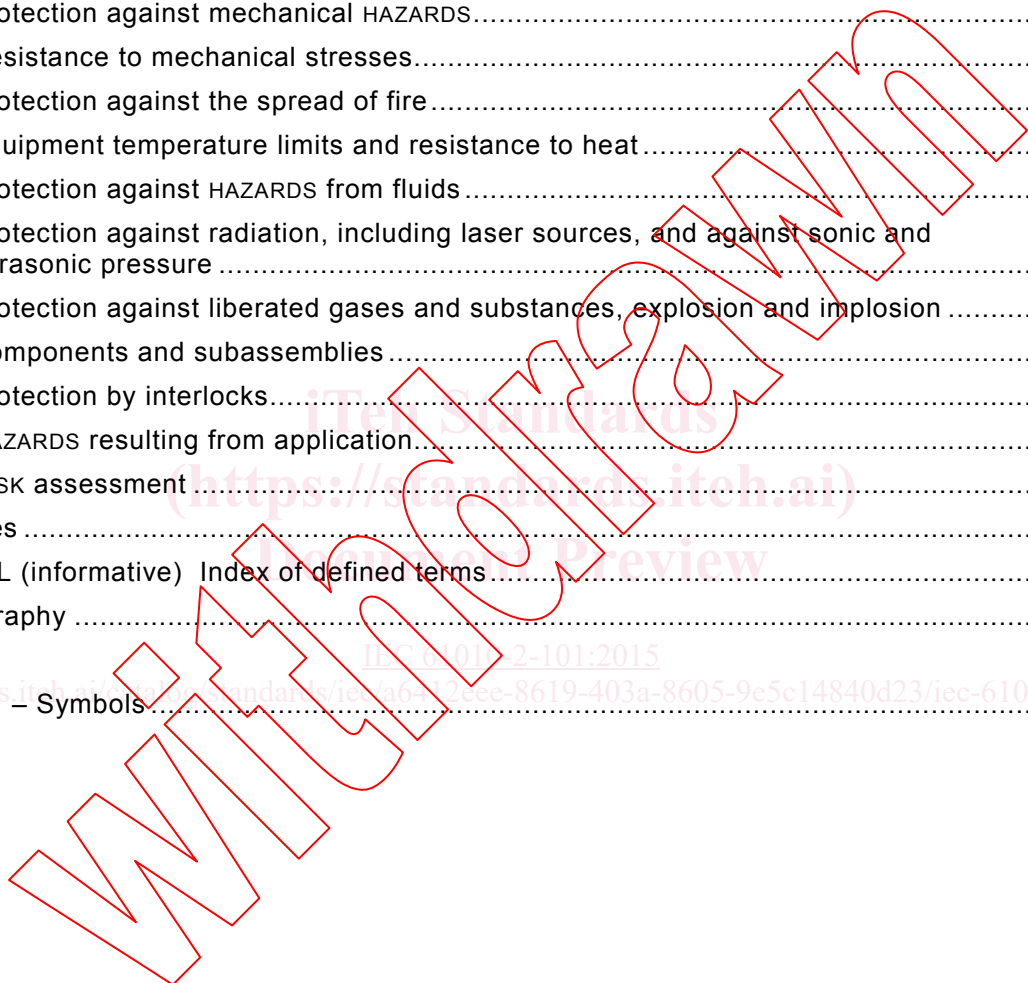

<https://standards.iteh.ai/> IEC 61010-2-101:2015  
<https://standards.iteh.ai/standards/iec/61010-2-101-2015/iec-8619-403a-8605-9e5c14840d23/iec-61010-2-101-2015>

## INTERNATIONAL ELECTROTECHNICAL COMMISSION

**SAFETY REQUIREMENTS FOR ELECTRICAL EQUIPMENT  
FOR MEASUREMENT, CONTROL AND LABORATORY USE –****Part 2-101: Particular requirements for  
in vitro diagnostic (IVD) medical equipment**

## FOREWORD

- 1) The International Electrotechnical Commission (IEC) is a worldwide organization for standardization comprising all national electrotechnical committees (IEC National Committees). The object of IEC is to promote international co-operation on all questions concerning standardization in the electrical and electronic fields. To this end and in addition to other activities, IEC publishes International Standards, Technical Specifications, Technical Reports, Publicly Available Specifications (PAS) and Guides (hereafter referred to as "IEC Publication(s)"). Their preparation is entrusted to technical committees; any IEC National Committee interested in the subject dealt with may participate in this preparatory work. International, governmental and non-governmental organizations liaising with the IEC also participate in this preparation. IEC collaborates closely with the International Organization for Standardization (ISO) in accordance with conditions determined by agreement between the two organizations.
- 2) The formal decisions or agreements of IEC on technical matters express, as nearly as possible, an international consensus of opinion on the relevant subjects since each technical committee has representation from all interested IEC National Committees.
- 3) IEC Publications have the form of recommendations for international use and are accepted by IEC National Committees in that sense. While all reasonable efforts are made to ensure that the technical content of IEC Publications is accurate, IEC cannot be held responsible for the way in which they are used or for any misinterpretation by any end user.
- 4) In order to promote international uniformity, IEC National Committees undertake to apply IEC Publications transparently to the maximum extent possible in their national and regional publications. Any divergence between any IEC Publication and the corresponding national or regional publication shall be clearly indicated in the latter.
- 5) IEC itself does not provide any attestation of conformity. Independent certification bodies provide conformity assessment services and, in some areas, access to IEC marks of conformity. IEC is not responsible for any services carried out by independent certification bodies.
- 6) All users should ensure that they have the latest edition of this publication.
- 7) No liability shall attach to IEC or its directors, employees, servants or agents including individual experts and members of its technical committees and IEC National Committees for any personal injury, property damage or other damage of any nature whatsoever, whether direct or indirect, or for costs (including legal fees) and expenses arising out of the publication, use of, or reliance upon, this IEC Publication or any other IEC Publications.
- 8) Attention is drawn to the Normative references cited in this publication. Use of the referenced publications is indispensable for the correct application of this publication.
- 9) Attention is drawn to the possibility that some of the elements of this IEC Publication may be the subject of patent rights. IEC shall not be held responsible for identifying any or all such patent rights.

International Standard IEC 61010-2-101 has been prepared by IEC technical committee 66: Safety of measuring, control and laboratory equipment.

It has the status of a group safety publication, as specified in IEC Guide 104.

This standard has been prepared in close collaboration with Working Group CENELEC BTTF 88.1.

This second edition cancels and replaces the first edition published in 2002. It constitutes a technical revision and includes the following significant changes from the first edition, as well as numerous other changes:

- excluded IEC 61010-2-081 (general laboratory equipment) from the scope. This separates IEC 61010-2-081 and IEC 61010-2-101 equipment;

- updated Biohazard and Lot symbols in Table 1 in Clause 5;
- added requirement for within expiration consumables and authorized representative details in Instructions for Use to Clause 5;
- added requirement for gas or liquid markings and ratings to Clause 5;
- added requirement to include OPERATOR instructions to deal with consumable or sample spills, jams or breakage inside equipment, disposal of hazardous waste, personal protection, RISK reduction procedures relating to flammable liquids, burns from surfaces, and loading and unloading of sample and reagents in Instructions for Use to Clause 5;
- added requirement for manufacturer to provide instructions on equipment transport, storage and removal from use to Clause 5;
- added normative reference ISO 18113-5 for instructions for use of self-test IVD medical equipment in Clause 5;
- added requirement for OPERATOR maintenance instructions to Clause 7;
- added requirements for sample zones and loading zones to Clause 7;
- excluded equipment whose size and weight make unintentional movement unlikely from drop test in Clause 8;
- added requirement for biohazard marking to Clause 13;
- added requirement for interlock systems containing electric/electronic or programmable components to Clause 15;
- added informative reference to Usability standard IEC 62366 to Clause 16;
- replaced Clause 17 with requirements of ISO 14971 for RISK assessment.
- Annex BB Instructions for use for self-testing IVD Medical Equipment deleted and a reference given to ISO 18113-5 in Clause 5.

The text of this standard is based on the following documents:

FDIS	Report on voting
66/545/FDIS	66/560/RVD

Full information on the voting for the approval of this standard can be found in the report on voting indicated in the above table.

This publication has been drafted in accordance with the ISO/IEC Directives, Part 2.

A list of all parts of the IEC 61010 series, under the general title: *Safety requirements for electrical equipment for measurement, control, and laboratory use*, may be found on the IEC website.

This Part 2-101 is intended to be used in conjunction with IEC 61010-1. It was established on the basis of the third edition (2010).

This Part 2-101 supplements or modifies the corresponding clauses in IEC 61010-1 so as to convert that publication into the IEC standard: *Safety requirements for in vitro diagnostic (IVD) medical equipment*.

Where a particular subclause of Part 1 is not mentioned in this Part 2, that subclause applies as far as is reasonable. Where this part states “addition”, “modification”, “replacement”, or “deletion” the relevant requirement, test specification or note in Part 1 should be adapted accordingly.

In this standard:

1) the following print types are used:

- requirements: in roman type;
- NOTES: in smaller roman type;
- *conformity and test: in italic type;*
- terms used throughout this standard which have been defined in clause 3: SMALL ROMAN CAPITALS;

2) subclauses, figures, tables and notes which are additional to those in part 1 are numbered starting from 101. Additional annexes are lettered starting from AA.

The committee has decided that the contents of this publication will remain unchanged until the stability date indicated on the IEC web site under "<http://webstore.iec.ch>" in the data related to the specific publication. At this date, the publication will be

- reconfirmed,
- withdrawn,
- replaced by a revised edition, or
- amended.

Withdrawing

iTech Standards  
(<https://standards.iteh.ai>)  
Document Preview

[IEC 61010-2-101:2015](https://standards.iteh.ai/catalog/standards/iec/a6412ccc-8619-403a-8605-9e5c14840d23/iec-61010-2-101-2015)

<https://standards.iteh.ai/catalog/standards/iec/a6412ccc-8619-403a-8605-9e5c14840d23/iec-61010-2-101-2015>



# SAFETY REQUIREMENTS FOR ELECTRICAL EQUIPMENT FOR MEASUREMENT, CONTROL AND LABORATORY USE –

## Part 2-101: Particular requirements for in vitro diagnostic (IVD) medical equipment

### 1 Scope and object

This clause of Part 1 is applicable except as follows:

#### 1.1.1 Equipment included in scope

*Replacement:*

*Replace the text by the following:*

This part of IEC 61010 applies to equipment intended for in vitro diagnostic (IVD) medical purposes, including self-test IVD medical purposes.

IVD medical equipment, whether used alone or in combination, is intended by the manufacturer to be used in vitro for the examination of specimens, including blood and tissue samples, derived from the human body, solely or principally for the purpose of providing information concerning one or more of the following:

- a physiological or pathological state; or
- a congenital abnormality;
- the determination of safety and compatibility with potential recipients;
- the monitoring of therapeutic measures.

Self-test IVD medical equipment is intended by the manufacturer for use by lay persons in a home environment.

NOTE If all or part of the equipment falls within the scope of one or more other part 2 standards of IEC 61010 as well as within the scope of this standard, considerations have to be given to those other part 2 standards.

#### 1.1.2 Equipment excluded from scope

*Addition:*

*Add the following item:*

- aa) Equipment in the scope of IEC 61010-2-081 unless they are specifically intended by their manufacturer to be used for in vitro diagnostic examination.

### 1.2 Object

#### 1.2.1 Aspects included in scope

*Addition:*

*Add two items:*

- aa) biohazards;
- bb) hazardous chemical substances.



### 1.2.2 Aspects excluded from scope

*Addition:*

*Add the following item and note:*

aa) the handling or manipulation outside the equipment of material under analysis.

NOTE Requirements covering these subjects are the responsibility of committees preparing relevant standards.

## 2 Normative references

This clause of Part 1 is applicable except as follows:

*Addition:*

*Add the following references:*

ISO 14971, *Medical devices – Application of risk management to medical devices*

ISO 18113-5, *In vitro diagnostic medical devices – Information supplied by the manufacturer (labelling) – In vitro diagnostic instruments for selftesting*

ISO 13857, *Safety of machinery – Safety distances to prevent hazard zones being reached by upper and lower limbs*

## 3 Terms and definitions

This clause of Part 1 is applicable except as follows:

### 3.1 Equipment and states of equipment

*Addition:*

*Add the following terms and definitions:*

#### 3.1.101

##### **SAMPLE ZONE**

area where OPERATOR access is typically unintended; the inside of this zone presents mechanical HAZARDS and a more likely probability of biohazardous human skin puncture

#### 3.1.102

##### **LOADING ZONE**

area of automated equipment where an OPERATOR handles sample or reagent material.

#### 3.5.12 RESPONSIBLE BODY

*Addition:*

*Add the following note:*

NOTE 1 This is not the European Community responsible authority.

## 4 Tests

This clause of Part 1 is applicable:

## 5 Marking and documentation

This clause of Part 1 is applicable except as follows:

### 5.1.1 General

*Replacement:*



*Replace the third paragraph by the following:*

Letter symbols for quantities and units shall be in accordance with IEC 60027. Internationally recognized symbols, including those of Table 1, shall be used as far as possible. If other additional symbols are required, it shall not be possible to confuse them with the internationally recognized symbols. There are no colour requirements for symbols. Graphic symbols shall be explained in the documentation.

**Table 1 – Symbols**

*Addition:*

*Add the following symbols to Table 1:*

Number	Symbol	Publication	Description
101	 <p>Background colour – optional; Symbol colour – optional; Outline / outline colour – optional;</p>	ISO 7000- 0659 (2004-01)	Biological RISKS
102		ISO 7000- 2492 (2004-01)	Batch code

### 5.1.2 Identification

*Replacement:*

*Replace the text by the following:*

Equipment shall, as a minimum, be marked with the following information:

- a) manufacturer's name or trade mark, and the address. The address shall include at least the city and country;

NOTE 1 National regulation may require more details on the address than required in a).

- b) model number, name, or other means of identifying the equipment;

The following additional information shall be marked on the equipment or packaging or in the instructions for use:

- 1) the serial number, for example SN XXXX or alternatively the batch code, preceded by 'LOT', using symbol 102 of Table 1;
- 2) the following information:

- i) a clear indication that the equipment is IVD medical equipment;
  - ii) if applicable, a clear indication that the equipment is self-test IVD medical equipment;
  - iii) if a potential RISK is posed, the identification of detachable components by manufacturer and part identification, and where appropriate the batch code, etc.
- 3) instructions for use shall require that the OPERATOR only use consumables that are within their expiration date. Where this is required by regulation, the name and address of the authorized representative of the manufacturer.

NOTE 2 For example, in the European Union this is the natural or legal person as established within the European Community.

### 5.1.5 TERMINALS, connections and operating devices

*Addition:*

*Add the following subclause:*

#### 5.1.5.101 Gas and liquid connections

If necessary for safety, the equipment shall be clearly marked near to the connector on the equipment with;

- a) a means of identifying the gas or liquid to be used. Where no internationally recognized symbol (including chemical formulae) exists, the equipment shall be marked with symbol 14 of Table 1;
- b) the maximum permitted pressure, or alternatively symbol 14 of Table 1 (see 5.4.3).

*Conformity is checked by inspection.*

*Addition:*

*Add the following subclause:*

#### 5.1.101 Transport and storage

Packaging of equipment shall be labelled to indicate any special conditions for transport or storage (see 5.4.102).

*Conformity is checked by inspection.*

### 5.2 Warning markings

*Replacement:*

*Replace the first paragraph by the following:*

Warning Markings specified in 5.1.5.1, 5.1.5.2 c), 5.1.5.2 d), 5.1.5.101, 6.1.2 b), 7.3.2 b) 3), 7.4, 10.1, 13.2.2 and 13.101 shall meet the following requirements:

### 5.3 Durability of markings

*Replacement:*

*Replace the first paragraph by the following paragraph:*

Markings required by 5.1.2 to 5.2 shall remain clear and legible under conditions of NORMAL USE, and resist the effects of temperature and rubbing, and of solvent and reagents likely to

be encountered in NORMAL USE, including cleaning and decontaminating agents specified by the manufacturer.

*Addition:*

*Add the following paragraph after the second paragraph:*

*If a solvent or reagent specified for use with the equipment could affect the durability of a particular marking, that marking is also rubbed for 30 s with the most frequently used and/or aggressive solvent or reagent to which the equipment is likely to be exposed in NORMAL USE*

*A representative sample of groups of solvents or reagents likely to have a similar effect can optional be used.*

#### **5.4.1 General**

*Deletion:*

*Delete the note 2 in the second paragraph.*

#### **5.4.3 Equipment installation**

*Replacement:*

*Replace subclause 5.4.3 by the following:*

#### **5.4.3 Equipment transportation, installation and assembly instructions**

Documentation for the RESPONSIBLE BODY shall include the following if applicable:

- a) instructions for transportation after delivery to the RESPONSIBLE BODY;
- b) floor loading requirements;  
 NOTE Mass and dimensions are sufficient information for floor loading.
- c) individual mass of heavy units;
- d) location and mounting instructions, including the space required for ventilation, and for safe and efficient OPERATOR maintenance;
- e) assembly instructions;
- f) instructions for protective earthing;
- g) the sound data required by 12.5.1;
- h) instructions relating to the handling, containment and exhaust of hazardous substances, including any requirements for preventing back-syphonage;
- i) any drainage systems required where a HAZARD could occur from the discharge of biological and chemical substances and hot fluids;
- j) details of protective measures relating to hazardous radiation (see clause 12);
- k) connections to the supply;
- l) for PERMANENTLY CONNECTED EQUIPMENT only:
  - 1) MAINS supply requirements and details of connections, including the RATED temperature of the cable required at maximum RATED ambient temperature;
  - 2) requirements for any external switch or circuit-breaker (see 6.11.2.1) and external overcurrent protection devices (see 9.6.1) and a recommendation that the switch or circuit-breaker be near the equipment if this is necessary for safety;
- m) requirements for special services (for example air, cooling liquid) including pressure limits.