

INTERNATIONAL STANDARD



Gas analyzers – Expression of performance –
Part 3: Paramagnetic oxygen analyzers

ITeH Standards
(<https://standards.iteh.ai>)
Document Preview

[IEC 61207-3:2019](#)

<https://standards.iteh.ai/catalog/standards/iec/b39cff24-c822-4f7b-91ad-e29c05cf6fd7/iec-61207-3-2019>



THIS PUBLICATION IS COPYRIGHT PROTECTED
Copyright © 2019 IEC, Geneva, Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either IEC or IEC's member National Committee in the country of the requester. If you have any questions about IEC copyright or have an enquiry about obtaining additional rights to this publication, please contact the address below or your local IEC member National Committee for further information.

IEC Central Office
3, rue de Varembe
CH-1211 Geneva 20
Switzerland

Tel.: +41 22 919 02 11
info@iec.ch
www.iec.ch

About the IEC

The International Electrotechnical Commission (IEC) is the leading global organization that prepares and publishes International Standards for all electrical, electronic and related technologies.

About IEC publications

The technical content of IEC publications is kept under constant review by the IEC. Please make sure that you have the latest edition, a corrigendum or an amendment might have been published.

IEC publications search - webstore.iec.ch/advsearchform

The advanced search enables to find IEC publications by a variety of criteria (reference number, text, technical committee,...). It also gives information on projects, replaced and withdrawn publications.

IEC Just Published - webstore.iec.ch/justpublished

Stay up to date on all new IEC publications. Just Published details all new publications released. Available online and once a month by email.

IEC Customer Service Centre - webstore.iec.ch/csc

If you wish to give us your feedback on this publication or need further assistance, please contact the Customer Service Centre: sales@iec.ch.

Electropedia - www.electropedia.org

The world's leading online dictionary on electrotechnology, containing more than 22 000 terminological entries in English and French, with equivalent terms in 16 additional languages. Also known as the International Electrotechnical Vocabulary (IEV) online.

IEC Glossary - std.iec.ch/glossary

67 000 electrotechnical terminology entries in English and French extracted from the Terms and Definitions clause of IEC publications issued since 2002. Some entries have been collected from earlier publications of IEC TC 37, 77, 86 and CISPR.

[IEC 61207-3:2019](https://standards.iteh.ai/catalog/standards/iec/b39cff24-c822-4f7b-91ad-e29c05cf6fd7/iec-61207-3-2019)

<https://standards.iteh.ai/catalog/standards/iec/b39cff24-c822-4f7b-91ad-e29c05cf6fd7/iec-61207-3-2019>



IEC 61207-3

Edition 3.0 2019-06
REDLINE VERSION

INTERNATIONAL STANDARD



**Gas analyzers – Expression of performance –
Part 3: Paramagnetic oxygen analyzers**

iteh Standards
(<https://standards.iteh.ai>)
Document Preview

[IEC 61207-3:2019](#)

<https://standards.iteh.ai/catalog/standards/iec/b39cff24-c822-4f7b-91ad-e29c05cf6fd7/iec-61207-3-2019>

INTERNATIONAL
ELECTROTECHNICAL
COMMISSION

ICS 19.040; 71.040.40

ISBN 978-2-8322-7117-9

Warning! Make sure that you obtained this publication from an authorized distributor.

CONTENTS

| | |
|---|----|
| FOREWORD..... | 4 |
| INTRODUCTION..... | 6 |
| 1 Scope and object | 7 |
| 2 Normative references | 7 |
| 3 Terms and definitions..... | 7 |
| 4 Procedures for specification | 16 |
| 4.1 General..... | 16 |
| 4.2 Specification of essential ancillary units and services | 16 |
| 4.2.1 Sampling system | 16 |
| 4.2.2 Services | 16 |
| 4.3 Additional characteristics related to specification of performance..... | 17 |
| 4.4 Important aspects related to specification of performance..... | 17 |
| 4.4.1 General | 17 |
| 4.4.2 Rated range of ambient temperature..... | 17 |
| 4.4.3 Rated range of sample gas temperature | 17 |
| 4.4.4 Rated range of ambient pressure..... | 18 |
| 4.4.5 Rated range of sample pressure | 18 |
| 4.4.6 Rated range of sample flow | 18 |
| 4.4.7 Rated range of sample dew point..... | 18 |
| 4.4.8 Rated range of sample particulate content..... | 18 |
| 4.4.9 Rated range of interference errors uncertainties | 19 |
| 4.4.10 Rated range of linearity error uncertainty..... | 19 |
| 4.4.11 Rated ranges of influence quantities | 19 |
| 5 Procedures for compliance testing..... | 19 |
| 5.1 Introduction Analyzer testing..... | 19 |
| 5.1.1 General | 19 |
| 5.1.2 Test equipment..... | 19 |
| 5.2 Testing procedures | 20 |
| 5.2.1 General | 20 |
| 5.2.2 Interference error uncertainty | 20 |
| 5.2.3 Wet samples..... | 21 |
| 5.2.4 Delay times, rise time, fall time | 21 |
| Annex A (informative) Interfering gases | 23 |
| Annex B (informative) Methods of preparation of water vapour in test gases..... | 27 |
| Bibliography..... | 29 |
| Figure 1 – Magnetic auto-balance system with current feedback..... | 10 |
| Figure 2 – Thermomagnetic oxygen sensor..... | 11 |
| Figure 3 – Differential pressure oxygen sensor | 12 |
| Figure 4 – Typical sampling systems – Filtered and dried system with pump for wet samples | 14 |
| Figure 5 – Typical sampling system – Steam-aspirated system with water wash for wet samples | 15 |
| Figure 6 – General test arrangement – Dry gases | 20 |
| Figure 7 – Test apparatus to apply gases and water vapour to analysis systems | 22 |

Table A.1 – Zero correction factors for current gases23

iTeh Standards
(<https://standards.iteh.ai>)
Document Preview

[IEC 61207-3:2019](#)

<https://standards.iteh.ai/catalog/standards/iec/b39cff24-c822-4f7b-91ad-e29c05cf6fd7/iec-61207-3-2019>

INTERNATIONAL ELECTROTECHNICAL COMMISSION

**GAS ANALYZERS –
EXPRESSION OF PERFORMANCE –****Part 3: Paramagnetic oxygen analyzers****FOREWORD**

- 1) The International Electrotechnical Commission (IEC) is a worldwide organization for standardization comprising all national electrotechnical committees (IEC National Committees). The object of IEC is to promote international co-operation on all questions concerning standardization in the electrical and electronic fields. To this end and in addition to other activities, IEC publishes International Standards, Technical Specifications, Technical Reports, Publicly Available Specifications (PAS) and Guides (hereafter referred to as “IEC Publication(s)”). Their preparation is entrusted to technical committees; any IEC National Committee interested in the subject dealt with may participate in this preparatory work. International, governmental and non-governmental organizations liaising with the IEC also participate in this preparation. IEC collaborates closely with the International Organization for Standardization (ISO) in accordance with conditions determined by agreement between the two organizations.
- 2) The formal decisions or agreements of IEC on technical matters express, as nearly as possible, an international consensus of opinion on the relevant subjects since each technical committee has representation from all interested IEC National Committees.
- 3) IEC Publications have the form of recommendations for international use and are accepted by IEC National Committees in that sense. While all reasonable efforts are made to ensure that the technical content of IEC Publications is accurate, IEC cannot be held responsible for the way in which they are used or for any misinterpretation by any end user.
- 4) In order to promote international uniformity, IEC National Committees undertake to apply IEC Publications transparently to the maximum extent possible in their national and regional publications. Any divergence between any IEC Publication and the corresponding national or regional publication shall be clearly indicated in the latter.
- 5) IEC itself does not provide any attestation of conformity. Independent certification bodies provide conformity assessment services and, in some areas, access to IEC marks of conformity. IEC is not responsible for any services carried out by independent certification bodies.
- 6) All users should ensure that they have the latest edition of this publication.
- 7) No liability shall attach to IEC or its directors, employees, servants or agents including individual experts and members of its technical committees and IEC National Committees for any personal injury, property damage or other damage of any nature whatsoever, whether direct or indirect, or for costs (including legal fees) and expenses arising out of the publication, use of, or reliance upon, this IEC Publication or any other IEC Publications.
- 8) Attention is drawn to the Normative references cited in this publication. Use of the referenced publications is indispensable for the correct application of this publication.
- 9) Attention is drawn to the possibility that some of the elements of this IEC Publication may be the subject of patent rights. IEC shall not be held responsible for identifying any or all such patent rights.

This redline version of the official IEC Standard allows the user to identify the changes made to the previous edition. A vertical bar appears in the margin wherever a change has been made. Additions are in green text, deletions are in strikethrough red text.

International Standard IEC 61207-3 has been prepared by sub-committee 65B: Measurement and control devices, of IEC technical committee 65: Industrial-process measurement, control and automation.

This third edition cancels and replaces the second edition published in 2002. This edition constitutes a technical revision.

This edition includes the following significant technical changes with respect to the previous edition:

- a) all references (normative and informative) have been updated, deleted or added to as appropriate;
- b) all the terms, descriptions and definitions relating to the document have been updated where appropriate;
- c) all references to “errors” have been replaced by “uncertainties” and appropriate updated definitions applied.

The text of this International Standard is based on the following documents:

| | |
|---------------|------------------|
| FDIS | Report on voting |
| 65B/1155/FDIS | 65B/1157/RVD |

Full information on the voting for the approval of this International Standard can be found in the report on voting indicated in the above table.

This document has been drafted in accordance with the ISO/IEC Directives, Part 2.

This International Standard is to be used in conjunction with IEC 61207-1:2010.

A list of all parts in the IEC 61207 series, published under the general title *Gas analyzers – Expression of performance*, can be found on the IEC website.

<https://standards.iteh.ai/catalog/standards/iec/b39cff24-c822-4f7b-91ad-e29c05cf6fd7/iec-61207-3-2019>

The committee has decided that the contents of this document will remain unchanged until the stability date indicated on the IEC website under "<http://webstore.iec.ch>" in the data related to the specific document. At this date, the document will be

- reconfirmed,
- withdrawn,
- replaced by a revised edition, or
- amended.

IMPORTANT – The “colour inside” logo on the cover page of this publication indicates that it contains colours which are considered to be useful for the correct understanding of its contents. Users should therefore print this publication using a colour printer.

INTRODUCTION

Paramagnetic oxygen analyzers respond to the partial pressure of oxygen in the measured gas, and ~~not~~ the volumetric concentration is then determined by knowledge of the total pressure, as in many other gas analyzers. Due to this fact, many paramagnetic oxygen analyzers use pressure compensation (see 4.4.4 and 4.4.5). They are used in a wide range of industrial, laboratory, medical, and other applications where the rated measuring range of the analyzer is between 0 % to 1 % and 0 % to 100 %, at reference pressure (usually near atmospheric).

Only a few gases display significant paramagnetism (for example, oxygen, nitric oxide and nitrogen dioxide), and oxygen has ~~a particularly strong~~ the strongest paramagnetic susceptibility (see Annex A) among gases. By employing this particular property of oxygen, analyzers have been designed that can be highly specific to the measurement in most industrial and medical applications, where, for example, high background levels of hydrocarbons or moisture may be present.

There are several different techniques described for measuring ~~the paramagnetic properties of~~ oxygen by its paramagnetic property, but three main methods have evolved over many years of commercial application.

The three methods are:

- automatic null balance;
- thermomagnetic or magnetic wind;
- differential pressure or Quincke.

These methods all require the sample gas to be clean and ~~dry~~ non-condensing, though some versions work at elevated temperatures so that samples that are likely to condense at a lower temperature can be analyzed. Because of this requirement, analyzers often require a sample system to condition the sample prior to measurement.

[IEC 61207-3:2019](https://standards.iteh.ai/)

<https://standards.iteh.ai/catalog/standards/iec/b39cff24-c822-4f7b-91ad-e29c05cf6fd7/iec-61207-3-2019>

GAS ANALYZERS – EXPRESSION OF PERFORMANCE –

Part 3: Paramagnetic oxygen analyzers

1 ~~Scope and object~~

This part of IEC 61207 applies to the three main methods for measuring oxygen by its paramagnetic property, which are outlined in the introduction. It considers essential ancillary units and applies to analyzers installed indoors and outdoors.

NOTE Safety-critical applications can require ~~an additional requirement of~~ requirements from system and analyzer specifications not covered in this document.

This document is intended

- to specify terminology and definitions related to the functional performance of paramagnetic gas analyzers for the measurement of oxygen in a source gas;
- to unify methods used in making and verifying statements on the functional performance of such analyzers;
- to specify what tests ~~should be~~ are performed to determine the functional performance and how such tests ~~should be~~ are carried out;
- to provide basic documents to support the application of internationally recognized quality management standards ~~of quality assurance (ISO 9001, ISO 9002 and ISO 9003).~~

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

~~IEC 60654-1:1993, Industrial process measurement and control equipment – Operating conditions – Part 1: Climatic conditions~~

~~IEC 61115:1992, Expression of performance of sample handling systems for process analyzers~~

IEC 61207-1:1994, Expression of performance of gas analyzers – Part 1: General

~~ISO 9001:2000, Quality management systems – Requirements~~

~~ISO 9002:1994, Quality systems – Model for quality assurance in production, installation and servicing~~

~~ISO 9003:1994, Quality systems – Model for quality assurance in final inspection and test~~

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

NOTE Although cgs (centimetre-gram-second) units have been used in this document, SI (Système International) units (such as defined in IUPAC [1]¹) can also be used.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- IEC Electropedia: available at <http://www.electropedia.org/>
- ISO Online browsing platform: available at <http://www.iso.org/obp>

3.1

magnetic susceptibility

measure (X) of the variation of the intensity of a magnetic field H , existing in a vacuum, when the vacuum is substituted (filled) by the test substance, expressed as:

$$X = \frac{H^1 - H}{H}$$

where

H is the magnetic field intensity in vacuum

H^1 is the magnetic field intensity in the test substance

Note 1 to entry: $H^1 - H$ is also known as the magnetisation MV (magnetic dipole per unit volume) and therefore this is also the volume magnetic susceptibility.

3.2

paramagnetism

property of substances causing an increase of the magnetic field intensity ($X > 0$)

3.3

diamagnetism

property of substances causing a diminution of the magnetic field intensity ($X < 0$ because $H^1 < H$)

3.4

specific magnetic susceptibility

ratio of magnetic susceptibility to the density derived as follows:

$$X_s = \frac{X}{D}$$

where

D is the density of the considered substance, expressed in $\text{g}\cdot\text{cm}^{-3}$ at 273,15 K (~~0 °C~~) and, 101,3 kPa (~~= 1 bar~~).

Note 1 to entry: The measuring unit of X_s is therefore $\text{cm}^3\cdot\text{g}^{-1}$. This is also known as the mass magnetic susceptibility.

3.5

molar magnetic susceptibility

X_m specific magnetic susceptibility multiplied by the molecular ~~weight~~ mass (M) of the substance considered:

$$X_m = X_s \cdot M$$

¹ Numbers in square brackets refer to the bibliography

where

M is expressed in g per mole ($\text{g}\cdot\text{mol}^{-1}$) (for oxygen $M = 32\ 31,998\ 8$)

Note 1 to entry: The measuring unit of X_m is therefore $\text{cm}^3\cdot\text{mol}^{-1}$.

Note 4.2 to entry: Electrons determine the magnetic properties of matter in two ways:

- an electron can be considered as a small sphere of negative charge spinning on its axis. This spinning charge produces a magnetic moment;
- an electron travelling in an orbit around a nucleus will also produce a magnetic moment.

It is the combination of the spin moment and the orbital moment that governs the resulting magnetic properties of an individual atom or ion.

In paramagnetic materials, the main contribution to the magnetic moment comes from unpaired electrons. It is the configuration of the orbital electrons and their spin orientations that establish the paramagnetism of the oxygen molecule and distinguish it from most other gases.

Note 2.3 to entry: When paramagnetic gases are placed within an external magnetic field, the flux within the gas is higher than it would be in a vacuum, thus paramagnetic gases are attracted to the part of the magnetic field with the strongest magnetic flux. On the contrary, diamagnetic substances contain magnetic dipoles which cancel out some lines of force from the external field; thus diamagnetic gases are subject to repulsion by the magnetic flux.

Note 3.4 to entry: The molar magnetic susceptibility of oxygen is inversely proportional to the absolute temperature T . According to Van Vleck [2] the molar susceptibility of oxygen can be approximated by Equation (4).

$$\text{For oxygen, } X_m = \frac{8L \cdot \mu_B^2}{3kT} \quad (4)$$

where

X_m is the molar susceptibility of oxygen, expressed in $\text{cm}^3\cdot\text{mol}^{-1}$;

L is the Avogadro constant = $6,022\ 7 \times 10^{23}\ \text{mol}^{-1}$;

μ_B is the Bohr magneton = $9,274 \times 10^{-24}\ \text{A}\cdot\text{m}^2$;

k is the Boltzmann constant = $1,38 \times 10^{-23}\ \text{J}\cdot\text{K}^{-1}$;

T is the temperature, expressed in K (kelvin).

Equation (4) can be written as follows:

$$X_m = \frac{1010557}{T} \times 10^{-6}\ \text{cm}^3\cdot\text{mol}^{-1} \text{ (only for oxygen).}$$


Note 5 to entry: A full understanding of paramagnetism and diamagnetism can be obtained from physics and inorganic chemistry textbooks. The explanation in this document is to give the user of paramagnetic oxygen analyzers a simple understanding of the physical property utilized.

3.6

automatic null balance analyzer

~~this type of~~ analyzer ~~that~~ uses, as a general principle of operation, the displacement of a body containing a vacuum or a diamagnetic gas, from a region of high magnetic field by paramagnetic oxygen molecules

Note 1 to entry: See Figure 1.

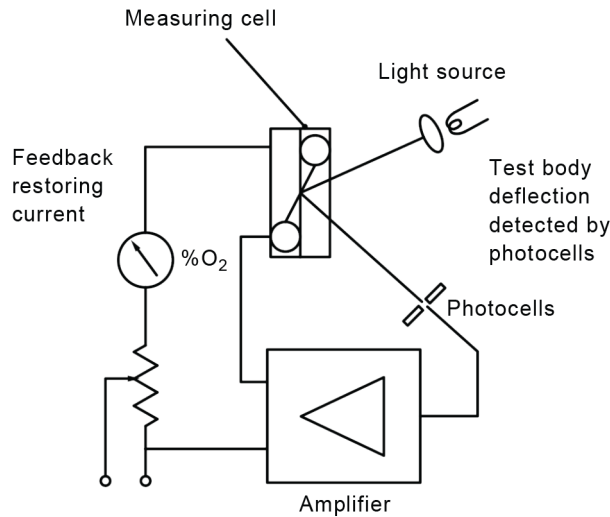

IEC

Figure 1 – Magnetic auto-balance system with current feedback

Note 2 to entry: The measuring cell typically employs a glass dumb-bell, with the spheres containing nitrogen, suspended on a torsion strip between magnetic pole pieces or magnets that concentrate the flux produce a very strong magnetic field gradient around the dumb-bell. The measuring cell has to be placed in a magnetic circuit. The dumb-bell is then deflected when oxygen molecules enter the measuring cell, a force being exerted on the dumb-bell by the oxygen molecules which are attracted to the strongest part of the magnetic field. By use of an optical levers, a feedback magnetic actuation coil, and suitable electronics to generate a feedback signal that nulls the magnetic susceptibility force, an output that is directly proportional to the partial pressure of oxygen can be achieved. The transducer is usually can be maintained at a constant temperature to prevent the variations in magnetic susceptibility with to temperature from introducing errors uncertainties. Alternatively, built-in temperature sensors may be used to provide temperature compensation of the oxygen reading. Additionally, the elevated temperature helps in applications where the sample is not particularly dry. Some analyzers are designed so that the transducer operates at a temperature in excess of 373,15 K (100 °C) to further facilitate applications where condensates would form at a lower temperature. Paramagnetic sensor orientation may also affect the oxygen measurement uncertainty and this may be corrected by using a compensation algorithm using, for example, a three-dimensional accelerometer to determine the sensor orientation relative to its orientation during calibration. Due to the mechanical nature of this type of device, there is some inherent susceptibility to vibrational and gyroscopic motion, potentially resulting in increased measurement uncertainty.

<https://standards.iteh.ai/catalog/standards/iec/b39cff24-c822-4f7b-91ad-e29c05cf6fd7/iec-61207-3-2019>

3.7 thermomagnetic (magnetic wind) analyzer

3.7.1 magnetic wind analyzer

this type of analyzer utilizes that uses the temperature dependence of the magnetic susceptibility to generate a magnetically induced gas flow which can then be measured by a flow sensor

Note 1 to entry: The sample gas passes into a chamber designed in such a way that the inlet splits the flow.

Note 2 to entry: See Figure 2.

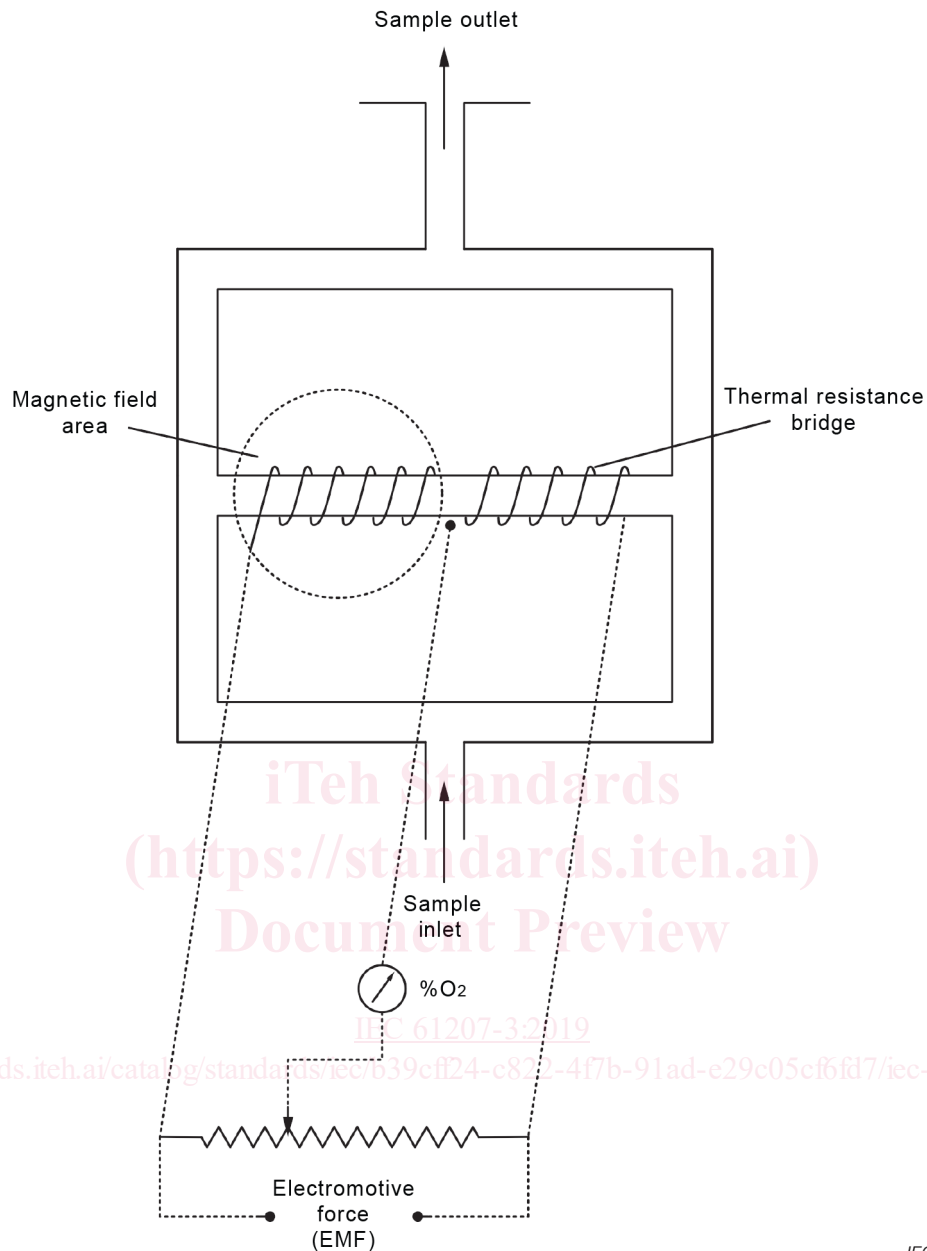


Figure 2 – Thermomagnetic oxygen sensor

Note 3 to entry: The two flows recombine at the outlet. A connecting tube is placed centrally with the flow sensor wound on it. Half of the connecting tube is placed between the poles of a strong magnet. The flow sensor is effectively two coils of wire heated to about 353,15 K (80 °C) by passage of a current. The cold oxygen molecules are diverted by the magnetic field into the central tube, and, as they heat up, their magnetic susceptibility is reduced and more cold oxygen molecules enter the connecting tube. A flow of oxygen is generated in this way through the transversal connecting tube, with the effect of cooling the first coil (which is placed in the magnetic field area), while the temperature of the second coil is not essentially influenced by this transversal flow. Since the two coils are wound with thermosensitive wire (for example, platinum wire) and connected together to build a Wheatstone bridge, the resulting unbalance current is a nearly proportional function of the oxygen partial pressure in the test gas.

More recent analyzers use more refined measuring cells, toroidal shaped resistors instead of the two-coil flow sensor, and employ temperature control to minimize ambient temperature changes.

As this method relies on heat transfer, the thermal conductivity of background gases will affect the oxygen reading and the composition of the background has to be known. Some analyzers can give a first-order correction for this by utilizing further compensation devices.

Thermomagnetic analyzers do not produce a strictly linear output and additional signal processing is required to linearize the output.

3.8
differential pressure (Quincke) analyzer

3.8.1
differential pressure analyzer

~~this type of analyzer utilizes~~ that uses a pneumatic balance system established by using a flowing reference gas (such as nitrogen or air)

Note 1 to entry: The measuring cell is designed so that at the reference gas inlet the flow is divided into two paths. These flows recombine at the reference gas outlet, where the sample is also introduced. A differential pressure sensor (or microflow sensor) is positioned across the two reference gas flows so that any imbalance is detected. A magnet is situated in the vicinity of the reference gas outlet in one arm of the measuring cell so that oxygen in the sample is attracted into the arm, thereby causing a small back pressure which is detected by the pressure sensor (see Figure 3).

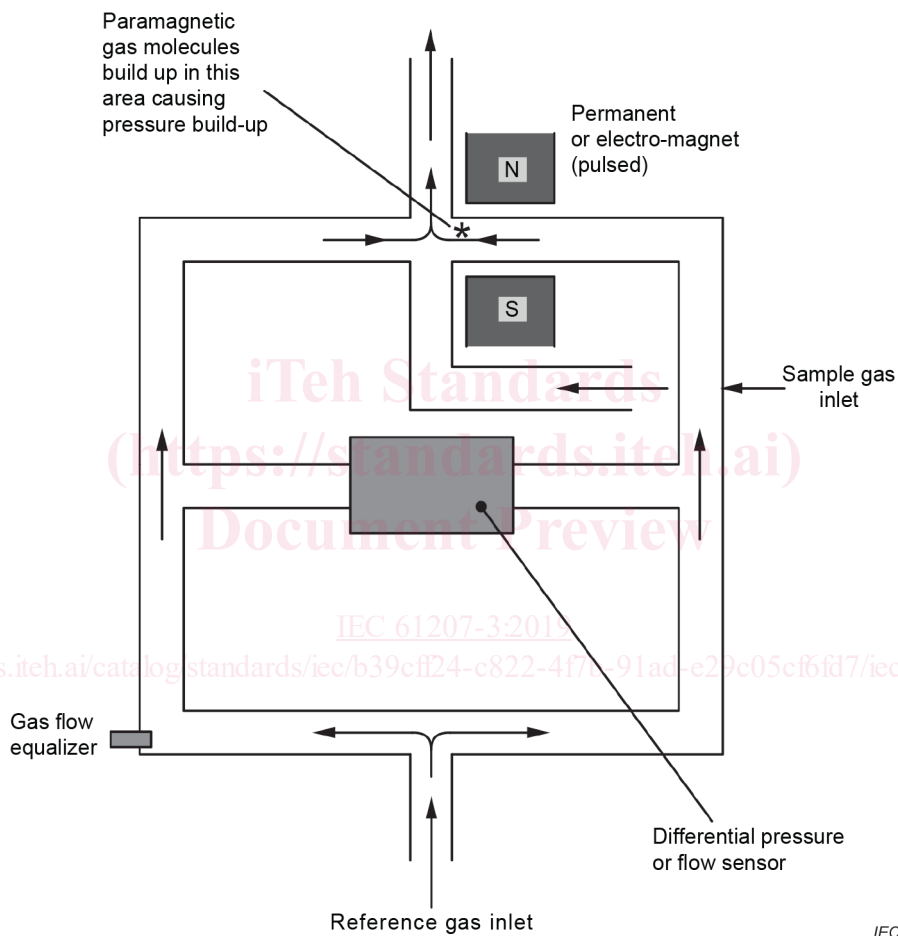


Figure 3 – Differential pressure oxygen sensor

Note 2 to entry: Differential pressure analyzers are independent of thermal conductivity of background gases, and as only the reference gas comes in contact with the sensor, corrosion problems are minimal. Some instruments use pulsed magnetic fields to improve tilt sensitivity, and certain designs compensate for vibration effects.

3.9
hazardous area

~~area where there is a possibility of release of potentially flammable gases, vapours or dusts. Restrictions in the use of electrical equipment apply in hazardous areas~~

area in which an explosive gas atmosphere is present, or may be expected to be present, in quantities such as to require special precautions for the construction, installation and use of devices