

INTERNATIONAL  
STANDARD

**ISO**  
**7206-1**

Second edition  
1995-09-01

---

---

**Implants for surgery — Partial and total  
hip joint prostheses —**

**Part 1:**

**Classification and designation of dimensions  
(standards.iteh.ai)**

*Implants chirurgicaux — Prothèses partielles et totales de l'articulation de  
la hanche —*  
<https://standards.iteh.ai/catalog/standards/sist/6b800f46-12b5-451f-9546-0952na7514ac/iso-7206-1-1995>  
*Partie 1. Classification et désignation des dimensions*



Reference number  
ISO 7206-1:1995(E)

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

International Standard ISO 7206-1 was prepared by Technical Committee ISO/TC 150, *Implants for surgery*, Subcommittee SC 4, *Bone and joint replacements*.

This second edition cancels and replaces the first edition (ISO 7206-1:1985), of which it constitutes a technical revision.

ISO 7206 consists of the following parts, under the general title *Implants for surgery — Partial and total hip joint prostheses*:

- Part 1: *Classification and designation of dimensions*
- Part 2: *Articulating surfaces made of metallic, ceramic and plastics materials*
- Part 3: *Determination of endurance properties of stemmed femoral components without application of torsion*
- Part 4: *Determination of endurance properties of stemmed femoral components with application of torsion*
- Part 5: *Determination of resistance to static load of head and neck region of stemmed femoral components*
- Part 6: *Determination of endurance properties of head and neck region of stemmed femoral components*

© ISO 1995

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from the publisher.

International Organization for Standardization  
Case Postale 56 • CH-1211 Genève 20 • Switzerland

Printed in Switzerland

- *Part 7: Endurance performance of stemmed femoral components without application of torsion*
- *Part 8: Endurance performance of stemmed femoral components with application of torsion*
- *Part 9: Determination of resistance to torque of head fixation of stemmed femoral components*

**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

[ISO 7206-1:1995](https://standards.iteh.ai/catalog/standards/sist/6b800f46-12b5-451f-9546-f0952aa524ac/iso-7206-1-1995)

<https://standards.iteh.ai/catalog/standards/sist/6b800f46-12b5-451f-9546-f0952aa524ac/iso-7206-1-1995>

## Introduction

Partial and total hip joint prostheses are designed to transmit load and allow movement under high stress conditions. The task of preparing International Standards to cover all eventualities is complicated by the limited range of biologically suitable materials.

The purpose of this part of ISO 7206 and of other International Standards relating to joint prostheses is to provide direction in the control of manufacture and standard specifications for the different components of prostheses.

Attention is drawn to ISO 5839:1985, *Implants for surgery — Orthopaedic joint prostheses — Basic requirements*.

## iTeh STANDARD PREVIEW (standards.iteh.ai)

[ISO 7206-1:1995](https://standards.iteh.ai/catalog/standards/sist/6b800f46-12b5-451f-9546-f0952aa524ac/iso-7206-1-1995)

<https://standards.iteh.ai/catalog/standards/sist/6b800f46-12b5-451f-9546-f0952aa524ac/iso-7206-1-1995>

# Implants for surgery — Partial and total hip joint prostheses —

## Part 1:

### Classification and designation of dimensions

#### 1 Scope

This part of ISO 7206 specifies the means of classification and standardizes the designation of dimensions for partial and total hip joint prostheses.

It does not give a comprehensive description of modular and anatomic prostheses but can be used for the description of specific features of such prostheses.

ISO 7206-1:1995  
<https://standards.iteh.ai/catalog/standards/sist/6b800f46-12b5-451f-9546-f0952aa524ac/iso-7206-1-1995>

#### 2 Classification


Hip joint prostheses shall be classified as follows:

- a) femoral prosthesis (consisting of one or more components);
- b) acetabular prosthesis (consisting of one or more components);
- c) a combination of a) and b).

#### 3 Designation of dimensions

Dimensions of hip joint prostheses shall be designated in accordance with figures 1 to 6.


NOTE 1 Figures 1 to 6 are intended to be illustrative of typical hip joint prostheses and to designate dimensions, but representation of the components does not otherwise form part of this International Standard.

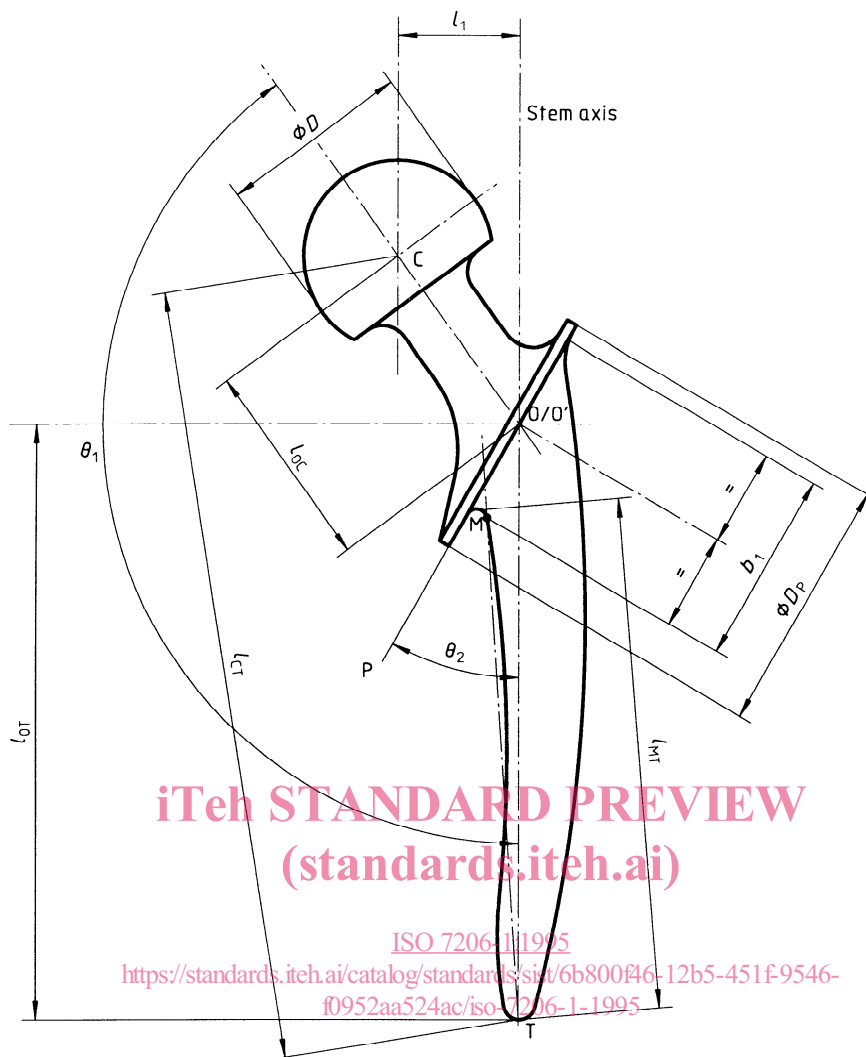

ISO 7206-1:1995  
<https://standards.iteh.ai/catalog/standards/sist/6b800f46-12b5-451f-9546-f0952aa524ac/iso-7206-1-1995>

- Key**
- C = head centre of curvature
  - CO' = neck axis of symmetry (O' is not necessarily coincident with O)
  - O = plateau stem centre (not necessarily coincident with O')
  - PO = plateau major axis
  - T = tip of stem
  - M = junction radius mid-point of medial side of stem with plateau
  - b<sub>1</sub> = width of stem adjoining plateau
  - D = head diameter
  - D<sub>p</sub> = mediolateral plateau diameter
  - l<sub>1</sub> = offset of head
  - l<sub>CT</sub> = length from head centre to tip of stem
  - l<sub>MT</sub> = medial stem length
  - l<sub>OC</sub> = neck length (OC) (not necessarily coincident with the neck axis)
  - l<sub>OT</sub> = stem length [length between tip and plateau (OT)]
  - θ<sub>1</sub> = neck angle (COT)
  - θ<sub>2</sub> = plateau angle (POT)
- Stem axis is the straight line from the centre of the stem tip in the intersection plane of the plateau  
 The stem axis mid-line is the straight line passing through the centres of two sections, 10 mm and 80 mm respectively from the tip (see figure 4)

**Figure 1 — Designation of dimensions of femoral components of hip joint prostheses with plateau**

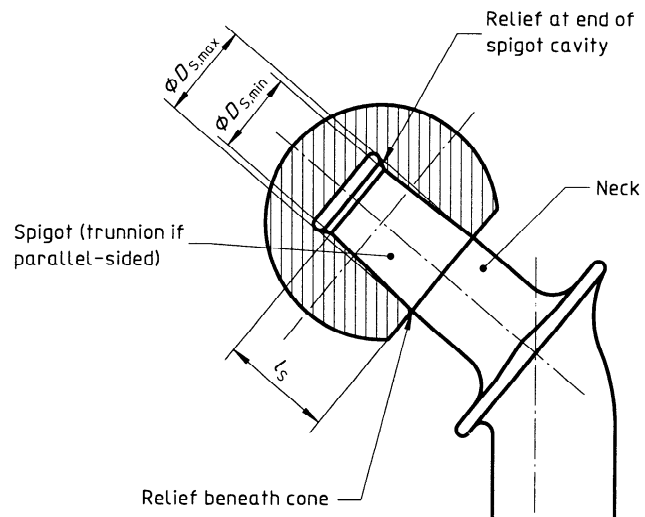

iTeh STANDARD PREVIEW  
(standards.iteh.ai)

**Key**

$D_{S,min}$  = spigot minimum diameter


$D_{S,max}$  = spigot maximum diameter

$l_S$  = spigot length

ISO 7206-1:1995  
<https://standards.iteh.ai/catalog/standards/sist/6b800f46-12b5-451f-9546-f0952aa524ac/iso-7206-1-1995>

**Figure 2 — Detail of head secured by spigot or trunnion** (alternative design of head)

Dimensions in millimetres

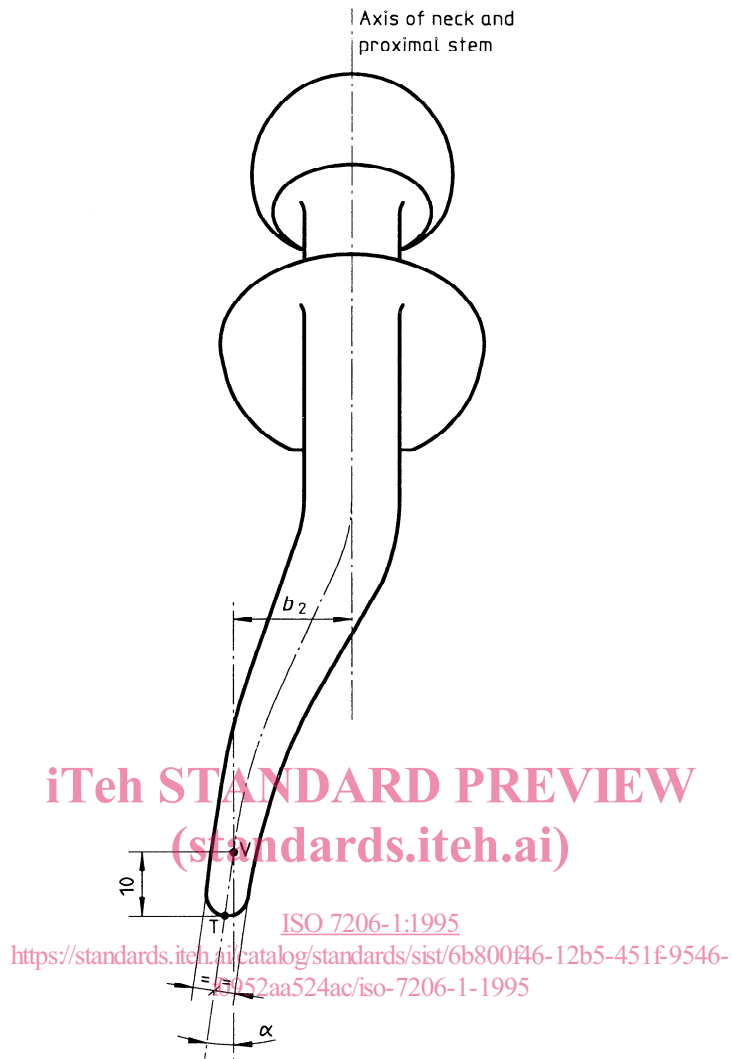


**Key**

- V = point on stem centreline 10 mm from T
- $b_2$  = offset of V from plane containing neck and proximal part of stem
- $\alpha$  = angle of stem distal end to centreline of neck and proximal stem

**Figure 3 — Lateral view of asymmetrical prosthesis illustrating dimensions required to specify antero/posterior offset**



Dimensions in millimetres

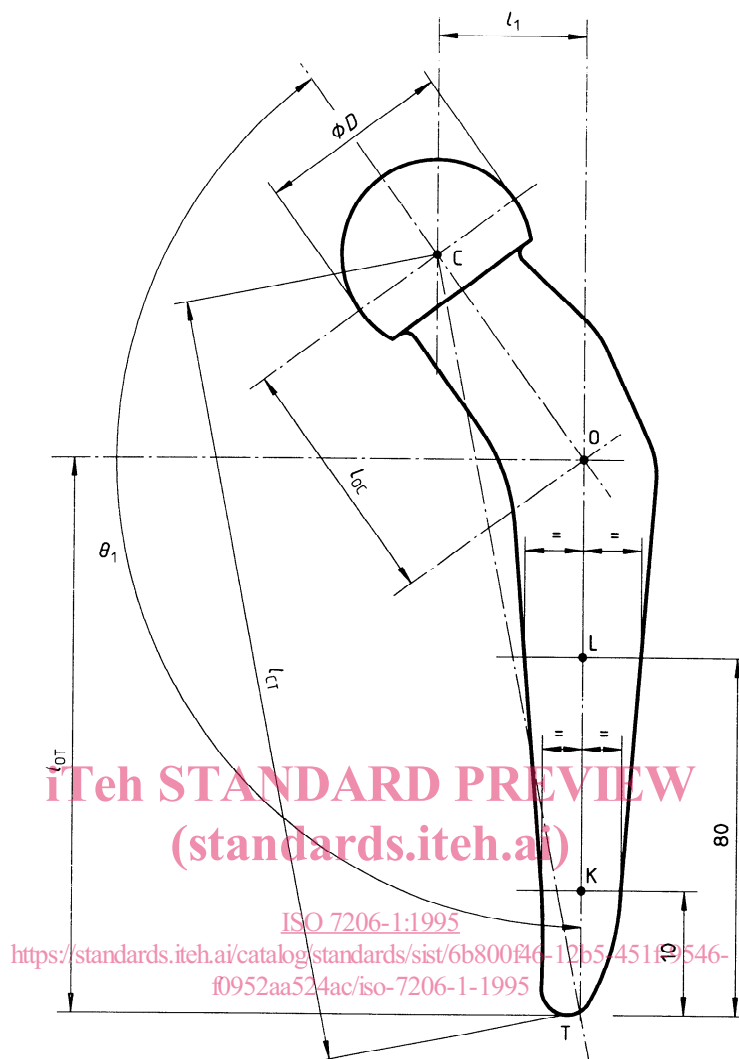**Key**

- C = head centre of curvature
- CO = neck nominal axis
- O = stem axis and midline intersection of neck nominal axis
- T = tip of stem
- KL = stem axis midline
- D = head diameter
- $l_1$  = offset of head
- $l_{CT}$  = length from head centre to tip of stem
- $l_{OC}$  = neck length (OC)
- $l_{OT}$  = effective stem length (OT)
- $\theta_1$  = neck angle (COL)

**Figure 4 — Designation of dimensions of femoral component of hip joint prostheses without plateau**