

INTERNATIONAL STANDARD



HORIZONTAL PUBLICATION

Electrostatics –
Part 2-1: Measurement methods – Ability of materials and products to dissipate static electric charge

[IEC 61340-2-1:2015](https://standards.iteh.ai/catalog/standards/sist/d1c2001d-0a89-49cb-91fe-a66919feecf/iec-61340-2-1-2015)

<https://standards.iteh.ai/catalog/standards/sist/d1c2001d-0a89-49cb-91fe-a66919feecf/iec-61340-2-1-2015>





THIS PUBLICATION IS COPYRIGHT PROTECTED
Copyright © 2022 IEC, Geneva, Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either IEC or IEC's member National Committee in the country of the requester. If you have any questions about IEC copyright or have an enquiry about obtaining additional rights to this publication, please contact the address below or your local IEC member National Committee for further information.

IEC Secretariat
3, rue de Varembe
CH-1211 Geneva 20
Switzerland

Tel.: +41 22 919 02 11
info@iec.ch
www.iec.ch

About the IEC

The International Electrotechnical Commission (IEC) is the leading global organization that prepares and publishes International Standards for all electrical, electronic and related technologies.

About IEC publications

The technical content of IEC publications is kept under constant review by the IEC. Please make sure that you have the latest edition, a corrigendum or an amendment might have been published.

IEC publications search - webstore.iec.ch/advsearchform

The advanced search enables to find IEC publications by a variety of criteria (reference number, text, technical committee, ...). It also gives information on projects, replaced and withdrawn publications.

IEC Products & Services Portal - products.iec.ch

Discover our powerful search engine and read freely all the publications previews. With a subscription you will always have access to up to date content tailored to your needs.

IEC Just Published - webstore.iec.ch/justpublished

Stay up to date on all new IEC publications. Just Published details all new publications released. Available online and once a month by email.

Electropedia - www.electropedia.org

The world's leading online dictionary on electrotechnology, containing more than 22 300 terminological entries in English and French, with equivalent terms in 19 additional languages. Also known as the International Electrotechnical Vocabulary (IEV) online.

IEC Customer Service Centre - webstore.iec.ch/csc

If you wish to give us your feedback on this publication or need further assistance, please contact the Customer Service Centre: sales@iec.ch.

[IEC 61340-2-1:2015](https://standards.iteh.ai/catalog/standards/sist/d1c2001d-0a89-49cb-91fe-a66919f6e6cf/iec-61340-2-1-2015)

<https://standards.iteh.ai/catalog/standards/sist/d1c2001d-0a89-49cb-91fe-a66919f6e6cf/iec-61340-2-1-2015>



IEC 61340-2-1

Edition 2.1 2022-06
CONSOLIDATED VERSION

INTERNATIONAL STANDARD



HORIZONTAL PUBLICATION

Electrostatics –
Part 2-1: Measurement methods – Ability of materials and products to dissipate static electric charge

IEC 61340-2-1:2015

<https://standards.iteh.ai/catalog/standards/sist/d1c2001d-0a89-49cb-91fe-a66919feecf/iec-61340-2-1-2015>

INTERNATIONAL
ELECTROTECHNICAL
COMMISSION

ICS 17.220.99; 29.020

ISBN 978-2-8322-3945-2

Warning! Make sure that you obtained this publication from an authorized distributor.

REDLINE VERSION



HORIZONTAL PUBLICATION

Electrostatics –
Part 2-1: Measurement methods – Ability of materials and products to dissipate static electric charge

IEC 61340-2-1:2015

<https://standards.iteh.ai/catalog/standards/sist/d1c2001d-0a89-49cb-91fe-a66919f6e6cf/iec-61340-2-1-2015>



CONTENTS

FOREWORD	4
INTRODUCTION	6
1 Scope	7
2 Normative references	7
3 Terms and definitions	8
4 Method of measurement of charge decay	9
4.1 Principles	9
4.2 Environmental conditions	9
4.3 Apparatus for measurement of corona charge decay	10
4.3.1 Physical design features	10
4.3.2 Containment of test material	11
4.3.3 Corona charge deposition	11
4.3.4 Fieldmeter	11
4.4 Apparatus for measurement of contact charge decay	12
4.4.1 Physical design features	12
4.4.2 Charge decay time (t_{SD})	13
5 Practical application of test methods and procedures	14
5.1 General	14
5.2 Charge decay test for textile materials	14
5.2.1 Selection of test method	14
5.2.2 Test surface preparation	14
5.2.3 Testing	15
5.2.4 Results	15
5.2.5 Test report	15
5.3 Charge decay test via gloves, finger cots or tools	16
5.3.1 Selection of test method	16
5.3.2 Common steps in testing	16
5.3.3 Test procedure for charge decay properties of finger cots as worn	16
5.3.4 Test procedure for the charge decay properties of gloves as worn	17
5.3.5 Test report for finger cots or gloves	17
5.3.6 Test procedure for the charge decay properties of tools	17
5.3.7 Test report for tools	20
5.4 Null test for CPM	20
Annex A (normative) Performance verification of measuring instrumentation	21
A.1 Verification of corona charge decay measuring instrumentation	21
A.1.1 Aspects to be verified	21
A.1.2 Surface potential sensitivity verification	21
A.1.3 Decay time verification	21
A.1.4 Verification procedure	21
A.2 Methods for verification of the capacitance of an isolated conductive plate	22
A.2.1 General	22
A.2.2 Capacitance meter method	22
A.2.3 Charge measuring method	22
A.2.4 Charge-sharing method	23
Bibliography	24

Figure 1 – Example of an arrangement for measurement of dissipation of charge using corona charging	10
Figure 2 – Example of an arrangement for measurement of dissipation of charge using a charged plate	12
Figure 3 – Charged plate detail	13
Figure 4 – Charge decay time (t_{sd}) and offset voltage (U_0)	14
Figure 5 – Examples of decay waveforms when testing tools	20
Figure A.1 – Equivalent circuit for CPM and reference capacitor	23

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[IEC 61340-2-1:2015](https://standards.iteh.ai/catalog/standards/sist/d1c2001d-0a89-49cb-91fe-a66919feecf/iec-61340-2-1-2015)

<https://standards.iteh.ai/catalog/standards/sist/d1c2001d-0a89-49cb-91fe-a66919feecf/iec-61340-2-1-2015>

INTERNATIONAL ELECTROTECHNICAL COMMISSION

ELECTROSTATICS –

Part 2-1: Measurement methods – Ability of materials and products to dissipate static electric charge

FOREWORD

- 1) The International Electrotechnical Commission (IEC) is a worldwide organization for standardization comprising all national electrotechnical committees (IEC National Committees). The object of IEC is to promote international co-operation on all questions concerning standardization in the electrical and electronic fields. To this end and in addition to other activities, IEC publishes International Standards, Technical Specifications, Technical Reports, Publicly Available Specifications (PAS) and Guides (hereafter referred to as “IEC Publication(s)”). Their preparation is entrusted to technical committees; any IEC National Committee interested in the subject dealt with may participate in this preparatory work. International, governmental and non-governmental organizations liaising with the IEC also participate in this preparation. IEC collaborates closely with the International Organization for Standardization (ISO) in accordance with conditions determined by agreement between the two organizations.
- 2) The formal decisions or agreements of IEC on technical matters express, as nearly as possible, an international consensus of opinion on the relevant subjects since each technical committee has representation from all interested IEC National Committees.
- 3) IEC Publications have the form of recommendations for international use and are accepted by IEC National Committees in that sense. While all reasonable efforts are made to ensure that the technical content of IEC Publications is accurate, IEC cannot be held responsible for the way in which they are used or for any misinterpretation by any end user.
- 4) In order to promote international uniformity, IEC National Committees undertake to apply IEC Publications transparently to the maximum extent possible in their national and regional publications. Any divergence between any IEC Publication and the corresponding national or regional publication shall be clearly indicated in the latter.
- 5) IEC itself does not provide any attestation of conformity. Independent certification bodies provide conformity assessment services and, in some areas, access to IEC marks of conformity. IEC is not responsible for any services carried out by independent certification bodies.
- 6) All users should ensure that they have the latest edition of this publication.
- 7) No liability shall attach to IEC or its directors, employees, servants or agents including individual experts and members of its technical committees and IEC National Committees for any personal injury, property damage or other damage of any nature whatsoever, whether direct or indirect, or for costs (including legal fees) and expenses arising out of the publication, use of, or reliance upon, this IEC Publication or any other IEC Publications.
- 8) Attention is drawn to the Normative references cited in this publication. Use of the referenced publications is indispensable for the correct application of this publication.
- 9) Attention is drawn to the possibility that some of the elements of this IEC Publication may be the subject of patent rights. IEC shall not be held responsible for identifying any or all such patent rights.

This consolidated version of the official IEC Standard and its amendment has been prepared for user convenience.

IEC 61340-2-1 edition 2.1 contains the second edition (2015-08) [documents 101/446/CDV and 101/462/RVC] and its amendment 1 (2022-06) [documents 101/639/CDV and 101/651/RVC].

In this Redline version, a vertical line in the margin shows where the technical content is modified by amendment 1. Additions are in green text, deletions are in strikethrough red text. A separate Final version with all changes accepted is available in this publication.

International Standard IEC 61340-2-1 has been prepared by IEC technical committee 101: Electrostatics.

This second edition constitutes a technical revision.

This edition includes the following significant technical changes with respect to the previous edition:

- a) the first edition supported requirements in IEC TR 61340-5-1, but with the revision of IEC TR 61340-5-1 into an International Standard, this support is no longer required; references to IEC 61340-5-1[1]¹ have been removed;
- b) the introduction gives additional information on when charge decay time measurements are appropriate, and the applications for which each of the two test methods are best suited;
- c) procedures for performance verification of measuring instruments for the corona charging method have been added.

This publication has been drafted in accordance with the ISO/IEC Directives, Part 2.

It has the status of a horizontal standard in accordance with IEC Guide 108[3].

A list of all the parts in the IEC 61340 series, published under the general title *Electrostatics*, can be found on the IEC website.

The committee has decided that the contents of the base publication and its amendment will remain unchanged until the stability date indicated on the IEC web site under webstore.iec.ch in the data related to the specific publication. At this date, the publication will be

- reconfirmed,
- withdrawn,
- replaced by a revised edition, or
- amended.

IMPORTANT – The 'colour inside' logo on the cover page of this publication indicates that it contains colours which are considered to be useful for the correct understanding of its contents. Users should therefore print this document using a colour printer.

¹ Numbers in square brackets refer to the Bibliography.

INTRODUCTION

Measurements of the rate of dissipation of static charge belong to the essential measurement techniques in the field of electrostatics.

For homogeneous conductive materials, this property can be evaluated indirectly by measuring resistance or resistivity parameters. Care should be exercised when determining the homogeneity of materials, as some materials that appear homogenous do exhibit non-homogeneous electrical characteristics. If the homogeneity of materials is not known and cannot be otherwise verified, it is possible that resistance measurements ~~may~~ will not be reliable or ~~may~~ will not give enough information. It is also possible that resistance measurements ~~may also~~ will not be reliable when evaluating materials in the dissipative or insulative range and especially for high ohmic materials ~~including~~ that include conductive fibres (e.g. textiles with a metallic grid). In such cases, the rate of dissipation of static charge should be measured directly.

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[IEC 61340-2-1:2015](#)

<https://standards.iteh.ai/catalog/standards/sist/d1c2001d-0a89-49cb-91fe-a66919feecf/iec-61340-2-1-2015>

ELECTROSTATICS –

Part 2-1: Measurement methods – Ability of materials and products to dissipate static electric charge

1 Scope

This part of IEC 61340 describes test methods for measuring the rate of dissipation of static charge of insulating and static dissipative materials and products.

It includes a generic description of test methods and detailed test procedures for specific applications.

The two test methods for measuring charge decay time, one using corona charging and one using a charged metal plate are different and it is possible that they ~~may~~ will not give equivalent results. Nevertheless, each method has a range of applications for which it is best suited. The corona charging method is suitable for evaluating the ability of materials, ~~e.g.~~ for example textiles, packaging, ~~etc.~~ to dissipate charge from their own surfaces. The charged metal plate method is suitable for evaluating the ability of materials and objects such as gloves, finger cots, hand tools, ~~etc.~~ to dissipate charge from conductive objects placed on or in contact with them. It is possible that the charged plate method ~~may~~ will not be suitable for evaluating the ability of materials to dissipate charge from their own surfaces.

In addition to its general application, this horizontal standard is also intended for use by technical committees in the preparation of standards in accordance with the principles laid down in IEC Guide 108.

61340-2-1-2015

One of the responsibilities of a technical committee is, wherever applicable, to make use of horizontal standards in the preparation of its publications. The contents of this horizontal standard shall not apply unless specifically referred to or included in the relevant publications.

2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

IEC 61010-1, *Safety requirements for electrical equipment for measurement, control, and laboratory use – Part 1: General requirements*

IEC 61010-2-030, *Safety requirements for electrical equipment for measurement, control, and laboratory use – Part 2-030: Particular requirements for equipment having testing or measuring circuits*

IEC 61340-4-6, *Electrostatics – Part 4-6: Standard test methods for specific applications – Wrist straps*

IEC 61340-4-7, *Electrostatics – Part 4-7: Standard test methods for specific applications – Ionization*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

3.1

charge decay

migration of charge across or through a material leading to a reduction of charge density or surface potential at the area where the charge was deposited

3.2

charge decay time

time from an initial voltage to a set fraction of the initial voltage

Note 1 to entry: $1/e$ and 10 % are appropriate fractions (e is the base of natural logarithms, equal to 2,718). If the initial voltage is low, the accuracy of decay time measurements to a small fraction of the initial voltage ~~may~~ can be susceptible to the noise level of the fieldmeter.

3.3

charged plate monitor

CPM

instrument using a charged metal plate of a defined capacitance and geometry which is discharged in order to measure charge dissipation/neutralization properties of products or materials

Note 1 to entry: This note only applies to the French language.

3.4

corona

corona discharge

generation of ions of either polarities by a high electric field

3.5

static dissipative material

material which allows charge to migrate over its surface and/or through its volume in a time which is short compared to the time scale of the actions creating the charge, or short compared to the time within which this charge will cause an electrostatic problem

Note 1 to entry: Materials that ~~may be~~ are considered conductive in other contexts are included within this definition for the purposes of this part of IEC 61340.

3.6

initial voltage

< corona charge decay > surface potential at a time after the end of charge deposition that is a sensible match to the time it takes material surfaces to separate in practical situations

Note 1 to entry: A time of 100 ms is appropriate for manual tribocharging actions.

3.7

initial voltage

<contact charge decay > voltage applied to the conductive plate of a charged plate monitor

3.8

insulator

material with very low mobility of charge so that any charge on the surface will remain there for a time which is long compared to the time scale of the actions creating the charge

4 Method of measurement of charge decay

4.1 Principles

Two methods are described.

The first method determines the dissipation of charge deposited on the surface of the material by a corona discharge. The resulting decrease in surface potential is observed using a fieldmeter or other equivalent equipment. This method is applicable to measurement of charge dissipation from surfaces and materials.

The second method determines the dissipation of charge from a charged plate through an object under test by applying a potential to the metallic plate, disconnecting the voltage source and observing the decrease in potential of the plate by means of a fieldmeter or other equivalent equipment. This method is applicable to measurement of charge dissipation via products such as finger cots, gloves and hand tools.

NOTE There are more methods to charge materials other than the charging methods described here (for example tribocharging or inductive charging) but they are not relevant for this standard.

CAUTION WARNING – The test methods specified in this ~~International Standard~~ document involve the use of high-voltage power supplies that ~~may~~ can present hazards if handled incorrectly, particularly by unqualified or inexperienced personnel. Users of this ~~International Standard~~ document are encouraged to carry out proper risk assessments and pay due regard to local regulations before undertaking any of the test procedures. Electrical equipment for measurements shall comply with the safety requirements specified in IEC 61010-1 and IEC 61010-2-030.

4.2 Environmental conditions

The electrical properties of materials vary with temperature and the absorption of moisture.


Unless otherwise agreed, the atmosphere for conditioning and testing shall be (23 ± 2) °C and (12 ± 3) % relative humidity, and the conditioning time prior to testing shall be at least 48 h.

For measurements in practical situations the ambient temperature and relative humidity shall be recorded.

4.3 Apparatus for measurement of corona charge decay

4.3.1 Physical design features

Dimensions in millimetres with a tolerance of ± 1 mm.

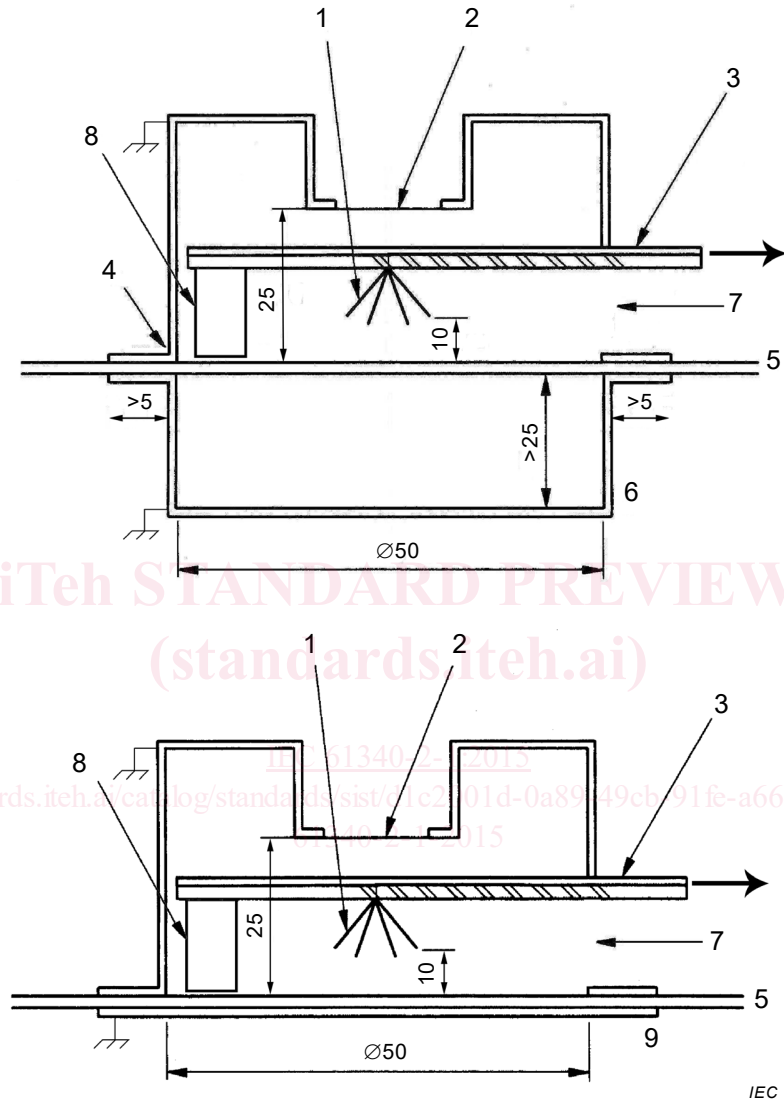

Key

- | | |
|--|---|
| 1 Array of corona points, the tips of which form a circle (10 ± 1) mm in diameter | 5 Sample |
| 2 Fieldmeter sensing aperture | 6 Metal plate (open backing) |
| 3 Movable plate:
– insulating plate to mount corona points (resistance to ground $> 10^{14} \Omega$)
– earthed top surface to shield fieldmeter | 7 Aperture through which the movable plate is withdrawn |
| 4 Earthed casing | 8 Air dam |
| | 9 Metal plate (earthed backing) |

Figure 1 – Example of an arrangement for measurement of dissipation of charge using corona charging

A typical arrangement and relevant dimensions of the test apparatus are shown in Figure 1. Other equipment giving similar results may be used.

The test aperture for deposition and measurement of deposited charge shall be (50 ± 1) mm diameter or an equivalent area quasi-square aperture. An array of corona points is mounted on a movable plate above the centre of the test aperture. The fieldmeter sensing aperture shall be (25 ± 1) mm above the centre of the test area. When the plate with the corona points is moved fully away, the test area shall be clear up to the plane of the fieldmeter sensing aperture.

4.3.2 Containment of test material

With an installed material, the test aperture in the instrument base plate shall rest directly on its surface. Sheet or flexible materials shall be supported as follows:

- a) for testing materials with open backing, the material shall be rested against an earthed metal plate with an aperture aligned with the instrument test aperture and with a width of at least 5 mm extending beyond the aperture. A shield over the reverse side of the test area shall be earthed and be at least 25 mm away over the whole test area;
- b) for testing materials against an earthed backing, the material shall be mounted between the instrument base plate and a flat earthed metal plate.

NOTE If charge moves more readily through the bulk test material than across its surface, then placing an earthed metal plate immediately behind the test area can increase the rate of charge dissipation. On the other hand, if charge moves more readily across the surface of the test material, then the rate of charge dissipation can decrease if an earthed metal plate is used because its presence will increase the capacitive loading. To gain a full understanding of charge dissipation from the test material, it is desirable to make measurements both with and without an earthed metal plate backing the test area.

In practical terms, earthed backing represents a material in intimate contact with an earthed surface, for example, a garment fitted close to the body of the wearer, or a work surface on top of a metal bench. Open-backed measurements represent the other practical extreme where materials are separated from earthed surfaces, for example, the bottom edge of a coat or smock which hangs away from the body of the wearer.

4.3.3 Corona charge deposition

Corona charging is achieved with at least five corona points, the tips of which form a (10 ± 1) mm diameter circle, (10 ± 1) mm above the centre of the test area. The corona points shall be made from non-corrosive metal wire of a diameter in the range 0,1 mm to 0,5 mm. The exact size and distribution of charge on the material is not well defined, particularly with the more conductive surfaces, but the arrangement provides a consistent pattern of deposited charge and decay time measurements.

NOTE 1 Typical voltages for corona charging equipment are between 5 kV and 10 kV.

The corona duration shall be no more than 50 ms, and 10 ms or 20 ms is usually appropriate in order to achieve an adequate initial peak voltage for measurements. Excessively long deposition times (more than some seconds) ~~may~~ can damage the material.

The materials shall be tested with positive and negative polarity.

The equipment for charge deposition shall move fully away from the region of fieldmeter observation in less than 20 ms.

NOTE 2 For corona voltages of 7 kV to 8 kV, the initial surface voltage with relatively high insulating materials will be up to about 3 kV. For materials with fast charge decay rates the initial voltage can be much lower – for example only 50 V to 100 V.

4.3.4 Fieldmeter

The fieldmeter shall be able to measure the surface voltage with an accuracy of ± 5 V to below the lower limit of surface voltage that is required to be measured. The response time (10 % to 90 %) shall be at least one-tenth of the faster decay time required to be measured. The stability of the zero shall allow measurement of surface voltage with this accuracy over the longest decay times to be measured. Therefore, a rotating vane 'field mill' type of fieldmeter is preferred.