

SLOVENSKI STANDARD**SIST EN 14397-2:2005****01-januar-2005**

; bc Č U]b`gfYXghj UnUUbdbYbY ē 8 c`c Yj UbYc[`1_cj Y[UX]c_g]XU ē &"XY.
A YtçXU nUgfYXghj UnUUbdbYbY

Fertilizers and liming materials - Determination of carbon dioxide - Part 2: Method for liming materials

Düngemittel und Calcium-/Magnesium-Bodenverbesserungsmittel - Bestimmung von Kohlenstoffdioxid - Teil 2: Verfahren für Calcium-/Magnesium-Bodenverbesserungsmittel

SIST EN STANDARD PREVIEW

(standards.iteh.ai)

Engrais et amendements minéraux basiques - Détermination de la teneur en dioxyde de carbone - Partie 2: Méthode pour amendements minéraux basiques

SIST EN 14397-2:2005

<https://standards.iteh.ai/catalog/standards/sist/13c5ff3c-1c22-4ea7-bbe5-f001e60ad376/sist-en-14397-2-2005>

Ta slovenski standard je istoveten z: EN 14397-2:2004

ICS:

65.080

Gnojila

Fertilizers

SIST EN 14397-2:2005**en,fr,de**

iTeh STANDARD PREVIEW
(standards.iteh.ai)

SIST EN 14397-2:2005

<https://standards.iteh.ai/catalog/standards/sist/13c5ff3c-1c22-4ea7-bbe5-f001e60ad376/sist-en-14397-2-2005>

EUROPEAN STANDARD
NORME EUROPÉENNE
EUROPÄISCHE NORM

EN 14397-2

July 2004

ICS 65.080

English version

**Fertilizers and liming materials - Determination of carbon dioxide
- Part 2: Method for liming materials**

Engrais et amendements minéraux basiques -
Détermination de la teneur en dioxyde de carbone - Partie
2: Méthode applicable aux amendements minéraux
basiques

Düngemittel und Calcium-/Magnesium-
Bodenverbesserungsmittel - Bestimmung von
Kohlenstoffdioxid - Teil 2: Verfahren für Calcium-
/Magnesium-Bodenverbesserungsmittel

This European Standard was approved by CEN on 1 April 2004.

CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration. Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the Central Secretariat or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the Central Secretariat has the same status as the official versions.

(standards.iteh.ai)

CEN members are the national standards bodies of Austria, Belgium, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Slovakia, Slovenia, Spain, Sweden, Switzerland and United Kingdom.

<https://standards.iteh.ai/catalog/standards/sist/13c5f3c-1c22-4ea7-bbe5-f001e60ad376/sist-en-14397-2-2005>



EUROPEAN COMMITTEE FOR STANDARDIZATION
COMITÉ EUROPÉEN DE NORMALISATION
EUROPÄISCHES KOMITEE FÜR NORMUNG

Management Centre: rue de Stassart, 36 B-1050 Brussels

Contents

| | |
|--------------------------------------|-----------|
| Foreword | 3 |
| 1 Scope | 4 |
| 2 Normative references | 4 |
| 3 Terms and definitions | 4 |
| 4 Principle | 4 |
| 5 Reagents | 4 |
| 6 Apparatus | 5 |
| 7 Sampling | 7 |
| 8 Procedure | 7 |
| 9 Expression of results | 8 |
| 10 Precision | 8 |
| 11 Test report | 9 |
| Bibliography | 10 |

iTeh STANDARD PREVIEW

(standards.iteh.ai)

SIST EN 14397-2:2005

<https://standards.iteh.ai/catalog/standards/sist/13c5ff3c-1c22-4ea7-bbe5-f001e60ad376/sist-en-14397-2-2005>

Foreword

This document (EN 14397-2:2004) has been prepared by Technical Committee CEN/TC 260 "Fertilizers and liming materials", the secretariat of which is held by DIN.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by January 2005, and conflicting national standards shall be withdrawn at the latest by January 2005.

EN 14397 "Fertilizers and liming materials — Determination of carbon dioxide" consists of two parts:

- *Part 1: Method for solid fertilizers (prCEN/TS 14397-1)*
- *Part 2: Method for liming materials*

According to the CEN/CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Slovakia, Slovenia, Spain, Sweden, Switzerland and United Kingdom.

iTeh STANDARD PREVIEW (standards.iteh.ai)

SIST EN 14397-2:2005

<https://standards.iteh.ai/catalog/standards/sist/13c5ff3c-1c22-4ea7-bbe5-f001e60ad376/sist-en-14397-2-2005>

EN 14397-2:2004 (E)

1 Scope

This document specifies a method for the determination of carbon dioxide in all liming materials.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

EN 1482, *Sampling of solid fertilizers and liming materials*.

EN 12944-3:2001, *Fertilizers and liming materials — Vocabulary — Part 3: Terms relating to liming materials*.

EN ISO 3696, *Water for analytical laboratory use — Specification and test methods (ISO 3696:1987)*.

3 Terms and definitions

For the purposes of this document, the terms and definitions given in EN 12944-3:2001 apply.

iTeh STANDARD PREVIEW
(standards.iteh.ai)

4 Principle

The carbon dioxide contained in liming materials in the form of carbonates is liberated by reaction with hydrochloric acid and determined volumetrically.

5 Reagents

5.1 General

During the analysis, unless otherwise stated, use only reagents of recognized analytical grade and water conforming to grade 3 in accordance with EN ISO 3696.

5.2 Concentrated hydrochloric acid, ρ_{20} (HCl) = 1,18 g/ml to 1,19 g/ml

5.3 Diluted hydrochloric acid, ρ_{20} (HCl) = 1,09 g/ml

Dilute one part by volume of concentrated hydrochloric acid (5.2) with one part by volume of water.

5.4 Concentrated sulfuric acid, ρ_{20} (H₂SO₄) = 1,84 g/ml

5.5 Sodium sulfate, Na₂SO₄

5.6 Sealing liquid

Add 20 g of sodium sulfate (5.5) and 5 ml of concentrated sulfuric acid (5.4) to water and make up to 100 ml. Colour with a few drops of methyl red solution (5.8). The sealing liquid shall be saturated with carbon dioxide.

5.7 Ethanol, w (C_2H_5OH) = 95,6 % (mass fraction)

5.8 Methyl red solution

Dissolve 0,1 mg of methyl red in 50 ml of ethanol (5.7). Dilute with water up to 100 ml and homogenize.

5.9 Potassium hydroxide solution, w (KOH) = 50 % (mass fraction)

5.10 Calcium carbonate, $CaCO_3$, pre-dried to constant mass at 250 °C

5.11 Copper sulfate, $CuSO_4 \cdot 5 H_2O$

6 Apparatus

6.1 Apparatus for liberation and determination of carbon dioxide as shown in Figure 1

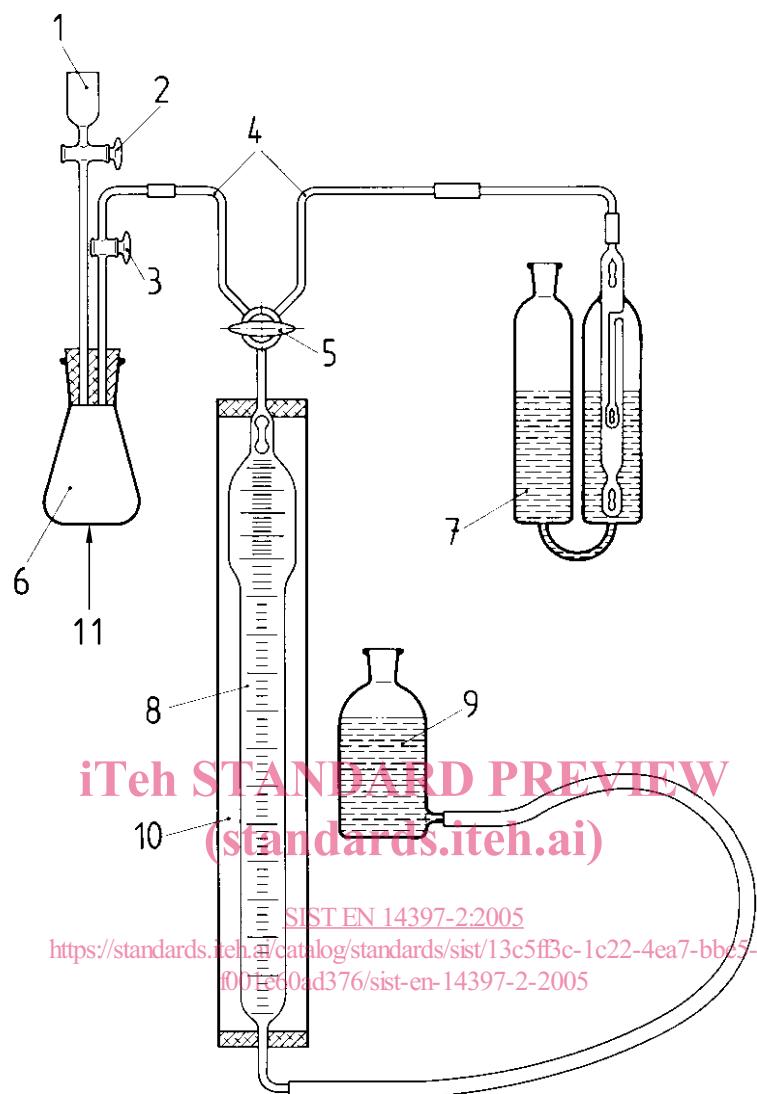
6.2 Laboratory balance capable of weighing to the nearest 0,0001 g

6.3 Heating device, electrical or gas-burning

iTeh STANDARD PREVIEW
(standards.iteh.ai)

SIST EN 14397-2:2005

<https://standards.iteh.ai/catalog/standards/sist/13c5ff3c-1c22-4ea7-bbe5-f001e60ad376/sist-en-14397-2-2005>

**Key**

- 1 Dropping funnel with a volume of 25 ml
- 2 Stopcock 1
- 3 Stopcock 2
- 4 Capillary tubes
- 5 Three-way tap
- 6 Heated decomposition flask with a volume of 50 ml
- 7 Absorption vessel with a volume of 100 ml containing KOH solution
- 8 Measuring burette with a volume of 100 ml
- 9 Levelling bottle with a volume of 200 ml containing sealing liquid
- 10 Tube filled with water
- 11 Heating device

Figure 1 — Apparatus for liberation and determination of carbon dioxide

7 Sampling

Sample the liming material in accordance with EN 1482.

8 Procedure

8.1 Test portion

The test portion used depends on the expected carbon dioxide content and shall be chosen according to Table 1.

Table 1 — Test portion

| Expected carbon dioxide content mass fraction | Test portion g |
|--|-------------------|
| > 15 % ≤ 50 % | 0,1 |
| > 10 % ≤ 15 % | 0,3 |
| > 5 % ≤ 10 % | 0,5 |
| > 2 % ≤ 5 % | 1,0 |
| 0 % ≤ 2 % | 2,0 |

8.2 Determination

(standards.iteh.ai)

Weigh the test portion (8.1) to the nearest 0,1 mg into the decomposition flask. Bond any hydrogen sulfide formed by adding a spatula-tip of copper sulfate (5.11) and suspend in a little water.

<https://standards.iteh.ai/catalog/standards/sist/13c5ff3c-1c22-4ea7-bbe5-001e9ad176/ist-en-14397-2-2005>

Connect the decomposition flask to the rest of the apparatus (see Figure 1) with a double-bored stopper. A dropping funnel and the feed tube to the measuring burette pass through the stopper. Open the stopcocks in these two lines. Bring the three-way tap to the position such that it connects the flask and measuring burette with one another. Fill the burette with sealing liquid (5.6) up to the three-way tap by raising the levelling bottle. Now close stopcock 1 and fill the funnel with diluted hydrochloric acid (5.3). Add diluted hydrochloric acid (5.3) to the flask through the dropping funnel until the flask is half full. With stopcock 1 closed a little acid remains as sealing liquid in the funnel.

Allow the mixture to react for about 3 min and then heat it to the boiling point and boil for about 3 min. Fill the decomposition flask completely with diluted hydrochloric acid (5.3) up to stopcock 2 through the dropping funnel to transfer the remaining gas mixture into the burette. Take care that no diluted hydrochloric acid overflows. Close the burette with the three-way tap. After about 5 min, bring the sealing liquid (5.6) in the burette and in the levelling bottle to the same level and record the gas volume V_1 .

Turn the three-way tap to connect the measuring burette with the absorption vessel and wash out the air-carbon dioxide-mixture collected. For this, raise the levelling bottle so that all the gas is forced through the potassium hydroxide solution (5.9) in the absorption vessel. The carbon dioxide is thereby absorbed. Repeat the absorption operation by raising the levelling bottle seven or eight times until, finally, the measuring burette contains only the residual gas. Close the three-way tap, bring the sealing liquid (5.6) in the burette and in the levelling bottle to the same level and record the gas volume V_2 .

NOTE The volume difference $V_1 - V_2$ corresponds to the carbon dioxide content of the sample.

8.3 Calibration of the apparatus

Weigh 0,1 g of calcium carbonate (5.10) to the nearest 0,0001 g into the decomposition flask (see Figure 1). Carry out the determination as described in 8.2.

NOTE The volume difference $V_3 - V_4$ corresponds to the carbon dioxide content of the calibration material.