



# SLOVENSKI STANDARD SIST EN ISO 18856:2005

01-december-2005

---

Water quality - Determination of selected phthalates using gas chromatography/mass spectrometry (ISO 18856:2004)

Wasserbeschaffenheit - Bestimmung ausgewählter Phthalate mittels Gaschromatographie/Massenspektrometrie (ISO 18856:2004)

Qualité de l'eau - Dosage de certains phtalates par chromatographie en phase gazeuse/spectrométrie de masse (ISO 18856:2004)

Ta slovenski standard je istoveten z: EN ISO 18856:2005

---

## ICS:

13.060.50 Examination of water for chemical substances

SIST EN ISO 18856:2005

en,fr,de

**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

[SIST EN ISO 18856:2005](#)

<https://standards.iteh.ai/catalog/standards/sist/f7e4dcc2-6cd2-47a7-9c78-6a831c04ca99/sist-en-iso-18856-2005>

EUROPEAN STANDARD

EN ISO 18856

NORME EUROPÉENNE

EUROPÄISCHE NORM

August 2005

ICS 13.060.50

English Version

## Water quality - Determination of selected phthalates using gas chromatography/mass spectrometry (ISO 18856:2004)

Qualité de l'eau - Dosage de certains phtalates par chromatographie en phase gazeuse/spectrométrie de masse (ISO 18856:2004)

Wasserbeschaffenheit - Bestimmung ausgewählter Phthalate mittels Gaschromatographie/Massenspektrometrie (ISO 18856:2004)

This European Standard was approved by CEN on 20 July 2005.

CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration. Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the Central Secretariat or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the Central Secretariat has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Slovakia, Slovenia, Spain, Sweden, Switzerland and United Kingdom.

<https://standards.iteh.ai/catalog/standards/sist/17e4dcc2-6cd2-47a7-9c78-6a831c04ca99/sist-en-iso-18856-2005>



EUROPEAN COMMITTEE FOR STANDARDIZATION  
COMITÉ EUROPÉEN DE NORMALISATION  
EUROPÄISCHES KOMITEE FÜR NORMUNG

Management Centre: rue de Stassart, 36 B-1050 Brussels

**EN ISO 18856:2005 (E)****Foreword**

The text of ISO 18856:2004 has been prepared by Technical Committee ISO/TC 147 "Water quality" of the International Organization for Standardization (ISO) and has been taken over as EN ISO 18856:2005 by Technical Committee CEN/TC 230 "Water analysis", the secretariat of which is held by DIN.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by February 2006, and conflicting national standards shall be withdrawn at the latest by February 2006.

According to the CEN/CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Slovakia, Slovenia, Spain, Sweden, Switzerland and United Kingdom.

**Endorsement notice**

The text of ISO 18856:2004 has been approved by CEN as EN ISO 18856:2005 without any modifications.

**(standards.iteh.ai)**

[SIST EN ISO 18856:2005](https://standards.iteh.ai/catalog/standards/sist/f7e4dcc2-6cd2-47a7-9c78-6a831c04ca99/sist-en-iso-18856-2005)

<https://standards.iteh.ai/catalog/standards/sist/f7e4dcc2-6cd2-47a7-9c78-6a831c04ca99/sist-en-iso-18856-2005>

# INTERNATIONAL STANDARD

**ISO**  
**18856**

First edition  
2004-09-15

---

---

## Water quality — Determination of selected phthalates using gas chromatography/mass spectrometry

*Qualité de l'eau — Dosage de certains phtalates par chromatographie  
en phase gazeuse/spectrométrie de masse*

**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

[SIST EN ISO 18856:2005](https://standards.iteh.ai/catalog/standards/sist/f7e4dcc2-6cd2-47a7-9c78-6a831c04ca99/sist-en-iso-18856-2005)

<https://standards.iteh.ai/catalog/standards/sist/f7e4dcc2-6cd2-47a7-9c78-6a831c04ca99/sist-en-iso-18856-2005>



Reference number  
ISO 18856:2004(E)

© ISO 2004

**ISO 18856:2004(E)****PDF disclaimer**

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

## iTeh STANDARD PREVIEW (standards.iteh.ai)

[SIST EN ISO 18856:2005](https://standards.iteh.ai/catalog/standards/sist/f7e4dcc2-6cd2-47a7-9c78-6a831c04ca99/sist-en-iso-18856-2005)

<https://standards.iteh.ai/catalog/standards/sist/f7e4dcc2-6cd2-47a7-9c78-6a831c04ca99/sist-en-iso-18856-2005>

© ISO 2004

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Case postale 56 • CH-1211 Geneva 20  
Tel. + 41 22 749 01 11  
Fax + 41 22 749 09 47  
E-mail [copyright@iso.org](mailto:copyright@iso.org)  
Web [www.iso.org](http://www.iso.org)

Published in Switzerland

## Contents

Page

Foreword.....	iv
Introduction .....	v
1 Scope.....	1
2 Normative references .....	2
3 Principle .....	2
4 Interferences.....	3
5 Reagents .....	3
6 Apparatus.....	5
7 Sampling and sample pre-treatment.....	7
8 Procedure.....	7
9 Calibration.....	10
10 Calculation .....	13
11 Expression of results.....	15
12 Precision .....	15
13 Test report.....	15
Annex A (informative) List of phthalates.....	16
Annex B (informative) General remarks.....	18
Annex C (normative) Precision data.....	19
Annex D (informative) Examples of solutions (overview) .....	22
Annex E (informative) Example of equipment to avoid contaminations.....	25
Annex F (informative) Examples of suitable capillary columns .....	29
Annex G (informative) Example of gas chromatographic conditions .....	30
Bibliography .....	32

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 18856 was prepared by Technical Committee ISO/TC 147, *Water quality*, Subcommittee SC 2, *Physical, chemical and biochemical methods*.

## iTeh STANDARD PREVIEW (standards.iteh.ai)

[SIST EN ISO 18856:2005](https://standards.iteh.ai/catalog/standards/sist/f7e4dcc2-6cd2-47a7-9c78-6a831c04ca99/sist-en-iso-18856-2005)

<https://standards.iteh.ai/catalog/standards/sist/f7e4dcc2-6cd2-47a7-9c78-6a831c04ca99/sist-en-iso-18856-2005>



## Introduction

The user should be aware that particular problems could require the specification of additional marginal conditions.

# iTeh STANDARD PREVIEW (standards.iteh.ai)

[SIST EN ISO 18856:2005](https://standards.iteh.ai/catalog/standards/sist/f7e4dcc2-6cd2-47a7-9c78-6a831c04ca99/sist-en-iso-18856-2005)

<https://standards.iteh.ai/catalog/standards/sist/f7e4dcc2-6cd2-47a7-9c78-6a831c04ca99/sist-en-iso-18856-2005>

**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

[SIST EN ISO 18856:2005](#)

<https://standards.iteh.ai/catalog/standards/sist/f7e4dcc2-6cd2-47a7-9c78-6a831c04ca99/sist-en-iso-18856-2005>

# Water quality — Determination of selected phthalates using gas chromatography/mass spectrometry

**WARNING** — Persons using this International Standard should be familiar with normal laboratory practice. This International Standard does not purport to address all of the safety problems, if any, associated with its use. It is the responsibility of the user to establish appropriate safety and health practices and to ensure compliance with any national regulatory conditions.

**IMPORTANT** — It is absolutely essential that tests conducted according to this International Standard be carried out by suitably trained staff.

## 1 Scope

This International Standard specifies a method for the determination of phthalates in water after solid phase extraction and gas chromatography/mass spectrometry.

This method is applicable to the determination of phthalates (see Table 1) in ground water, surface water, wastewater and drinking water in mass concentrations ranging from above 0,02 µg/l up to 0,150 µg/l, depending on the individual substance and the value of the blank.

The applicability of this method to other phthalates not specified in Table 1 is not excluded, but it is necessary to determine its applicability in each case (see Annex A for the list of phthalates).

General remarks concerning the recovery and use of internal standards is given in Annex B.

**Table 1 — Phthalates determined by this method**

No	Name	Formula	Abbreviation	Molar mass g/mol	CAS <sup>a</sup> number
1	Dimethyl phthalate	C <sub>10</sub> H <sub>10</sub> O <sub>4</sub>	DMP	194,2	131-11-3
2	Diethyl phthalate	C <sub>12</sub> H <sub>14</sub> O <sub>4</sub>	DEP	222,24	84-66-2
3	Dipropyl phthalate	C <sub>14</sub> H <sub>18</sub> O <sub>4</sub>	DPP	250,3	131-16-8
4	Diisobutyl phthalate	C <sub>16</sub> H <sub>22</sub> O <sub>4</sub>	DiBP	278,4	84-69-5
5	Dibutyl phthalate	C <sub>16</sub> H <sub>22</sub> O <sub>4</sub>	DBP	278,4	84-74-2
6	Butyl benzyl phthalate	C <sub>19</sub> H <sub>20</sub> O <sub>4</sub>	BBzP	312,4	85-68-7
7	Dicyclohexyl phthalate	C <sub>20</sub> H <sub>26</sub> O <sub>4</sub>	DCHP	330,4	84-61-7
8	Di(2-ethylhexyl) phthalate	C <sub>24</sub> H <sub>38</sub> O <sub>4</sub>	DEHP	390,6	117-81-7
9	Di( <i>n</i> -octyl) phthalate	C <sub>24</sub> H <sub>38</sub> O <sub>4</sub>	DOP	390,6	117-84-0
10	Didecyl phthalate	C <sub>28</sub> H <sub>46</sub> O <sub>4</sub>	DDcP	446,7	84-77-5
11	Diundecyl phthalate	C <sub>30</sub> H <sub>50</sub> O <sub>4</sub>	DUP	474,4	3648-20-2

<sup>a</sup> CAS: Chemical Abstracts System.

## ISO 18856:2004(E)

## 2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the reference document (including any amendments) applies.

ISO 5667-1, *Water quality — Sampling — Part 1: Guidance on the design of sampling programmes*

ISO 5667-2, *Water quality — Sampling — Part 2: Guidance on sampling techniques*

ISO 5667-3, *Water quality — Sampling — Part 3: Guidance on the preservation and handling of water samples*

## 3 Principle

Extraction of the compounds from the water by solid-phase extraction. Then separation is accomplished using capillary columns by gas chromatography and followed by identification and quantification of the phthalates by mass spectrometry. The principle of this method is outlined in Figure 1.

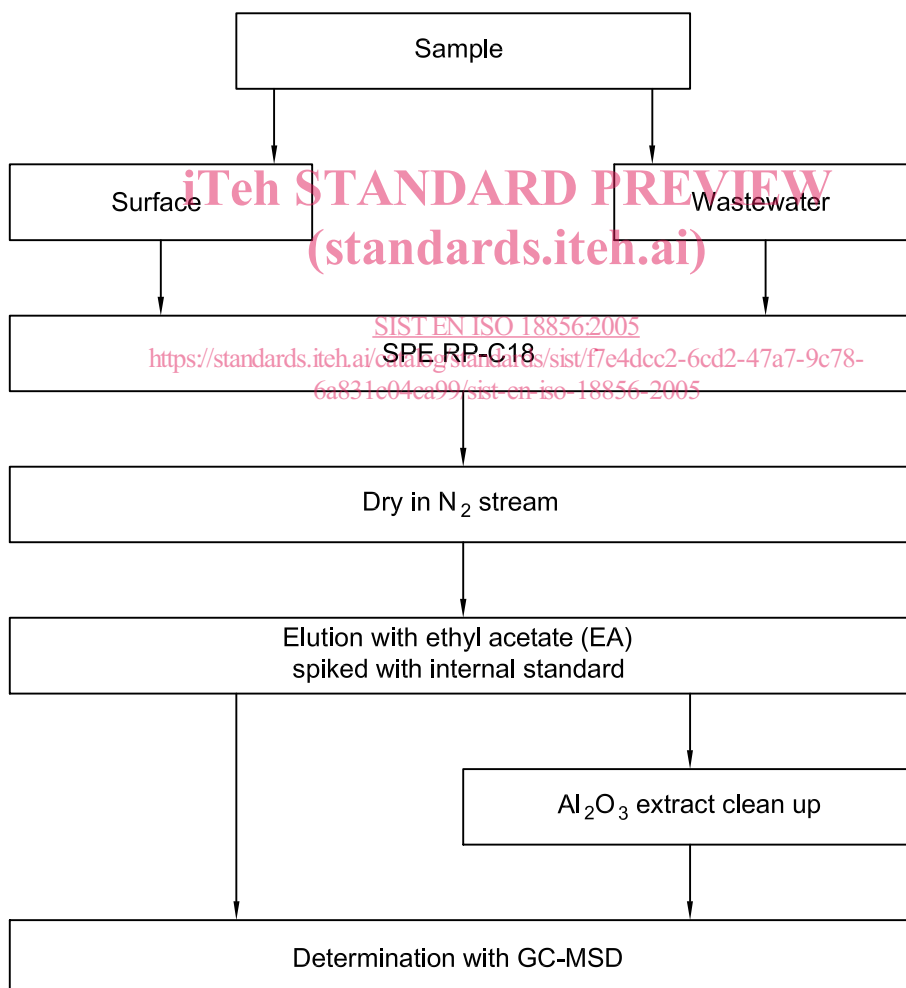


Figure 1 — Flowchart of the analysis

## 4 Interferences

**IMPORTANT** — Due to their use as plasticizer agents, phthalates are ubiquitous. Therefore, pay special attention to avoid any contamination.

### 4.1 Interferences during sampling

In order to avoid interferences and cross-contamination, do not use plastics materials (pipes, etc.).

### 4.2 Interferences during enrichment

Commercially available adsorbent materials are often of varying quality. Considerable batch-to-batch differences in quality and selectivity of this material are possible. The recovery of single substances may vary with concentration. Therefore, check the recovery regularly at different concentration levels and whenever new batches are used. Perform calibration and analysis with material from the same batch.

Cross-contamination is likely to occur with laboratory air. Therefore, remove, as far as possible, plastics materials from the laboratory. Cleaning agents often contain phthalates and may severely contaminate the laboratory air if in use regularly. Therefore, refrain from using these agents during application of this procedure.

The use of plastics gloves during pre-treatment may increase the contamination.

The maximum allowed blank level for each phthalate is 80 ng/l with reference to water (see Annex C).

### 4.3 Interferences in gas chromatography

Phthalates may bleed from the septa of the injector into the gas chromatograph, therefore use septa that are not likely to contaminate the system.

Fittings of syringes, for example, or equipment and septa of the sampling bottles (see 6.7) may as well contain phthalates. Therefore make sure that uncontaminated septa are used.

## 5 Reagents

Use, as far as available, reagents of analytical quality, or better. Use only reagents with negligibly low concentrations of phthalates and verify by blank determinations and, if necessary, apply additional cleaning steps.

**5.1 Water**, having a negligibly low concentration of phthalates.

In some cases, it may be preferable to use surface water instead of distilled water, because the concentration levels of the blank of surface water can be lower (9.3). Other waters with negligibly low concentrations of phthalates may be used as well.

**5.2 Nitrogen**, N<sub>2</sub> of high purity, at least a volume fraction of 99,9 %, for drying and eventually for concentration by evaporation.

**5.3 Helium**, He of high purity, at least a volume fraction of 99,999 %.

**5.4 Operating gases for gas chromatography/mass spectrometry**, of high purity and in accordance with manufacturer's specifications.

**5.5 Ethyl acetate**, highest purity, C<sub>4</sub>H<sub>8</sub>O<sub>2</sub>.

**5.6 Methanol**, CH<sub>3</sub>OH.