

INTERNATIONAL STANDARD

ISO
8319-1

Second edition
1996-05-15

Orthopaedic instruments — Drive connections —

Part 1:

Keys for use with screws with hexagon socket
heads

iTeh STANDARD PREVIEW
(standards.iteh.ai)

Instruments orthopédiques — Raccords d'entraînement —

Partie 1: Clés à utiliser pour les vis à tête à six pans creux



Reference number
ISO 8319-1:1996(E)

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

International Standard ISO 8319-1 was prepared by Technical Committee ISO/TC 150, *Implants for surgery*, Subcommittee SC 5, *Osteosynthesis*.

This second edition cancels and replaces the first edition (ISO 8319-1:1986), which has been technically revised.

ISO 8319 consists of the following parts, under the general title *Orthopaedic instruments — Drive connections*:

- Part 1: *Keys for use with screws with hexagon socket heads*
- Part 2: *Screwdrivers for single slot head screws, screws with cruciate slot and cross-recessed head screws*

Annexes A and B of this part of ISO 8319 are for information only.

© ISO 1996

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from the publisher.

International Organization for Standardization
Case postale 56 • CH-1211 Genève 20 • Switzerland

Printed in Switzerland

Introduction

Essential requirements for all varieties of screw keys are that

- a) the working end of the screw key should accurately engage the head of the screw;
- b) the materials used for the manufacture of the screw keys should be satisfactory from all clinical aspects;
- c) the screw key should have adequate strength.

The purpose of this part of ISO 8319 is to ensure that this is achieved without imposing undue restriction on design features.

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 8319-1:1996

<https://standards.iteh.ai/catalog/standards/sist/3c5cf29d-3ae8-4cea-a873-f430f80ceb16/iso-8319-1-1996>

iTeh STANDARD PREVIEW
This page intentionally left blank
(standards.iteh.ai)

ISO 8319-1:1996

<https://standards.iteh.ai/catalog/standards/sist/3c5cf29d-3ae8-4cea-a873-f430f80ceb16/iso-8319-1-1996>

Orthopaedic instruments — Drive connections —

Part 1:

Keys for use with screws with hexagon socket heads

1 Scope

This part of ISO 8319 specifies the dimensions, tolerances, mechanical properties and performance requirements of the working end of keys to be used for inserting and removing metal bone screws with hexagon drive sockets, used as surgical implants.

Screw keys with a working end specified in this part of ISO 8319 are suitable for use with screws that conform to ISO 5835.

2 Normative references

The following standards contain provisions which, through reference in this text, constitute provisions of this part of ISO 8319. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this part of ISO 8319 are encouraged to investigate the possibility of applying the most recent editions of the standards indicated below. Members of IEC and ISO maintain registers of currently valid International Standards.

ISO 5832-5:1993, *Implants for surgery — Metallic materials — Part 5: Wrought cobalt-chromium-tungsten-nickel alloy.*

ISO 5835:1991, *Implants for surgery — Metal bone screws with hexagonal drive connection, spherical under-surface of head, asymmetrical thread — Dimensions¹⁾.*

ISO 6508:1986, *Metallic materials — Hardness test — Rockwell test (scales A - B - C - D - E - F - G - H - K).*

ISO 7153-1:1991, *Surgical instruments — Metallic materials — Part 1: Stainless steel.*

3 Dimensions and tolerances

The dimensions and tolerances shall be as specified in figure 1 and table 1.

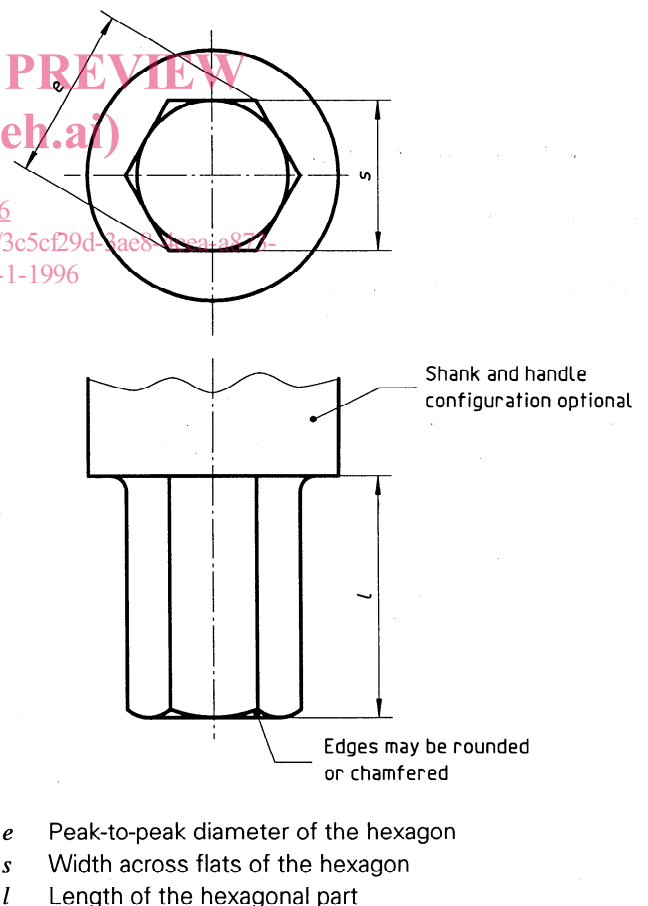


Figure 1 — Designation of dimensions of screw keys

1) See annex A for information on the interrelationship between International Standards dealing with bone screws, bone plates and relevant tools.

Table 1 — Dimensions and tolerances of screw keys

Dimensions in millimetres

Screws in accordance with ISO 5835	Screw key dimensions					
	<i>s</i>			<i>e</i>		<i>l</i>
	nom.	max.	min.	max.	min.	min.
HA 1,5; HA 2,0	1,5	1,500	1,475	1,690	1,650	2
HA 2,7; HA 3,5; HB 4;	2,5	2,500	2,475	2,840	2,800	4
HA 4; HA 4,5; HA 5; HB 6; HB 6,5;	3,5	3,500	3,470	3,980	3,932	5
	4,5	4,500	4,470	5,130	5,082	6

4 Material and grades

Screw keys shall be made of one of the following metals:

- martensitic stainless steel (for example, in accordance with grade reference letters C, D, H or I of ISO 7153-1).
- cold-worked wrought cobalt-chromium-tungsten-nickel alloy in accordance with ISO 5832-5, or other equivalent cobalt alloy.

5 Performance requirements

5.1 Hardness

The Rockwell hardness shall be within the range given in table 2 when tested in accordance with ISO 6508.

Table 2 — Hardness of screw keys

Material	Rockwell hardness HRC
Stainless steel	48 to 54
Wrought cobalt-chromium-tungsten-nickel alloy	45 to 50

5.2 Torque test requirements

Following the application of the minimum test torque as given in clause 6 and table 3, the key for screws with hexagon socket heads shall not fracture or show permanent deformation.

6 Torque test

6.1 Apparatus

6.1.1 Female hexagon socket adaptor, with an opening in accordance with table 3. The socket adaptor shall be hardened to a Rockwell hardness higher than that of the screw key.

6.2 Procedure

Insert the working end of the key in the adaptor and apply the corresponding torque as given in table 3.

Do not jerk or strike the key when testing. Apply the load gradually until the minimum testing torque is reached.

Table 3 — Dimensions and torques used in testing

Key nom. mm	Width across flats, <i>s</i>		Depth of key engagement min. mm	Torque min. N·m
	Female hexagon socket adaptor nom.	tol. mm		
1,5	1,5	+ 0,046	0,9	0,7
2,5	2,5	+ 0,006	1,2	3,8
3,5	3,5	+ 0,058 + 0,010	2,8	9,7
4,5	4,5	+ 0,058 + 0,010	3,8	12

7 Marking

The key shall be permanently and legibly marked with the following information:

- a) size of the screw (code and thread diameter, in accordance with ISO 5835) with which it is intended to be used;
- b) manufacturer's name or trademark;
- c) number of this part of ISO 8319, if there is space available;
- d) material of which it is made, if there is space available.

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 8319-1:1996


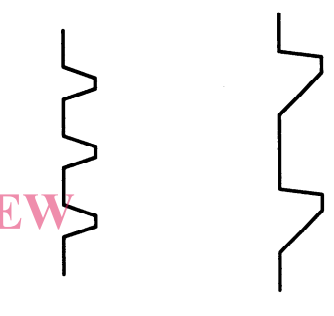




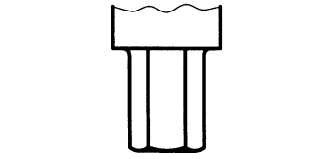
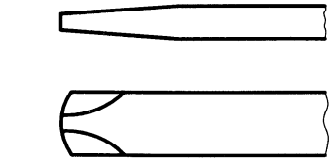
<https://standards.iteh.ai/catalog/standards/sist/3c5cf29d-3ae8-4cea-a873-f430f80ceb16/iso-8319-1-1996>

Annex A
(informative)

Interrelationship of International Standards dealing with bone screws, bone plates and relevant tools

It has been decided that the set of International Standards dealing with bone screws, bone plates and relevant tools should be divided into two parallel series, based on the essentially different designs of the threads of the bone screws (HA and HB type screws as opposed to HC to HD type screws).

A simplified schematic guide illustrating the interrelationship between screws, plates and tools covered by the two parallel series of International Standards is given below.

		ISO 5835	ISO 9268
Screws	Thread	 HA HB	 HC HD
	Head undersurface	 Spherical	 Conical
	Drive connection	 Hexagon	 Single slot Cruciate slot Cross-recessed head
	Mechanical requirements	ISO 6475 Breaking torque/ angle of rotation	In preparation
	Holes and slots	ISO 5836	ISO 9269
Plates	Mechanical requirements	In preparation	In preparation
Driving tools	Keys and screwdrivers	ISO 8319-1  Hexagon keys	ISO 8319-2  Screwdrivers

Annex B (informative)

Bibliography

- [1] ISO 5836:1988, *Implants for surgery — Metal bone plates — Holes corresponding to screws with asymmetrical thread and spherical under-surface.*
- [2] ISO 6475:1989, *Implants for surgery — Metal bone screws with asymmetrical thread and spherical under-surface — Mechanical requirements and test methods.*
- [3] ISO 8319-2:1986, *Orthopaedic instruments — Drive connections — Part 2: Screwdrivers for single slot head screws, screws with cruciate slot and cross-recessed head screws.*
- [4] ISO 9268:1988, *Implants for surgery — Metal bone screws with conical under-surface of head — Dimensions.*
- [5] ISO 9269:1988, *Implants for surgery — Metal bone plates — Holes and slots corresponding to screws with conical under-surface.*

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 8319-1:1996

<https://standards.iteh.ai/catalog/standards/sist/3c5cf29d-3ae8-4cea-a873-f430f80ceb16/iso-8319-1-1996>