

INTERNATIONAL STANDARD

NORME INTERNATIONALE

AMENDMENT 1
AMENDEMENT 1

**Medical electrical equipment –
Part 2-35: Particular requirements for the basic safety and essential performance
of heating devices using blankets, pads or mattresses and intended for heating
in medical use**

<https://standards.iteh.ai/catalog/standards/sist/932348c5-6dea-4a85-9ce8-109076f4de/iec-80601-2-35-2009-amd1-2016>

**Appareils électromédicaux –
Partie 2-35: Exigences particulières pour la sécurité de base et les performances
essentielle des dispositifs de réchauffage utilisant des couvertures, des
coussins ou des matelas chauffants et destinés au réchauffage des patients en
usage médical**



THIS PUBLICATION IS COPYRIGHT PROTECTED

Copyright © 2016 IEC, Geneva, Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either IEC or IEC's member National Committee in the country of the requester. If you have any questions about IEC copyright or have an enquiry about obtaining additional rights to this publication, please contact the address below or your local IEC member National Committee for further information.

Droits de reproduction réservés. Sauf indication contraire, aucune partie de cette publication ne peut être reproduite ni utilisée sous quelque forme que ce soit et par aucun procédé, électronique ou mécanique, y compris la photocopie et les microfilms, sans l'accord écrit de l'IEC ou du Comité national de l'IEC du pays du demandeur. Si vous avez des questions sur le copyright de l'IEC ou si vous désirez obtenir des droits supplémentaires sur cette publication, utilisez les coordonnées ci-après ou contactez le Comité national de l'IEC de votre pays de résidence.

IEC Central Office
3, rue de Varembe
CH-1211 Geneva 20
Switzerland

Tel.: +41 22 919 02 11
Fax: +41 22 919 03 00
info@iec.ch
www.iec.ch

About the IEC

The International Electrotechnical Commission (IEC) is the leading global organization that prepares and publishes International Standards for all electrical, electronic and related technologies.

About IEC publications

The technical content of IEC publications is kept under constant review by the IEC. Please make sure that you have the latest edition, a corrigenda or an amendment might have been published.

IEC Catalogue - webstore.iec.ch/catalogue

The stand-alone application for consulting the entire bibliographical information on IEC International Standards, Technical Specifications, Technical Reports and other documents. Available for PC, Mac OS, Android Tablets and iPad.

IEC publications search - www.iec.ch/searchpub

The advanced search enables to find IEC publications by a variety of criteria (reference number, text, technical committee,...). It also gives information on projects, replaced and withdrawn publications.

IEC Just Published - webstore.iec.ch/justpublished

Stay up to date on all new IEC publications. Just Published details all new publications released. Available online and also once a month by email.

Electropedia - www.electropedia.org

The world's leading online dictionary of electronic and electrical terms containing 20 000 terms and definitions in English and French, with equivalent terms in 15 additional languages. Also known as the International Electrotechnical Vocabulary (IEV) online.

IEC Glossary - std.iec.ch/glossary

65 000 electrotechnical terminology entries in English and French extracted from the Terms and Definitions clause of IEC publications issued since 2002. Some entries have been collected from earlier publications of IEC TC 37, 77, 86 and CISPR.

IEC Customer Service Centre - webstore.iec.ch/csc

If you wish to give us your feedback on this publication or need further assistance, please contact the Customer Service Centre: csc@iec.ch.

A propos de l'IEC

La Commission Electrotechnique Internationale (IEC) est la première organisation mondiale qui élabore et publie des Normes internationales pour tout ce qui a trait à l'électricité, à l'électronique et aux technologies apparentées.

A propos des publications IEC

Le contenu technique des publications IEC est constamment revu. Veuillez vous assurer que vous possédez l'édition la plus récente, un corrigendum ou amendement peut avoir été publié.

Catalogue IEC - webstore.iec.ch/catalogue

Application autonome pour consulter tous les renseignements bibliographiques sur les Normes internationales, Spécifications techniques, Rapports techniques et autres documents de l'IEC. Disponible pour PC, Mac OS, tablettes Android et iPad.

Recherche de publications IEC - www.iec.ch/searchpub

La recherche avancée permet de trouver des publications IEC en utilisant différents critères (numéro de référence, texte, comité d'études,...). Elle donne aussi des informations sur les projets et les publications remplacées ou retirées.

IEC Just Published - webstore.iec.ch/justpublished

Restez informé sur les nouvelles publications IEC. Just Published détaille les nouvelles publications parues. Disponible en ligne et aussi une fois par mois par email.

Electropedia - www.electropedia.org

Le premier dictionnaire en ligne de termes électroniques et électriques. Il contient 20 000 termes et définitions en anglais et en français, ainsi que les termes équivalents dans 15 langues additionnelles. Egalement appelé Vocabulaire Electrotechnique International (IEV) en ligne.

Glossaire IEC - std.iec.ch/glossary

65 000 entrées terminologiques électrotechniques, en anglais et en français, extraites des articles Termes et Définitions des publications IEC parues depuis 2002. Plus certaines entrées antérieures extraites des publications des CE 37, 77, 86 et CISPR de l'IEC.

Service Clients - webstore.iec.ch/csc

Si vous désirez nous donner des commentaires sur cette publication ou si vous avez des questions contactez-nous: csc@iec.ch.

INTERNATIONAL STANDARD

NORME INTERNATIONALE

AMENDMENT 1
AMENDEMENT 1

Medical electrical equipment –
Part 2-35: Particular requirements for the basic safety and essential performance
of heating devices using blankets, pads or mattresses and intended for heating
in medical use

[IEC 80601-2-35:2009/AMD1:2016](https://standards.iteh.ai/catalog/standards/sist/932348c5-6dea-4a85-9ce8-c2-01976fade/iec-80601-2-35-2009-amd1-2016)

[https://standards.iteh.ai/catalog/standards/sist/932348c5-6dea-4a85-9ce8-](https://standards.iteh.ai/catalog/standards/sist/932348c5-6dea-4a85-9ce8-c2-01976fade/iec-80601-2-35-2009-amd1-2016)

[c2-01976fade/iec-80601-2-35-2009-amd1-2016](https://standards.iteh.ai/catalog/standards/sist/932348c5-6dea-4a85-9ce8-c2-01976fade/iec-80601-2-35-2009-amd1-2016)

Appareils électromédicaux –
Partie 2-35: Exigences particulières pour la sécurité de base et les performances
essentielle des dispositifs de réchauffage utilisant des couvertures, des
coussins ou des matelas chauffants et destinés au réchauffage des patients en
usage médical

INTERNATIONAL
ELECTROTECHNICAL
COMMISSION

COMMISSION
ELECTROTECHNIQUE
INTERNATIONALE

FOREWORD

This amendment has been prepared by a joint working group of IEC subcommittee 62D: Electromedical equipment of IEC technical committee 62: Electrical equipment in medical practice and ISO subcommittee TC121/SC1: Breathing attachments and anaesthetic machines, of ISO technical committee 121: Anaesthetic and respiratory equipment.

It is published as a double logo standard.

The text of this amendment is based on the following documents:

FDIS	Report on voting
62D/1328/FDIS	62D/1355/RVD

Full information on the voting for the approval of this amendment can be found in the report on voting indicated in the above table. In ISO, the standard has been approved by 15 P-members out of 15 having cast a vote.

The committee has decided that the contents of this amendment and the base publication will remain unchanged until the stability date indicated on the IEC website under "http://webstore.iec.ch" in the data related to the specific publication. At this date, the publication will be

iTeh STANDARD PREVIEW
(standards.iteh.ai)

- reconfirmed,
- withdrawn,
- replaced by a revised edition, or [IEC 80601-2-35:2009/AMD1:2016](http://standards.iteh.ai/catalog/standards/sist/932348c5-6dea-4a85-9ce8-bc8b9f76fade/iec-80601-2-35-2009-amd1-2016)
- amended. <https://standards.iteh.ai/catalog/standards/sist/932348c5-6dea-4a85-9ce8-bc8b9f76fade/iec-80601-2-35-2009-amd1-2016>

INTRODUCTION

Replace, in the second paragraph, "IEC 60601-1 (third edition, 2005)" by "IEC 60601-1".

201.1 Scope, object and related standards

Replace, in footnote 1), "IEC 60601-1:2005" by "IEC 60601-1".

201.2 Normative references

Replace "IEC 60601-1-2:2007" by "IEC 60601-1-2".

Replace "IEC 60601-1-8:2006" by "IEC 60601-1-8".

Replace "IEC 60601-1-10:2007" by "IEC 60601-1-10".

Delete the following reference:

ISO 3743-1:1994, *Acoustics – Determination of sound power levels of noise sources – Engineering methods for small, movable sources in reverberant fields – Part 1: Comparison method for hard-walled test rooms*

201.3 Terms and definitions

Replace, in the first paragraph, “IEC 60601-1:2005” by “IEC 60601-1”.

201.7.2.1.101.2 CONTROLLERS

Replace the text in item a) by the following new text:

- a) The HOSE shall be marked within 15 cm of the NOZZLE to caution that the NOZZLE needs to be connected to a BLANKET. The following statement and the safety sign ISO 7010-M002 (see IEC 60601-1, Table D.2, safety sign 10) shall accompany the “NO FREE HOSING” safety sign of IEC 60878, shown in Annex D of this particular standard:

201.8.5.1.2.101 * Additional requirements for MEANS OF PATIENT PROTECTION (MOPP)

Replace the first two paragraphs by the following:

The electrical circuit within the APPLIED PART shall be isolated from earth by at least one MOPP and from MAINS by at least two MOPP. Where a transformer is used to achieve this isolation, it need not meet 15.5.3.

201.12.3.104 Disconnection or short-circuiting of sensors ALARM CONDITION

Replace the second paragraph by the following:

The HEATING DEVICE shall be equipped with an ALARM SYSTEM that includes at least a MEDIUM PRIORITY TECHNICAL ALARM CONDITION for HIGH HEAT TRANSFER DEVICES and at least a LOW PRIORITY ALARM for LOW HEAT TRANSFER DEVICES and FORCED AIR DEVICES that indicates when leads to either the temperature control sensors or the THERMAL CUT-OUT sensors are damaged or otherwise disconnected from the control unit.

202 Electromagnetic compatibility – Requirements and tests

Replace, in the first paragraph, “IEC 60601-1-2:2007” by “IEC 60601-1-2”.

202.6.2.3 Radiated RF electromagnetic fields

Replace the number, title and entire text by the following new subclause number, title and text:

202.8.9 IMMUNITY TEST LEVELS

Addition:

For radiated radio-frequency electromagnetic fields, the HEATING DEVICE and/or system shall

- continue to perform its intended function as specified by the MANUFACTURER at the level up to 3 V/m for the frequency range of the collateral standard of EMC.

NOTE A HEATING DEVICE is not considered to be used in a HOME HEALTHCARE ENVIRONMENT.

208 General requirements, tests and guidance for ALARM SYSTEMS IN MEDICAL ELECTRICAL EQUIPMENT and MEDICAL ELECTRICAL SYSTEMS

Replace, in the first paragraph, “IEC 60601-1-8:2006” by “IEC 60601-1-8”.

210 Requirements for the development of physiologic closed-loop controllers

Replace both instances of “IEC 60601-1-10:2007” by “IEC 60601-1-10”.


Annex AA (informative)

Particular guidance and rationale

Add, immediately after the annex title, the following new text and figure:

AA.1 Requirements and the safety concept of this standard

Compliance with the minimum safety requirements specified in this particular standard is predominantly checked by measurement of physical quantities such as the temperature. In most cases the spatial location of the measuring site or the temporal development of the quantity is of interest. Therefore, the expert group of this standard considered it helpful to provide a synopsis of the requirements of this standard. Hence, Figure AA.1 illustrates the requirements and their schematic measuring sites or expected temporal development. The requirements as given by their clauses are set in brackets.

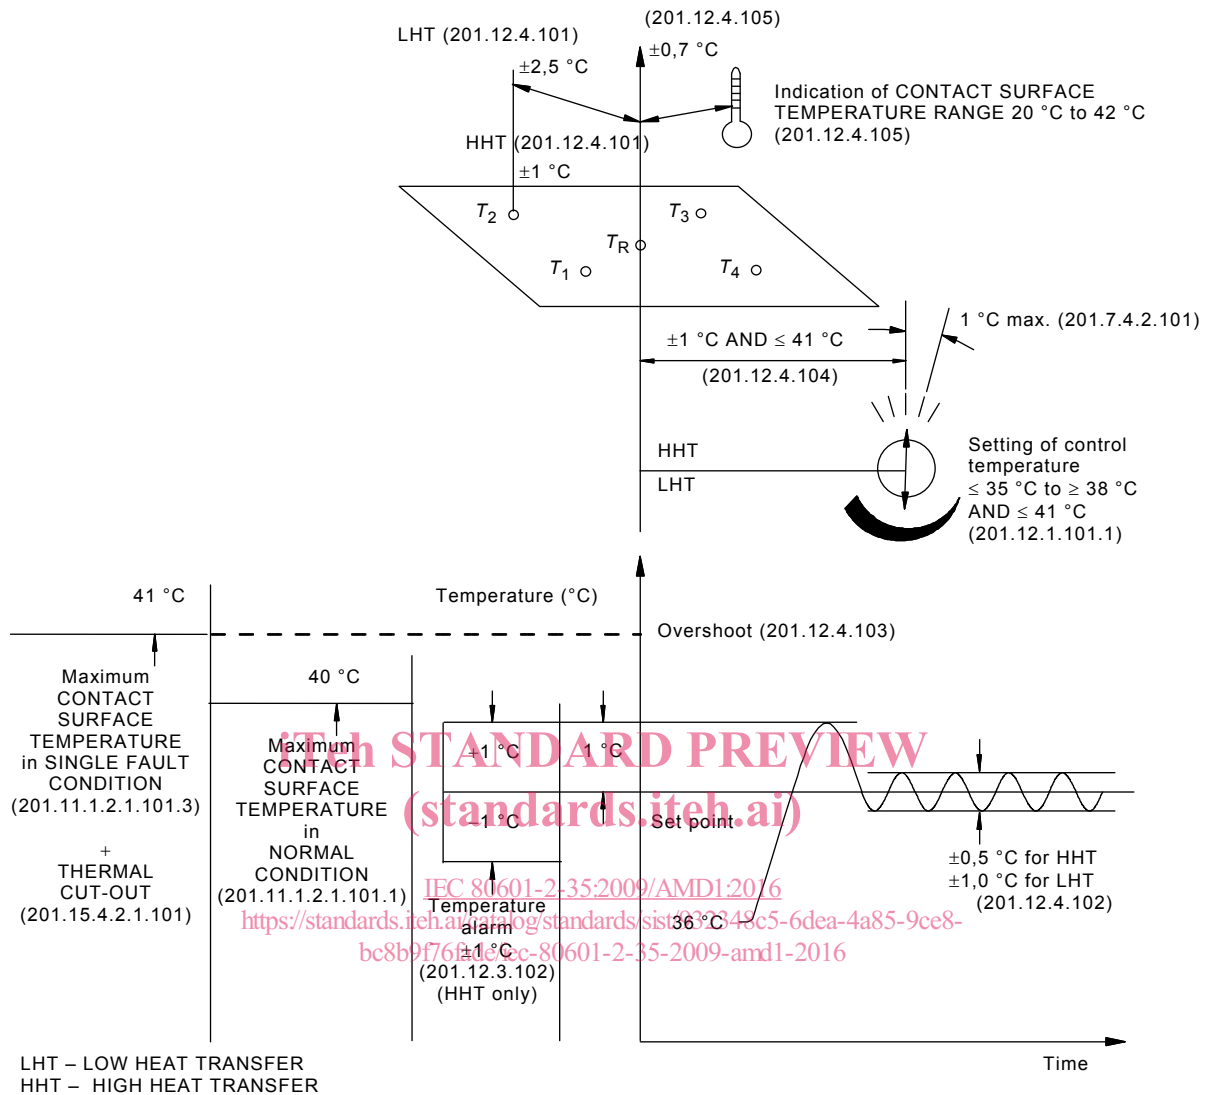

IEC

NOTE Numbers in brackets indicate the relevant subclauses.

Figure AA.1 – Illustration of the main requirements of this standard

AA.2 Particular guidance

Subclause 201.11.1.2.1.102.1 – Maximum CONTACT SURFACE TEMPERATURE in NORMAL CONDITION

Add, after the existing text, the following new text:

The CONTACT SURFACE TEMPERATURE of HEATING DEVICES may rise when combined with other heat sources such as heating BLANKETS or PADS. Hence, it is important to specifically consider the impact of such additional heat sources in the RISK MANAGEMENT.

Subclause 202.6.2 – IMMUNITY

Delete the entire reference to subclause 202.6.2 and its rationale.

Subclause 210 – Requirements for the development of physiologic closed-loop controllers

Replace, in the first paragraph, “IEC 60601-1-10-1” by “IEC 60601-1-10”.

Annex FF
(normative)

Test procedure for maximum CONTACT SURFACE TEMPERATURE for FORCED AIR DEVICES

Replace the entire existing text of item a) by the following new text:

a) LAGGING MATERIAL

The LAGGING MATERIAL has the following characteristics:

Material: Polyurethane or polystyrene insulation material;

Thermal resistance: A minimum R-Value rating of 10 when tested in accordance with ASTM C578 [8];

Size: Not less than the size of the active heating area of the test blanket and not less than 25 mm thick.

ITeH STANDARD PREVIEW
(standards.iteh.ai)

Bibliography

[IEC 80601-2-35:2009/AMD1:2016](https://standards.iteh.ai/catalog/standards/sist/932348c5-6dea-4a85-9ce8-81411e518812/iec-80601-2-35-2009-amd1-2016)

[https://standards.iteh.ai/catalog/standards/sist/932348c5-6dea-4a85-9ce8-](https://standards.iteh.ai/catalog/standards/sist/932348c5-6dea-4a85-9ce8-81411e518812/iec-80601-2-35-2009-amd1-2016)

Delete “:2009” in references [10], [11] and [12].

Index of defined terms used in this particular standard

Replace all instances of “IEC 60601-1:2005” by “IEC 60601-1”.

Replace all instances of “IEC 60601-1-8:2006” by “IEC 60601-1-8”.

Replace all instances of “IEC 60601-1-10:2007” by “IEC 60601-1-10”.

Replace the term

LIFE SUPPORTING ME EQUIPMENT OR ME SYSTEM IEC 60601-1-2:2007, 3.18

by the following new term:

HOME HEALTHCARE ENVIRONMENT IEC 60601-1-11, 3.2



iTeh STANDARD PREVIEW
(standards.iteh.ai)

[IEC 80601-2-35:2009/AMD1:2016](https://standards.iteh.ai/catalog/standards/sist/932348c5-6dea-4a85-9ce8-bc8b9f76fade/iec-80601-2-35-2009-amd1-2016)

<https://standards.iteh.ai/catalog/standards/sist/932348c5-6dea-4a85-9ce8-bc8b9f76fade/iec-80601-2-35-2009-amd1-2016>