INTERNATIONAL STANDARD



First edition 1999-04-15

Pen systems —

Part 2: Plungers and discs for pen-injectors for medical use

iTeh Systèmes de stylos-injecteurs - VIEW

Partie 2: Bouchons-pistons et rondelles d'étanchéité pour stylos-injecteurs à usage médical S. Iten. al)



Contents

1 Scope	1
2 Normative references	1
3 Dimensions and designation	
4 Material	3
5 Requirements	3
6 Marking	5
Annex A (normative) Test for fragmentation	6
Annex B (normative) Leakage test1	0
Annex C (normative) Test for sliding characteristics1	1
Bibliography1 ITeh STANDARD PREVIEW	3

(standards.iteh.ai)

<u>ISO 13926-2:1999</u> https://standards.iteh.ai/catalog/standards/sist/6b7901eb-b4ac-43c1-a867-3d72931b8b22/iso-13926-2-1999

© ISO 1999

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from the publisher.

International Organization for Standardization Case postale 56 • CH-1211 Genève 20 • Switzerland Internet iso@iso.ch

Printed in Switzerland

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 3.

Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

International Standard ISO 13926-2 was prepared jointly by Technical Committees ISO/TC 76, *Transfusion, infusion and injection equipment for medical use* and ISO/TC 84, *Medical devices for injections.*

ISO 13926 consists of the following parts, under the general title Pen systems:

— Part 1: Glass cylinders for pen-injectors for medical use

— Part 2: Plungers and discs for pen-injectors for medical use PREVIEW

Annexes A, B and C form an integral part of this part of ISO 13926.

iTeh STANDARD PREVIEW (standards.iteh.ai)

Pen systems —

Part 2: Plungers and discs for pen-injectors for medical use

1 Scope

This part of ISO 13926 specifies the design, dimensions, material performance requirements and marking of plungers and discs for medical pen systems. It is applicable to primary packs used in direct contact with drugs.

NOTE The potency, purity, stability and safety of a drug during its manufacture and storage can be strongly affected by the nature and performance of the primary pack.

This part of ISO 13926 does not apply to laminated or lacquered plungers. iTeh STANDARD PREVIEW

(standards.iteh.ai)

2 Normative references

The following normative documents contain provisions which, through reference in this text, constitute provisions of this part of ISO 13926. For dated references, subsequent amendments to, or revisions of, any of these publications do not apply. However, parties to agreements based on this part of ISO 13926 are encouraged to investigate the possibility of applying the most recent editions of the normative documents indicated below. For undated references, the latest edition of the normative document referred to applies. Members of ISO and IEC maintain registers of currently valid International Standards.

ISO 48:1994, Rubber, vulcanized or thermoplastic – Determination of hardness (hardness between 10 IRHD and 100 IRHD).

ISO 3302:1990, Rubber – Dimensional tolerances for use with products.

ISO 7864:1993, Sterile hypodermic needles for single use.

ISO 8871:1990, Elastomeric parts for aqueous parenteral preparations.


ISO 11040-3:1993, Prefilled syringes – Part 3: Aluminium caps for dental local anaesthetic cartridges.

ISO 13926-1:1998, Pen systems – Part 1: Glass cylinders for pen-injectors for medical use.

3 Dimensions and designation

3.1 Dimensions

The plungers shall be type PSF, with dimensions as shown in Figure 1 and given in Table 1, and for discs as shown in Figure 2 and given in Table 2.





Toh STANDARD Dimensions in milimetres				
Nominal volume	(stand	Diameter	teh.ai)	Height
ml https://standar	d_1 $\pm 0,1$ d_2 iteb avcatalo	SO 13926-2:19 ±0,1	99 ^d 3 +0,15 6b790 cb-b4a	h ₁ -43cl-a867-
1,5	3 , <u></u> 272931	b8b226;9-1392	.6-2-1 <mark>6,4</mark> 9	5,5
2	9,1	8,8	8,3	8,1
2,5	9,6	9,3	8,8	8,7
3	10	9,7	9,2	11,0
4	12,5	12,1	11,7	11
5	12,35	11,95	11,55	11
6	16,6	16,15	15,7	13

Table 1 — Dimensions of the plunger

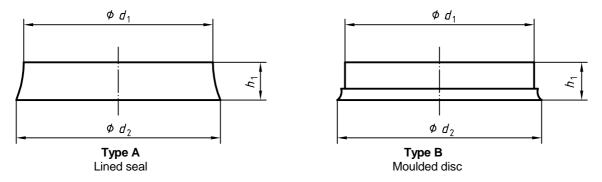


Figure 2 — Dimensions and configuration of discs for medical pen-injectors

			Dimensio	ns in millimetres
Nominal volume	Туре	Diameter		Height
ml		<i>d</i> ₁	<i>d</i> ₂	<i>h</i> ₁ ± 0,15
1,5	А, В	7,1 min.	7,8 max.	
³ Tel	STA, ANI	7,65±0,1	R7,85 max .	1,5
4 to 6	(stond	9,85 ± 0,15	10 max.	· ·
(stanuarus.tten.ar)				

Table 2 — Dimensions of the disc

3.2 Designation

<u>ISO 13926-2:1999</u>

Plungers and discs for medical pen systems shall be designated with the appropriate block descriptor followed by a reference to this part of ISO 13926, followed by the type of disc (if applicable), followed by the nominal volume, expressed in millilitres, of the glass cylinder with which it is to be used.

EXAMPLE 1 Designation of a plunger for a glass cylinder with a nominal volume of 1,5 ml complying with the requirements in this part of ISO 13926:

Plunger ISO 13926-2 - 1,5

EXAMPLE 2 Designation of a disc type A for a glass cylinder with a nominal volume of 3 ml complying with the requirements in this part of ISO 13926:

Disc ISO 13926-2 - A - 3

4 Material

The type of elastomeric material used shall be chosen such that the plungers and discs meet the requirements specified in clause 5.

5 Requirements

5.1 Physical requirements

5.1.1 Dimensions

If not otherwise specified, general dimensional tolerances shall be in accordance with ISO 3302.

The trimmed part of the disc may be slightly conical and eccentric. The trimming edge shall not extend beyond diameter d_2 .

Discs may be knurled on one or both sides in order to avoid sticking together in a package.

In order to avoid adhesion of the plungers to each other, interrupted rings or bridges should be used as spacers in packaging. The height of the spacers shall not exceed 0,2 mm.

Sprues, if present on the surface of the plunger, shall not protrude beyond spacers.

5.1.2 Hardness

The hardness shall be agreed between manufacturer and user; hardness shall be determined in accordance with ISO 48.

5.1.3 Fragmentation (coring)

When testing discs for fragmentation in accordance with annex A, not more than three fragments per 50 piercings shall be observed.

5.1.4 Leakage

When testing discs or plungers according to annex B, no leakage of liquid from the glass cylinder shall be observed.

5.1.5 Sliding properties

When testing plungers according to annex C, the break-loose force and restarting force shall not exceed 30 N. The force to sustain continuous movement shall not exceed 15 N and there shall be no chattering¹)

5.2 Chemical requirement**§Teh STANDARD PREVIEW**

The chemical properties of the material of the plungers and discs shall not exceed the limits specified in Table 3.

Test	3d72931b8b22/so-13926-2-1999 Requirement	Test procedure as described in ISO 8871:1990, annexª
Reducing matter (oxidizables)	\leq 7 ml of $c(KMnO_4) = 2 mmol/l per 20 ml$	С
Heavy metals (calculated as Pb ²⁺)	\leq 10 µg Pb ²⁺ /10 ml	D
Ammonium (calculated as NH ₄ +)	\leq 20 µg NH ₄ +/10 ml	E
Acidity/alkalinity	\leq 1 ml of c(HCl) or c(NaOH) = 5 mmol/l per 20 ml	G
Residue on evaporation (total solids)	≤ 4 mg/100 ml	Н
Volatile sulfides (at pH \approx 2)	coloration of lead acetate paper $\leq 50 \ \mu g \ Na_2 S/20 \ cm^2$ rubber surface	J
Zinc (calculated as Zn ²⁺)	$Zn^{2+} \leqslant 30 \ \mu g/10 \ ml$	К
Conductivity	\leq 40 μ S/cm	L
Turbidity	not exceeding opalescence suspension number 3	М

Table 3 — Chemical limits for plungers and discs_867-

¹⁾ Chatter (stick-slip) is the phenomenon of irregular motion of the plunger.

5.3 Biological requirements

The elastomeric plunger shall not release any substances which may adversely affect the therapeutic effectiveness of the injectable products or substances which may exhibit toxic, pyrogenic or haemolytic reactions.

NOTE Since biological tests are usually requested by most of the national Pharmacopoeias or related regulations of health authorities, they are mandatory for producers and users in countries where they exist. If this is not the case, reference should be made to biological tests, e.g. as described in the United States Pharmacopoeia, European Pharmacopoeia, national Pharmacopoeias or ISO 10993 series.

6 Marking

The package of plungers or discs may be marked with a designation in accordance with 3.2.

iTeh STANDARD PREVIEW (standards.iteh.ai)