
Prostheses — Structural testing of hip units

Prothèses — Essais portant sur la structure des prothèses de hanche

iTeh Standards
(<https://standards.iteh.ai>)
Document Preview

ISO 15032:2000

<https://standards.iteh.ai/catalog/standards/iso/2c2d872c-cfeb-464f-9779-2e703cd7e5d3/iso-15032-2000>



Reference number
ISO 15032:2000(E)

© ISO 2000

PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

iTeh Standards
(<https://standards.iteh.ai>)
Document Preview

ISO 15032:2000

<https://standards.iteh.ai/catalog/standards/iso/2c2d872c-cfeb-464f-9779-2e703cd7e5d3/iso-15032-2000>

© ISO 2000

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 734 10 79
E-mail copyright@iso.ch
Web www.iso.ch

Printed in Switzerland

Contents

Page

Foreword.....	iv
Introduction	v
1 Scope	1
2 Normative reference	1
3 Terms and definitions	1
4 Test configurations	2
4.1 General.....	2
4.2 Axes of coordinate system	2
4.3 Reference planes	2
4.4 Reference points.....	5
4.5 Test force.....	5
4.6 Load line	5
4.7 Reference distances.....	5
5 Test samples	5
5.1 Types of test sample	5
5.2 Responsibilities regarding selection, preparation and alignment of test samples	6
5.3 Selection of test samples.....	6
5.4 Preparation of test samples.....	6
5.5 Alignment of test samples	7
6 Test requirements and conditions	8
6.1 Types of test.....	8
6.2 Test loading requirements	8
6.3 Requirements and conditions relevant to test procedures and equipment	9
6.4 A-P and M-L test procedures	12
6.5 Torsional test procedures.....	18
6.6 Number of tests required	23
6.7 Restrictions on multiple use of test samples	23
6.8 Accuracy	23
7 Test loading parameters	24
7.1 Test loads and references	24
7.2 Details of loading	25
8 Test submission document	27
8.1 Document need	27
8.2 General requirements.....	27
8.3 Information required for test samples	28
8.4 Information required for tests	28
9 Test report	29
9.1 General requirements.....	29
9.2 Records required for all test samples	29
9.3 Records required for all tests.....	30
9.4 Records required for results of A-P and M-L tests	30
9.5 Records required for results of torsional tests	31
Annex A (normative) Description of internal loads and their effects	32
Annex B (informative) Reference data for the specification of the A-P, M-L and torsional test loading conditions at different test loading levels.....	35
Bibliography	38

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 3.

Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this International Standard may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

International Standard ISO 15032 was prepared by Technical Committee ISO/TC 168, *Prosthetics and orthotics*.

Annex A forms an integral part of this International Standard. Annex B is given for information only.

iteh Standards
(<https://standards.iteh.ai>)
Document Preview

ISO 15032:2000

<https://standards.iteh.ai/catalog/standards/iso/2c2d872c-cfeb-464f-9779-2e703cd7e5d3/iso-15032-2000>

Introduction

Throughout this International Standard, the term prosthesis means an externally applied device used to replace wholly, or in part, an absent or deficient limb segment.

During use a prosthesis is subject to a series of load actions each varying individually with time. The test methods specified in this International Standard use simplified static and cyclic strength tests in which antero-posterior (A-P) and medio-lateral (M-L) components of loading are produced in separate tests by the application of test forces in two different test planes.

The static tests relate to the worst loads generated in any activity. The cyclic tests relate to normal walking activities where loads occur regularly with each step. This International Standard specifies fatigue testing of structural components. The tests specified do not provide sufficient data to predict actual service life.

The evaluation of hip disarticulation prostheses and their components requires controlled field trials in addition to the laboratory tests specified in this International Standard.

The laboratory tests and field trials should be repeated when significant design changes are made to a load-bearing part of a prosthesis.

Ideally, additional laboratory tests should be carried out to deal with function, wear and tear, new material developments, environmental influences, and amputee activities as part of the evaluation procedure. There are no standards for such tests, so appropriate procedures will need to be specified.

Document Preview

[ISO 15032:2000](https://standards.iteh.ai/catalog/standards/iso/2c2d872c-cfeb-464f-9779-2e703cd7e5d3/iso-15032-2000)

<https://standards.iteh.ai/catalog/standards/iso/2c2d872c-cfeb-464f-9779-2e703cd7e5d3/iso-15032-2000>

Prostheses — Structural testing of hip units

1 Scope

This International Standard specifies test methods for components and assemblies of hip disarticulation prostheses which are arranged at hip and thigh level. It does not apply to other components of lower limb prostheses for which test methods are given in ISO 10328.

This International Standard specifies procedures for simplified static and cyclic strength tests in which the antero-posterior (A-P) and medio-lateral (M-L) components of loading are produced in separate tests by the application of test forces in two different test planes. The components of loading produced in the test sample relate to the peak values of the components of loading which normally occur at different instants during the stance phase of walking.

2 Normative reference

The following normative document contains provisions which, through reference in this text, constitute provisions of this International Standard. For dated references, subsequent amendments to, or revisions of, any of these publications do not apply. However, parties to agreements based on this International Standard are encouraged to investigate the possibility of applying the most recent edition of the normative document indicated below. For undated references, the latest edition of the normative document referred to applies. Members of ISO and IEC maintain registers of currently valid International Standards.

ISO 8549-1:1989, *Prosthetics and orthotics — Vocabulary — Part 1: General terms for external limb prostheses and external orthoses*.

[ISO 15032:2000](https://standards.iso.org/iso/15032-2000)

<https://standards.iso.org/iso/15032-2000>

3 Terms and definitions

For the purposes of this International Standard, the terms and definitions given in ISO 8549-1 and the following apply.

3.1

brittle failure

fracture of any component without significant plastic deformation at the fracture

3.2

ductile failure

⟨...⟩ fracture of any component with significant plastic deformation at the fracture

3.3

ductile failure

⟨...⟩ gross plastic deformation of the test sample

3.4

test equipment

any test machine or device adapted or specifically designed to the test requirements of this International Standard and complying with the requirements on accuracy of 6.8

4 Test configurations

4.1 General

4.1.1 For ease in interpretation, presentation and application of this International Standard, two test configurations are specified, one for right-sided application and a mirror image for left-sided application. This approach enables the application of uniform sign conventions for corresponding components of loading generated in the load-bearing structures of right and left prostheses or asymmetrically designed prosthetic components.

4.1.2 Each test configuration is defined in a three-dimensional, rectangular coordinate system, containing a geometric system of planes, lines and points (see Figures 1 and 2).

4.1.3 Each test configuration specifies reference parameters both for the position of the line of application of the test force and for the alignment of test samples within the coordinate system.

4.2 Axes of coordinate system

4.2.1 The axes of each of the coordinate systems have an origin at ground level and are specified in 4.2.2 to 4.2.4 in relation to a prosthesis which is standing on the ground in a vertical position.

If a test sample is not in a vertical position, the axes of the coordinate system shall be rotated to correspond.

4.2.2 The u' -axis is a line extending from the origin and passing through the effective knee-joint centre (see 5.5.2.2) and the effective hip-joint centre (see 5.5.2.4). Its positive direction is upwards (in the proximal direction).

4.2.3 The o' -axis is perpendicular to the u' -axis and parallel to the effective hip-joint centreline (see 5.5.2.3). Its positive direction is outward (in the lateral direction), which is to the left for a left prosthesis and to the right for a right prosthesis.

4.2.4 The f' -axis is perpendicular to both the o' -axis and the u' -axis. Its positive direction is forward towards the toe (in the anterior direction).

4.3 Reference planes

The reference planes (see Figure 1) shall be parallel planes perpendicular to the u' -axis of the coordinate system.

4.3.1 Bottom reference plane, BK

The bottom reference plane, BK, is located at a distance $u' = u'_{BK}$ from the origin. It contains the bottom load application point P_{BK} .

4.3.2 Knee reference plane, K

The knee reference plane, K, is located at a distance $u' = u'_K$ from the origin. It contains the effective knee-joint centre (see 5.5.2.2).

4.3.3 Hip reference plane, H

The hip reference plane, H, is located at a distance $u' = u'_H$ from the origin. It contains the effective hip-joint centre (see 5.5.2.4).

4.3.4 Top reference plane, TH

The top reference plane, TH, is located at a distance $u' = u'_{TH}$ from the origin. It contains the top load application point P_{TH} .



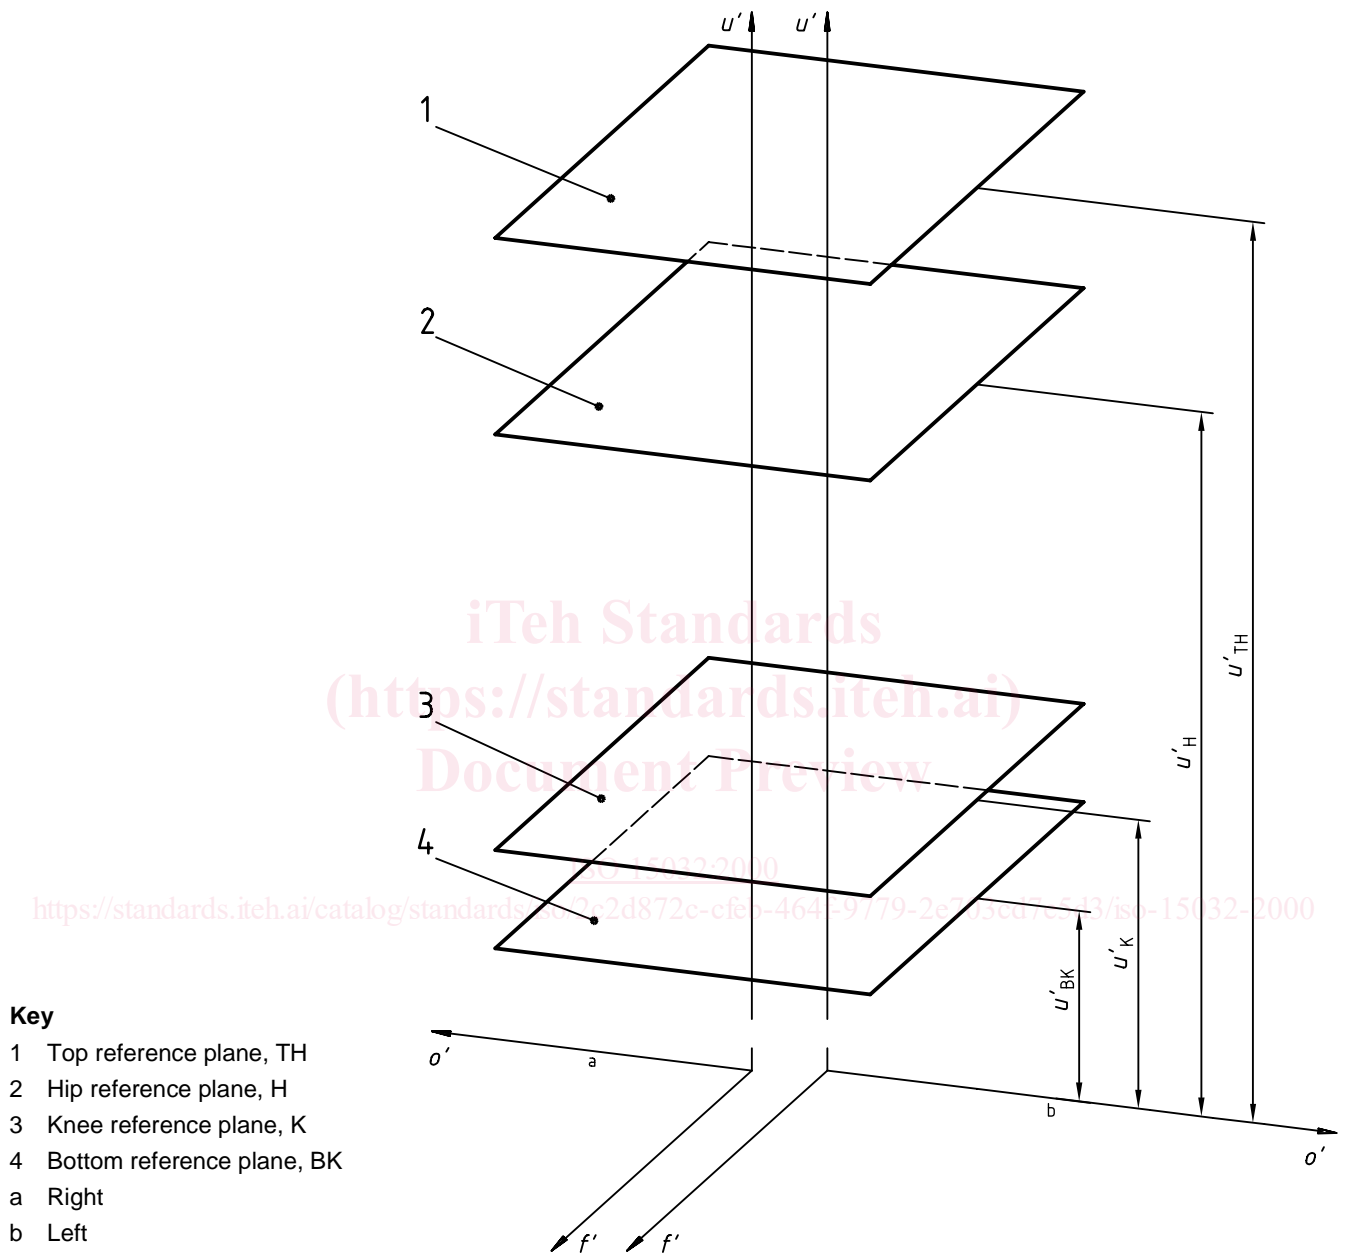


Figure 1 — Coordinate system according to 4.2 with reference planes

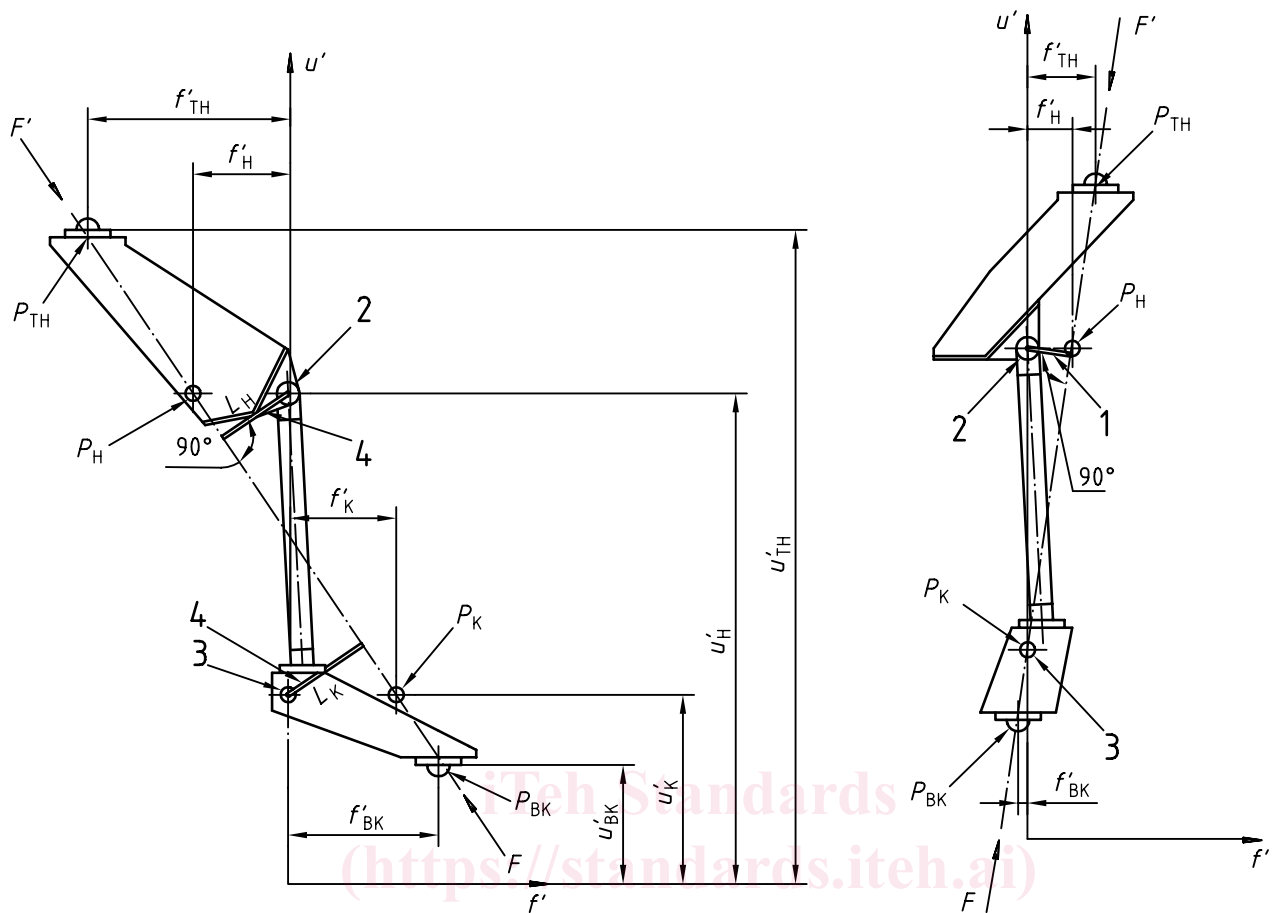

a) A-P ext. test loading condition

b) A-P flex. test loading condition

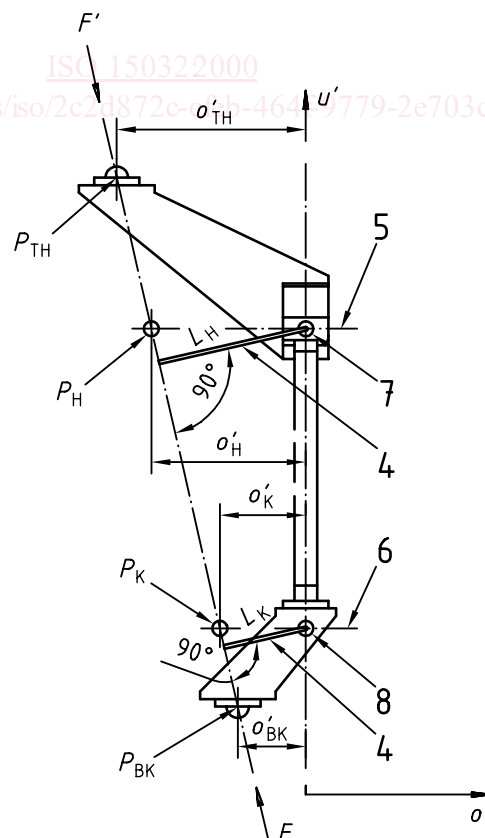

c) M-L test loading condition

Key

- 1 Effective lever arm, L_H
- 2 Effective hip joint centre
- 3 Effective knee joint centre
- 4 Effective lever arm
- 5 Effective hip joint centre line
- 6 Effective knee joint centre line
- 7 Effective hip joint centre
- 8 Effective knee joint centre

Figure 2 — Test configurations for A-P and M-L tests in f' - u' - and o' - u' - plane

4.4 Reference points

The reference points shall be the points of intersection of the load line (see 4.6) with the reference planes. The coordinates of the reference points are as follows:

bottom load application point P_{BK} (f'_{BK} , o'_{BK} , u'_{BK});

knee load reference point P_K (f'_K , o'_K , u'_K);

hip load reference point P_H (f'_H , o'_H , u'_H);

top load application point P_{TH} (f'_{TH} , o'_{TH} , u'_{TH}).

NOTE In the following text the f' - and o' -coordinates are also referred to as offsets (see also 4.7).

4.5 Test force

The test force F shall be a single compressive load applied to the bottom and top load application points P_{BK} and P_{TH} .

4.6 Load line

The load line shall be the line of application of the test force F which passes through the reference points P_K and P_H .

4.7 Reference distances

4.7.1 Offsets

The offsets shall be the perpendicular distances of the reference points (see 4.3.1 and 4.4) from the o - u -plane and the u - f -plane of the coordinate systems (see 4.1 and 4.2). They are identical with the corresponding f' - or o' -coordinates, respectively, of these reference points.

4.7.2 Effective lever arms

The effective lever arms shall be the perpendicular distances from the load line to the effective joint centres (see 5.5.2.2 and 5.5.2.4), where L_K represents the knee effective lever arm and L_H the hip effective lever arm.

4.7.3 Distance L_{BK-TH}

L_{BK-TH} shall be the distance between the bottom load application point P_{BK} (see 4.3.1 and 4.4) and the top load application point P_{TH} (see 4.3.4 and 4.4).

5 Test samples

5.1 Types of test sample

5.1.1 Number of types

There are two types of test sample, as described in 5.1.2 and 5.1.3.

5.1.2 Complete structure

The complete structure shall comprise the hip unit and at least the following:

- a) thigh segment or suitable attachment;
- b) any special attachment at the knee; and/or
- c) any parts above the hip unit including the socket.

5.1.3 Hip unit

The hip unit shall be attached to suitable attachments to give the same overall dimensions as the complete structure.

The interface of such attachments shall have mechanical characteristics similar to those of the intended adjacent components.

5.2 Responsibilities regarding selection, preparation and alignment of test samples

5.2.1 The manufacturer/submitter shall be responsible for the selection and assembly of the components to be tested, and for the provision of specified parts to be replaced during the cyclic tests.

5.2.2 The manufacturer/submitter shall be responsible for preparing the test submission document complete with alignment and/or service instructions, as necessary.

5.2.3 The manufacturer/submitter shall apply a unique and traceable identification to each test sample.

5.2.4 The load application levers (see 6.2.1) shall be attached by either the manufacturer/submitter or the test laboratory/facility.

5.2.5 The test laboratory/facility shall seek the advice of the manufacturer/submitter if the specific design of hip units incorporates any special characteristics.

5.2.6 The test laboratory/facility shall be responsible for adjustment of the alignment to give the correct offsets and effective lever arms during test.

5.3 Selection of test samples

If appropriate, the prosthetic structures selected for test shall be drawn from standard production. Details of the selection shall be recorded in the test submission document. If the manufacturer/submitter supplies a certificate stating that the test sample has been taken from the normal production, this certificate shall be included in the test submission document, together with details of the sampling method.

5.4 Preparation of test samples

Any cosmetic components shall be omitted from the test sample, unless they contribute to the structural strength.

The test samples shall include all parts normally fitted.

NOTE During the course of the cyclic tests, specified parts are replaced when the number of cycles has reached a value at which such replacement is indicated in accordance with the manufacturer's/submitter's service instructions and/or the test submission document.

The test sample including any end fittings shall be assembled in accordance with the responsibilities regarding the preparation of the test sample and the test submission document.