
**Fine ceramics (advanced ceramics,
advanced technical ceramics) — Sample
preparation for the determination of particle
size distribution of ceramic powders**

*Céramiques techniques — Préparation de l'échantillon pour la
détermination de la répartition granulométrique des poudres céramiques*

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[ISO 14703:2000](https://standards.iteh.ai/catalog/standards/sist/09718370-380a-4b76-a1e7-6752cb72e930/iso-14703-2000)

<https://standards.iteh.ai/catalog/standards/sist/09718370-380a-4b76-a1e7-6752cb72e930/iso-14703-2000>



PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 14703:2000

<https://standards.iteh.ai/catalog/standards/sist/09718370-380a-4b76-a1e7-6752cb72e930/iso-14703-2000>

© ISO 2000

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 734 10 79
E-mail copyright@iso.ch
Web www.iso.ch

Printed in Switzerland

Contents

Page

Foreword..... iv

1 Scope 1

2 Normative references 1

3 Terms and definitions 1

4 Sampling..... 2

5 Dispersing media 2

6 Deagglomeration of sample..... 4

7 Suspension and dispersion of sample 4

8 Treatment of suspension 5

9 Record of preparation conditions 6

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 14703:2000

<https://standards.iteh.ai/catalog/standards/sist/09718370-380a-4b76-a1e7-6752cb72e930/iso-14703-2000>

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 3.

Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this International Standard may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

International Standard ISO 14703 was prepared by Technical Committee ISO/TC 206, *Fine ceramics*.

iTeh STANDARD PREVIEW (standards.iteh.ai)

ISO 14703:2000

<https://standards.iteh.ai/catalog/standards/sist/09718370-380a-4b76-a1e7-6752cb72e930/iso-14703-2000>

Fine ceramics (advanced ceramics, advanced technical ceramics) — Sample preparation for the determination of particle size distribution of ceramic powders

1 Scope

This International Standard establishes a general wet sample preparation technique common to the size analysis of powdered fine ceramic materials. The analyzed size distribution of fine particles is strongly dependent on the sample preparation.

2 Normative references

The following normative documents contain provisions which, through reference in this text, constitute provisions of this International Standard. For dated references, subsequent amendments to, or revisions of, any of these publications do not apply. However, parties to agreements based on this International Standard are encouraged to investigate the possibility of applying the most recent editions of the normative documents indicated below. For undated references, the latest edition of the normative document referred to applies. Members of ISO and IEC maintain registers of currently valid International Standards.

ISO 3696:1987, *Water for analytical laboratory use — Specification and test methods*.

<https://standards.iteh.ai/catalog/standards/sist/09718370-380a-4b76-a1e7->

ISO 8213:1986, *Chemical products for industrial use Sampling techniques — Solid chemical products in the form of particles varying from powders to coarse lumps*.

3 Terms and definitions

For the purpose of this International Standard, the following terms and definitions apply.

3.1

fine particles

particles of whose sizes are less than a few micrometres

3.2

sample preparation

process that includes deagglomeration, dispersion of a test sample and treatment of suspension in stages up to taking the test portion

3.3

test sample

representative part taken from a quantity of material

3.4

test portion

quantity of material taken from the test sample entirely used in the test

**3.5
dispersing medium**

liquid in which the sample is dispersed and suspended

**3.6
Na-HMP**

sodium hexametaphosphate

4 Sampling

The sampling method, from a quantity of material to the test sample, shall comply with the requirements specified in ISO 8213, otherwise the methods specified in a national standard or as mutually agreed upon shall be complied with.

5 Dispersing media

5.1 Types of dispersing media

5.1.1 Aqueous solution of Na-HMP

A solution of Na-HMP with mass concentration of 0,01 % to 0,1 % should be used for the samples that are insoluble or can be regarded as insoluble. The dispersing medium shall be used no more than two days after preparation. The water should be equivalent to the water of type 1 as defined in ISO 3696.

5.1.2 Ethanol

Analytical grade or better ethanol should be used for samples soluble in, or reactive with, water.

<https://standards.iteh.ai/catalog/standards/sist/09718370-380a-4b76-a1e7-6752cb72e930/iso-14703-2000>

5.1.3 Other dispersing media

In case sufficient dispersing effects are not obtained with Na-HMP water solution or ethanol, other dispersing media, like polymer dispersant solution, can be used but the following conditions shall be satisfied.

- a) The dispersing medium shall not contain solid or liquid particles.
- b) The dispersing medium shall wet the sample material thoroughly.
- c) The sample shall not cause the particulate material to dissolve, swell, shrink or coagulate.
- d) The dispersing medium shall not foam during ultrasonic agitation.
- e) Analytical grade or better reagents shall be used for the dispersing medium.
- f) For wet sedimentation methods, the dispersing medium and the sample material shall have different densities.
- g) For the laser diffraction method, the dispersing medium and the sample material shall have different refractive indices.

5.2 Evaluation of dispersed conditions for the selection of dispersing medium

The evaluation of dispersed conditions should be made by one or more of the following techniques, for selection of the dispersant medium or the dispersant concentration.

- a) Measurement of zeta-potential: the greatest absolute value of zeta-potential, preferably more than 60 mV shall be required.

- b) Observation of sedimentation process: no clear boundary between the supernatant and the settling suspension shall be detected (Figure 1).
- c) Observation of sediment: the sediment shall be as dense as possible (Figure 2).
- d) Measurement of particle size distribution: the finest particle size distribution curve shall be obtained from the best dispersed particles.

NOTE The method of zeta-potential measurement should comply with the methods specified in a national standard or as mutually agreed upon.

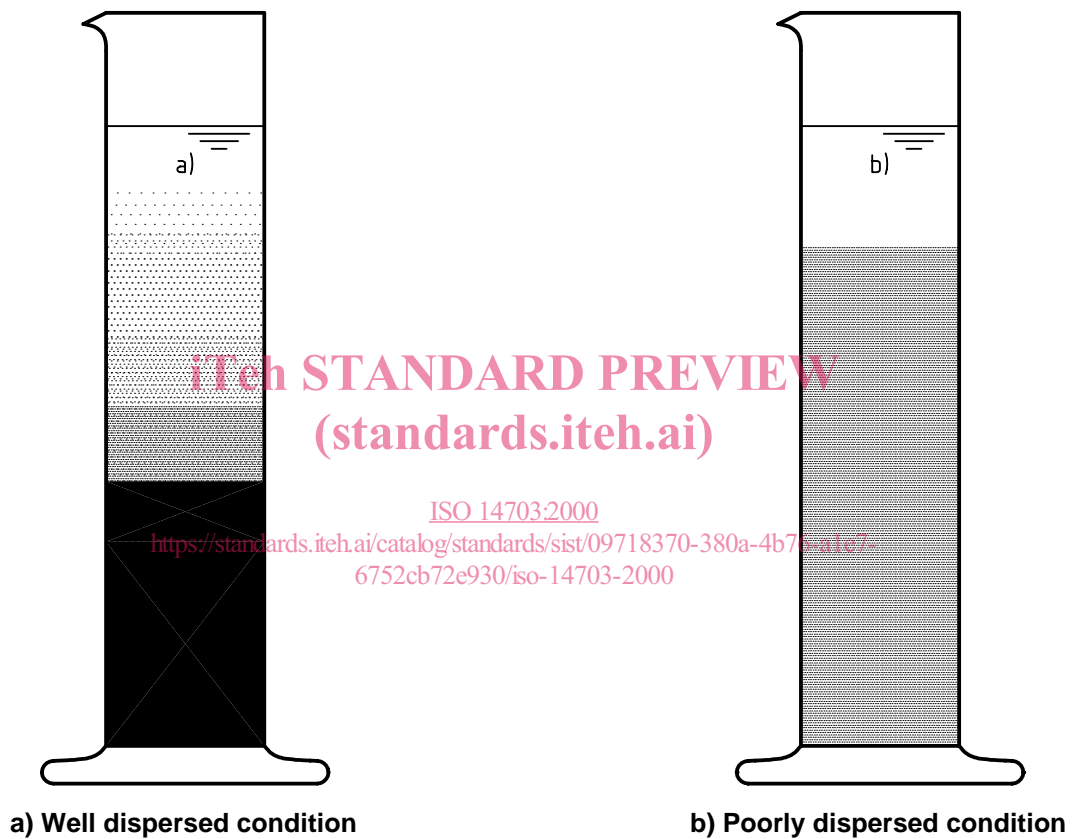


Figure 1 — Sedimentation process

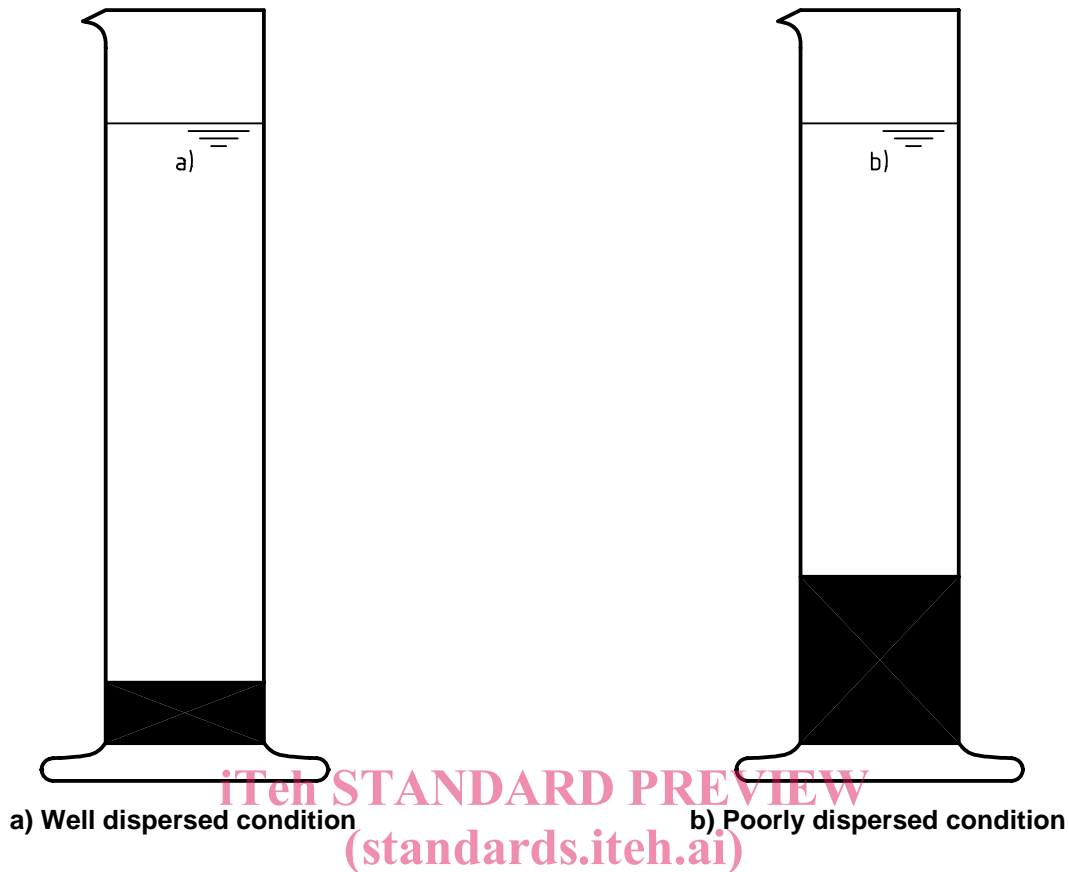


Figure 2 — Sediments

ISO 14703:2000

<https://standards.iteh.ai/catalog/standards/sist/09718370-380a-4b76-a1e7-6752cb72e930/iso-14703-2000>

6 Deagglomeration of sample

6.1 In order to improve the reproducibility of size analysis, the test sample should be deagglomerated by means of a mortar and pestle using the following procedure.

6.2 The weighed sample is placed in a dry mortar.

6.3 The sample is strongly disintegrated with a pestle using the whole inner wall of the mortar until most of the sample adheres to it.

6.4 The sample adhering to the mortar wall is scraped off with a spatula or equivalent and collected at the bottom of the mortar.

6.5 6.3 and 6.4 are repeated five times.

NOTE 1 Where it is known that the sample consists of separated primary particles, deagglomeration is not needed.

NOTE 2 Deagglomeration is not needed to determine the particle size of the sample "as received" or "as is".

7 Suspension and dispersion of sample

7.1 Suspension of sample

The sample shall be suspended in the dispersing medium at a given concentration. The concentration shall be dilute but denser than the proper concentration for the instrumental technique used. As the beaker capacity and the amount of suspension could affect the dispersing conditions, they shall be recorded.

7.2 Ultrasonic agitation of sample

7.2.1 Ultrasonic agitation of sample

Dispersion of the sample shall be made with any one of the following devices.

- a) Ultrasonic bath: the dispersion shall be made with the amount of water in the ultrasonic bath controlled in order to obtain the strongest dispersing effect and with the beaker set at the position undergoing the strongest ultrasonic intensity.
- b) Ultrasonic homogenizer: the suspension shall not be contaminated by foreign particles generated from its tip. Its output, tip size and tip position may influence the dispersing condition and therefore shall be recorded.

NOTE 1 Where foreign particles are magnetic materials, they can be eliminated by mixing with a magnet stirrer.

NOTE 2 If the ultrasonic agitation causes a noticeable increase in temperature of more than a few degrees centigrade, the sample should be cooled using water chilled with ice.

7.2.2 Ultrasonic agitation time

The sample suspension shall be agitated until the obtained particle size, e.g. median diameter, becomes constant independent of agitation time. If the obtained particle size does not become constant and continues to decrease with the agitation time, the agitation can be stopped at a certain point at which time the size analysis shall be conducted and recorded.

NOTE Ultrasonic agitation is not needed for size analysis of the sample "as received" or "as is".

iTech STANDARD PREVIEW
(standards.iteh.ai)

8 Treatment of suspension

ISO 14703:2000

8.1 Concentration control

<https://standards.iteh.ai/catalog/standards/sist/09718370-380a-4b76-a1e7-6752cb72e930/iso-14703-2000>

After ultrasonic agitation, and just before the size measurement, the concentration shall be adjusted, using the same dispersing media, to the concentration suitable for the instrument technique.

8.2 Change with passage of time

The suspension shall be kept agitated in order to prevent the sedimentation of coarse particles and reagglomeration when it is left to stand. If reagglomeration is not prevented by the agitation, the type and concentration of dispersant should be re-examined.

8.3 Taking test portion

When a test portion is taken from the suspension of the test sample, the suspension shall be agitated sufficient to avoid segregation.