
Ophthalmic optics — Contact lens care products — Microbiological requirements and test methods for products and regimens for hygienic management of contact lenses

iTeh STANDARD PREVIEW
Optique ophtalmique — Produits d'entretien des lentilles de contact — Exigences microbiologiques et méthodes d'essai des produits et protocoles d'entretien des lentilles de contact
(standards.iteh.ai)

[ISO 14729:2001](https://standards.iteh.ai/catalog/standards/sist/cdf29bd5-1b63-4ba4-bb4d-27f6be5b1c97/iso-14729-2001)

<https://standards.iteh.ai/catalog/standards/sist/cdf29bd5-1b63-4ba4-bb4d-27f6be5b1c97/iso-14729-2001>



PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 14729:2001

<https://standards.iteh.ai/catalog/standards/sist/cdf29bd5-1b63-4ba4-bb4d-27f6be5b1c97/iso-14729-2001>

© ISO 2001

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.ch
Web www.iso.ch

Printed in Switzerland

Contents

Page

Foreword.....	iv
Introduction.....	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Principle.....	2
4.1 General.....	2
4.2 Stand-alone test (Inoculum challenge test)	2
4.3 Regimen test	3
5 Performance requirements.....	3
5.1 Stand-alone test: Primary criteria (see also Table 1)	3
5.2 Stand-alone test: Secondary criteria (see also Table 1)	4
5.3 Regimen test: Regimen criteria (see also Table 1).....	4
6 Test methods.....	5
6.1 Materials and reagents.....	5
6.2 Preparation of microbial challenge (Inoculum)	6
6.3 Stand-alone procedure.....	7
6.4 Regimen procedure	10
Annex A (informative) Test organisms from other culture collections	13
Annex B (informative) Example of a membrane filtration procedure	14
Annex C (informative) Technical report: Virus testing	16
Annex D (informative) Technical report: <i>Acanthamoeba</i> testing	17
Annex E (informative) Technical report: Artificial tears (organic soil) in laboratory testing	18
Bibliography	19

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 3.

Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this International Standard may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

International Standard ISO 14729 was prepared by Technical Committee ISO/TC 172, *Optics and optical instruments*, Subcommittee SC 7, *Ophthalmic optics and instruments*.

Annexes A to E of this International Standard are for information only.

ITEH STANDARD PREVIEW
(standards.iteh.ai)

[ISO 14729:2001](https://standards.iteh.ai/catalog/standards/sist/cdf29bd5-1b63-4ba4-bb4d-27f6be5b1c97/iso-14729-2001)

<https://standards.iteh.ai/catalog/standards/sist/cdf29bd5-1b63-4ba4-bb4d-27f6be5b1c97/iso-14729-2001>

Introduction

Products for contact lens disinfection by chemical means are intended to reduce microbial contamination introduced during lens wear and removal, cleaning and storage and are required to contain antimicrobial agents capable of achieving this.

It is essential that all liquid contact lens care products are sterile until opened. Dry products (tablets, granules, etc.) should be subject to control of microbial contamination and should be dissolved in a suitable diluent immediately prior to use. Multidose contact lens care products must be adequately preserved or be packaged in a container designed and labelled to minimize the risk of injury resulting from in-use contamination.

Contact lenses are normally subject to a regimen of cleaning and contact lens disinfection between periods of wear. Aqueous solutions containing cleaning and/or disinfecting agents are commonly used for this purpose. These products may be marketed as solutions or as tablets for dissolution immediately prior to use in a suitable diluent such as saline.

The past 20 years of experience in the use and regulation of contact lens disinfecting products has shown distinct disinfecting antimicrobial criteria for this class of medical devices. Ocular toxicology concerns, process convenience and product comfort on the eye, have meant an evolution of products which maintain a low incidence of contact lens associated ocular infection when used as instructed by the manufacturer. This International Standard gives these distinct contact lens disinfecting antimicrobial criteria along with annexes to explain why viruses (annex C) and Acanthamoeba (annex D) are not included as challenges. Organic soil is not required for evaluation of contact lens care disinfecting products but may be used; an informative annex (annex E) is included to discuss organic soil in the context of contact lenses and contact lens care products.

[ISO 14729:2001](https://standards.iteh.ai/catalog/standards/sist/cdf29bd5-1b63-4ba4-bb4d-27f6be5b1c97/iso-14729-2001)

<https://standards.iteh.ai/catalog/standards/sist/cdf29bd5-1b63-4ba4-bb4d-27f6be5b1c97/iso-14729-2001>

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 14729:2001

<https://standards.iteh.ai/catalog/standards/sist/cdf29bd5-1b63-4ba4-bb4d-27f6be5b1c97/iso-14729-2001>

Ophthalmic optics — Contact lens care products — Microbiological requirements and test methods for products and regimens for hygienic management of contact lenses

1 Scope

This International Standard specifies two test methods for evaluating the antimicrobial activity of products to be marketed for contact lens disinfection by chemical means and for products that are part of a contact lens care regimen.

This International Standard is not applicable to the hygienic management of trial lenses.

NOTE General disinfection product standards are not applicable to contact lens care products, e.g. EN 1040:1997 and EN 1275:1997.

2 Normative references

The following normative documents contain provisions which, through reference in this text, constitute provisions of this International Standard. For dated references, subsequent amendments to, or revisions of, any of these publications do not apply. However, parties to agreements based on this International Standard are encouraged to investigate the possibility of applying the most recent editions of the normative documents indicated below. For undated references, the latest edition of the normative document referred to applies. Members of ISO and IEC maintain registers of currently valid International Standards.

ISO 8320-1:—¹⁾, *Contact lenses and contact lens care products — Vocabulary — Part 1: Contact lenses.*

ISO 8320-2:—¹⁾, *Contact lenses and contact lens care products — Vocabulary — Part 2: Contact lens care products.*

3 Terms and definitions

For the purposes of this International Standard, the definitions given in ISO 8320 apply together with the following.

3.1

contact lens disinfecting product

product that possesses cidal activity (kills, destroys and/or inactivates) meeting the primary criteria of the stand-alone test specified in this International Standard

3.2

contact lens disinfecting regimen

contact lens care regimen designed to meet both the secondary criteria of the stand-alone test and the regimen test as specified in this International Standard

1) To be published. (Revision of ISO 8320:1986)

3.3

contact lens disinfection

chemical or physical process to reduce the number of viable microorganisms as specified in the performance requirement sections of this International Standard

4 Principle

4.1 General

The stand-alone test is designed to qualify individual solutions with a suitable level of antimicrobial activity as contact lens disinfection products. The regimen test is designed to qualify individual solutions as part of a contact lens disinfecting regimen. Products meeting the regimen test criteria shall also meet the minimum performance requirements of the stand-alone test. It is fundamental that such products (unopened containers) are capable of meeting the requirements of the test throughout their labelled shelf life.

As described in Figure 1, contact lens care solutions which are designed to possess disinfecting properties shall be tested in the stand-alone test first. If the respective primary criteria are met (see 5.1), the product may be labelled as a contact lens disinfecting product. If the product fails the primary criteria of the stand-alone test, the product must exhibit sufficient antimicrobial activity to meet the secondary criteria of the stand-alone test as listed in 5.2. If these secondary criteria are met, the regimen test shall be performed in order to qualify the product as part of a contact lens disinfecting regimen by meeting the regimen criteria (see 5.3). If the product meets both the secondary criteria of the stand-alone test and the regimen test but fails the primary criteria of the stand-alone test, it shall be labelled as part of a contact lens disinfecting regimen.

The design of contact lens care products for cleaning and contact lens disinfection shall take into consideration the needs of patient compliance and the probability of non-compliance. For example, disinfecting time must be appropriate for contact lens wear.

NOTE Use of multiple or mixed microbial challenges can influence the apparent disinfecting activity of a particular product. The evaluation of these variables together with testing against a larger panel of microorganisms and testing of samples from partially used containers may be of value in developing a contact lens care product but are excluded from the scope of this International Standard. (See annexes C and D).


4.2 Stand-alone test (Inoculum challenge test)

The stand-alone test challenges a disinfecting product with a standard inoculum of a representative range of microorganisms and establishes the extent of their viability loss at pre-determined time intervals comparable with those during which the product may be used. The size of the microbial challenge chosen in this test is not intended to be representative of the likely challenge in practice but to provide countable numbers from which estimation of the rate and extent of viability loss can be determined.

In carrying out the test for antimicrobial activity the qualitative and quantitative compositions of the product have to be known at the time of testing by either analytical testing or extrapolation.

Appropriate measures shall be taken to inactivate or remove residual antimicrobial agents during culturing and counting of challenge organism survivors, and the effectiveness of these measures shall be validated. The action of this process during the test shall be demonstrated by the construction of suitable controls.

NOTE For information about virus testing, see annex C, and for *Acanthamoeba* testing, see annex D.

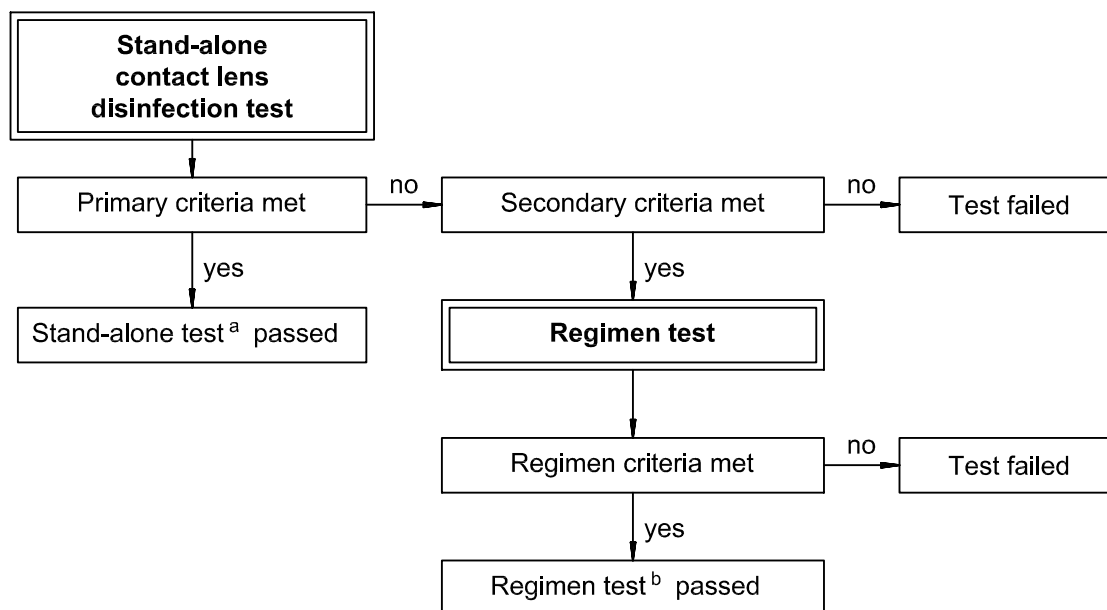

^a Product may be labelled as a contact lens disinfecting product.

^b Product shall be labelled as part of a contact lens disinfecting regimen.

Figure 1 — Flow chart for stand-alone test and regimen test

4.3 Regimen test

This is a test which challenges a multifunctional disinfecting regimen with a standard inoculum of a representative range of micro-organisms and which measures the viability loss after a predetermined time interval; the inoculum is carried through the regimen by being applied to a contact lens.

This procedure is applicable to multifunctional disinfecting regimens which may include the steps of cleaning, rinsing and soaking. In carrying out the regimen test procedure, the products are used in the manner and quantity recommended in product labelling and/or patient instructions.

The disinfecting stage of any proposed contact lens disinfecting regimen evaluated by this test shall satisfy the minimum requirements of the stand-alone test as described in Figure 1. Only those products that satisfy the minimum performance requirements for the stand-alone test may be incorporated into a disinfecting regimen.

In carrying out the test, qualitative and quantitative composition of all products used in the test regimen have to be known at the time of testing, either by analytical testing or extrapolation.

Appropriate measures shall be taken to inactivate or remove residual antimicrobial activity during culturing and counting of challenge organism survivors, and the effectiveness of these measures shall be validated. The action of this process during the test shall be demonstrated by the construction of suitable controls.

NOTE For problems associated with the use of human-worn lenses, see annex E.

5 Performance requirements

5.1 Stand-alone test: Primary criteria (see also Table 1)

5.1.1 Bacteria

The number of each challenge organism recovered per millilitre shall be reduced by an average value of not less than 99,9 % (3,0 logs) within the minimum recommended soaking period.

NOTE The value is determined by taking the average of the log reductions for each challenge organism for the individual lots tested.

5.1.2 Moulds and yeasts

The number of each challenge organism recovered per millilitre shall be reduced by an average value of not less than 90 % (1,0 log) within the minimum recommended soaking period with no increase at not less than four times the minimum recommended soaking period within an experimental error of $\pm 0,5$ logs.

NOTE The value is determined by taking the average of the log reductions for each challenge organism for the individual lots tested.

5.2 Stand-alone test: Secondary criteria (see also Table 1)

Products failing to meet the criteria in 5.1.1 or 5.1.2 shall be evaluated by the regimen test procedure described in 6.4, provided the sum of the averages is a minimum of 5,0 log units reduction for the three species of bacteria within the recommended soaking period with a minimum average of 1,0 log unit reduction for any single bacteria. Stasis for the yeast and mould shall be observed for the recommended soaking period within an experimental error of $\pm 0,5$ logs.

5.3 Regimen test: Regimen criteria (see also Table 1)

For each microbial species, the average regimen recovery count (for all lots tested) shall be no more than 10 cfu for each lens type/storage solution combination.

Data from more than one lens type should not be combined to calculate the average.

NOTE When qualifying a lens care product regimen for use with one lens type, the average count for each species requires averaging the data from the 24 inoculated and treated lenses of the one lens type. When qualifying a lens care product regimen for use with more than one lens type, the average count for each species by lens type would require averaging the data from the 12 inoculated and treated lenses for each lens type. See Table 4 for numbers of lenses to be used.

iTeh STANDARD PREVIEW
(standards.iteh.ai)
ISO 14729:2001
27f6be5b1c97/iso-14729-2001

Table 1 — Summary of performance requirements criteria for contact lens disinfection procedures

Test	Average log reduction at soaking time				
	Fungi		Bacteria		
	FS ^a	CA ^a	SM ^a	PA ^a	SA ^a
Stand-alone test: Primary Criteria	1	1	3	3	3
Stand-alone test: Secondary Criteria	b	b	c	c	c
Regimen test: Regimen criteria ^d	≈ 4 to 5	≈ 4 to 5	≈ 4 to 5	≈ 4 to 5	≈ 4 to 5
^a PA = <i>P. aeruginosa</i> ATCC 9027; SA = <i>S. aureus</i> ATCC 6538; SM = <i>S. marcescens</i> ATCC 13880; CA = <i>C. albicans</i> ATCC 10231; FS = <i>F. solani</i> ATCC 36031. ^b Stasis at the soaking time. ^c The minimum acceptable log reduction for all three bacteria combined is 5. The minimum acceptable log reduction for any single bacterial type is 1. ^d Equivalent to an average of not more than 10 cfu per lens type/storage solution combination.					

6 Test methods

ISO 14729:2001

<https://standards.iteh.ai/catalog/standards/sist/cdf29bd5-1b63-4ba4-bb4d-27f6be5b1c97/iso-14729-2001>

6.1 Materials and reagents

The materials and reagents (i.e. the test organisms, media and reagents, equipment and samples) are common to both the stand-alone procedure for disinfecting products and the regimen procedure for contact lens disinfection.

6.1.1 Test organisms

The strains listed in Table 2 shall be used.

NOTE Test organisms from other culture collections that may be used are listed in annex A.

Table 2 — Test organisms

<i>Pseudomonas aeruginosa</i>	ATCC 9027
<i>Staphylococcus aureus</i>	ATCC 6538
<i>Serratia marcescens</i>	ATCC 13880
<i>Candida albicans</i>	ATCC 10231
<i>Fusarium solani</i>	ATCC 36031

6.1.2 Culture media and reagents

6.1.2.1 Potato dextrose agar (PDA).