



Designation: C1269 – 97 (Reapproved 2003)

Standard Practice for Adjusting the Operational Sensitivity Setting of In-Plant Walk-Through Metal Detectors¹

This standard is issued under the fixed designation C1269; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

INTRODUCTION

Nuclear regulatory authorities require personnel entering designated security areas to be screened for concealed weapons. Additionally, in security areas containing specified quantities of special nuclear materials, personnel exiting the facility are required to be screened for metallic nuclear shielding material. Walk-through metal detectors are widely used to implement these requirements. Nuclear regulatory authorities usually specify an assortment of metal detector test objects that must all be detected by walk-through metal detectors. This practice provides a procedure for adjusting the operational sensitivity setting to the lowest setting necessary to detect the least likely to-be-detected test object in its least likely to-be-detected orientation while passing through the detection zone in the weakest known detection path. All other test objects will then be detected at this sensitivity setting anywhere in the detection zone.

1. Scope

1.1 This practice covers a procedure for adjusting the operational sensitivity of in-plant walk-through metal detectors. Performance of this procedure should result with in-plant walk-through metal detectors being adjusted to an initial operational sensitivity setting suitable for performance testing.

1.2 This practice does not set test object specifications or specify specific test objects. These should be specified by the regulatory authority.

1.3 This practice uses information developed by Practice C1270, or an equivalent procedure, which identifies the critical test object (from a specified set of test objects), its critical orientation, and the critical test path through the detection zone. In the case of Practice C1270, the information is found on the detection sensitivity map(s) for each in-plant walk-through metal detector.

1.4 This practice is one of several developed to assist operators of nuclear facilities with meeting the metal detection performance requirements of the regulatory authorities (see Appendix).

1.5 This standard practice is neither intended to set performance levels nor limit or constrain technologies.

1.6 This practice does not address safety or operational issues associated with the use of walk-through metal detectors.

1.7 The values stated in SI units are to be regarded as standards. The values given in parentheses are for information only.

2. Referenced Documents

2.1 ASTM Standards:²

C1238 Guide for Installation of Walk-Through Metal Detectors

C1270 Practice for Detection Sensitivity Mapping of In-Plant Walk-Through Metal Detectors

C1309 Practice for Performance Evaluation of In-Plant Walk-Through Metal Detectors

F1468 Practice for Evaluation of Metallic Weapons Detectors for Controlled Access Search and Screening

3. Terminology

3.1 Definitions of Terms Specific to This Standard:

3.1.1 *clean-tester, n*—a person who does not carry any extraneous metallic objects that would significantly alter the signal produced when the person carries a test object.

3.1.1.1 *Discussion*—Smaller test objects require more complete elimination of metallic objects. By example but not limitation, such extraneous metallic objects may include: metallic belt buckles, metal buttons, cardiac pacemakers, coins, metal frame eyeglasses, hearing aids, jewelry, keys, mechanical pens and pencils, shoes with metal shanks or arch supports,

¹ This practice is under the jurisdiction of ASTM Committee C26 on Nuclear Fuel Cycle and is the direct responsibility of Subcommittee C26.12 on Safeguard Applications.

Current edition approved Feb. 10, 2003. Published February 2003. Originally approved in 1994. Last previous edition approved in 1997 as C1269 – 97. DOI: 10.1520/C1269-97R03.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

metallic surgical implants, undergarment support metal, metal zippers, etc. In the absence of other criteria, a clean tester passing through a metal detector shall not cause a disturbance signal greater than 10 % of that produced when carrying the critical test object through the detector. Test objects requiring more complete elimination of extraneous metal to obtain less than 10 % signal disturbance.

3.1.1.2 *Discussion*—The tester shall have a weight between 50 to 104 kg (110 to 230 lb) and a height between 1.44 to 1.93 m (57 to 75 in.). Should a given detector be sensitive to body size because of design or desired sensitivity, the physical size of testers should be smaller and within a narrower range.

3.1.1.3 *Discussion*—It is recommended that the clean tester be surveyed with a high sensitivity hand-held metal detector to ensure that no metal is present.

3.1.2 *critical orientation*—the orthogonal orientation of a test object that produces the smallest detection signal or weakest detection anywhere in the detection zone; the orthogonal orientation of a test object that requires a higher sensitivity setting to be detected compared to the sensitivity settings required to detect the object in all other orthogonal orientations. See Fig. 1 for handgun orientations

3.1.2.1 *Discussion*—Critical orientations are determined by testing using a mapping procedure such as described in Practice C1270.

3.1.2.2 *Discussion*—The term critical orientation can be applied in two ways. Critical orientation can refer to the worst case orthogonal orientation in a single test path or the worst case orthogonal orientation for all the test paths (the entire detection zone). The two are coincident in the critical test path.

3.1.3 *critical sensitivity setting, n*—the lowest sensitivity setting of a detector at which the critical test object in its critical orientation is consistently detected (10 out of 10 test passes) when passed through the detection zone on the critical test path.

3.1.4 *critical test element, n*—see **test element**.

3.1.5 *critical test object, n*—see **test object**.

3.1.6 *critical test path, n*—the straight-line shortest-course path through the portal aperture, as defined by an element on the detection sensitivity map, that produces the smallest detection signal or weakest detection for the critical test object in its critical orientation. (see Figs. 2 and 3)

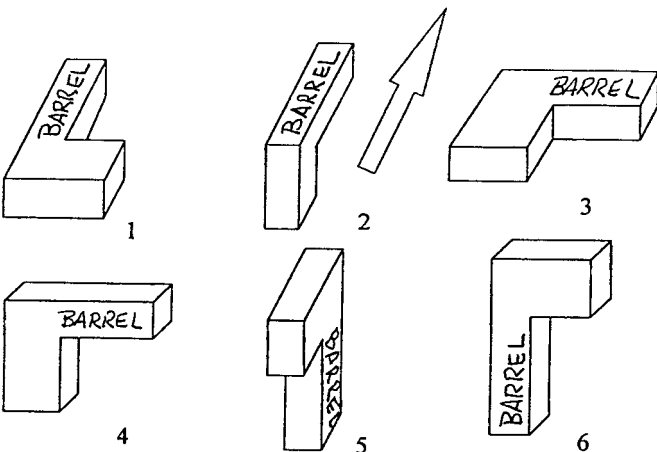


FIG. 1 Six Standard Orthogonal Orientations for a Handgun

52	68	52	52
49	55	75	71
50	52	75	73
48	58	74	70
35	63	81	72
47	62	89	74
47	69	79	75
57	71	81	79
62	74	74	69

critical test element

NOTE 1—Numbers are sensitivity setting values for a hypothetical detector. The numbers represent the lowest sensitivity setting at which the object was detected ten out of ten consecutive test passes through the indicated test path.

FIG. 2 Example of Detection Sensitivity Map

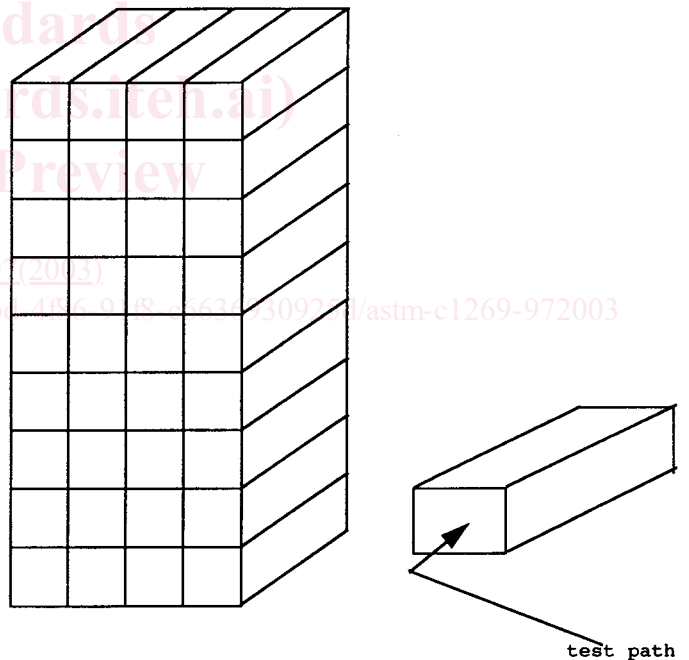


FIG. 3 3-D View of Detection Zones and Test Grid

3.1.7 *detection sensitivity map, n*—(see Fig. 2) a depiction of the grid used to define test paths through the detection zone with each element of the grid containing a value, usually the sensitivity setting of the detector, that is indicative of the detectability of the test object.

3.1.7.1 *Discussion*—These values are relative and describe the detection sensitivity pattern within the detection zone for the specific test object. The values are derived by identically testing each defined test path using a specific test object in a

single orthogonal orientation. The value is usually the minimum sensitivity setting of the detector that will cause a consistent alarm (10 out of 10 test passes) when the test object is passed through the detection field. **Appendix X2** is a sample form for a potential detection sensitivity map configuration.

3.1.8 *detection zone*, *n*—the volume within the portal aperture.

3.1.9 *detector*, *n*—see **walk-through metal detector**.

3.1.10 *element*, *n*—see **test element**.

3.1.11 *grid*, *n*—see **test grid**.

3.1.12 *grid element*, *n*—(1) a single block on a detection sensitivity map; (2) the rectilinear volume through the detection zone defined by coincident elements of identical grid works placed on either side of the portal aperture. (see **Figs. 2 and 3**)

3.1.12.1 *test path*, *n*—as defined by an element on a detection sensitivity map, a straight-line shortest-course path through the detection zone of a detector undergoing mapping, detection sensitivity, or detection sensitivity verification testing. (see **Fig. 3**)

3.1.13 *in-plant*, *adj*—installed in the location, position, and operating environment where the device will be used.

3.1.14 *orthogonal orientation*—as used in this practice, orthogonal orientation refers to alignment of the longitudinal axis of a test object along the *xyz* axes of the Cartesian coordinate system; *x* is horizontal and across the portal, *y* is vertical, and *z* is in the direction of travel through the portal.

3.1.15 *portal*, *n*—see **walk-through metal detector**. (See **Fig. 1** for handgun orientations)

3.1.16 *test element*, *n*—(see **Figs. 2 and 3**) for the purpose of testing, it is necessary to define discrete and repeatable straight-line shortest-course test paths through the detection zone. This can be done by using two identical networks (grids) made of nonconductive/nonmagnetic material attached across the entry and exit planes of the portal aperture so the networks coincide. A test object on the end of a probe can then be passed from one side of the portal aperture to the other side through corresponding openings, which results in the test object taking a reasonably straight-line shortest-course path through the detection zone. If the networks are constructed so that they can be put in-place identically each time they are used, then the test paths through the detection zone are repeatable over time. Thus, a test element is the volume of space defined by the boundaries of two corresponding network openings and it represents a straight-line shortest-course path through the detection zone.

3.1.16.1 *Discussion*—On a detection sensitivity map the corresponding networks appear as a rectangular grid with each element of the grid representing a test path through the detection zone. The element defining the critical test path is the critical test element.

3.1.17 *test grid*, *n*—a network of nonconductive/nonmagnetic material, such as string or tape, can be stretched across the entry and exit planes of the portal aperture to define test paths through the portal aperture; the material should not be hygroscopic.

3.1.17.1 *Discussion*—See **Fig. 2** for an example of a 4 by 9 element test grid.

3.1.18 *test object*, *n*—metallic item meeting dimension and material criteria used to evaluate detection performance.

3.1.18.1 *critical test object*—the one test object out of any given group of test objects that, in its critical orientation, produces the weakest detection signal anywhere in the detection zone. The group referred to consists of one or more objects that are to be detected at the same detector setting.

3.1.18.2 *Discussion*—Depending on the particular detector, some orientation sensitive test objects may have orientations at different locations in the detection zone that result in near critical sensitivity settings. Hence, care must be taken in determining the critical test object, its critical orientation, and the critical test path.

3.1.18.3 *shielding test object*—a test object representing special nuclear material shielding that might be used in a theft scenario.

3.1.18.4 *Discussion*—It is usually a metallic container or metallic material configured as a credible gamma-radiation shield for a specific type and quantity of special nuclear material. The object is specified by a regulatory authority or is based on the facility threat analysis, or both.

3.1.18.5 *weapon test object*, *n*—a handgun(s) or simulated handgun designated by or satisfying the regulatory authority requirement for a weapon test object.

3.1.18.6 *Discussion*—Care must be taken when selecting or designing a mock handgun. Simple blocks of metal shaped like a handgun will likely not cause a metal detector to react the same as it would to the intricate shapes and variable components of a real handgun. Most government agencies use actual guns for testing.

3.1.19 *walk-through metal detector (detector, portal)*, *n*—a free-standing screening device, usually an arch-type portal, using an electromagnetic field within its portal structure (aperture) for detecting metallic objects, specifically weapons or metallic shielding material, or both, on persons walking through the portal.

3.1.20 *walk speed (normal)*, *n*—walk speed is between 0.5 to 1.3 m/s (1½ to 2½ steps/s).

3.1.20.1 *Discussion*—The average casual walk rate is about 1¾ steps/s.

3.1.20.2 *shielding test object*, *n*—see **test object**.

3.1.20.3 *weapon test object*, *n*—see **test object**.

4. Summary of Practice

4.1 A clean-tester carries the critical test object in the critical orientation through the critical test element in the normal operating fashion. The metal detector sensitivity is adjusted upward, starting from a setting where no alarms occur, until the lowest sensitivity setting is found where 10 consecutive passes result with 10 consecutive alarms. This value is the initial operational sensitivity setting.

5. Significance and Use

5.1 Performing this procedure from this practice should result in a properly adjusted walk-through metal detector operating at or near the optimum sensitivity setting for the environment in which it is installed.