



Designation: E 2194 – 03

# Standard Practice for Multiangle Color Measurement of Metal Flake Pigmented Materials<sup>1</sup>

This standard is issued under the fixed designation E 2194; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

## INTRODUCTION

Surfaces that exhibit different colors depending on the angles of illumination or sensing are said to be “gonioapparent.” Colorimetric values of reflecting gonioapparent materials are derived from spectrophotometric (narrow band) or colorimetric (broad band) measurements of reflectance factor, at various angles of illuminating or sensing. When using spectral values, tristimulus values are computed using the CIE Standard Observer and the spectrum of the illuminant, as described in Practice E 308. This practice, E 2194, specifies the measurement of color observed at various aspecular angles.

## 1. Scope

1.1 This practice covers the instrumental requirements, standardization procedures, material standards, and parameters needed to make precise instrumental measurements of the colors of gonioapparent materials. This practice is designed to encompass gonioapparent materials; such as, automotive coatings, paints, plastics, and inks.

1.2 This practice addresses measurement of materials containing metal flake and pigments. The optical characteristics of materials containing pearlescent and interference materials are not covered by this practice. The measurement of materials containing metal flakes requires three angles of measurement to characterize the colors of the specimen.

NOTE 1—Data taken by utilizing this practice are for appearance quality control purposes. This procedure may not necessarily supply appropriate data for pigment identification.

1.3 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

## 2. Referenced Documents

### 2.1 ASTM Standards:

- D 2244 Practice for Calculation of Color Differences from Instrumentally Measured Color Coordinates<sup>2</sup>
- E 284 Terminology of Appearance<sup>2</sup>

E 308 Practice for Computing the Colors of Objects by Using the CIE System<sup>2</sup>

E 805 Practice for Identification of Instrumental Methods of Color or Color-Difference Measurement of Materials<sup>2</sup>

E 1164 Practice for Obtaining Spectrophotometric Data for Object Color Evaluation<sup>2</sup>

E 1345 Practice for Reducing the Effect of Variability of Color Measurement by Use of Multiple Measurements<sup>2</sup>

E 1708 Practice for Electronic Interchange of Color and Appearance Data<sup>2</sup>

E 1767 Practice for Specifying the Geometry of Observations and Measurements to Characterize the Appearance of Materials<sup>2</sup>

2.2 *CIE Document*:<sup>3</sup> 13b90c83/astm-e2194-03  
Publication No. 15.2 Colorimetry 2nd Edition

2.3 *NIST (NBS) Publication*:<sup>4</sup>

LC 1017 Standards for Checking the Calibration of Spectrophotometers

## 3. Terminology

3.1 Terms and definitions in Terminology E 284 are applicable to this practice. See Section “Specialized Terminology on Gonioapparent Phenomena.”

3.2 *Definitions*—Usually the term metallic refers to a metal material. However, this standard employs the alternative definition given in Terminology E 284 as:

3.2.1 *metallic, adj*—pertaining to the appearance of a gonioapparent material containing metal flakes.

<sup>1</sup> This practice is under the jurisdiction of ASTM Committee E12 on Color and Appearance and is the direct responsibility of Subcommittee E12.12 on Metallic and Pearlescent Colors.

Current edition approved Feb. 10, 2003. Published May 2003.

<sup>2</sup> *Annual Book of ASTM Standards*, Vol 06.01.

<sup>3</sup> Available from The U.S. National Committee of the CIE (International Commission on Illumination), C/o Thomas M. Lemons, TLA-Lighting Consultants, Inc., 7 Pond St., Salem, MA 01970.

<sup>4</sup> Available from National Institute of Standards and Technology (NIST), 100 Bureau Dr., Stop 3460, Gaithersburg, MD 20899-3460.

#### 4. Summary of Practice

4.1 This practice describes the procedures for the spectrophotometric and colorimetric measurement of metal flake pigmented materials. The results are reported in terms of CIE tristimulus values and other color coordinate systems. Standardization of the instrument used to measure these materials is defined. Guidelines are given for the selection of specimens and a measurement protocol given. Characterization of these materials requires measurement at a near-specular angle, a face (mid-aspecular angle) and a flop (far-specular) angle. These preferred aspecular angles are 15°, 45°, and 110°.

#### 5. Significance and Use

5.1 *Instrumental Measurement Angles*—This practice is designed to provide color data at specific measurement angles that can be utilized for quality control, color matching, and formulating in the characterization of metal flake pigmented materials.

5.2 *Materials*—This practice provides meaningful color information for metal flake pigmented materials, but has not been evaluated for use with pearlescent materials or other gonioapparent materials. This practice has been tested and verified on paint and coatings, and the same principles should apply to plastics containing metallic flake.

5.3 *Utilization*—This practice is appropriate for measurement and characterization of metal flake pigmented materials. These data may be used for quality control, incoming inspection, or color correction purposes.

5.4 *Specimen Requirements*—Even though a pair of specimens have the same color values at three angles, if there are differences in gloss, orange peel, texture, or flake orientation, they may not be a visual match.

NOTE 2—Information presented in this practice is based upon data taken on metallic materials coatings. Applicability of this practice to other materials should be confirmed by the user.

#### 6. Apparatus


6.1 *Instrument*—This practice requires measurement at multiple angles of illumination and sensing, usually accomplished by the use of a multiangle spectrophotometer as specified in this practice to characterize metal flake pigmented materials. Measurement with a single geometry cannot characterize the gonioappearance of these materials.

6.2 *Standardization*—A standardization plaque with assigned spectral reflectance factor or tristimulus values traceable to a national standardizing laboratory for each specified aspecular angle is required to standardize the instrument. The instrument manufacturer typically assigns the values to this plaque.

#### 7. Geometric Conditions

7.1 *Conventional Color Measurement*—In general purpose colorimetry, the common geometry involves illuminating at 45° and sensing at 0°. This geometry is designated 45:0 (45/0). Reverse geometry has the illumination at 0° and the sensing at 45°. That is, the illuminator and sensing geometries are interchanged. This reciprocal geometry is designated 0:45 (0/45). Either geometry is used.

7.1.1 A single bi-directional geometry is specified by illumination and sensing angles with respect to the normal of the plane of the specimen. Angles are measured relative to the normal. Angles on the same side of the normal as the illumination beam are written as positive angles; those on the other side are shown as negative, as shown in Fig. 1.

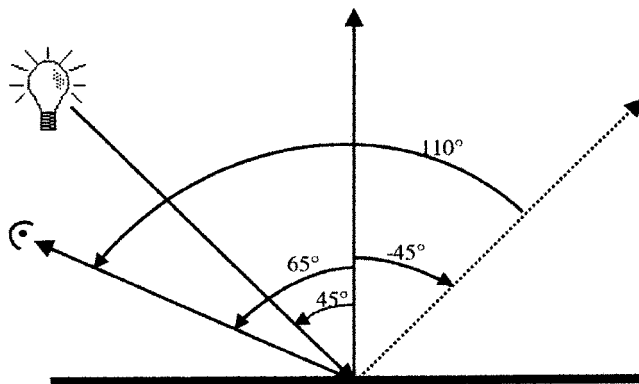

NOTE 1—A normal illumination angle = 45° and anormal sensing angle = 65°; therefore, aspecular angle = 45 + 65 = 110°.

FIG. 1 Example of Illuminating and Sensing Geometry

7.2 *Multiangle Uniplanar Measurement*—The color of metallic materials specimens varies with the angle of view. Thus measurements must be taken at more than one angle to characterize the change of color with angle. The measurement geometry for multiangle measurements is specified by aspecular angles. The aspecular angle is the sensing angle measured from the specular direction, in the illuminator plane. The angle is considered positive when measured from the specular direction towards the normal direction. Thus, if the specimen is illuminated at 45° to the normal the specular reflection will be at -45° (See Fig. 1). Sensing at 65° from the normal, and on the same side of normal as the illumination, is sensing 110° away from the specular direction; that is an aspecular angle of 110°. Thus, the aspecular angle is the sum of the materials colors, a specific aspecular angle gives the same measurement regardless of angle of illumination.<sup>5</sup>

7.3 *Annular and Circumferential Geometry*—Annular illumination provides incident light to a sample at all azimuthal angles. This type of illumination minimizes the contribution from directional effects such as the venetian blind effect and surface irregularities. Circumferential illumination is an approximation to annular illumination, incident light being provided from a discrete number of representative azimuthal angles. A large number or an odd number of illumination sources more closely approximates annular illumination. Annular or circumferential illumination minimizes directional effects. Therefore, measurements with annular or circumferential illumination may or may not correlate with how that specimen appears under directional illumination. For example, this system averaging may cause the measured color values of

<sup>5</sup> Rodrigues, *Die Farbe* 37, pp. 65-78 (1990).

two specimens to be the same or similar, even though these same two specimens would not match visually due to the fact that one specimen exhibits the venetian blind effect.

**7.4 Recommended Geometry**—The instrument shall conform to the following geometric requirements for measurement of reflectance factor unless otherwise agreed upon between the buyer and the seller. The preferred aspecular angles for measurement are 15°, 45°, and 110°.

**NOTE 3**—Given a geometric configuration, the reverse geometry is considered equivalent, if all other components of the instrument design are equivalent; for example, in the example shown in Fig. 1, the same result would be obtained with the illumination angle at 65° and the sensing angle at 45°. The aspecular angle would still be 110°.

**NOTE 4**—Measurement angles below are stated in terms of aspecular angles. It has been established that for metallic materials colors, a specific aspecular angle gives the same measurement regardless of angle of illumination. For pearlescent materials, it is known that color is also a function of angle of illumination. The importance of this phenomenon in measurement of pearlescent and interference materials for color difference for quality control or color correction purposes has not been established.


**NOTE 5**—Uniplanar instruments can measure the venetian blind effect. Circumferential and annular illumination will not quantify this gonioapparent effect.

**NOTE 6**—There are instruments commercially available with uniplanar, multiangle geometries that give results that characterize gonioapparent materials. These instruments will detect the venetian blind effect and other anomalies. Table 1 delineates the preferred angles. Note that circumferential geometry is limited to <90° aspecular angle. With the variety of instrumentation in common usage, it is incumbent upon the user to determine if an instrument with angles other than the preferred angles is appropriate in their application. Fig. 2

**7.4.1 Near Specular Angle**—The near specular angle used should be as close to the specular direction as possible, without detecting specular light. Surface imperfections can cause light to be reflected in a direction slightly away from the nominal specular direction. Measurement at 15° from the specular minimizes the effects of surface imperfections encountered in most practical industrial specimens. Differences in surface texture may result from spray application differences which can cause flake orientation differences. Measurement at 20° or 25° from specular may be chosen when less sensitivity to application differences between standard and batch is desired. In critical color matching applications, batches should be resampled and resprayed to eliminate surface differences and measurements shall be performed at 15°.5

**7.4.2 Face Angle**—The face color measurement shall be at an aspecular angle of 45° conforming to the geometrical specifications of CIE 15.2. The geometrical requirements are specified as follows:

**7.4.3 Flop Angle**—Visual observation of color differences in a few cases detects sidetone scattering better at angles further away from specular; hence, 110° is the preferred aspecular angle for flop measurement. In most but not all cases,

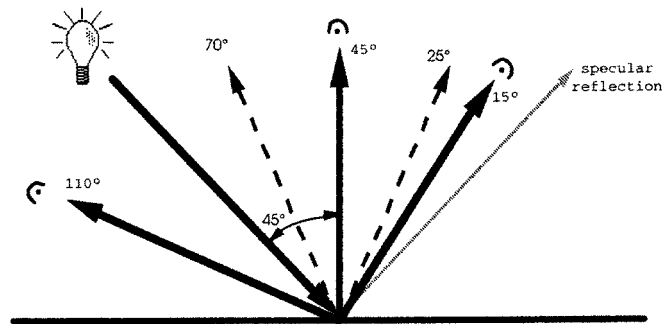

NOTE 1—Solid lines indicate preferred angles.  
**FIG. 2 Diagram of Aspecular Angles**

angles down to 70° give acceptable results. (**Warning**—Visual assessments of gonioapparent matches typically cover a wide range of aspecular angles, from very near specular, all the way to flop angles of 110° or even higher. Therefore, instrumental measurement at flop angles below 110° may occasionally result in measurements not agreeing with typical visual assessments. This will occur when specimens are an acceptable visual and instrumental match at angles such as 75° but unacceptable at 110°.)

**7.4.4 Illuminating and Sensing Beam Aperture Angles**—The illuminating beam aperture angle and the sensing beam aperture angle must be less than 8°.

**7.4.5 Tolerances on Measurement Geometries**—Instrumental measurement of specimens entails illumination of a sample and detection of light reflected at an aspecular angle. Illumination and detection may be collimated or non-collimated. The specimen may be under-illuminated or over-illuminated. The size of the illuminator, detector, and specimen, the distance between them, and uniformity of illumination or detection, will all provide different effective aspecular angles. The following ray tracing-procedure must be used to determine the effective aspecular angle and the distribution of the aspecular angles to ensure that the instrument design meets the specifications in Table 2. This ensures equivalent color readings between instruments differing in optical design. Fig. 3 schematically shows a procedure for ray tracing in 2-dimensional space. In actuality, we are dealing with 3-dimensional space and all angles must be calculated in 3-dimensional space relative to the surface normal of the specimen.

**7.4.5.1** All rays from the illuminator ( $I_1$  to  $I_n$ ) to all points on the sample area ( $S_1$  to  $S_n$ ) result in mirrored rays in the specular direction ( $Sp_1$  to  $Sp_n$ ). For each of these specular rays and for each point on the detector area ( $D_1$  to  $D_n$ ) the aspecular angles have to be calculated. In Fig. 3 the aspecular angles  $A_{111}$ ,  $A_{11n}$ ,  $A_{nn1}$ , and  $A_{nnn}$  are shown. They are all different, as

**TABLE 1**


| Uniplanar Angle | Preferred Angle |
|-----------------|-----------------|
| Near specular   | 15°             |
| Face angle      | 45°             |
| Flop angle      | 110°            |

**TABLE 2**

| Nominal aspecular angle                                   | 15°  | 25°  | 45°  | 75°  | 110° |
|---|------|------|------|------|------|
| Percentage of rays within 0.5° of nominal aspecular angle | ≥13% | ≥15% | ≥10% | ≥10% | ≥5%  |
| Maximum deviation from nominal aspecular angle            | ±8°  | ±8°  | ±8°  | ±10° | ±17° |

NOTE 1—Other geometries in common usage are: 25°, 70°, or 75°.



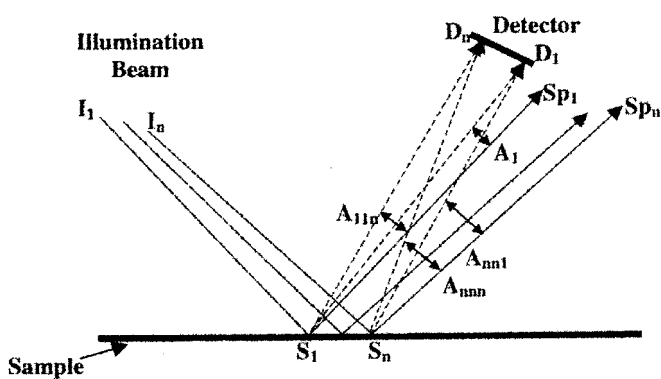

NOTE 1—Example is for 15° aspecular angle.

FIG. 3 Diagram of Ray Tracing Used to Calculate Effective Aspecular Angles and their Distribution

they result from different illumination directions, different points on the sample, and different points on the active detector area.

7.4.5.2 A minimum of 3000 such rays reaching the detector and their individual aspecular angles must be determined. All rays originating at the illuminator and striking the sample are to be included. The rays must be distributed evenly over the illuminator and the entire areas of the effective illuminated sample. The distribution of aspecular angles of all rays reaching the active detector area for each nominal aspecular angle must meet the specifications in Table 2.

7.4.5.3 For example, for the 15° nominal aspecular angle, instrument design must be such that no ray reaching the detector has an aspecular angle less than 7° or more than 23°, and at least 13 % of the rays have aspecular angles between 14.5° and 15.5°.

7.4.5.4 In calculation of aspecular angles, one must consider the distance between illuminator, sample, and receiver as it affects the relative intensity of the rays. In addition, non-uniformities of illumination and detection have to be included as weighting factors on each calculated aspecular angle, so that the effective distribution will be described.

NOTE 7—It will be useful for the user if the manufacturer of the instrument discloses the geometry of the instrument and references the appropriate ASTM standard.

## 8. Test Specimen

8.1 Measured values depend on the quality of the test specimens. The specimens must be statistically representative of the lot being tested and should meet the requirements listed below. If the specimens do not meet these requirements, include this information in Section 13.

8.2 *Specimen Handling*—Handle the specimens carefully. Touch them by their edges only. Never lay the measurement surface of the specimen down on another surface or stack specimens without a protective medium as recommended by the provider.

8.3 *Specimen Cleaning*—If necessary, clean the specimens following the providers' cleaning procedure.

8.4 *Specimen Conditioning*—Allow specimens to stabilize in the measurement environment for a period of 4 or more

hours before measurement, unless a different time period is agreed to by the parties concerned. Instrument heating may induce the effect of specimen thermochromism.

### 8.5 Specimen Physical Requirements:

8.5.1 The test specimen shall be 8 × 8 cm (approximately 3 × 3 in.) minimum.

NOTE 8—The recommendation for specimen size corresponds to the physical size required for observation by the CIE 1964 Supplemental Observer (10°). The specimen must subtend >10° when being observed. This observation usually occurs at approximately 45 cm (17.7 in.) from the eye. This specimen size is well suited for instrumental measurement and visual assessment.

8.5.2 The surface of the specimen to be measured should be essentially planar.

### 8.6 Specimen Optical Requirements:

8.6.1 *Uniformity*—Reference specimens and test specimens should be uniform in color and appearance when viewed in a lighting booth. They must be similar in appearance to make meaningful observations. There should be no appearance of mottling or banding in the specimens.

8.6.2 *Gloss*—Specimens should be uniform and similar in gloss when viewed in a lighting booth.

8.6.3 *Surface Texture*—The standard and batch being compared should have substantially similar surface textures. Orange peel is a common example of surface texture.

8.6.4 *Specimen Flake Distribution*—Examine the specimens to ensure that they have similar flake size and distribution. Dissimilar flake distributions will cause results to vary significantly.

8.6.5 *Orientation*—Consistent orientation of the specimen for presentation to the measuring instrument must be controlled for repeatable measurements. This is necessary to minimize errors due to indiscriminate matching of the directionality of the specimen to that of the instrument.

## 9. Instrument Standardization

9.1 Standardization is essential to ensure that spectrophotometric or tristimulus measurements with minimum bias are reported. For the measurement of reflectance factor, two standardizations are required, namely,

9.1.1 *Optical Zero (0) Level Standardization*—To verify the optical zero, the instrument manufacturer normally supplies a highly polished black glass or a black trap that has an assigned reflectance factor value.

9.1.2 *Full Scale Standardization*—To standardize the instrument relative to the perfect reflecting diffuser, the instrument manufacturer should provide a standardization plaque with multiangle calibration traceable to a standardizing laboratory.

9.1.3 *Photometric Scale Validation*—To ascertain proper standardization, measure a reference plaque immediately after the standardization sequence and validate that the measured values agree with the assigned values within 0.05 reflectance unit.

9.1.4 *Discussion*—Typically a neutral gray of >50 % reflectance is used for this purpose.

## 10. Instrumental Performance Verification

10.1 The use of validation standards to verify spectrophotometric performance of an instrument is recommended. These