



SLOVENSKI STANDARD

SIST ISO 10705-4:2007

01-februar-2007

Kakovost vode - Ugotavljanje prisotnosti in števila bakteriofagov - 4. del – Štetje bakteriofagov, ki okužijo *Bacteroides fragilis*

Water quality -- Detection and enumeration of bacteriophages -- Part 4: Enumeration of bacteriophages infecting *Bacteroides fragilis*

iTeh STANDARD PREVIEW

Qualité de l'eau -- Détection et dénombrement des bactériophages -- Partie 4: Dénombrement des bactériophages infectant *Bacteroides fragilis*

[SIST ISO 10705-4:2007](https://standards.itih.ai/catalog/standards/sist/96843da6-1214-4809-8705-c0068a472519/sist-iso-10705-4-2007)

Ta slovenski standard je istoveten z: **ISO 10705-4:2001**

ICS:

07.100.20 Mikrobiologija vode Microbiology of water

SIST ISO 10705-4:2007

en

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[SIST ISO 10705-4:2007](#)

<https://standards.iteh.ai/catalog/standards/sist/96843da6-1214-4809-8705-e00b8a4725f9/sist-iso-10705-4-2007>

INTERNATIONAL
STANDARD

ISO
10705-4

First edition
2001-12-15

**Water quality — Detection and enumeration
of bacteriophages —**

Part 4:

**Enumeration of bacteriophages infecting
*Bacteroides fragilis***

iTeh STANDARD PREVIEW

Qualité de l'eau — Détection et dénombrement des bactériophages —

(standards.iteh.ai)

Partie 4: Dénombrement des bactériophages infectant Bacteroides fragilis

[SIST ISO 10705-4:2007](https://standards.iteh.ai/catalog/standards/sist/96843da6-1214-4809-8705-e00b8a4725f9/sist-iso-10705-4-2007)

<https://standards.iteh.ai/catalog/standards/sist/96843da6-1214-4809-8705-e00b8a4725f9/sist-iso-10705-4-2007>



Reference number
ISO 10705-4:2001(E)

© ISO 2001

ISO 10705-4:2001(E)

PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

iTeh STANDARD PREVIEW (standards.iteh.ai)

SIST ISO 10705-4:2007

<https://standards.iteh.ai/catalog/standards/sist/96843da6-1214-4809-8705-e00b8a4725f9/sist-iso-10705-4-2007>

© ISO 2001

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.ch
Web www.iso.ch

Printed in Switzerland

Contents

	Page
1 Scope	1
2 Normative references	1
3 Term and definition	1
4 Safety precautions	2
5 Principle	2
6 Reagents	2
7 Apparatus	2
8 Microbiological reference cultures	3
9 Sampling	4
10 Preparation of test materials	4
11 Procedure	7
12 Expression of results	9
13 Test report	10

Annexes

A General description of bacteriophages infecting <i>Bacteroides fragilis</i>	11
B Culture media and diluents	12
C Alternative method for preparing inoculum cultures.....	17
D Culturing of Bacteriophage B56-3.....	18
Bibliography.....	19

iTeh STANDARD PREVIEW
(standards.iteh.ai)

SIST ISO 10705-4:2007

[https://standards.iteh.ai/catalog/standards/sist/96843da6-1214-4809-](https://standards.iteh.ai/catalog/standards/sist/96843da6-1214-4809-8705-e00b8a4725d9/sist-iso-10705-4-2007)

[8705-e00b8a4725d9/sist-iso-10705-4-2007](https://standards.iteh.ai/catalog/standards/sist/96843da6-1214-4809-8705-e00b8a4725d9/sist-iso-10705-4-2007)

ISO 10705-4:2001(E)

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 3.

Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this part of ISO 10705 may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

International Standard ISO 10705-4 was prepared by Technical Committee ISO/TC 147, *Water quality*, Subcommittee SC 4, *Microbiological methods*.

ISO 10705 consists of the following parts, under the general title *Water quality — Detection and enumeration of bacteriophages*:

- Part 1: Enumeration of F-specific RNA bacteriophages
- Part 2: Enumeration of somatic coliphages
- Part 3: Validation of methods for concentration of bacteriophages from water
- Part 4: Enumeration of bacteriophages infecting *Bacteroides fragilis*

Annexes A, B, C and D of this part of ISO 10705 are for information only.

Water quality — Detection and enumeration of bacteriophages —

Part 4: Enumeration of bacteriophages infecting *Bacteroides fragilis*

1 Scope

This part of ISO 10705 specifies a method for the detection and enumeration of bacteriophages infecting *Bacteroides fragilis* by incubating the sample with an appropriate host-strain. The method is applicable to all kinds of water, sediments and sludge extracts, where necessary after dilution. In the case of low phage numbers, a pre-concentration step may be necessary for which a separate International Standard has been developed. The method is also applicable to shellfish extracts.

NOTE It is desirable for International Standards to be adopted as widely as possible. This part of ISO 10705 includes reference to alternative procedures which obviate the need for expensive materials or equipment which may not be readily available in developing countries. Use of these alternatives will not affect the performance of this method.

2 Normative references

The following normative documents contain provisions which, through reference in this text, constitute provisions of this part of ISO 10705. For dated references, subsequent amendments to, or revisions of, any of these publications do not apply. However, parties to agreements based on this part of ISO 10705 are encouraged to investigate the possibility of applying the most recent editions of the normative documents indicated below. For undated references, the latest edition of the normative document referred to applies. Members of ISO and IEC maintain registers of currently valid International Standards.

ISO 3696, *Water for analytical laboratory use — Specification and test methods*

ISO 5667-1, *Water quality — Sampling — Part 1: Guidance on the design of sampling programmes*

ISO 5667-2, *Water quality — Sampling — Part 2: Guidance on sampling techniques*

ISO 5667-3, *Water quality — Sampling — Part 3: Guidance on the preservation and handling of samples*

ISO 6887-1, *Microbiology of food and animal feeding stuffs — Preparation of test samples, initial suspension and decimal dilutions for microbiological examination — Part 1: General rules for the preparation of the initial suspension and decimal dilutions*

ISO 8199, *Water quality — General guide to the enumeration of micro-organisms by culture*

3 Term and definition

For the purposes of this part of ISO 10705, the following term and definition applies.

3.1

bacteriophage infecting *Bacteroides fragilis*

bacterial virus which is capable of infecting selected *Bacteroides fragilis* host strains by attachment to the bacterial cell wall as the first step of the infectious process

NOTE 1 Such bacteriophages produce visible plaques (clearance zones) in a confluent lawn of host bacteria grown under appropriate culture conditions.

ISO 10705-4:2001(E)

NOTE 2 A general description of bacteriophages infecting *B. fragilis* is given in annex A.

4 Safety precautions

The host strain used in this part of ISO 10705 is non-pathogenic to man and animals and should be handled in accordance with the normal (national or international) safety procedures for bacteriological laboratories. Bacteriophages infecting *Bacteroides fragilis* are non-pathogenic for man and animals, but some types are very resistant to drying. Appropriate precautions shall be taken to prevent cross-contamination of test materials, particularly when examining or handling cultures of high titre or when inoculating cultures of the host strains. Such procedures shall be carried out in a biohazard cabinet or a separate area of the laboratory. Chloroform is a carcinogenic substance. Observe relevant safety precautions or use an alternative method of equal efficacy.

It is recommended that personnel using this method have or acquire some experience in handling anaerobic bacteria.

5 Principle

The sample is mixed with a small volume of semi-solid nutrient medium. A culture of host-strain is added and plated on a solid nutrient medium. After this, incubation and reading of plaques take place. The results are expressed as the number of plaque-forming particles (also named plaque-forming units, pfu) per unit of volume (pfp/ml, pfp/l, etc.).

6 Reagents

6.1 Basic materials.

Use ingredients of uniform quality and chemicals of analytical grade for the preparation of culture media and reagents and follow the instructions given in annex B. For information on storage see ISO 8199, except where indicated in this part of ISO 10705. Alternatively, use dehydrated complete media and follow strictly the manufacturer's instructions.

Other grades of chemicals may be used provided they can be shown to lead to the same results.

6.2 Water, for the preparation of media, glass-distilled or deionized, free from substances which might inhibit bacterial growth under the conditions of the test, and complying with ISO 3696.

6.3 Diluent, for making sample dilution, such as peptone-saline solution or another diluent complying with ISO 6887-1.

7 Apparatus

Apart from apparatus supplied sterile, sterilize any glassware and other equipment in accordance with ISO 8199.

Usual sterile, microbiological laboratory equipment and glassware or disposable plastics-ware in accordance with ISO 8199 and including the following:

7.1 Hot-air oven, for dry-heat sterilization, and an **autoclave**.

7.2 Incubator or **water bath**, thermostatically maintained at $(36 \pm 2) ^\circ\text{C}$.

7.3 Incubator or **water bath**, thermostatically maintained at $(36 \pm 2) ^\circ\text{C}$ with a shaking device.

7.4 Water bath or **heating block**, thermostatically maintained at $(45 \pm 1) ^\circ\text{C}$.

7.5 Water bath or **equivalent device**, for melting of agar media.

7.6 pH meter, and **pH paper**.

- 7.7 Counting apparatus**, with indirect, oblique light.
- 7.8 Deep freezer**, thermostatically maintained at $(-20 \pm 5) ^\circ\text{C}$.
- 7.9 Deep freezer**, thermostatically maintained at $(-70 \pm 10) ^\circ\text{C}$ or **liquid nitrogen storage vessel**.
- 7.10 Spectrophotometer**, equipped with a filter for the range of 500 nm to 650 nm with a maximum bandwidth of ± 10 nm, capable of holding cuvettes (7.21) having an optical path length of 1 cm or Hungate glass tubes (7.20) with butyl rubber stopper and screw cap or screw-capped glass culture tubes.
- 7.11 Anaerobic cabinet**, or **jars** or **bags**, as well as **anaerobiosis generators** and **anaerobiosis indicators**.
- 7.12 Refrigerator**, temperature set at $(5 \pm 3) ^\circ\text{C}$.
- 7.13 Petri dishes**, having a diameter of 9 cm, and vented.
- 7.14 Graduated pipettes**, having a capacity of 0,1 ml, 1 ml, 5 ml and 10 ml and **Pasteur pipettes**.
- 7.15 Glass bottles**, of suitable volumes.
- 7.16 Screw-capped glass bottles**, of suitable volumes.
- 7.17 Culture tubes**, with caps or suitable alternatives.
- 7.18 Screw-capped glass culture tubes**.
- 7.19 Measuring cylinders**, of suitable capacity.
- 7.20 Hungate glass tubes**, with butyl rubber stopper and screw cap or screw-capped glass culture tubes which can fit in the spectrophotometer (see Figure 1).
- 7.21 Cuvettes**, having an optical path length of 1 cm.
- 7.22 Membrane filter units**, for decontamination, having a pore size of $0,2 \mu\text{m}$, preferably low protein-binding membranes, as for example, those composed of polyvinylidene difluoride.
- 7.23 Plastics vials**, lidded, having a capacity of 3 ml.
- 7.24 Glass vials**, screw-capped, having a capacity of 3 ml.
- 7.25 Syringes and needles**.
- 7.26 Cotton swabs**.

8 Microbiological reference cultures

The recommended host strain is *Bacteroides fragilis* RYC2056 (ATCC 700786).^[1]

Use bacteriophage B56-3 (ATCC 700786-B1) infecting *Bacteroides fragilis* RYC2056 for the preparation of reference materials (11.4).

NOTE The ATCC strains are available from American Type Culture Collection (ATCC), 10801 University Boulevard, Manassas, VA 20110-2209, USA. This information is given for the convenience of users of this part of ISO 10705 and does not constitute an endorsement by ISO of the product named. Equivalent products may be used if they can be shown to lead to the same results.

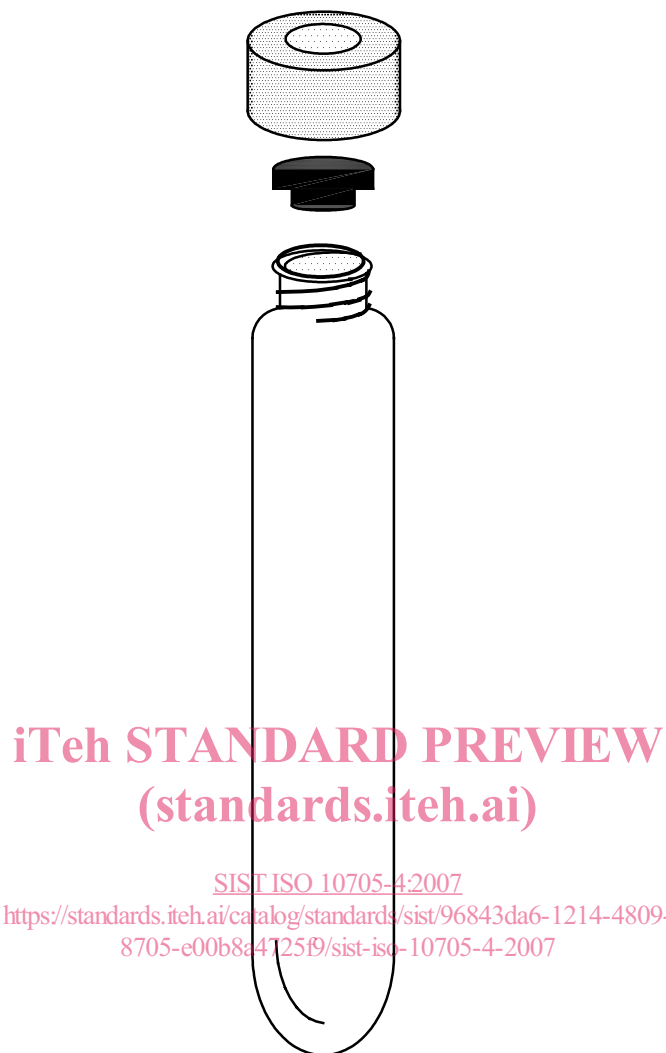


Figure 1 — Hungate glass tube with rubber stopper and screw cap

9 Sampling

Take samples and deliver them to the laboratory in accordance with ISO 8199, ISO 5667-1, ISO 5667-2 and ISO 5667-3.

10 Preparation of test materials

10.1 Culturing and maintenance of host strains

10.1.1 General

The culturing and maintenance of host strains involves several stages which are summarized in Figure 2.

Bacteroides fragilis is an obligate anaerobe. However, it does not require handling under conditions of strict anaerobiosis. Incubation of cultures in solid media should be carried out in an anaerobic cabinet, or anaerobic jars or bags. When using liquid media it is sufficient to ensure that containers are completely filled and closed with a screw cap.

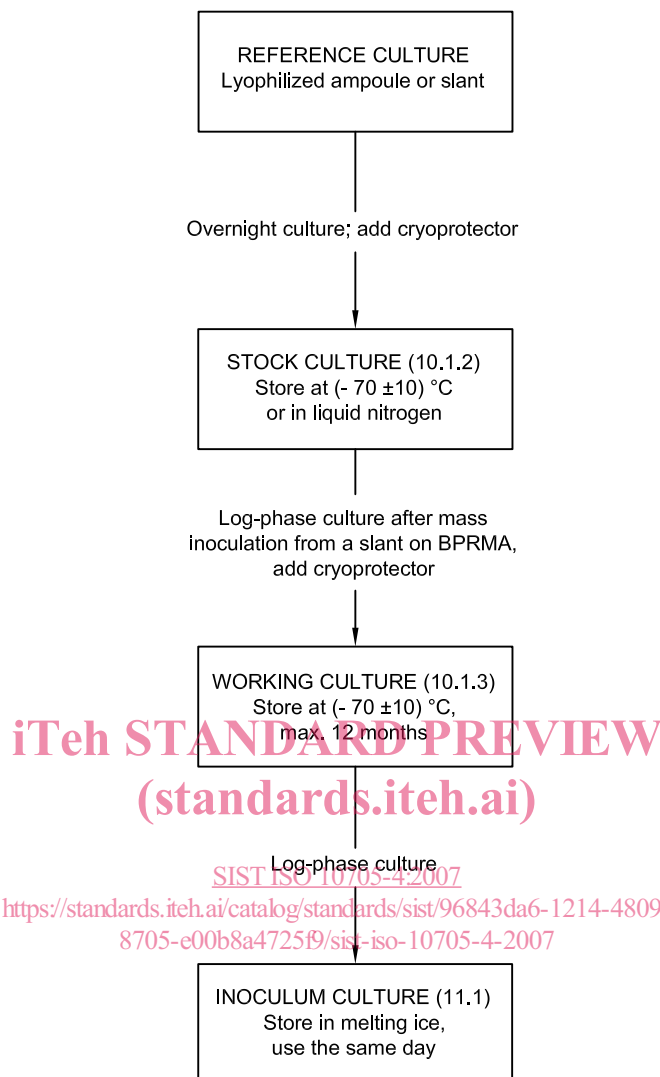


Figure 2 — Scheme for the culturing and maintenance of host strains

10.1.2 Preparation of stock cultures

Rehydrate the content of a lyophilized ampoule of the reference culture of the host strain in 1 ml of *Bacteroides* phage recovery medium broth (BPRMB) (B.1) using a Pasteur pipette (7.14). Inoculate the suspensions in 10 ml of BPRMB (B.1) in a 10 ml screw-capped glass tube (see 10.1.1) and incubate at $(36 \pm 2) ^\circ\text{C}$ for (21 ± 3) h. Aseptically soak a sterile cotton swab with the culture and streak it onto a plate of *Bacteroides* phage recovery medium agar (BPRMA) (B.2). Incubate the culture in an anaerobic cabinet, jar or bag at $(36 \pm 2) ^\circ\text{C}$ for (44 ± 4) h.

Alternatively, if a culture in slant is available, streak it with a sterile cotton swab directly onto a plate of BPRMA (B.2). Incubate the culture in an anaerobic cabinet, jar or bag at $(36 \pm 2) ^\circ\text{C}$ for (44 ± 4) h.

Inoculate cells (mass inoculation with a sterile cotton swab) from the plate into 10 ml of BPRMB (B.1) in a 10 ml screw-capped glass tube (7.18). Be sure that the tube is completely filled (see 10.1.1). If dense growth occurs, inoculate 1/8 of the growth onto the BPRMA plate; if poor growth occurs, use 1/2 of the growth onto the plate. Incubate the culture at $(36 \pm 2) ^\circ\text{C}$ for (21 ± 3) h.