INTERNATIONAL STANDARD

ISO 5362

Third edition 2000-12-01

Anaesthetic reservoir bags

Ballons réservoirs d'anesthésie

iTeh STANDARD PREVIEW (standards.iteh.ai)

ISO 5362:2000 https://standards.iteh.ai/catalog/standards/sist/3af3e907-60a6-49e4-b8d9c591ba509137/iso-5362-2000



PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

iTeh STANDARD PREVIEW (standards.iteh.ai)

ISO 5362:2000 https://standards.iteh.ai/catalog/standards/sist/3af3e907-60a6-49e4-b8d9c591ba509137/iso-5362-2000

© ISO 2000

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.ch
Web www.iso.ch

Printed in Switzerland

Contents		Page
1	Scope	1
2	Normative references	1
3	Terms and definitions	1
4	General requirements	2
	Prevention of electrostatic charges	
	Requirements for bags supplied sterile	
7	Marking	4
	Information to be supplied by the manufacturer	
An	nnexes	
Α	Test for leakage	5
A. 1	Principle	5
A.2	2 Apparatus	5
A.3	Procedure	5
A. 4	Procedure Expression of results ITEH STANDARD PREVIEW	5
В	Determination of capacity(standards.iteh.ai)	
B.1		6
B.2	2 Apparatus <u>ISO.5362:2000</u>	6
B.3	Procedure https://standards.iteh.ai/catalog/standards/sist/3af3e907-60a6-49e4-b8d9-	6
B.4	Expression of results	6
С	Test for security of attachment of plain neck to 22 mm male conical connector	
C.1		
C.2	2 Apparatus and materials	7
C.3	Procedure	7
D	Test for security of attachment of adaptor of assembled neck to bag	8
D.1		
D.2	P Apparatus	8
D.3	Procedure	8
Е	Test for resistance to pressure required to distend the bag (pressure/volume)	9
E.1		
E.2	P. Apparatus	9
E.3	Procedure	9
E.4	Expression of results	9
F	Test for resistance to pressure required to distend the bag using air (pressure/volume)	
F.1		
F.2	·	
F.3		
F.4		
G	Recommendations for materials	
Bib	liography	

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 3.

Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this International Standard may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

International Standard ISO 5362 was prepared by Technical Committee ISO/TC 121, *Anaesthetic and respiratory equipment*, Subcommittee SC 2, *Tracheal tubes and other equipment*.

This third edition cancels and replaces the second edition (ISO 5362:1986), which has been technically revised. This edition differs from the previous edition primarily in that it contains test methods for leakage and for security of attachment of the necks of reservoir bags. It also differs in that the maximum pressure used to test resistance to distension of the bag has been increased to 6,0 kPa (see annex E).

Annexes B, C, D and E form a normative part of this International Standard. Annexes A, F and G of this International Standard are for information only.//standards.iteh.ai/catalog/standards/sist/3af3e907-60a6-49e4-b8d9-

c591ba509137/iso-5362-2000

Introduction

This International Standard is one of a series dealing with anaesthetic and respiratory equipment. This International Standard is primarily concerned with the design of the neck, size designation and resistance to pressure required to distend anaesthetic reservoir bags.

The requirement that reservoir bags should be electrically conductive when used with a flammable anaesthetic is widely recognized and is of particular importance when such bags are rhythmically compressed by the anaesthetic provider in order to provide intermittent positive-pressure ventilation.

This International Standard gives requirements for both antistatic and non-antistatic bags. Only antistatic bags are suitable for use with flammable anaesthetic agents.

This International Standard includes requirements for both single-use and reusable bags. Reusable bags are intended to comply with the requirements of this International Standard for the recommended product life.

The reference test method given as annex E is not practical for routine use in manufacturing control, because it involves filling the bag with water. For this reason, another test method using air rather than water has been provided for information in annex F. This may ultimately be suitable as the reference test method if it can be shown to give results equivalent to annex E.

A test method for leakage of bags using air rather than water is given as annex A for information only. Recommendations for materials are given in annex G. (standards.iteh.ai)

ISO 5362:2000 https://standards.iteh.ai/catalog/standards/sist/3af3e907-60a6-49e4-b8d9c591ba509137/iso-5362-2000

iTeh STANDARD PREVIEW (standards.iteh.ai)

ISO 5362:2000 https://standards.iteh.ai/catalog/standards/sist/3af3e907-60a6-49e4-b8d9-c591ba509137/iso-5362-2000

Anaesthetic reservoir bags

1 Scope

This International Standard specifies requirements for antistatic and non-antistatic reservoir bags for use with anaesthetic apparatus or lung-ventilator breathing systems. It includes requirements for the design of the neck, size designation, distension and, where relevant, for electrical resistance.

This International Standard is not applicable to special-purpose bags, for example bellows and self-expanding bags. Bags for use with anaesthetic gas scavenging systems are not considered to be anaesthetic reservoir bags and are thus outside the scope of this International Standard.

2 Normative references

The following normative documents contain provisions which, through reference in this text, constitute provisions of this International Standard. For dated references, subsequent amendments to, or revisions of, any of these publications do not apply. However, parties to agreements based on this International Standard are encouraged to investigate the possibility of applying the most recent editions of the normative documents indicated below. For undated references, the latest edition of the normative document referred to applies. Members of ISO and IEC maintain registers of currently valid International Standards.

ISO 4287, Geometrical Product Specifications (GPS) — Surface texture: Profile method — Terms, definitions and surface texture parameters. ISO 53622000

https://standards.iteh.ai/catalog/standards/sist/3af3e907-60a6-49e4-b8d9-

ISO 5356-1, Anaesthetic and respiratory equipment : Conical connectors — Part 1: Cones and sockets.

ISO 7000, Graphical symbols for use on equipment — Index and synopsis.

ISO 11607, Packaging for terminally sterilized medical devices.

IEC 60601-1:1988, Medical electrical equipment — Part 1: General requirements for safety.

EN 556:1994, Sterilization of medical devices — Requirements for medical devices to be labelled "sterile".

EN 980, Terminology, symbols and information provided with medical devices — Graphic symbols for use in the labelling of medical devices.

3 Terms and definitions

For the purposes of this International Standard, the following terms and definitions apply.

3 1

anaesthetic reservoir bag

collapsible gas container which is a component in a breathing system

[ISO 4135:—]

3.2

assembled neck

neck incorporating an adaptor

3.3

adaptor

specialized connector to establish functional continuity between otherwise disparate or incompatible components, one end of which is intended to be inserted into the neck of the bag, the other end having a conical connector complying with ISO 5356-1

3.4

plain neck

neck designed to fit directly over a male conical connector complying with ISO 5356-1

3.5

tai

tubular extension of the bag at the end opposite to the neck

4 General requirements

4.1 Reusable bags

Reusable bags shall comply with the requirements of this International Standard throughout the recommended product life as given in clause 8.

4.2 Size designation

iTeh STANDARD PREVIEW

The size of the bag shall be designated by the nominal capacity expressed in litres. (standards.iteh.ai)

4.3 Leakage

ISO 5362:2000

Bags of nominal capacity 1 I or less shall not leak at a rate of more than 10 ml \cdot min at an internal overpressure of (3 ± 0.3) kPa.

Bags of nominal capacity greater than 1 I shall not leak at a rate of more than 25 ml \cdot min⁻¹ at an internal overpressure of (3 ± 0.3) kPa.

NOTE 1 For the purpose of this International Standard, the flowrate of air required to maintain the specified internal gas pressure is assumed to equal the leakage rate.

NOTE 2 A suitable test method is given in annex A. This draws attention to the possible sites of leakage.

4.4 Capacity

The actual capacity of the bag when tested in accordance with annex B shall be the marked value, subject to a tolerance of ± 15 %.

4.5 Design

4.5.1 Neck


- **4.5.1.1** Necks shall be either plain or assembled.
- **4.5.1.2** Plain necks shall fit directly on to 22 mm male conical connectors complying with ISO 5356-1, or on to adaptors that fit 15 mm or 22 mm male conical connectors complying with ISO 5356-1.

NOTE Plain necks may be reinforced internally or externally or made of a material thicker than that of the bag.

4.5.1.3 Plain necks of bags intended to fit directly on to 22 mm male conical connectors shall have an axial length of not less than 26 mm from the open end, when measured in the unstretched condition. Plain necks shall not become detached from a 22 mm male conical connector when tested in accordance with annex C.

NOTE Plain necks may be constructed to engage with the recess at the base of a 22 mm male conical connector.

4.5.1.4 Assembled necks shall incorporate an adaptor (see Figure 1) bearing a female conical connector in accordance with ISO 5356-1. The adaptor of the assembled neck shall not become detached from the bag when tested in accordance with annex D.

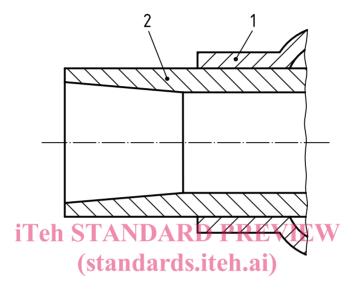

Key

Neck of reservoir bag

- ISO 5362:2000
- 2 Adaptor, which may be flanged, grooved on recessed and sist/3af3e907-60a6-49e4-b8d9-

Figure 1 — Typical adaptor with (female) conical connector

4.5.2 Tail

The tail, if open and not provided with a closure mechanism, shall have a minimum length of 20 mm.

NOTE A loop for suspending the bag may be provided near the tail of the bag.

4.6 Resistance to pressure required to distend the bag (pressure/volume)

- **4.6.1** When tested in accordance with annex E (see E.3.6), the final pressure head shall be not less than 3,0 kPa and not more than 6,0 kPa.
- **4.6.2** A bag tested in accordance with annex E shall revert within 30 min of the test to its previously measured capacity (i.e. capacity V_1 , see E.3.2) within a tolerance of \pm 10 %.

NOTE Another method for testing resistance to pressure to distend the bag, involving filling the bag with air rather than water, has been included for information as annex F.

5 Prevention of electrostatic charges

- **5.1** Antistatic bags shall comply with the requirements specified in IEC 60601-1:1988, 39.3b.
- **5.2** Bags coloured black shall be antistatic and comply with 5.1.

6 Requirements for bags supplied sterile

6.1 Sterility assurance

Bags supplied and marked as "STERILE" shall satisfy the requirements of EN 556:1994, 4.1.

6.2 Packaging for bags supplied sterile

Each bag supplied and marked as "STERILE" shall be contained in an individual pack. The pack shall serve as an effective barrier to the penetration of microorganisms and particulate material in accordance with ISO 11607. The pack shall permit the extraction of the contents and shall not be capable of reclosure without clearly revealing that it has been opened.

NOTE The individual pack may also contain other breathing system components.

7 Marking

7.1 Use of symbols

The requirements of 7.2 and 7.3 may be met by the use of appropriate symbols as given in ISO 7000 or EN 980.

7.2 Reusable bags iTeh STANDARD PREVIEW

Bags intended for reuse shall be marked with the following information: ai)

- a) the name or trade mark of the manufacturer and/or supplier:
- b) the nominal capacity (seet4:2);tandards.iteh.ai/catalog/standards/sist/3af3e907-60a6-49e4-b8d9-
- c) for bags and integrally attached non-metallic components for use with flammable anaesthetic agents, the word "ANTISTATIC".

It is recommended that reservoir bags be additionally marked with the "use-by" date.

The marking should be legible, durable and resistant to the methods of cleaning and disinfection or sterilization recommended by the manufacturer.

NOTE Reusable bags may be black or coloured and/or bear an indelible yellow-coloured marking.

7.3 Single-use bags

The packaging or an insert shall be marked in accordance with 7.2 and with the words "single use" or equivalent.

An indication shall be given if any natural rubber (latex) is present in the device.

NOTE Single-use bags may be black or coloured and/or bear an indelible yellow-coloured marking.

8 Information to be supplied by the manufacturer

Unless the bag is intended and labelled as being for single use, the manufacturer shall recommend methods of cleaning and disinfection or sterilization, and the maximum number or period of reuses. For reusable devices, the manufacturer shall indicate if any natural rubber (latex) is present in the device.

Marking, labelling and information to be supplied by the manufacturer should comply with EN 1041.

Annex A

(informative)

Test for leakage

A.1 Principle

Leakage rate is measured by applying and maintaining an internal gas pressure by introducing air into the anaesthetic reservoir bag, and recording the flowrate of air required to maintain that internal pressure. This will test for leakage from the body of the bag. In the case of bags with assembled necks, it will test for leakage from the bag, the adaptor and their connection; in the case of bags with plain necks, it will test for leakage from the connection of the bag to an appropriately-sized male conical connector.

A.2 Apparatus

- **A.2.1** Appropriately-sized male conical connector, complying with ISO 5356-1.
- **A.2.2** Means of applying and maintaining an internal overpressure of (3 ± 0.3) kPa.
- A.2.3 Suitable safety cage, for surrounding the inflated bag.
- **A.2.4** Means of recording the flowrate of air required to maintain the specified internal gas pressure in the bag being tested, accurate to within 5 % of the flowrates indicated in 4.3.

(standards.iteh.ai)

A.3 Procedure

- **A.3.1** Carry out the test procedure at an ambient femperature of $(23 \pm 2)^{\circ}$ C.
- **A.3.2** Fit the neck of the bag over the appropriately-sized male conical connector, closing off the tail if this is openended.
- **A.3.3** Establish an internal overpressure of (3 ± 0.3) kPa by introducing air into the bag and allowing the pressure to stabilize. Record the flowrate of air required to maintain that internal gas pressure.

A.4 Expression of results

The flowrate of air required to maintain the specified internal gas pressure (= leakage rate) shall be expressed in millilitres per minute.