



Designation: D3999 – 91 (Reapproved 2003)

Standard Test Methods for the Determination of the Modulus and Damping Properties of Soils Using the Cyclic Triaxial Apparatus¹

This standard is issued under the fixed designation D3999; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 These test methods cover the determination of the modulus and damping properties of soils in either undisturbed or reconstituted states by either load or stroke controlled cyclic triaxial techniques.

1.2 The cyclic triaxial properties of soil are evaluated relative to a number of factors including: strain level, density, number of cycles, material type, saturation, and effective stress.

1.3 These test methods are applicable to both fine-grained and coarse-grained soils as defined by the unified soil classification system or by Classification D2487. Test specimens may be undisturbed or reconstituted by compaction in the laboratory.

1.4 Two test methods are provided for using a cyclic loader to determine Young's modulus (E) and damping (D) properties. The first test method (A) permits the determination of E and D using a constant load apparatus. The second test method (B) permits the determination of E and D using a constant stroke apparatus. The test methods are as follows:

1.4.1 *Test Method A*—This test method requires the application of a constant cyclic load to the test specimen. It is used for determining the Young's modulus and damping under a constant load condition.

1.4.2 *Test Method B*—This test method requires the application of a constant cyclic deformation to the test specimen. It is used for determining the Young's modulus and damping under a constant stroke condition.

1.5 The development of relationships to aid in interpreting and evaluating test results are left to the engineer or office requesting the test.

1.6 *Limitations*—There are certain limitations inherent in using cyclic triaxial tests to simulate the stress and strain conditions of a soil element in the field during an earthquake.

1.6.1 Nonuniform stress conditions within the test specimen are imposed by the specimen end platens.

1.6.2 A90° change in the direction of the major principal stress occurs during the two halves of the loading cycle on isotropically confined specimens and at certain levels of cyclic stress application on anisotropically confined specimens.

1.6.3 The maximum cyclic axial stress that can be applied to a saturated specimen is controlled by the stress conditions at the end of confining stress application and the pore-water pressures generated during testing. For an isotropically confined specimen tested in cyclic compression, the maximum cyclic axial stress that can be applied to the specimen is equal to the effective confining pressure. Since cohesionless soils are not capable of taking tension, cyclic axial stresses greater than this value tend to lift the top platen from the soil specimen. Also, as the pore-water pressure increases during tests performed on isotropically confined specimens, the effective confining pressure is reduced, contributing to the tendency of the specimen to neck during the extension portion of the load cycle, invalidating test results beyond that point.

1.6.4 While it is advised that the best possible undisturbed specimens be obtained for cyclic testing, it is sometimes necessary to reconstitute soil specimens. It has been shown that different methods of reconstituting specimens to the same density may result in significantly different cyclic behavior. Also, undisturbed specimens will almost always be stronger than reconstituted specimens of the same density.

1.6.5 The interaction between the specimen, membrane, and confining fluid has an influence on cyclic behavior. Membrane compliance effects cannot be readily accounted for in the test procedure or in interpretation of test results. Changes in pore-water pressure can cause changes in membrane penetration in specimens of cohesionless soils. These changes can significantly influence the test results.

1.6.6 Despite these limitations, with due consideration for the factors affecting test results, carefully conducted cyclic triaxial tests can provide data on the cyclic behavior of soils

¹ These test methods are under the jurisdiction of ASTM Committee D18 on Soil and Rock and are the direct responsibility of Subcommittee D18.09 on Dynamic Properties of Soils.

Current edition approved August 15, 1991. Published October 1991. DOI: 10.1520/D3999-91R03.

with a degree of accuracy adequate for meaningful evaluations of modulus and damping below a shearing strain level of 0.5 %.

1.7 The values stated in either SI or inch-pound units shall be regarded separately as standard. The values in each system may not be exact equivalents, therefore, each system must be used independently of the other, without combining values in any way.

1.8 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 *ASTM Standards:*²

- D422 Test Method for Particle-Size Analysis of Soils
- D653 Terminology Relating to Soil, Rock, and Contained Fluids
- D854 Test Methods for Specific Gravity of Soil Solids by Water Pycnometer
- D1587 Practice for Thin-Walled Tube Sampling of Soils for Geotechnical Purposes
- D2216 Test Methods for Laboratory Determination of Water (Moisture) Content of Soil and Rock by Mass
- D2435 Test Methods for One-Dimensional Consolidation Properties of Soils Using Incremental Loading
- D2487 Practice for Classification of Soils for Engineering Purposes (Unified Soil Classification System)
- D2488 Practice for Description and Identification of Soils (Visual-Manual Procedure)
- D3740 Practice for Minimum Requirements for Agencies Engaged in Testing and/or Inspection of Soil and Rock as Used in Engineering Design and Construction
- D4220 Practices for Preserving and Transporting Soil Samples
- D4318 Test Methods for Liquid Limit, Plastic Limit, and Plasticity Index of Soils
- D4767 Test Method for Consolidated Undrained Triaxial Compression Test for Cohesive Soils

2.2 *USBR Standard:*

USBR 5210 Practice for Preparing Compacted Soil Specimens for Laboratory Use³

3. Terminology

3.1 *Definitions:*

3.1.1 The definitions of terms used in these test methods shall be in accordance with Terminology D653.

3.2 *Definitions of Terms Specific to This Standard:*

3.2.1 *back pressure*—a pressure applied to the specimen pore-water to cause air in the pore space to pass into solution in the pore-water, that is, to saturate the specimen.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard’s Document Summary page on the ASTM website.

³ Available from U.S. Department of the Interior, Bureau of Reclamation.

3.2.2 *cycle duration*—the time interval between successive applications of a deviator stress.

3.2.3 *deviator stress* [FL⁻²]*—*the difference between the major and minor principal stresses in a triaxial test.

3.2.4 *effective confining stress*—the confining pressure (the difference between the cell pressure and the pore-water pressure) prior to shearing the specimen.

3.2.5 *effective force, (F)*—the force transmitted through a soil or rock mass by intergranular pressures.

3.2.6 *hysteresis loop*—a trace of load versus deformation resulting from the application of one complete cycle of either a cyclic load or deformation. The area within the resulting loop is due to energy dissipated by the specimen and apparatus, see Fig. 1.

3.2.7 *load duration*—the time interval the specimen is subjected to a cyclic deviator stress.

3.2.8 *principal stress*—the stress normal to one of three mutually perpendicular planes on which the shear stresses at a point in a body are zero.

3.2.9 *Young’s modulus (modulus of elasticity)* [FL⁻²]*—*the ratio of stress to strain for a material under given loading conditions; numerically equal to the slope of the tangent or the secant of a stress-strain curve (same as Terminology D653).

4. Summary of Test Method

4.1 The cyclic triaxial test consists of imposing either a cyclic axial deviator stress of fixed magnitude (load control) or cyclic axial deformation (stroke control) on a cylindrical soil specimen enclosed in a triaxial pressure cell. The resulting axial strain and axial stress are measured and used to calculate either stress-dependent or stroke-dependent modulus and damping.

5. Significance and Use

5.1 The cyclic triaxial modulus and damping test provides parameters that may be considered for use in dynamic, linear and non-linear analytical methods. These test methods are used for the performance evaluation of both natural and engineered structures under dynamic of cyclic loads such as caused by earthquakes, ocean wave, or blast.

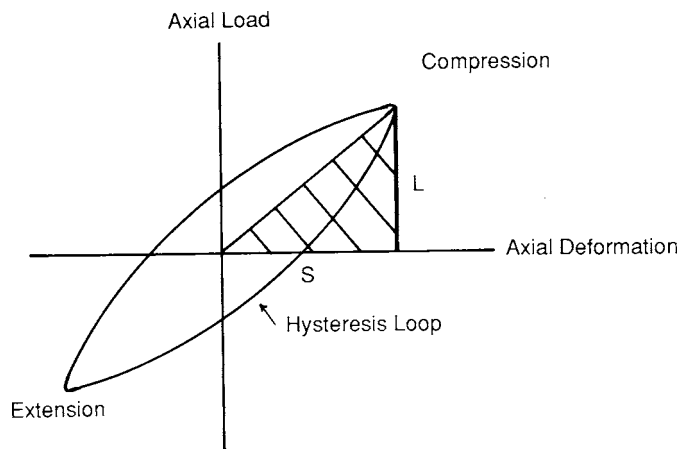


FIG. 1 Schematic of Typical Hysteresis Loop Generated by Cyclic Triaxial Apparatus

5.2 One of the primary purposes of these test methods is to obtain data that are used to calculate Young's modulus.

NOTE 1—The quality of the result produced by this standard is dependent on the competence of the personnel performing it, and the suitability of the equipment and facilities used. Agencies that meet the criteria of Practice D3740 are generally considered capable of competent and objective testing/sampling/inspection/etc. Users of this standard are cautioned that compliance with Practice D3740 does not in itself assure reliable results. Reliable results depend on many factors; Practice D3740 provides a means of evaluating some of those factors.

6. Apparatus

6.1 General—In many ways, triaxial equipment suitable for cyclic triaxial modulus and damping tests is similar to equipment used for the consolidated-undrained triaxial compression test (see Test Method D4767). However, there are special features described in the following sections that are required to perform acceptable cyclic triaxial tests. A schematic representation of the various components comprising a typical triaxial modulus and damping test setup is shown in Fig. 2.

6.2 Triaxial Pressure Cell—The primary considerations in selecting the cell are tolerances for the piston, top platen, and low friction piston seal, Fig. 3.

6.2.1 Two linear ball bushings or similar bearings should be used to guide the load rod to minimize friction and to maintain alignment.

6.2.2 The load rod diameter should be large enough to minimize lateral bending. A minimum load rod diameter of 1/8 the specimen diameter has been used successfully in many laboratories.

6.2.3 The load rod seal is a critical element in triaxial cell design for cyclic soils testing if an external load cell connected to the loading rod is employed. The seal must exert negligible friction on the load rod. The maximum acceptable piston friction tolerable without applying load corrections is com-

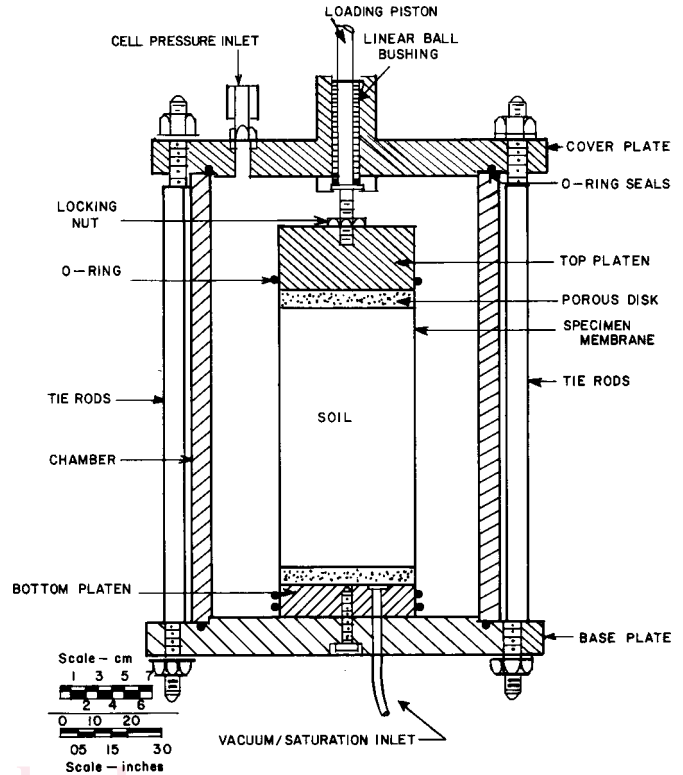


FIG. 3 Typical Cyclic Triaxial Pressure Cell

monly considered to be ±2 % of the maximum single amplitude cyclic load applied in the test, refer to Fig. 4. The use of


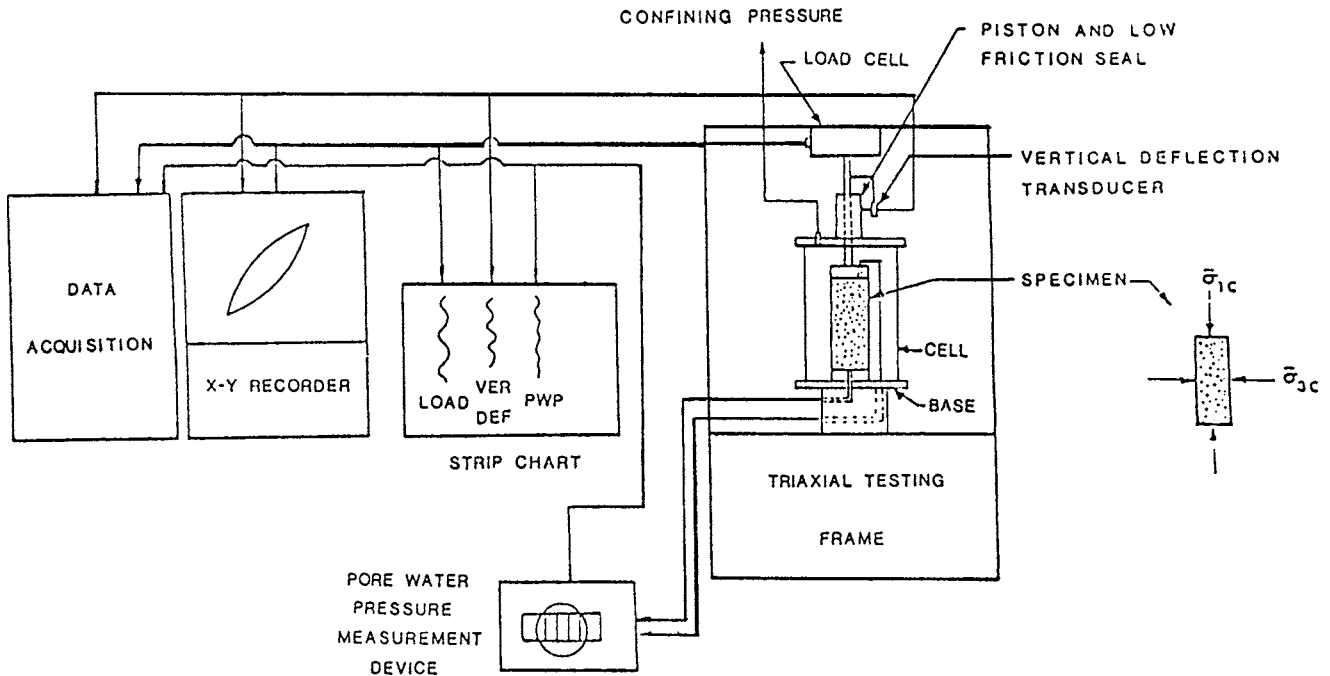


FIG. 2 Schematic Representation of Load or Stroke-Controlled Cyclic Triaxial Test Setup

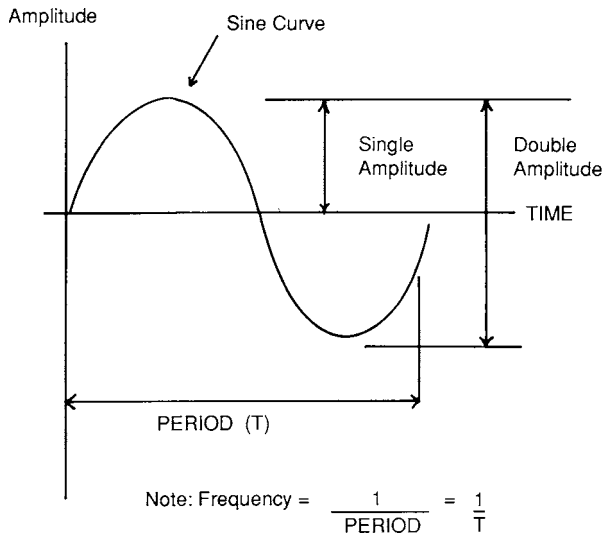

NOTE 1—Frequency = $\frac{1}{\text{PERIOD}} = \frac{1}{T}$.
FIG. 4 Definitions Related to Cyclic Loading

a seal described in 9.1 and described by Ladd and Dutko⁴, and Chan⁵ will meet these requirements.

6.2.4 Top and bottom platen alignment is critical to avoid increasing a nonuniform state of stress in the specimen. Internal tie-rod triaxial cells have worked well at a number of laboratories. These cells allow the placement of the cell wall after the specimen is in place between the loading platens. Acceptable limits on platen eccentricity and parallelism are shown in Fig. 5.

6.2.5 Since axial loading in cyclic triaxial tests is in extension as well as in compression, the load rod shall be rigidly connected to the top platen by a method such as one of those shown in Fig. 6.

6.2.6 There shall be provision for specimen drainage at both the top and bottom platens.

6.3 Cyclic Loading Equipment:

6.3.1 Cyclic loading equipment used for load controlled cyclic triaxial tests must be capable of applying a uniform sinusoidal load at a frequency within the range of 0.1 to 2 Hz. The loading device must be able to maintain uniform cyclic loadings to at least 0.5 % double amplitude stress, refer to Fig. 4. Unsymmetrical compression-extension load peaks, nonuniformity of pulse duration, “ringing”, or load fall-off at large strains must not exceed tolerances illustrated in Fig. 7. The equipment must also be able to apply the cyclic load about an initial static load on the loading rod.

6.3.2 Cyclic loading equipment used for deformation-controlled cyclic triaxial tests must be capable of applying a uniform sinusoidal deformation at a frequency range of 0.1 to 2 Hz. The equipment must also be able to apply the cyclic deformation about either an initial datum point or follow the

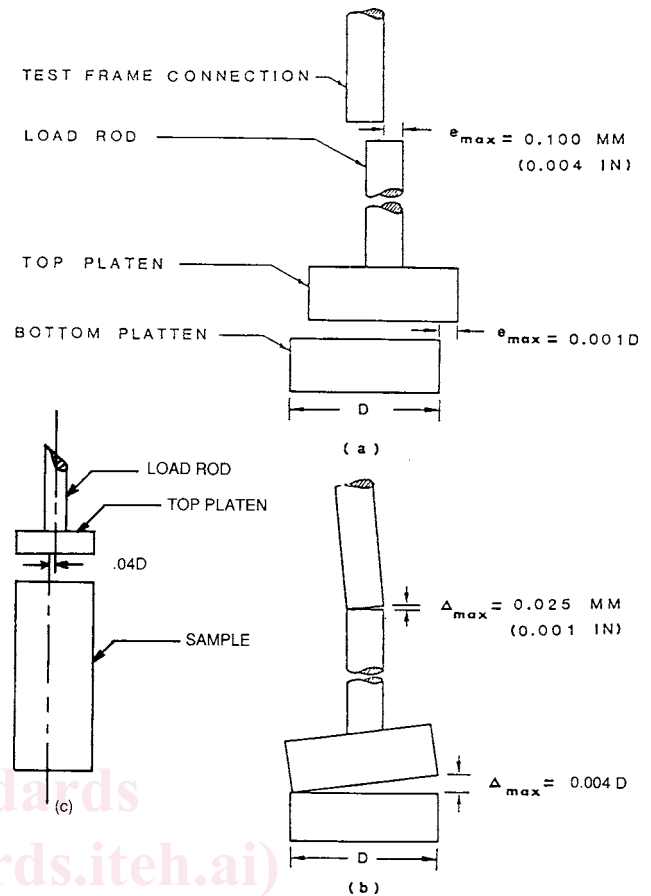


FIG. 5 Limits on Acceptable Platen and Load Rod Alignment: (a) eccentricity, (b) parallelism, (c) eccentricity between Top Platen and Sample

⁴ Ladd, R. S., and Dutko, P., “Small Strain Measurements Using Triaxial Apparatus,” *Advances In The Art of Testing Soils Under Cyclic Conditions*, V. Khosla, ed., American Society of Civil Engineers, 1985.

⁵ Chan, C. K., “Low Friction Seal System” *Journal of the Geotechnical Engineering Division*, American Society of Civil Engineers, Vol. 101, GT-9, 1975, pp. 991-995.

specimen as it deforms. The type of apparatus typically employed can range from a simple cam to a closed loop electro-hydraulic system.

6.4 Recording Equipment:

6.4.1 Load, displacement, and pore water pressure transducers are required to monitor specimen behavior during cyclic loading; provisions for monitoring the chamber pressure during cyclic loading are optional.

6.4.2 *Load Measurement*—Generally, the load cell capacity should be no greater than five times the total maximum load applied to the test specimen to ensure that the necessary measurement accuracy is achieved. The minimum performance characteristics of the load cell are presented in Table 1.

6.4.3 *Axial Deformation Measurement*—Displacement measuring devices such as linear variable differential transformer (LVDT), Potentiometer-type deformation transducers, and eddy current sensors may be used if they meet the required performance criteria (see Table 1). Accurate deformation measurements require that the transducer be properly mounted to avoid excessive mechanical system compression between the load frame, the triaxial cell, the load cell, and the loading piston.

6.4.4 *Pressure- and Vacuum-Control Devices*—The chamber pressure and back pressure control devices shall be capable of applying and controlling pressures to within ± 2 psi (14 kPa)

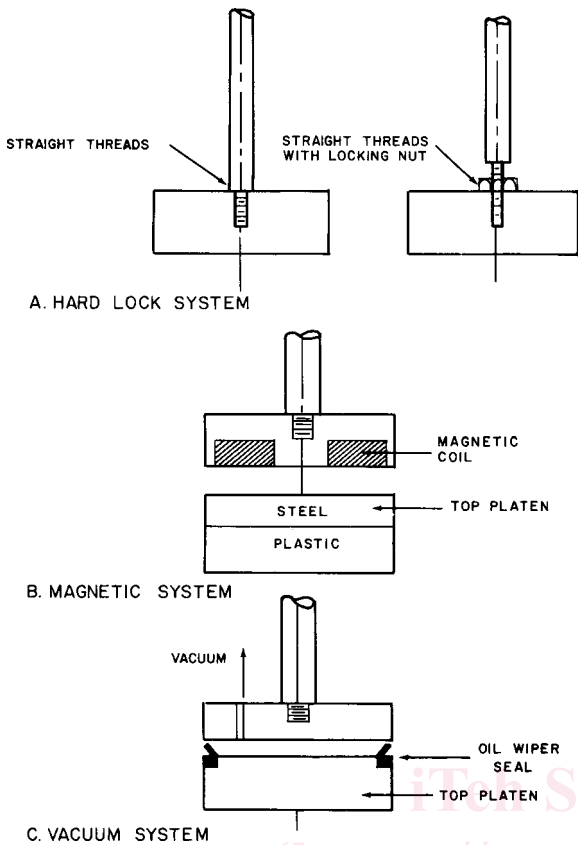


FIG. 6 Top Platen Connections

for effective consolidation pressures. The vacuum control device shall be capable of applying and controlling partial vacuums to within ± 2 psi (14 kPa). The devices may consist of self-compensating mercury pots, pneumatic pressure regulators, combination pneumatic pressure and vacuum regulators, or any other device capable of applying and controlling pressures or partial vacuums to the required tolerances.

6.4.5 Pressure- and Vacuum-Measurement Devices—The chamber pressure, back pressure, and vacuum measuring devices shall be capable of measuring pressures or partial vacuums to the tolerances given in Table 1. They may consist of Bourdon gages, pressure manometers, electronic pressure transducers, or any other device capable of measuring pressures, or partial vacuums to the stated tolerances. If separate devices are used to measure the chamber pressure and back pressure, the devices must be calibrated simultaneously and against the same pressure source. Since the chamber pressure and back pressure are the pressures taken at the midheight of the specimen, it may be necessary to adjust the calibration of the devices to reflect the hydraulic head of fluid in the chamber and back pressure control systems (see Fig. 2).

6.4.6 Pore-Water Pressure Measurement Device—The specimen pore-water pressure shall also be measured to the tolerances given in Table 1. During cyclic loading on a saturated specimen the pore-water pressure shall be measured in such a manner that as little water as possible is allowed to go into or out of the specimen. To achieve this requirement a very stiff electronic pressure transducer must be used. With an electronic pressure transducer the pore-water pressure is read

directly. The measuring device shall have a rigidity of all the assembled parts of the pore-water pressure measurement system relative to the total volume of the specimen satisfying the following requirement:

$$\frac{(\Delta v/v)}{\Delta u} < 3.2 \times 10^{-6} \text{ m}^2/\text{kN} (2.2 \times 10^{-5} \text{ in.}^2/\text{lb}) \quad (1)$$

where:

- ΔV = change in volume of the pore-water measurement system due to a pore pressure change, in.³ (mm³),
- V = the total volume of the specimen, in.³ (mm³), and
- δu = the change in pore pressure, psi (kPa).

NOTE 2—To meet the rigidity requirement, tubing between the specimen and the measuring device should be short and thick walled with small bores. Thermoplastic, copper, and stainless steel tubing have been used successfully in many laboratories.

6.4.7 Volume Change Measurement Device—The volume of water entering or leaving the specimen shall be measured with an accuracy of within ± 0.05 % of the total volume of the specimen. The volume measuring device is usually a burette but may be any other device meeting the accuracy requirement. The device must be able to withstand the maximum chamber pressure.

6.5 Specimen Cap and Base—The specimen cap and base shall be designed to provide drainage from both ends of the specimen. They shall be constructed of a rigid, noncorrosive, impermeable material, and each shall, except for the drainage provision, have a circular plane surface of contact with the porous discs and a circular cross section. The weight of the specimen cap and top porous disc shall be less than 0.5 % of the applied axial load at failure as determined from an undrained static triaxial test. The diameter of the cap and base shall be equal to the initial diameter of the specimen. The specimen base shall be connected to the triaxial compression chamber to prevent lateral motion or tilting, and the specimen cap shall be designed such that eccentricity of the piston-to-cap contact relative to the vertical axis of the specimen does not exceed $0.04 D$ (D = diameter of specimen) as shown in Fig. 5(c). The cylindrical surface of the specimen base and cap that contacts the membrane to form a seal shall be smooth and free of scratches.

6.6 Porous Discs—The specimen shall be separated from the specimen cap and base by rigid porous discs fastened to the specimen cap and base of a diameter equal to that of the specimen. The coefficient of permeability of the discs shall be approximately equal to that of fine sand 1×10^{-3} mm/s (3.9×10^{-5} in./s). The discs shall be regularly checked by passing air or water under pressure through them to determine whether they have become clogged. Care must be taken to ensure that the porous elements of the end platens are open sufficiently so as not to impede drainage or pore water movement from specimen into the volume change or pore pressure measuring devices, and with openings sufficiently fine to prevent movement of fines out of the specimen.

NOTE 3—Filter-paper discs of a diameter equal to that of the specimen may not be placed between the porous discs and specimen to avoid clogging of the porous discs when measuring moduli values on stiff specimens.

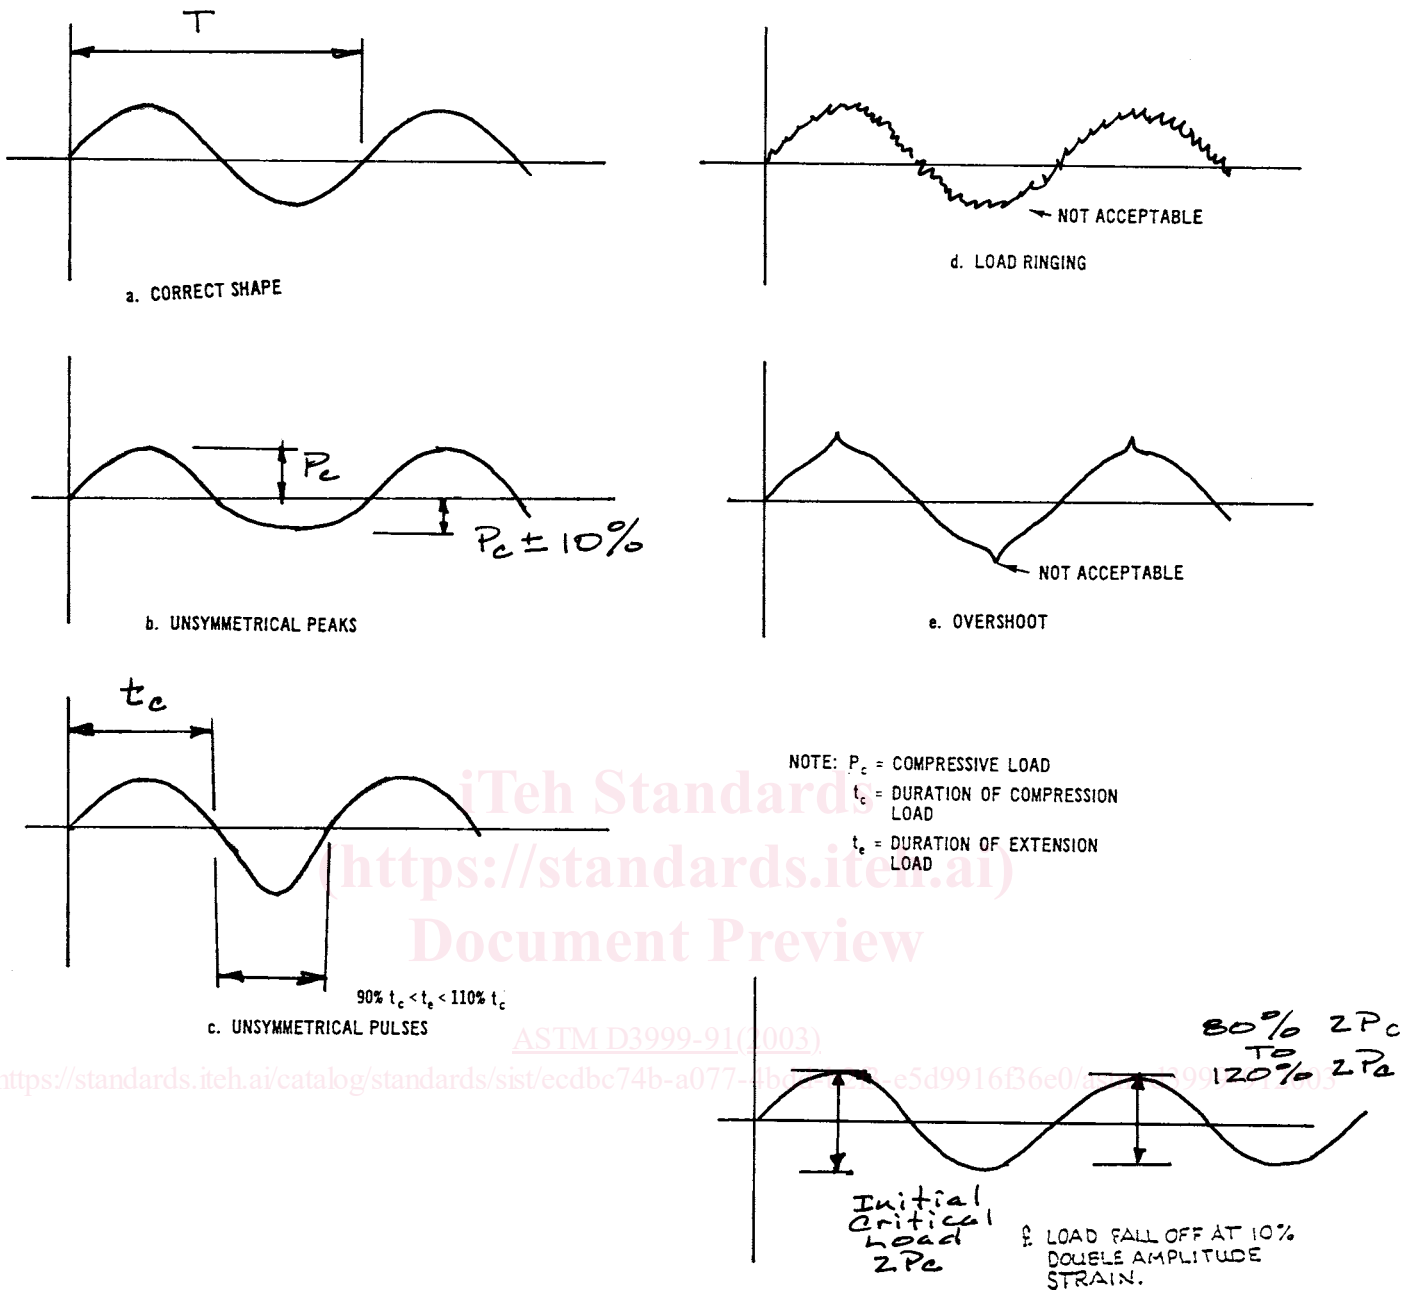


FIG. 7 Examples of Acceptable and Unacceptable Sinusoidal Loading Wave Forms For Cyclic Triaxial Load Control Tests

6.7 *Filter-Paper Strips*—Filter-paper strips are used by many laboratories to decrease the time required for testing. If filter strips are used, they shall be of a type that does not dissolve in water. The coefficient or permeability of the filter paper shall not be less than 1×10^{-4} mm/s (3.9×10^{-6} in./s) for a normal pressure of 550 kPa (80 psi). To avoid hoop tension, filter strips should cover no more than 50 % of the specimen periphery.

NOTE 4—The filter paper given in Footnote 6 has been found to meet the permeability and durability requirements.⁶

⁶ Whatman's No. 54 filter paper has been found suitable for this purpose.

6.8 *Rubber Membrane*—The rubber membrane used to encase the specimen shall provide reliable protection against leakage. To check a membrane for leakage, the membrane shall be placed around a cylindrical form, sealed at both ends with rubber O-rings, subjected to a small air pressure on the inside, and immersed in water. If air bubbles appear from any point on the membrane it shall be rejected. To offer minimum restraint to the specimen, the unstretched membrane diameter shall be between 90 and 95 % of that of the specimen. The membrane thickness shall not exceed 1 % of the diameter of the specimen. The membrane shall be sealed to the specimen cap and base with rubber O-rings for which the unstressed inside diameter is