



SLOVENSKI STANDARD
SIST ISO 13318-2:2002
01-junij-2002

8 c`c Yj Ub`Y[fUbi `UM`Y`n`a YrcXUa]`W`b`f]Z [UbY`gYX]a YbHUM`Y`j `hY_c]b]!`&`XY.
: c`c`W`b`f]Z [UbUa YrcXU

Determination of particle size distribution by centrifugal liquid sedimentation methods --
Part 2: Photocentrifuge method

iTeh STANDARD PREVIEW

Détermination de la distribution granulométrique par les méthodes de sédimentation
centrifuge dans un liquide -- Partie 2: Méthode photocentrifuge

[SIST ISO 13318-2:2002](https://standards.iteh.ai/catalog/standards/sist/f9bbe57-bb37-4163-b8ca-64702d57a9f6/sist-iso-13318-2-2002)

Ta slovenski standard je istoveten z: **ISO 13318-2:2001**

ICS:

19.120	Analiza velikosti delcev. Sejanje	Particle size analysis. Sieving
--------	--------------------------------------	---------------------------------

SIST ISO 13318-2:2002

en

iTeh STANDARD PREVIEW
(standards.iteh.ai)

SIST ISO 13318-2:2002

<https://standards.iteh.ai/catalog/standards/sist/f9bbe57-bb37-4163-b8ca-b4762d37a9f6/sist-iso-13318-2-2002>

INTERNATIONAL STANDARD

ISO 13318-2

First edition
2001-12-01

Determination of particle size distribution by centrifugal liquid sedimentation methods —

Part 2: Photocentrifuge method

iTeh **STANDARD PREVIEW**

*Détermination de la distribution granulométrique par les méthodes de
sédimentation centrifuge dans un liquide —*

Partie 2: Méthode photocentrifuge

[SIST ISO 13318-2:2002](https://standards.iso.org/iso/13318-2:2002)

<https://standards.itih.ai/catalog/standards/sist/f9bbe57-bb37-4163-b8ca-b4762d37a9f6/sist-iso-13318-2-2002>



Reference number
ISO 13318-2:2001(E)

© ISO 2001

ISO 13318-2:2001(E)**PDF disclaimer**

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

iTeh STANDARD PREVIEW (standards.iteh.ai)

[SIST ISO 13318-2:2002](https://standards.iteh.ai/catalog/standards/sist/f9bbe57-bb37-4163-b8ca-b4762d37a9f6/sist-iso-13318-2-2002)

<https://standards.iteh.ai/catalog/standards/sist/f9bbe57-bb37-4163-b8ca-b4762d37a9f6/sist-iso-13318-2-2002>

© ISO 2001

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.ch
Web www.iso.ch

Printed in Switzerland

Contents

Page

Foreword.....	iv
Introduction.....	v
1 Scope	1
2 Normative references	1
3 Terms, definitions and symbols.....	2
3.1 Terms and definitions	2
3.2 Symbols	2
4 Principle.....	2
5 Apparatus	3
6 Sampling.....	5
7 Preparation.....	5
7.1 Sample preparation	5
7.2 Temperature	5
7.3 Dispersion	5
8 Procedure	5
8.1 Line-start methods	5
8.2 Homogeneous technique.....	6
9 Tests in duplicate and validation	7
9.1 Tests in duplicate.....	7
9.2 Validation.....	7
10 Calculation of results	7
10.1 General.....	7
10.2 Calculation of particle size	7
10.3 Calculation of cumulative mass percentage	7
11 Reporting of results.....	8
Annex A (informative) Worked example	10
Annex B (informative) Extinction curve, example for titanium dioxide.....	14
Annex C (informative) Effect of radial dilution.....	15

iTech STANDARD PREVIEW

(standards.itech.ai)

<https://standards.itech.ai/catalog/standards/sist/dbbcf57-bb37-4163-b8ca-b4762d37a9f6/sist-iso-13318-2-2002>

ISO 13318-2:2001(E)

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 3.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this part of ISO 13318 may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 13318-2 was prepared by Technical Committee ISO/TC 24, *Sieves, sieving and other sizing methods*, Subcommittee SC 4, *Sizing by methods other than sieving*.

ISO 13318 consists of the following parts, under the general title *Determination of particle size distribution by centrifugal liquid sedimentation methods*: **(standards.iteh.ai)**

- *Part 1: General principles and guidelines* [SIST ISO 13318-2:2002](https://standards.iteh.ai/catalog/standards/sist/19bbe57-bb37-4163-b8ca-b4762d37a9f6/sist-iso-13318-2-2002)
- *Part 2: Photocentrifuge method* <https://standards.iteh.ai/catalog/standards/sist/19bbe57-bb37-4163-b8ca-b4762d37a9f6/sist-iso-13318-2-2002>
- *Part 3: Centrifugal X-ray method*

Annexes A to C of this part of ISO 13318 are for information only.

Introduction

The sample suspension in a photo-centrifuge may be contained in a cuvet or a disc. Sample concentration is determined by changes in a light signal monitored at a known radius. The cuvet photo-centrifuge can only be run in the homogeneous mode whereas the disc photo-centrifuge may be run in either the homogeneous or the line-start mode. Some systems permit the coarse end of the distribution to be measured in a gravitational mode and the fine end in the centrifugal mode. The use of light to determine particle size distribution requires a calibration factor to be applied as the particle size approaches the wavelength of the light, due to the inapplicability of the laws of geometric optics.

iTeh STANDARD PREVIEW (standards.iteh.ai)

[SIST ISO 13318-2:2002](https://standards.iteh.ai/catalog/standards/sist/f9bbe57-bb37-4163-b8ca-b4762d37a9f6/sist-iso-13318-2-2002)

<https://standards.iteh.ai/catalog/standards/sist/f9bbe57-bb37-4163-b8ca-b4762d37a9f6/sist-iso-13318-2-2002>

iTeh STANDARD PREVIEW
(standards.iteh.ai)

SIST ISO 13318-2:2002

<https://standards.iteh.ai/catalog/standards/sist/f9bbe57-bb37-4163-b8ca-b4762d37a9f6/sist-iso-13318-2-2002>

Determination of particle size distribution by centrifugal liquid sedimentation methods —

Part 2: Photocentrifuge method

WARNING — This part of ISO 13318 may involve hazardous materials, operations and equipment. This part of ISO 13318 does not purport to address all of the safety problems associated with its use. It is the responsibility of the user of this part of ISO 13318 to establish appropriate safety and health practices and determine the applicability of the regulatory limitations prior to its use.

1 Scope

This part of ISO 13318 covers methods for determining the particle size distribution of particulate materials by means of centrifugal sedimentation in a liquid. Solids concentrations are determined by the transmission of a light beam. The resulting signal enables conversion to a particle size distribution.

The method of determining the particle size distribution described in this part of ISO 13318 is applicable to powders that can be dispersed in liquids, powders that are present in slurry form and some emulsions. Typical particle size range for analysis is from about 0,1 μm to 5 μm . The method is applicable to powders in which all particles have the same density and comparable shapes and do not undergo chemical or physical change in the suspension liquid. It is usually necessary that the particles have a density higher than that of the liquid.

2 Normative references

The following normative documents contain provisions which, through reference in this text, constitute provisions of this part of ISO 13318. For dated references, subsequent amendments to, or revisions of, any of these publications do not apply. However, parties to agreements based on this part of ISO 13318 are encouraged to investigate the possibility of applying the most recent editions of the normative documents indicated below. For undated references, the latest edition of the normative document referred to applies. Members of ISO and IEC maintain registers of currently valid International Standards.

ISO 13318-1, *Determination of particle size distribution by centrifugal liquid sedimentation methods — Part 1: General principles and guidelines*

ISO 14887, *Sample preparation — Dispersing procedures for powders in liquids*

ISO 13318-2:2001(E)

3 Terms, definitions and symbols

3.1 Terms and definitions

For the purposes of this part of ISO 13318 the terms and definitions of ISO 13318-1 apply.

3.2 Symbols

For the purposes of this this part of ISO 13318 the symbols of ISO 13318-1 and the following apply:

- D optical density
- E_i extinction coefficient for a particle of diameter x_i
- G constant dependent upon the geometry of the system, the dimensions of the light beam and on the shape of the particles
- I transmission of the emergent light beam, at the time t , after the start of sedimentation
- I_0 transmission of the emergent light beam when no particles are present
- M distance from rotation axis to measurement zone (mm)
- n_i number of particles of diameter x_i in the beam
- R distance from rotation axis to centrifuge wall, inner disc radius (mm)
- S distance from rotation axis to liquid-air interface of sample (mm)
- x_0 diameter of the smallest particle in the light beam (μm)
- x_{St} diameter of the largest particle in the light beam i.e. the Stokes diameter (μm)

4 Principle

A stable, finely collimated beam of light passes through a spinning disc or cuvet and sedimenting sample and is detected at a known radius. Light rays, typically from either a white light source (e.g. incandescent bulb) or a monochromatic coherent source (e.g. laser), pass through the suspension and are detected by a photodiode or photomultiplier. The disc photocentrifuge can be operated in the line-start or homogeneous mode whereas the cuvet photocentrifuge can be operated only in the homogeneous mode. The signal of the light beam is monitored over the analysis time. The mass percentage of sample present in the beam is determined by calculating the ratio of the light transmission signal, by use of a clear dispersing liquid, to the light transmission signal with the sample present.

In the line-start mode the disc initially contains clear fill liquid to give maximum light transmission. Then the sample is injected as a thin layer on top of the spinning fill liquid and begins to settle outward radially. When the largest particles present reach the light beam the light transmission decreases, returning to the original transmission value when the smallest particle present passes through the beam. A buffer layer is usually injected over the fill liquid to prevent suspension breaking through the interface in a phenomenon known as "streaming".


5 Apparatus

5.1 Disc photocentrifuge, with a chamber consisting of a hollow disc with an entry port coaxial with the axis of rotation (see Figure 1). Typically this is mounted vertically, or at a small angle to the vertical, on to the shaft of an electric motor with a digitally variable speed typically between $500 \text{ r}\cdot\text{min}^{-1}$ and $15\,000 \text{ r}\cdot\text{min}^{-1}$. A white light source and detector assembly measures transmittance through the suspension as a function of time. The instrument can be used in either a line-start or homogeneous mode. Extinction coefficient corrections need to be applied for the breakdown in the laws of geometric optics for both line-start and homogeneous modes. Additionally a correction is required for radial dilution effects when the homogeneous mode is used. Software is provided with commercial equipment to convert the data directly into size distributions in the form of tables or graphs of cumulative mass percentage versus particle size.

5.2 Cuvet photocentrifuge, in which the disc is replaced with a rectangular cell containing a homogeneous suspension (see Figure 2). Corrections need to be made for both radial dilution and light scattering effects as described in ISO 13318-1. Cuvet photocentrifuges can typically be run in both the gravitational and centrifugal modes. Additionally, some systems may offer a gradient mode permitting the centrifuge to accelerate throughout the analysis in order to reduce the measurement time.

5.3 Ancillary apparatus, consisting of:

- dispersing vessel e.g. glass beaker or bottle, of appropriate dimensions;
- flexible spatula;
- ultrasonic bath or probe, a bottle shaker or high speed mechanical stirrer capable of rotating at $500 \text{ r}\cdot\text{min}^{-1}$ to $1\,000 \text{ r}\cdot\text{min}^{-1}$.

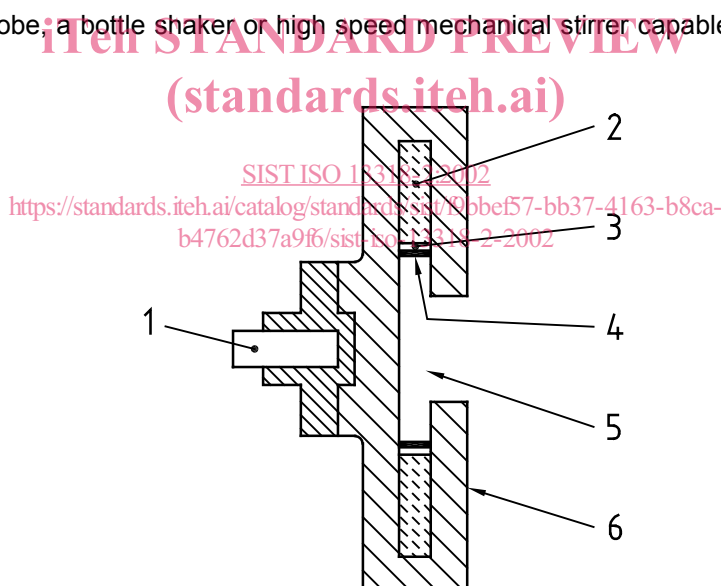

Key

- | | |
|---|-----------------------------|
| 1 | Motor shaft |
| 2 | Spin fluid |
| 3 | Buffer layer |
| 4 | Suspension |
| 5 | Entry port |
| 6 | Polymethylmethacrylate disc |

Figure 1 — Side view of the disc of a disc photocentrifuge