

First edition
2004-09-01

Corrected version
2005-03-01

**Water quality — Application of
inductively coupled plasma mass
spectrometry (ICP-MS) —**

**Part 1:
General guidelines**

*Qualité de l'eau — Application de la spectrométrie de masse avec
plasma à couplage inductif (ICP-MS) —*

Partie 1: Lignes directrices générales

Document Preview

ISO 17294-1:2004

<https://standards.iteh.ai/catalog/standards/iso/df981861-12f7-418c-8bb3-b937863e4680/iso-17294-1-2004>



Reference number
ISO 17294-1:2004(E)

© ISO 2004

PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

iTeh Standards
(<https://standards.iteh.ai>)
Document Preview

ISO 17294-1:2004

<https://standards.iteh.ai/catalog/standards/iso/df981861-12f7-418c-8bb3-b937863e4680/iso-17294-1-2004>

© ISO 2004

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

Page

Foreword	iv
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Principle	5
5 Apparatus	5
6 Interferences by concomitant elements	13
7 Adjustment of the apparatus	19
8 Preparatory steps	21
9 Procedure	26
Annex A (informative) Spectral interferences, choice of isotopes and method detection limits for quadrupole ICP-MS instruments	29
Bibliography	33

iTeh Standards
(<https://standards.itih.ai>)
Document Preview

[ISO 17294-1:2004](https://standards.itih.ai/catalog/standards/iso/df981861-12f7-418c-8bb3-b937863e4680/iso-17294-1-2004)

<https://standards.itih.ai/catalog/standards/iso/df981861-12f7-418c-8bb3-b937863e4680/iso-17294-1-2004>

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 17294-1 was prepared by Technical Committee ISO/TC 147, *Water quality*, Subcommittee SC 2, *Physical, chemical and biochemical methods*.

ISO 17294 consists of the following parts, under the general title *Water quality — Application of inductively coupled plasma mass spectrometry (ICP-MS)*:

- *Part 1: General guidelines*
- *Part 2: Determination of 62 elements*

This corrected version of ISO 17294-1:2004 incorporates correction of symbols for instrument detection limit and method detection limit, corrections to Equations (1) and (3), and various minor editorial corrections.

Water quality — Application of inductively coupled plasma mass spectrometry (ICP-MS) —

Part 1: General guidelines

1 Scope

This part of ISO 17294 specifies the principles of inductively coupled plasma mass spectrometry (ICP-MS) and provides general directions for the use of this technique for determining elements in water. Generally, the measurement is carried out in water, but gases, vapours or fine particulate matter may be introduced too. This International Standard applies to the use of ICP-MS for water analysis.

The ultimate determination of the elements is described in a separate International Standard for each series of elements and matrix. The individual parts of this International Standards refer the reader to these guidelines for the basic principles of the method and for configuration of the instrument.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the reference document (including any amendments) applies.

ISO Guide 30, *Terms and definitions used in connection with reference materials*

ISO Guide 32, *Calibration in analytical chemistry and use of certified reference materials*

ISO Guide 33, *Uses of certified reference materials*

ISO 3534-1, *Statistics — Vocabulary and symbols — Part 1: Probability and general statistical terms*

ISO 3696:1987, *Water for analytical laboratory use — Specification and test methods*

ISO 5725-1, *Accuracy (trueness and precision) of measurement methods and results — Part 1: General principles and definitions*

ISO 5725-2, *Accuracy (trueness and precision) of measurement methods and results — Part 2: Basic method for the determination of repeatability and reproducibility of a standard measurement method*

ISO 6206, *Chemical products for industrial use — Sampling — Vocabulary*

ISO 6955, *Analytical spectroscopic methods — Flame emission, atomic absorption and fluorescence — Vocabulary*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 5725-1, ISO 6206, ISO 6955 and ISO Guide 32 and the following apply.

3.1

accuracy

closeness of agreement between test result and the accepted reference value

NOTE The term accuracy, when applied to a set of observed values, describes a combination of random error components and common systematic error components. Accuracy includes precision and trueness.

3.2

analyte

element(s) to be determined

3.3

blank calibration solution

solution prepared in the same way as the calibration solution but leaving out the analyte

3.4

calibration solution

solution used to calibrate the instrument, prepared from (a) stock solution(s) or from a certified standard

3.5

check calibration solution

solution of known composition within the range of the calibration solutions, but prepared independently

3.6

determination

entire process from preparing the test sample solution up to and including measurement and calculation of the final result

3.7

laboratory sample

sample sent to the laboratory for analysis

3.8

linearity

straight line relationship between the (mean) result of measurement (signal) and the quantity (concentration) of the component to be determined

3.9

linearity verification solution

solution with a known concentration of the matrix components compared to the calibration solutions, but having an analyte concentration half that of the (highest) calibration solution

3.10

instrument detection limit

L_{DI}
smallest concentration that can be *detected* with a defined statistical probability using a contaminant-free instrument and a blank calibration solution

3.11

mean result

mean value of n results, calculated as intensity (ratio) or as mass concentration (ρ)

NOTE The mass concentration is expressed in units of milligrams per litre.

3.12

method detection limit

L_{DM}
smallest analyte concentration that can be *detected* with a specified analytical method with a defined statistical probability

3.13**net intensity** I

signal obtained after correction for (poly)atomic ion interferences using an elemental equation

3.14**net intensity ratio** I_R

net intensity divided by the signal of a reference element

3.15**optimization solution**

solution serving for mass calibration and for the optimization of the apparatus conditions

EXAMPLE Adjustment of maximal sensitivity with respect to minimal oxide formation rate and minimal formation of doubly charged ions.

3.16**precision**

closeness of agreement between independent test results obtained under prescribed conditions

NOTE Precision depends only on the distribution of random errors and does not relate to true value or the specified value.

3.17**“pure chemical”**

chemical with the highest available purity and known stoichiometry and for which the content of analyte and contaminants should be known with an established degree of certainty

3.18**raw intensity** I_{raw}

obtained uncorrected signal

3.19**reagent blank solution**

solution prepared by adding to the solvent the same amounts of reagents as those added to the test sample solution and with the same final volume

3.20**reproducibility** R

precision under reproducibility conditions

[ISO 3534-1]

3.21**reproducibility conditions**

conditions where test results are obtained with the same method on identical test items in different laboratories with different operators using different equipment

[ISO 3534-1]

3.22**reproducibility standard deviation**

standard deviation of test results obtained under reproducibility conditions

[ISO 3534-1]

3.23

reproducibility limit

value less than or equal to which the absolute difference between two single test results obtained under reproducibility conditions may be expected to be, with a probability of, generally, 95 %

3.24

repeatability

r

precision under repeatability conditions

[ISO 3534-1]

3.25

repeatability conditions

conditions where independent test results are obtained with the same method on identical test items in the same laboratory by the same operator using the same equipment within a short interval of time

[ISO 3534-1]

3.26

repeatability standard deviation

standard deviation of test results obtained under repeatability conditions

[ISO 3534-1]

3.27

repeatability limit

value less than or equal to which the absolute difference between two single test results obtained under repeatability conditions may be expected to be, with a probability of, generally, 95 %

3.28

result

outcome of a measurement

3.29

sensitivity

S

ratio of the variation of the magnitude of the signal (*dI*) to the corresponding variation in the concentration of the analyte (*dC*) expressed by the equation:

$$S = \frac{dI}{dC}$$

3.30

stock solution

solution with accurately known analyte concentration(s), prepared from "pure chemicals".

NOTE Stock solutions are reference materials within the meaning of ISO Guide 30.

3.31

test sample

sample prepared from the laboratory sample, for example by grinding or homogenizing

3.32

test sample solution

solution prepared with the fraction (test portion) of the test sample according to the appropriate specifications, such that it can be used for the envisaged measurement

3.33**trueness
bias**

closeness of agreement between the average value obtained from a large series of test results and an accepted reference value

NOTE The measure of trueness is usually expressed in terms of bias, which equals the sum of the systematic error components.

3.34**uncertainty of measurement**

parameter, associated with the result of a measurement, that characterises the dispersion of the values that could reasonably be attributed to the analyte concentration

4 Principle

ICP-MS stands for Inductively Coupled Plasma Mass Spectrometry. In the present context, a plasma is a small cloud of hot (6 000 K to 10 000 K) and partly ionized (approximately 1 %) argon gas. Cool plasmas have temperatures of only about 2 500 K. The plasma is sustained by a radio-frequency field. The sample is brought into the plasma as an aerosol. Liquid samples are converted into an aerosol using a nebulizer. In the plasma, the solvent of the sample evaporates, and the compounds present decompose into the constituent atoms (dissociation, atomization). The analyte atoms are in most cases almost completely ionized.

In the mass spectrometer, the ions are separated and the elements identified according to their mass-to-charge ratio, m/z , while the concentration of the element is proportional to the number of ions.

ICP-MS is a relative technique. The proportionality factor between response and analyte concentration relates to the fact that only a fraction of the analyte atoms that are aspirated reach the detector as an ion. The proportionality factor is determined by measuring calibration solutions (calibration).

5 Apparatus

ISO 17294-1:2004

<https://standards.iteh.ai/catalog/standards/iso/d1981861-12f7-418c-8bb3-b937863e4680/iso-17294-1-2004>

5.1 General

The principal components of the ICP-mass spectrometer are as shown in Figure 1 in the form of a schematic block diagram.

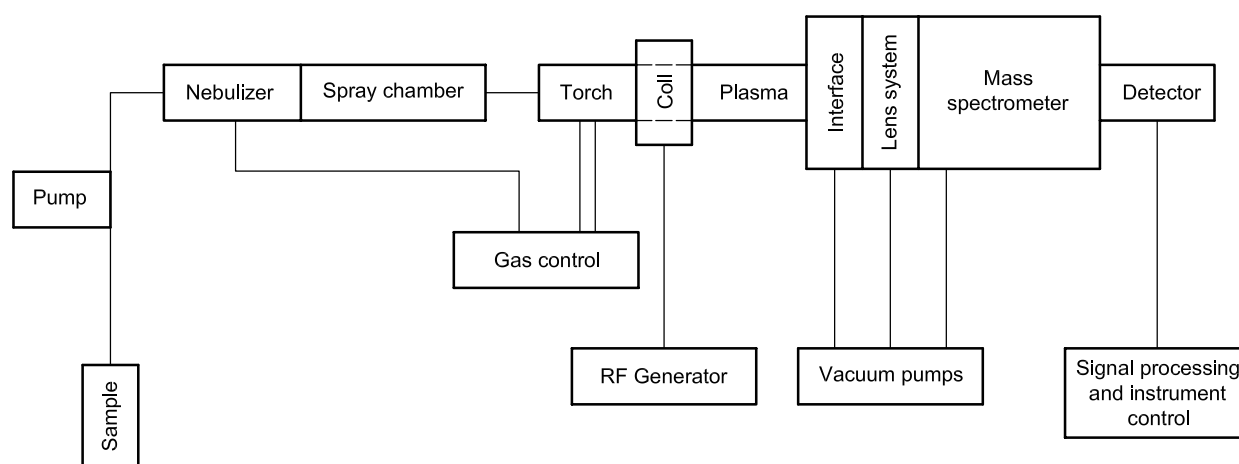


Figure 1 — Schematic block diagram of an ICP-mass spectrometer

5.2 Sample introduction

5.2.1 General

To introduce solutions to be measured into the plasma, a pump, a nebulizer and a spray chamber are generally used. The pump supplies the solution to the nebulizer. In the nebulizer, the solution is converted into an aerosol by an (argon) gas flow, except when an ultrasonic nebulizer is used; see 5.2.3. Large drops are removed from the aerosol in the spray chamber by means of collisions with the walls or other parts of the chamber and they are drained off as liquid. The resulting aerosol is then transferred into the plasma via the injector tube of the torch (see 5.3) with the help of the nebulizer gas (sample-introduction gas).

The sample introduction system is designed in such a way that

- a) the average mass per aerosol droplet is as low as possible;
- b) the mass of the aerosol transported to the plasma in each period of time is as constant as possible;
- c) the droplet size distribution and the added mass of the aerosol in each period of time is, as far as possible, independent of the solution to be measured (matrix effect, see 6.3);
- d) the time the aerosol takes to stabilize after introduction of a solution is as short as possible;
- e) the parts of the system in contact with the sample or the aerosol are not corroded, degraded or contaminated by the solution;
- f) carry-over from one sample to subsequent samples is minimized.

The components of the sample introduction system shall be able to withstand corrosive substances that may be in the solutions, such as strong acids. The material used for pump tubing should be resistant to dissolution and chemical attack by the solution to be nebulized. Components that come into contact with the solution are often made of special plastics. The use of glass and quartz shall be avoided if hydrofluoric acid is nebulized. In those cases, the nebulizer, spray chamber and torch injector tube shall be made of suitable inert materials.

The various components of the sample introduction system are discussed hereafter in relation to the above requirements and some "examples" are compared.

5.2.2 Sample pump

The use of a peristaltic pump to feed the solution to the nebulizer is not necessary with some nebulizers (see 5.2.3), but is desirable in almost all cases in order to render the supply of the solution less dependent on the composition of the solution. A sampling pump is used on all modern instruments.

It is advisable to use a peristaltic pump having the largest possible number of rollers and a velocity as high as possible to avoid major surges in the supply of the solution. The quantity of solution that is pumped is mostly between 0,1 ml and 1,5 ml per minute.

5.2.3 Nebulizer

The most common nebulizers are the concentric nebulizer [for example Meinhard¹⁾], the cross-flow nebulizer, the V-groove nebulizer and the ultrasonic nebulizer (USN). The first one is self-aspirating, and the second one can be, and these nebulizers can then be used without a pump (but seldom are). Nebulizers (except for the USN) can be made of glass or of hard, inert plastic.

1) The Meinhard nebulizer is an example of a suitable product available commercially. This information is given for the convenience of users of this part of ISO 17294 and does not constitute an endorsement by ISO of this product.

The concentric nebulizer consists of two concentric tubes, the outer one being narrowed at the end. The solution flows through the central tube and the nebulizer gas (see 5.4) through the tube around it, creating a region of lower pressure around the tip of the central tube and disrupting the solution flow into small droplets (the aerosol). This nebulizer performs best with solutions with a low content of dissolved matter, although there are also models that are less sensitive to significant amounts of dissolved matter in the solution to be nebulized.

The cross-flow nebulizer consists of two capillary tubes mounted at a right angle, one being used for the supply of the solution and the other for the supply of the nebulizer gas. Depending on the distance between the openings of the capillary tubes and their diameters, the nebulizer can be self-aspirating. With larger diameters, the chance of blockages occurring is of course smaller, but a pump will have to be used to supply the solution.

In the V-groove nebulizer, the solution flows through a vertical V-groove to the outflow opening of the nebulizer gas. The solution is nebulized by the high linear speed of this gas at the very small diameter outflow opening. The V-groove nebulizer was developed for solutions with a high concentration of dissolved matter and/or with suspended particles, although it is also used successfully with diluted and/or homogenous solutions. Similar nebulizers are the Burgener²⁾ nebulizer and the cone-spray nebulizer, with similar outer shapes as the concentric nebulizer. With these nebulizers, the solution flows out into a cone-shaped area at the tip of the nebulizer instead of a V-groove and flows over the outflow opening of the nebulizer gas.

In the ultrasonic nebulizer, the solution is pumped through a tube that ends near the transducer plate that vibrates at an ultrasonic frequency. The amount of aerosol produced (the efficiency) is typically 10 % to 20 % of the quantity of the pumped solution. This is so high that the aerosol has to be dried (desolvated) before being introduced into the plasma, which would otherwise be extinguished. The aerosol is transported to the plasma by the nebulizer gas. Disadvantages of the ultrasonic nebulizer include its greater susceptibility to matrix effects, diminished tolerance to high dissolved solid contents and a longer rinsing time.

For the other nebulizers described above, the efficiency is typically only a few percent. The efficiency increases when the solution introduction rate is decreased. Specially designed concentric micro-nebulizers made of special types of hard plastic operate at solution flow rates of 10 µl/min to 100 µl/min and efficiencies approaching 100 %. These concentric micro-nebulizers often show a very good precision (low relative standard deviation of the signal) and can also be combined with a membrane desolvator [see 6.2.1 a)].

Several other types of nebulizer may be used for specific applications.

5.2.4 Spray chamber

In the spray chamber [for example Scott (double concentric tubes), cyclonic or impact bead], the larger drops of the aerosol are drained off in liquid form. To create and keep over-pressure in the chamber, the liquid shall be removed via a sealed drain tube utilizing hydrostatic pressure or by pumping. The liquid shall be removed evenly in order to avoid pressure variations in the chamber, which can result in variations in the signal.

By cooling the spray chamber to 2 °C to 5 °C, the water vapour formed in the nebulization process condenses, thereby reducing the water load of the plasma. This results in a reduction in the formation of interfering polyatomic ions (oxides); see 6.2.2.

5.2.5 Other systems

There are other types of introduction systems for particular applications. They include laser or spark ablation of a solid sample, evaporation of the solution by means of a graphite furnace or a metal filament, introduction of a gas or a gas form of the analyte (as in the hydride generation technique), systems for the direct introduction of solid matter into the plasma (for example in the form of a slurry of a finely dispersed powder in a solvent) and the introduction with a graphite rod directly into the plasma.

2) The Burgener nebulizer is an example of a suitable product available commercially. This information is given for the convenience of users of this part of ISO 17294 and does not constitute an endorsement by ISO of this product.