
**Infusion equipment for medical use —
Part 8:
Infusion equipment for use with pressure
infusion apparatus**

*Matériel de perfusion à usage médical —
Partie 8: Matériel de perfusion pour utilisation avec des appareils de
perfusion sous pression*

[ISO 8536-8:2004](https://standards.iteh.ai/catalog/standards/sist/8ee77121-6b01-41e0-9edd-de0da1693f0d/iso-8536-8-2004)

<https://standards.iteh.ai/catalog/standards/sist/8ee77121-6b01-41e0-9edd-de0da1693f0d/iso-8536-8-2004>



PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 8536-8:2004

<https://standards.iteh.ai/catalog/standards/sist/8ee77121-6b01-41e0-9edd-de0da1693f0d/iso-8536-8-2004>

© ISO 2004

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

Page

Foreword	iv
1 Scope	1
2 Normative references	1
3 General requirements	1
4 Designation	4
4.1 Infusion set	4
4.2 Air-inlet device	4
5 Materials	4
6 Physical requirements	5
6.1 Particulate contamination	5
6.2 Tensile strength	5
6.3 Leakage	5
6.4 Male conical fitting	5
6.5 Injection site	5
6.6 Fluid filter	5
6.7 Flow rate of infusion fluid	5
6.8 Closure-piercing device	5
6.9 Air-inlet device	5
6.10 Drip chamber and drip tube	5
6.11 Tubing	5
6.12 Flow regulator	5
6.13 Protective caps	6
6.14 Storage volume	6
7 Chemical requirements	6
8 Biological requirements	6
9 Packaging	6
10 Labelling	6
10.1 Unit container	6
10.2 Shelf or multi-unit container	7
Annex A (normative) Physical tests	8
Annex B (normative) Chemical tests	9
Annex C (normative) Biological tests	10
Bibliography	11

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 8536-8 was prepared by Technical Committee ISO/TC 76, *Transfusion, infusion and injection equipment for medical and pharmaceutical use*.

ISO 8536 consists of the following parts, under the general title *Infusion equipment for medical use*:

- *Part 1: Infusion glass bottles*
- *Part 2: Closures for infusion bottles*
- *Part 3: Aluminium caps for infusion bottles*
- *Part 4: Infusion sets for single use, gravity feed*
- *Part 5: Burette infusion sets for single use, gravity feed*
- *Part 6: Freeze drying closures for infusion bottles*
- *Part 7: Caps made of aluminium-plastics combinations for infusion bottles*
- *Part 8: Infusion equipment for use with pressure infusion apparatus*
- *Part 9: Fluid lines for use with pressure infusion equipment*
- *Part 10: Accessories for fluid lines for use with pressure infusion equipment*
- *Part 11: Infusion filters for use with pressure infusion equipment*

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 8536-8:2004

<https://standards.iteh.ai/catalog/standards/sist/8ee77121-6b01-41e0-9edd-de0da1693f0d/iso-8536-8-2004>

Infusion equipment for medical use —

Part 8: Infusion equipment for use with pressure infusion apparatus

1 Scope

This part of ISO 8536 gives users information on sterilized infusion sets for single use with pressure infusion equipment up to a maximum of 200 kPa (2 bar).

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 594-2:1998, *Conical fittings with 6 % (Luer) taper for syringes, needles and certain other medical equipment — Part 2: Lock fittings*


ISO 8536-4:2004, *Infusion equipment for medical use — Part 4: Infusion sets for single use, gravity feed*

ISO 15223, *Medical devices — Symbols to be used with medical device labels, labelling and information to be supplied*

IEC 60601-2-24, *Medical electrical equipment — Part 2-24: Particular requirements for the safety of infusion pumps and controllers*

3 General requirements

3.1 The nomenclature to be used for components of infusion sets and of a separate air-inlet device is given in Figures 1, 2 and 3. These figures illustrate examples of the configuration of infusion sets and air-inlet devices; other configurations may be used provided they lead to the same results. Infusion sets as illustrated in Figure 2 should only be used for collapsible plastics containers. Infusion sets as illustrated in Figure 2 used with separate air-inlet devices as illustrated in Figure 3, or infusion sets as illustrated in Figure 1 shall be used for rigid containers.

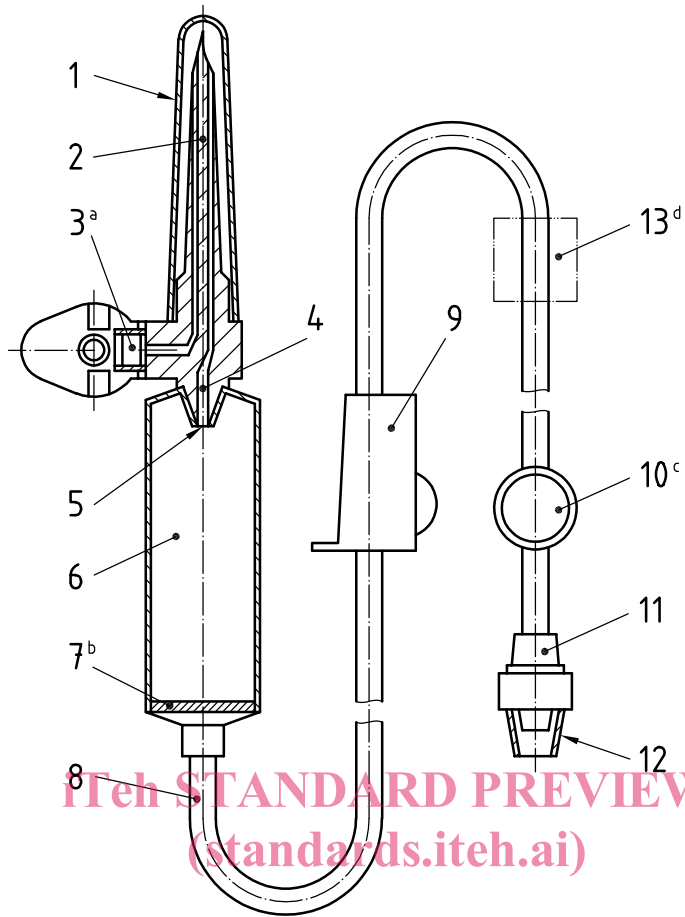


ISO 8536-8:2004
<https://standards.iteh.ai/catalog/standards/sist/8ee77121-6b01-41e0-9edd-de0da1693f0d/iso-8536-8-2004>

Key

- | | |
|---------------------------------------------|-------------------------------------------|
| 1 protective cap of closure-piercing device | 8 tubing |
| 2 closure-piercing device | 9 flow regulator |
| 3 air-inlet with air filter and closure | 10 injection site |
| 4 fluid channel | 11 male conical fitting |
| 5 drip tube | 12 protective cap of male conical fitting |
| 6 drip chamber | 13 flow element |
| 7 fluid filter | |

- a Closure of air inlet is optional.
- b The fluid filter may be positioned at other sites, preferably near the patient access. Generally, the fluid filter used has a nominal pore size of 15 µm.
- c Injection site is optional.
- d Optional element of infusion set which interfaces with pressure infusion equipment.

Figure 1 — Example of a vented infusion set

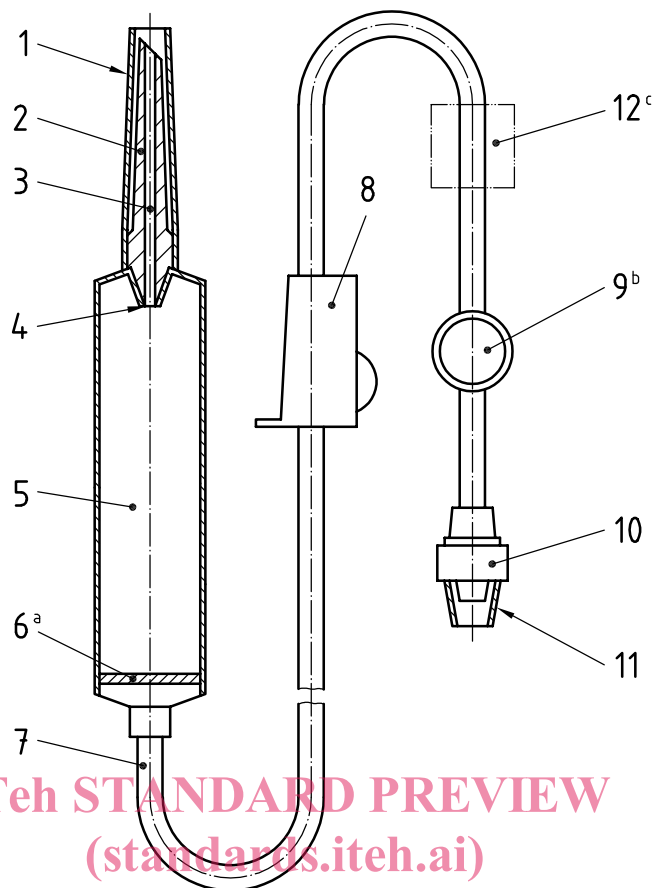

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 8536-8:2004

Key


- | | | | |
|---|-----------------------------------------------|----|--------------------------------------------|
| 1 | protective cap of the closure-piercing device | 7 | tubing |
| 2 | closure-piercing device | 8 | flow regulator |
| 3 | fluid channel | 9 | injection site |
| 4 | drip tube | 10 | male conical fitting |
| 5 | drip chamber | 11 | protective cap of the male conical fitting |
| 6 | fluid filter | 12 | flow element |

^a The fluid filter may be positioned at other sites, preferably near the patient access. Generally, the fluid filter used has a nominal pore size of 15 µm.

^b Injection site is optional.

^c Optional element of infusion set which interfaces with pressure infusion equipment.

Figure 2 — Example of a non-vented infusion set

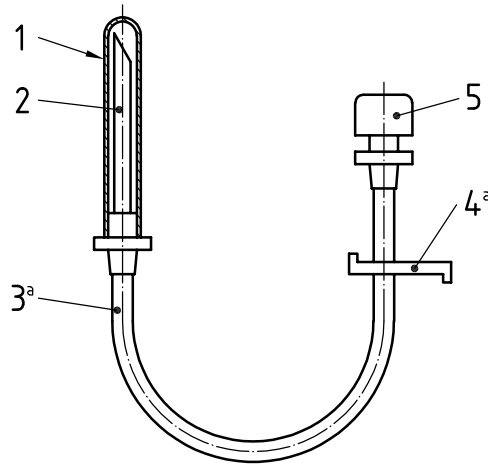

Key

- | | | | |
|---|-----------------------------------|---|---------------------------|
| 1 | protective cap | 4 | clamp ^a |
| 2 | closure-piercing device or needle | 5 | air-inlet with air filter |
| 3 | tubing | | |

^a Other designs are acceptable if the same safety aspects are ensured.

Figure 3 — Example of an air-inlet device

3.2 The infusion set shall be provided with protective caps to maintain sterility of the internal parts of the set until the set is used. The air-inlet device shall be provided with a protective cap over the closure-piercing device or needle.

ISO 8536-8:2004
<https://standards.iteh.ai/catalog/standards/sist/8ee77121-6b01-41e0-9edd-de0da1693f0d/iso-8536-8-2004>

4 Designation

4.1 Infusion set

Infusion sets complying with the requirements specified in this part of ISO 8536 shall be designated by the descriptor words, followed by a reference to this part of ISO 8536, followed by the letters IS, followed by the letter P:

Infusion set ISO 8536-8 — IS — P

4.2 Air-inlet device

Air-inlet devices complying with the requirements specified in this part of ISO 8536 shall be designated by the descriptor words, followed by a reference to this part of ISO 8536, followed by the letters AD.

Air-inlet device ISO 8536-8 — IS — AD

5 Materials

The materials from which the infusion set and its components as given in Clause 3 are manufactured shall comply with the requirements as specified in Clause 6. Where components of the infusion set come into contact with the infusion solution, the materials additionally shall comply with the requirements as specified in Clauses 7 and 8.

6 Physical requirements

6.1 Particulate contamination

ISO 8536-4 applies.

6.2 Tensile strength

When tested as specified in A.2, the infusion set, excluding protective caps, shall withstand a static tensile force of not less than 15 N for 15 s.

6.3 Leakage

The infusion set shall be impermeable to air, microorganisms and fluids.

Neither air nor water shall escape when tested according to A.3.2 and A.3.4, and no air shall enter when tested according to A.3.3.

6.4 Male conical fitting

The male conical fitting must be in accordance with ISO 594-2. No water shall leak from the point of connection when tested according to A.4.

6.5 Injection site iTeh STANDARD PREVIEW

The injection site shall enable injection into the tubing. There shall be no leakage of more than one falling drop of water when tested according to A.5.

6.6 Fluid filter <https://standards.iteh.ai/catalog/standards/sist/8ee77121-6b01-41e0-9edd-de0da1693f0d/iso-8536-8-2004>

ISO 8536-4 applies.

6.7 Flow rate of infusion fluid

ISO 8536-4 applies.

6.8 Closure-piercing device

ISO 8536-4 applies.

6.9 Air-inlet device

ISO 8536-4 applies.

6.10 Drip chamber and drip tube

ISO 8536-4 applies.

6.11 Tubing

ISO 8536-4 applies.

6.12 Flow regulator

ISO 8536-4 applies.