
Single-use sterile rubber surgical gloves — Specification

*Gants en caoutchouc à usage chirurgical, stériles, non réutilisables —
Spécifications*

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[ISO 10282:2002](https://standards.iteh.ai/catalog/standards/sist/ffd5d249-0f2c-415d-b64c-a43ae0d3e08d/iso-10282-2002)

<https://standards.iteh.ai/catalog/standards/sist/ffd5d249-0f2c-415d-b64c-a43ae0d3e08d/iso-10282-2002>



Reference number
ISO 10282:2002(E)

© ISO 2002

PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 10282:2002

<https://standards.iteh.ai/catalog/standards/sist/fd5d249-0f2c-415d-b64c-a43ae0d3e08d/iso-10282-2002>

© ISO 2002

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.ch
Web www.iso.ch

Printed in Switzerland

Contents

Page

Foreword	iv
1 Scope	1
2 Normative references	1
3 Classification	1
4 Materials	2
5 Sampling and selection of test pieces	3
6 Requirements	3
7 Packaging	6
8 Marking	6
Annex A (normative) Test for watertightness	8

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 10282:2002

<https://standards.iteh.ai/catalog/standards/sist/fd5d249-0f2c-415d-b64c-a43ae0d3e08d/iso-10282-2002>

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 3.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this International Standard may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 10282 was prepared by Technical Committee ISO/TC 45, *Rubber and rubber products*, Subcommittee SC 4, *Products (other than hoses)*.

This second edition cancels and replaces the first edition (ISO 10282:1994), which has been technically revised.

Annex A forms a normative part of this International Standard.

iTeh STANDARD PREVIEW
(standards.iteh.ai)
ISO 10282:2002
<https://standards.iteh.ai/catalog/standards/sist/fd5d249-0f2c-415d-b64c-a43ae0d3e08d/iso-10282-2002>

Single-use sterile rubber surgical gloves — Specification

1 Scope

This International Standard specifies requirements for packaged sterile rubber gloves intended for use in surgical procedures to protect the patient and the user from cross-contamination. It is applicable to single-use gloves that are worn once and then discarded. It does not apply to examination or procedure gloves. It covers gloves with smooth surfaces and gloves with textured surfaces over part or all of the glove.

This standard is intended as a reference for the performance and safety of rubber surgical gloves. The safe and proper usage of surgical gloves and sterilization procedures with subsequent handling, packaging and storage procedures are outside the scope of this International Standard.

2 Normative references

The following normative documents contain provisions which, through reference in this text, constitute provisions of this International Standard. For dated references, subsequent amendments to, or revisions of, any of these publications do not apply. However, parties to agreements based on this International Standard are encouraged to investigate the possibility of applying the most recent editions of the normative documents indicated below. For undated references, the latest edition of the normative document referred to applies. Members of ISO and IEC maintain registers of currently valid International Standards.

ISO 37:1994, *Rubber, vulcanized or thermoplastic — Determination of tensile stress-strain properties*

ISO 188:1998, *Rubber, vulcanized or thermoplastic — Accelerated ageing and heat resistance tests*

ISO 2859-1:1999, *Sampling procedures for inspection by attributes — Part 1: Sampling schemes indexed by acceptance quality limit (AQL) for lot-by-lot inspection*

ISO 4648:1991, *Rubber, vulcanized or thermoplastic — Determination of dimensions of test pieces and products for test purposes*

ISO 10993 (all parts), *Biological evaluation of medical devices*

ISO 15223:2000, *Medical devices — Symbols to be used with medical device labels, labelling and information to be supplied*

3 Classification

3.1 General

Gloves are classified by type, design and finish, as given in 3.2 to 3.4.

3.2 Type

Two types are classified:

- a) type 1: gloves made primarily from natural rubber latex;
- b) type 2: gloves made primarily from nitrile rubber latex, polychloroprene rubber latex, styrene-butadiene rubber solution, styrene-butadiene rubber emulsion or thermoplastic elastomer solution.

3.3 Design

Two designs are classified:

- a) gloves with straight fingers;
- b) gloves with fingers curved in the palmar direction.

The glove shall be anatomically correct, with the thumb positioned towards the palmar surface of the index finger rather than lying flat. The fingers and thumb may be straight or curved in the palmar direction.

3.4 Finish

Four finishes are classified:

- a) textured surface over part or all of the glove;
 - b) smooth surface;
 - c) powdered surface;
 - d) powder-free surface.
- ITeC STANDARD PREVIEW**
(standards.iteh.ai)
<https://standards.iteh.ai/catalog/standards/sist/fd5d249-0f2c-415d-b64c-a43ae0d3e08d/iso-10282-2002>

NOTE 1 Powdered gloves are gloves where a powder has been added as a part of the manufacturing process, generally to facilitate donning. Powder-free gloves are gloves which have been manufactured without the deliberate addition of powdered materials to facilitate donning.

NOTE 2 The cuff termination of the glove may be cut or in the form of a rolled rim.

4 Materials

Gloves shall be manufactured from compounded natural rubber or nitrile rubber or polychloroprene rubber latex, or compounded styrene-butadiene rubber or thermoplastic elastomer solution, or compounded styrene-butadiene rubber emulsion. To facilitate donning the gloves, any surface treatment, lubricant, powder or polymer coating may be used subject to compliance with ISO 10993.

Any pigment used shall be non-toxic. It is essential that substances used for surface treatment which are capable of being transferred are bio-absorbable.

Gloves as supplied to the user shall comply with the relevant part(s) of ISO 10993. The manufacturer shall make available to the purchaser, on request, data to support compliance with these requirements.

NOTE 1 Other suitable polymeric materials may be included in future editions of this International Standard.

NOTE 2 It is recognized that some individuals may, over a period of time, become sensitized to a particular rubber compound (allergic reaction) and require gloves of an alternative formulation.

NOTE 3 Limits of extractable proteins, allergenic proteins, residual chemicals, endotoxins and residual powder in gloves may be specified in future editions of this International Standard, subject to the availability of relevant ISO standard test methods.

5 Sampling and selection of test pieces

5.1 Sampling

For reference purposes, gloves shall be sampled and inspected in accordance with ISO 2859-1. The inspection levels and acceptable quality limits (AQLs) shall conform to those specified in Table 1 for the characteristics listed.

When a lot size cannot be determined, a lot of 35 001 to 150 000 shall be assumed.

Table 1 — Inspection levels and AQLs

Characteristic	Inspection level	AQL
Physical dimensions (width, length, thickness)	S-2	4,0
Watertightness	I	1,5
Force at break and elongation at break (before and after accelerated ageing) and force at 300 % elongation (before accelerated ageing)	S-2	4,0

5.2 Selection of test pieces

Where test pieces are required, they shall be taken from the palm or back of gloves.

6 Requirements

6.1 Dimensions

ISO 10282:2002
<https://standards.iteh.ai/catalog/standards/sist/fd5d249-0f2c-415d-b64c-a43ae0d3e08d/iso-10282-2002>

When measured at the points shown in Figure 1, gloves shall comply with the dimensions for palm width and length given in Table 2, using the inspection level and AQL given in Table 1.

The measurement of length shall be the shortest distance between the tip of the second finger and the cuff termination.

NOTE The length measurement may be taken by hanging the glove on a suitable mandrel with a tip radius of 5 mm.

The measurement of width shall be at the midpoint between the base of the index finger and the base of the thumb. The width measurement shall be made with the glove placed on a flat surface.

The thickness of the double wall of an intact glove shall be measured in accordance with ISO 4648, with a pressure on the foot of $22 \text{ kPa} \pm 5 \text{ kPa}$, at each of the locations shown in Figure 2: a point $13 \text{ mm} \pm 3 \text{ mm}$ from the extreme tip of the second finger, the approximate centre of the palm and a point $25 \text{ mm} \pm 5 \text{ mm}$ from the cuff termination. The single-wall thickness at each point shall be reported as half the measured double-wall thickness and shall comply with the dimensions given in Table 2, using the inspection level and AQL given in Table 1.

If visual inspection indicates the presence of thin spots, then single-wall thickness measurements shall be made in such areas. The thickness at the smooth area and textured area of a single wall when measured as described in this subclause shall not be less than 0,10 mm and 0,13 mm respectively.

NOTE The thickness of the cuff termination measured in accordance with ISO 4648 should preferably not exceed 2,50 mm.


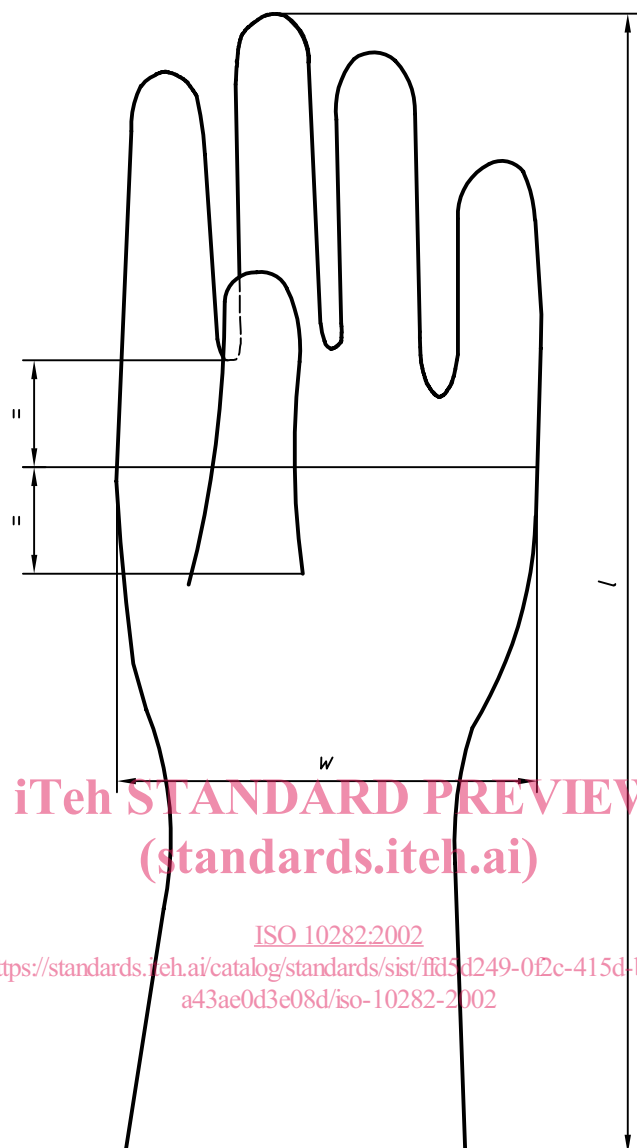


Figure 1 — Measurement points for width and length

Table 2 — Dimensions and tolerances

Size code	Width (dimension w , Figure 1) mm	Minimum length (dimension l , Figure 1) mm	Minimum thickness (at the locations shown in Figure 2) mm
5	67 ± 4	250	For all sizes: Smooth area: 0,10 Textured area: 0,13
5,5	72 ± 4	250	
6	77 ± 5	260	
6,5	83 ± 5	260	
7	89 ± 5	270	
7,5	95 ± 5	270	
8	102 ± 6	270	
8,5	108 ± 6	280	
9	114 ± 6	280	
9,5	121 ± 6	280	

Dimensions in millimetres

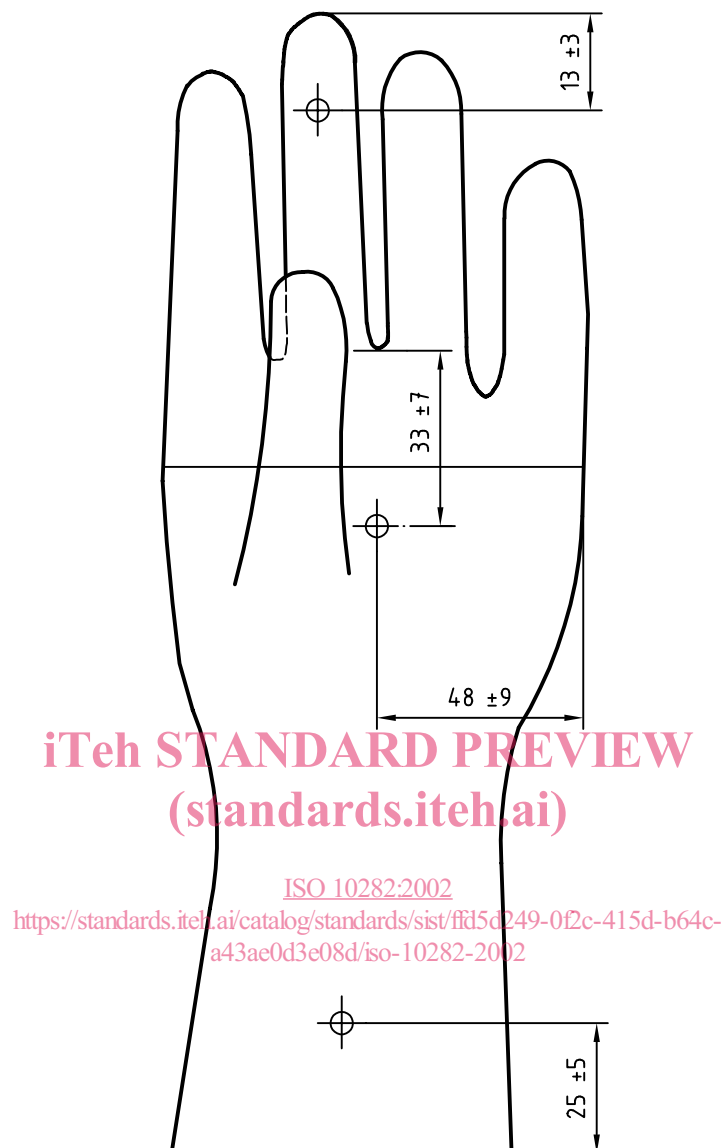

NOTE The distance $48 \text{ mm} \pm 9 \text{ mm}$ locates the approximate centre of the palm for different glove sizes.

Figure 2 — Measurement points for thickness

6.2 Watertightness

When gloves are tested for watertightness as described in annex A, the sample size and allowable number of non-conforming (leaking) gloves in the sample shall be determined in accordance with the inspection level and AQL given in Table 1.

6.3 Tensile properties

6.3.1 General

Tensile properties shall be measured in accordance with ISO 37, taking three test pieces from each glove and using the median value as the test result. Test pieces shall be taken from the palm or back of gloves.