
Compressed air —

Part 8:

**Test methods for solid particle content by
mass concentration**

Air comprimé —
iTeh STANDARD PREVIEW
*Partie 8: Méthodes d'essai pour la détermination de la teneur en
particules solides par concentration massique*
(standards.iteh.ai)

ISO 8573-8:2004

<https://standards.iteh.ai/catalog/standards/sist/f794b3b3-f10d-4bde-97cf-eacafad6e761/iso-8573-8-2004>



PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 8573-8:2004

<https://standards.iteh.ai/catalog/standards/sist/f794b3b3-f10d-4bde-97cf-eacafad6e761/iso-8573-8-2004>

© ISO 2004

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

Page

| | |
|---|-----------|
| Foreword | iv |
| 1 Scope | 1 |
| 2 Normative references | 1 |
| 3 Terms and definitions | 1 |
| 4 Units and symbols | 2 |
| 5 Selection of methods | 2 |
| 6 Sampling techniques | 2 |
| 7 Measurement methods | 3 |
| 8 Evaluation of test results | 6 |
| 9 Uncertainty | 6 |
| 10 Test report | 7 |
| Annex A (informative) Sample test report | 8 |

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[ISO 8573-8:2004](https://standards.iteh.ai/catalog/standards/sist/f794b3b3-f10d-4bde-97cf-eacafad6e761/iso-8573-8-2004)

<https://standards.iteh.ai/catalog/standards/sist/f794b3b3-f10d-4bde-97cf-eacafad6e761/iso-8573-8-2004>

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 8573-8 was prepared by Technical Committee ISO/TC 118, *Compressors, pneumatic tools and pneumatic machines*, Subcommittee SC 4, *Quality of compressed air*.

ISO 8573 consists of the following parts, under the general title *Compressed air*.

- *Part 1: Contaminants and purity classes*
- *Part 2: Test methods for aerosol oil content* [ISO 8573-8:2004](https://standards.iteh.ai/catalog/standards/sist/f794b3b3-f10d-4bde-97cf-82ca9d6761/iso-8573-8-2004)
- *Part 3: Test methods for measurement of humidity*
- *Part 4: Test methods for solid particle content*
- *Part 5: Test methods for oil vapour and organic solvent content*
- *Part 6: Test methods for gaseous contaminant content*
- *Part 7: Test methods for viable microbiological contaminant content*
- *Part 8: Test methods for solid particle content by mass concentration*
- *Part 9: Test methods for liquid water content*

Part 2 is under revision.

Compressed air —

Part 8:

Test methods for solid particle content by mass concentration

1 Scope

This part of ISO 8573 specifies test methods for determining the solid particle mass concentration in compressed air, expressed as the mass of solid particles with maximum particle size limits. The limitations of the methods are also given. One of a series of standards aimed at harmonizing air contamination measurements, it identifies sampling techniques and also gives requirements for evaluation, uncertainty considerations and reporting for the air purity parameter solid particles by mass concentration. The test methods are suitable for determining purity classes in accordance with ISO 8573-1. (Particle content based on counting particles is dealt with in ISO 8573-4.)

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 1219-1, *Fluid power systems and components — Graphic symbols and circuit diagrams — Part 1: Graphic symbols*

ISO 3857-1, *Compressors, pneumatic tools and machines — Vocabulary — Part 1: General*

ISO 5598, *Fluid power systems and components — Vocabulary*

ISO 8573-1, *Compressed air — Part 1: Contaminants and purity classes*

ISO 8573-2, *Compressed air — Part 2: Test methods for aerosol oil content*

ISO 8573-4, *Compressed air — Part 4: Test methods for solid particle content*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 3857-1, ISO 5598, ISO 8573-1 and ISO 8573-4 apply.

4 Units and symbols

For the purposes of this part of ISO 8573, the following, including non-SI-preferred, units are used:

- 1 bar = 100 000 Pa;
- 1 l (litre) = 0,001 m³;
- bar(a), used for expressing absolute pressure;
- bar(e), used for expressing effective pressure.

For the graphic symbols used in Figure 1, see ISO 1219-1.

5 Selection of methods

The gravimetric method to be used is suitable for mass concentration measurement, however, where water and oil is present in the compressed air, it shall be reduced to a minimum.

A suitable method for solid particle diameter measurement may be selected from those given in Table 1.

Table 1 — Solid particle diameter measurement methods

| Type of method | Maximum solid particle diameter <i>d</i> µm | Liquid water and oil contaminant mg/m ³ |
|-----------------------|---|---|
| Microscope method | $d \geq 0,5$ | ≤ 20 |
| Particle sizer method | $0,1 \leq d \leq 40$ | Not admitted |

6 Sampling techniques

The sampling shall be made at or near the actual pressure and at a constant flow rate.

The choice of sampling method will depend upon the actual level of contamination and the compressed air flow in the compressed air system. For sampling methods, see ISO 8573-2 and ISO 8573-4.

For partial flow sampling, it should be noted that, where large particle sizes are involved, the effects of gravity could introduce sampling errors.

Compressed air samples may be routed back into the main pipe or vent to the atmosphere after measurement. The value of air sample parameters (pressure, temperature, air velocity, etc.) shall be within the ranges specified by the test equipment manufacturer. Method B1 uses full flow sampling from the main pipe flow by means of a Y-piece.

7 Measurement methods

7.1 General

The test equipment and instruments shall be in good working order. Consideration shall be given to the calibration requirements of the measurement equipment used as given in the applicable instructions.

The indicated methods may be used at any point in a compressed air system using portable instruments where conditions of measurement are satisfied and available connectors and shut-off valves exist for connection to the compressed air system.

In order to guarantee the required accuracy of determination of solid particle content by the gravimetric method, the total content of water and oil aerosols in the compressed air sampling shall be less than 20 mg/m³ for sampling Method A and less than 5 mg/m³ for sampling Methods B1 and B2.

Reference should be made to the measurement equipment manufacturer in respect of the applicability of the equipment.

The gravimetric method deals with the separation and the weighing of solid particles that are present in a compressed air sample. The influence of temperature, pressure, humidity and other contaminants of compressed air shall be taken into consideration.

7.2 Test equipment


7.2.1 General

Air flow is passed through the test equipment via suitable in-line valves which have been previously checked to ensure they do not contribute to the level of contamination already present.

The general arrangement of the test equipment for the gravimetric method shall be in accordance with Figure 1.

NOTE The numbers given between parentheses in the subclause titles refer to the numbering of the elements in Figure 1.

For symbols, see ISO 1219-1.

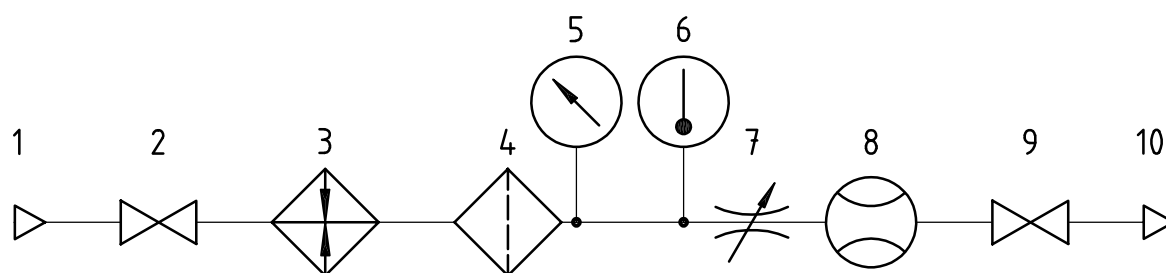

Key

| | | | |
|---|----------------------|----|--------------------|
| 1 | sampling point | 6 | thermometer |
| 2 | shut-off valve | 7 | flow control valve |
| 3 | heater (if required) | 8 | air flowmeter |
| 4 | membrane holder | 9 | shut-off valve |
| 5 | pressure gauge | 10 | discharge outlet |

Figure 1 — Circuit diagram of test equipment for gravimetric method

7.2.2 Membrane holder (4)

The membrane shall be manufactured from hydrophobic high-efficiency material.

NOTE For a description of a typical membrane and its holder, see ISO 8573-2.

7.2.3 Flow control valve (7)

In order to adjust the flow accurately, use a valve with fine adjustment.

7.2.4 Pressure gauge (5)

The pressure values shall be recorded during the entire period of the test.

The accuracy of measurement of the pressure shall be better than $\pm 2\%$ of reading.

7.2.5 Thermometer (6)

The temperature values shall be recorded during the entire period of the test.

The accuracy of measurement of the temperature shall be better than $\pm 1^\circ\text{C}$.

7.2.6 Air flowmeter (8)

The flow rate values shall be recorded during the entire period of the test.

The accuracy of measurement of the flow rate shall be better than $\pm 5\%$.

7.2.7 Pipes, connectors, shut-off valves (2 and 9)

ISO 8573-8:2004
<https://standards.iteh.ai/catalog/standards/sist/f794b3b3-f10d-4bde-97cf-4a6656761560/iso-8573-8-2004>

The requirements for pipes, connectors and shut-off valves shall be according to ISO 8573-2.

7.2.8 Heater (3)

The heater may be used to decrease the level of liquid water and oil contaminant content in the compressed air sample to the value specified in 7.1. Reducing the amount of liquid water and oil content by heating and/or the reduction of the pressure of the compressed air shall not have an influence on solid particle content in the compressed air sample.

7.3 Test procedure

7.3.1 Preparation for measuring

The procedures for preparation for measuring shall be in accordance with ISO 8573-2. The weight of the dry membrane shall be determined before the sample is taken.

7.3.2 Duration of test

The optimum duration of the compressed air sampling may be determined after the first proof measurement to determine the tentative solid particle concentration.

Approximate duration of test, t , in minutes can also be determined by the following inequality:

$$\frac{m_{\min}}{c_{p \text{ lim } q}} < t < \frac{m_{\max}}{c_{p \text{ lim } q}} \tag{1}$$

where

m_{\min} is the minimum required amount of solid particle content on the membrane, in milligrams;

m_{\max} is the maximum permitted amount of solid particle content on the membrane, in milligrams;

$C_{p \text{ lim}}$ is the assumed or maximum permitted amount of solid particle content in the compressed air, in milligrams per cubic metre;

q is the compressed air discharge through the membrane, in cubic metres per minute.

The mass of solid particles collected on the membrane shall be in range $1 \text{ mg} \leq m \leq 5 \text{ mg}$ on 1 cm^2 of the membrane surface.

7.3.3 Measurement of solid particle mass concentration

If liquid water and oil contaminants are absent in the compressed air flow, the solid particle mass concentration for each sample is determined as a difference between masses of the test membrane before and after air sampling, divided by the total volume of air passed through the membrane. After air sampling and before weighing, the test membrane should be placed in a desiccator over a suitable desiccant, e.g. silica gel, for 10 - 15 min or until the mass of membrane is stable.

If there are liquid water and oil contaminants in the compressed air flow, they shall be removed after air sampling and before weighing of the test membrane. For this purpose, the test membrane shall be placed in the desiccator over sulphuric acid for 2 h. Then, the test membrane is carried in the chemical funnel on the conical wall (the filtrate is over the membrane), pressed to the conic wall with the glass stick and treated several times by small portions of a suitable solvent of total volume 10 - 15 ml for dissolving and removing of the oil. After that, the test membrane shall be maintained for 2 - 3 min at a temperature of 20 - 30 °C and then weighed.

Other methods for removal of water and oil from the test membrane are permitted if they have no influence on solid particle content of the test membrane after sampling the compressed air.

The maximum uncertainty of measurement of mass shall be better than $\pm 2 \%$.

7.4 Calculation of results

It is necessary to ensure that results are stable, repeatable and presented in a form that shows that they are so.

The solid particle mass concentration c_{pn} in mg/m^3 for each measurement shall be determined by the formula:

$$c_{\text{pn}} = \frac{m_n - m_0}{q_n t_n} \quad (2)$$

where

m_0 is the mass of test membrane before sampling, in milligrams;

m_n is the mass of test membrane after sampling, in milligrams;

q_n is the flow rate of sampling air through the membrane, in cubic metres per minute;

t_n is the sampling time, in minutes.

7.5 Determination of maximum diameter of solid particles

The measurement methods of maximum diameter of solid particles identified in Table 1 shall be carried out in accordance with ISO 8573-4.