
**Iron ores — Determination of sulfur
content —**

**Part 3:
Combustion/infrared method**

Minerais de fer — Dosage du soufre —

Partie 3: Méthode par combustion et infrarouge
(standards.iteh.ai)

[SIST ISO 4689-3:2005](https://standards.iteh.ai/catalog/standards/sist/2c590690-255e-41fb-80a6-27895ab916e3/sist-iso-4689-3-2005)

<https://standards.iteh.ai/catalog/standards/sist/2c590690-255e-41fb-80a6-27895ab916e3/sist-iso-4689-3-2005>



PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[SIST ISO 4689-3:2005](https://standards.iteh.ai/catalog/standards/sist/2c590690-255e-41fb-80a6-27895ab916e3/sist-iso-4689-3-2005)

<https://standards.iteh.ai/catalog/standards/sist/2c590690-255e-41fb-80a6-27895ab916e3/sist-iso-4689-3-2005>

© ISO 2004

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

	Page
1 Scope	1
2 Normative references	1
3 Principle	1
4 Reagents	2
5 Apparatus	2
6 Sampling and samples	5
7 Procedure	5
8 Expression of results	6
9 Test report	9
Annex A (normative) Flowsheet of the procedure for the acceptance of analytical values for test samples	10
Annex B (informative) Derivation of repeatability and permissible tolerance equations	11
Annex C (informative) Precision data obtained by international analytical trial	12
Bibliography	14

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[SIST ISO 4689-3:2005](https://standards.iteh.ai/catalog/standards/sist/2c590690-255e-41fb-80a6-27895ab916e3/sist-iso-4689-3-2005)

<https://standards.iteh.ai/catalog/standards/sist/2c590690-255e-41fb-80a6-27895ab916e3/sist-iso-4689-3-2005>

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 4689-3 was prepared by Technical Committee ISO/TC 102, *Iron ore and direct reduced iron*, Subcommittee SC 2, *Chemical analysis*.

This first edition, in part cancels and replaces ISO 4690:1986, which has been technically revised.

ISO 4689 consists of the following parts, under the general title *Iron ores — Determination of sulfur content*:

- *Part 2: Combustion/titration method* [SIST ISO 4689-3:2005](http://standards.iteh.ai/catalog/standards/sist/2c590690-255e-41fb-80a6-27895ab916e3/sist-iso-4689-3-2005)
- *Part 3: Combustion/infrared method* <http://standards.iteh.ai/catalog/standards/sist/2c590690-255e-41fb-80a6-27895ab916e3/sist-iso-4689-3-2005>

The following part is under preparation:

- *Part 1: Barium sulfate gravimetric method*

Introduction

This part of ISO 4689 is a new procedure. ISO 4689-2 was originally published as ISO 4690:1986, *Iron ores — Determination of sulfur content — Combustion method*. Under a policy of rationalization of the numbering system used in ISO/TC 102, it has been decided to re-designate ISO 4690:1986 as ISO 4689-2. It was further decided to introduce a combustion/infrared method, numbered ISO 4689-3, i.e. this part of ISO 4689.

When next revised, ISO 4689:1986, *Iron ores — Determination of sulfur content — Barium sulfate gravimetric method*, will be re-designated 4689-1.

iTeh STANDARD PREVIEW (standards.iteh.ai)

[SIST ISO 4689-3:2005](https://standards.iteh.ai/catalog/standards/sist/2c590690-255e-41fb-80a6-27895ab916e3/sist-iso-4689-3-2005)

<https://standards.iteh.ai/catalog/standards/sist/2c590690-255e-41fb-80a6-27895ab916e3/sist-iso-4689-3-2005>

iTeh STANDARD PREVIEW
(standards.iteh.ai)

SIST ISO 4689-3:2005

<https://standards.iteh.ai/catalog/standards/sist/2c590690-255e-41fb-80a6-27895ab916e3/sist-iso-4689-3-2005>

Iron ores — Determination of sulfur content —

Part 3: Combustion/infrared method

WARNING — This part of ISO 4689 may involve hazardous materials, operations and equipment. This part of ISO 4689 does not purport to address all of the safety problems associated with its use. It is the responsibility of the user of this part of ISO 4689 to establish appropriate health and safety practices and determine the applicability of regulatory limitations prior to use.

1 Scope

This part of ISO 4689 specifies a combustion/infrared method, using a high-frequency induction furnace, for the determination of the sulfur content of iron ores.

This method is applicable to sulfur contents between 0,002 % (mass fraction) and 0,25 % (mass fraction) in natural iron ores, iron ore concentrates and agglomerates, including sinter products. The method is not applicable to iron ores containing more than 1,0 % (mass fraction) of combined water. The apparatus, of which the metal filter is equipped with a heating device, can be applied to iron ores containing less than 3,0 % (mass fraction) of combined water.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 385-1:1984, *Laboratory glassware — Burettes — Part 1: General requirements*

ISO 648:1977, *Laboratory glassware — One-mark pipettes*

ISO 1042:1998, *Laboratory glassware — One-mark volumetric flasks*

ISO 3082:2000, *Iron ores — Sampling and sample preparation procedures*

ISO 7764:1985, *Iron ores — Preparation of predried test samples for chemical analysis*

3 Principle

The sample is mixed with a flux containing iron, tin and tungsten and heated in a high-frequency induction furnace, using oxygen as a supporting fuel and carrier gas.

The evolved sulfur dioxide is carried by oxygen into the cell of an infrared detector, where the absorption scale is read.

4 Reagents

During analysis, use only reagents of recognized analytical grade, and only distilled water or water of equivalent purity.

- 4.1 Metallic iron**, particle size 0,2 mm to 1,2 mm and containing less than 0,001 % sulfur.
- 4.2 Magnesium perchlorate**, $Mg(ClO_4)_2$ anhydrous, free flowing, particle size 0,5 mm to 2 mm.
- 4.3 Iron(III) oxide**, containing less than 0,003 % sulfur.
- 4.4 Metallic tin**, particle size 0,2 mm to 1,2 mm, containing less than 0,001 % sulfur.
- 4.5 Metallic tungsten**, particle size 0,2 mm to 1,2 mm, containing less than 0,001 % sulfur.
- 4.6 Soda-asbestos**, particle size 0,5 mm to 2 mm.
- 4.7 Sodium hydroxide**, particle size 0,5 mm to 2 mm.
- 4.8 Standard sulfur solution**, prepared as follows.

Dry 8 g of potassium sulfate (purity > 99,9 % (mass fraction) to constant mass at 105 °C to 110 °C and cool in a desiccator. Weigh the dried masses of potassium sulfate specified in Table 1 and dissolve each portion in water. Cool, transfer each portion to separate 100 ml volumetric flasks and dilute to volume with water.

Table 1 — Sulfur standard solution (calibration series)

Solution No.	Mass of potassium sulfate	Concentration of sulfur
1	0,543 5	1,00
2	1,087 0	2,00
3	1,902 2	3,50
4	2,717 4	5,00


5 Apparatus

Ordinary laboratory apparatus, including one-mark pipettes and one-mark volumetric flasks complying with the specifications of ISO 648:1977 and ISO 1042 respectively as well as the following.

- 5.1 Oxygen supply.**
- 5.2 Absorption tower**, containing soda-asbestos (4.6) or sodium hydroxide (4.7).
- 5.3 Drying tower**, containing magnesium perchlorate (4.2).
- 5.4 High-frequency induction furnace**, having a heating induction coil (height 30 mm to 55 mm, 4 to 5 rolls), capable of heating to a temperature of 1 200 °C.

An example of a combustion furnace, with combustion gas-refining section, is given in Figure 1.

- 5.5 Combustion tube**, quartz.
- 5.6 Refractory combustion crucible.**

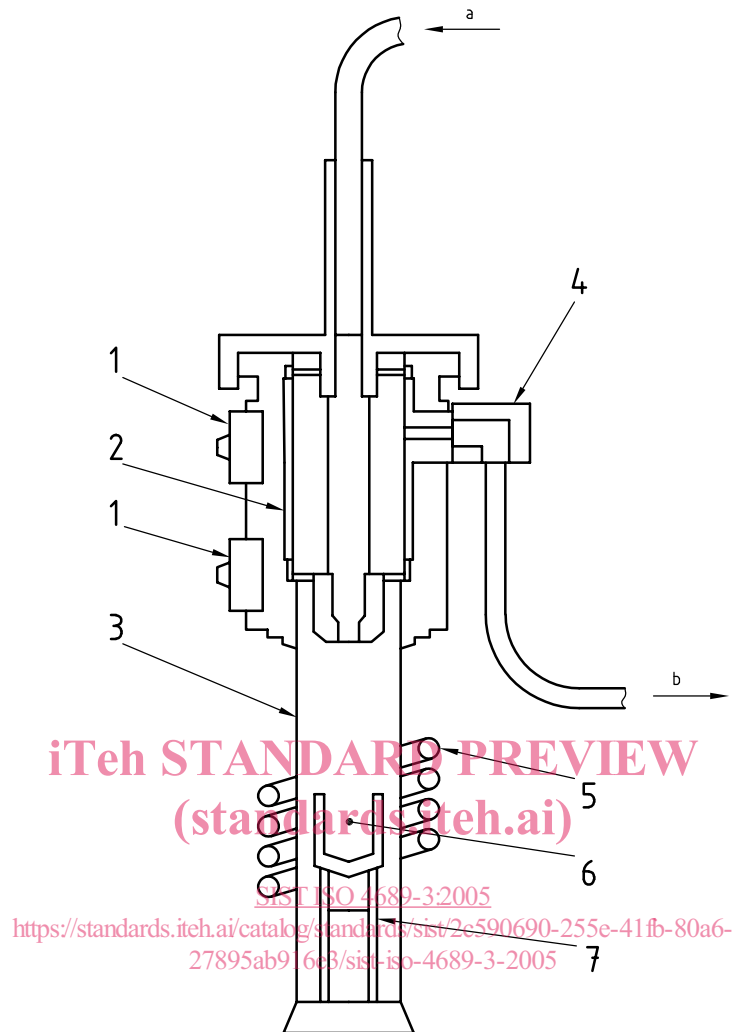

Key

- 1 metal filter
- 2 heating device
- 3 quartz combustion tube
- 4 dust trap
- 5 high-frequency induction coil
- 6 crucible
- 7 holder

a Oxygen.

b Combustion gas.

Figure 1 — Example of combustion furnace with combustion gas-refining section

5.7 Tin capsule.

The following dimensions may be used as guidelines.


Combustion tube		Combustion crucible		Tin capsule	
Length	140 mm to 220 mm	Height	26 mm	Diameter	6 mm
Outer diameter	30 mm to 44 mm	Internal diameter	10 mm	Height	18 mm
Inner diameter	26 mm to 37 mm	Outer diameter	26 mm	Mass	0,3 g
				Volume	0,4 ml

5.8 Metal filter.

5.9 Dust trap, containing glass wool.

5.10 Detector for infrared absorption, an example of which is shown in Figure 2.

5.11 Micro-pipette, 100 µl capacity, accurate to 1 µl.

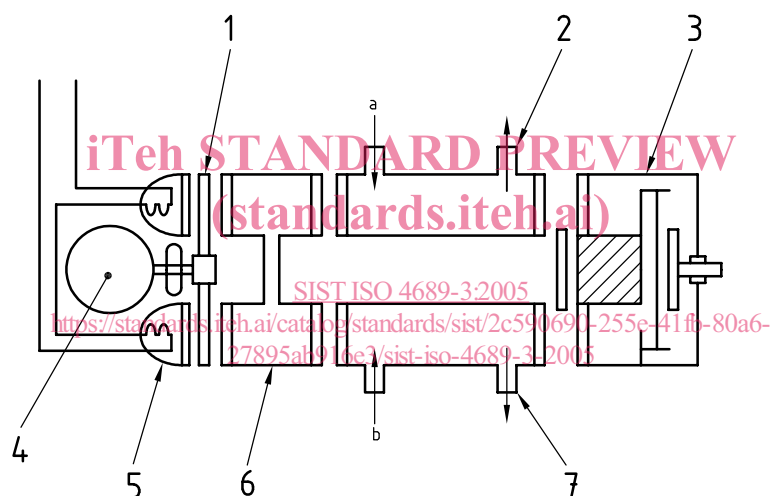

- Key**
- 1 chopper
 - 2 measuring cell
 - 3 infrared detector
 - 4 motor
 - 5 infrared source
 - 6 filter cell
 - 7 reference cell
 - a Combustion gas.
 - b Oxygen.

Figure 2 — Example of an infrared detection system

6 Sampling and samples

6.1 Laboratory sample

For analysis, use a laboratory sample of $-100\ \mu\text{m}$ particle size which has been taken and prepared in accordance with ISO 3082. In the case of ores having significant contents of combined water or oxidizable compounds, use a particle size of $-160\ \mu\text{m}$.

NOTE A guideline on significant contents of combined water and oxidizable compounds is incorporated in ISO 7764.

6.2 Preparation of predried test samples

Thoroughly mix the laboratory sample and, taking multiple increments, extract a test sample in such a manner that it is representative of the entire contents of the container. Dry the test sample at $105\ ^\circ\text{C} \pm 2\ ^\circ\text{C}$ as specified in ISO 7764. This is the predried test sample.

7 Procedure

7.1 Number of determinations

Carry out the analysis at least in duplicate in accordance with Annex A, independently, on one predried test sample.

NOTE The expression "independently" means that the second and any subsequent result is not affected by the previous result(s). For this particular analytical method, this condition implies that the repetition of the procedure is carried out either by the same operator at a different time or by a different operator, including in either case, appropriate recalibration.

7.2 Test portion

Taking several increments, weigh, to the nearest 0,000 2 g, approximately 0,5 g of the predried test sample obtained in accordance with 6.2. For samples containing in excess of 0,1 % (mass fraction) sulfur, 0,2 g should be taken.

NOTE The test portion should be taken and weighed quickly to avoid re-absorption of moisture.

7.3 Blank test and check test

In each run, one blank test and one analysis of a certified reference material of the same type of ore shall be carried out in parallel with the analysis of the ore sample(s) under the same conditions. A predried test sample of the certified reference material shall be prepared as specified in 6.2.

NOTE The certified reference material should be of the same type as the sample to be analysed and the properties of the two materials should be sufficiently similar to ensure that in either case no significant changes in the analytical procedure will become necessary.

Where the analysis is carried out on several samples at the same time, the blank value may be represented by one test, provided that the procedure is the same and the reagents are from the same reagent bottles.

Where the analysis is carried out on several samples of the same type of ore at the same time, the analytical value of one certified reference material may be used.

7.4 Determination

Connect the furnace (5.4) with components (5.1), (5.2), (5.3), (5.5), (5.8), (5.9) and (5.10) and switch on the power. Set the condition for heating in accordance with manufacturer's instructions after stabilization of the apparatus.