

---

---

**Optics and photonics — Lasers and  
laser-related equipment — Measurement  
of phase retardation of optical  
components for polarized laser radiation**

*Optique et photonique — Lasers et équipements associés aux lasers —  
Mesurage du retard de phase des composants optiques pour le  
rayonnement laser polarisé.*

iTeh STANDARD PREVIEW  
(standards.iteh.ai)

ISO 24013:2006

<https://standards.iteh.ai/catalog/standards/sist/263e0c12-1f09-4309-9aa5-4b65da3cfc7/iso-24013-2006>



**PDF disclaimer**

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

ISO 24013:2006

<https://standards.iteh.ai/catalog/standards/sist/263e0c12-1f09-4309-9aa5-4b65da3cfc7/iso-24013-2006>

© ISO 2006

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Case postale 56 • CH-1211 Geneva 20  
Tel. + 41 22 749 01 11  
Fax + 41 22 749 09 47  
E-mail [copyright@iso.org](mailto:copyright@iso.org)  
Web [www.iso.org](http://www.iso.org)

Published in Switzerland

## Contents

Page

Foreword.....	iv
Introduction .....	v
1 Scope .....	1
2 Normative references .....	1
3 Terms and definitions .....	1
4 Symbols and abbreviated terms .....	1
5 Measurement principle.....	2
6 Preparation of test sample and measuring arrangement.....	3
6.1 General.....	3
6.2 Laser beam preparation .....	3
6.3 Sample adjustment and system calibration.....	3
6.4 Detection system .....	4
7 Test procedure .....	5
7.1 Test procedure for zero phase retardation .....	5
7.2 Test procedure for $\pi/2$ phase retardation.....	5
8 Evaluation.....	6
8.1 General.....	6
8.2 Evaluation for zero phase retardation.....	6
8.3 Evaluation for $\pi/2$ phase retardation.....	6
9 Test report .....	6
Annex A (informative) Theoretical background .....	8
Bibliography .....	15

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 24013 was prepared by Technical Committee ISO/TC 172, *Optics and photonics*, Subcommittee SC 9, *Electro-optical systems*.

## iTeh STANDARD PREVIEW (standards.iteh.ai)

ISO 24013:2006

<https://standards.iteh.ai/catalog/standards/sist/263e0c12-1f09-4309-9aa5-4b65da3cfec7/iso-24013-2006>

## Introduction

Normally it is desirable that the state of polarization be not influenced by the optical components used. For the generation or maintenance of specific states of polarization the influence of optical components on the beam polarization is crucial. For generating circularly polarized radiation from linearly polarized radiation  $\pi/2$  phase retarders are used.

This International Standard describes methods to determine the relative phase retardation of optical components with respect to the x- and y-axes of the polarization and s- and p-polarization, respectively. This International Standard is necessary for optics manufacturers, suppliers and customers of such optics for the determination of the influence of phase retardation of optical components.

## iTeh STANDARD PREVIEW (standards.iteh.ai)

[ISO 24013:2006](https://standards.iteh.ai/catalog/standards/sist/263e0c12-1f09-4309-9aa5-4b65da3cfc7/iso-24013-2006)

<https://standards.iteh.ai/catalog/standards/sist/263e0c12-1f09-4309-9aa5-4b65da3cfc7/iso-24013-2006>

**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

ISO 24013:2006

<https://standards.iteh.ai/catalog/standards/sist/263e0c12-1f09-4309-9aa5-4b65da3cfc7/iso-24013-2006>

# Optics and photonics — Lasers and laser-related equipment — Measurement of phase retardation of optical components for polarized laser radiation

## 1 Scope

This International Standard specifies test methods for the determination of the optical phase retardation of optical components by polarized laser beams.

## 2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 11145, *Optics and photonics — Lasers and laser-related equipment — Vocabulary and symbols*

ISO 12005, *Lasers and laser-related equipment — Test methods for laser beam parameters — Polarization*

ISO 14644-1:1999, *Cleanrooms and associated controlled environments — Part 1: Classification of air cleanliness*

## 3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 11145 and ISO 12005 apply.

## 4 Symbols and abbreviated terms

Symbols used and units of measure

Symbol	Unit	Term
$\rho$	1	degree of linear polarization
$\phi$	rad	angle of analyser
$a_1$	V/m	amplitude of electric field in x-direction
$a_2$	V/m	amplitude of electric field in y-direction
a, b	V/m	principal axes of the vibrational ellipse
$\delta$	rad	phase difference
$\Delta\delta$	rad	phase retardation
$E$	V/m	electric field vector
$\alpha_x$	1	absorptance in x-direction
$\alpha_y$	1	absorptance in y-direction
$\psi$	rad	angle of the principle axis of the vibrational ellipse


## 5 Measurement principle

The optical component under test is irradiated by a laser beam with a defined state of polarization. After passing the component the state of polarization of the beam is determined by using an analyser. The phase retardation is then evaluated from the change of the state of polarization.


There are two cases to distinguish:

- a) the expected phase retardation is near zero: in this case a circularly polarized beam shall be used for the test;
- b) the expected phase retardation is near  $\pi/2$ : in this case a linearly polarized beam shall be used for the test.

Figure 1 shows the measuring set up.

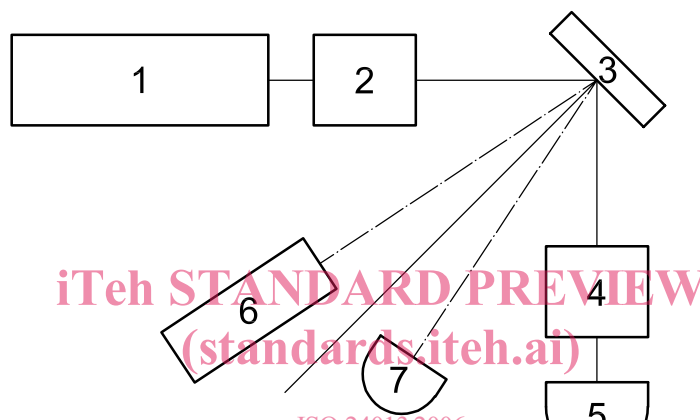

a) Optical path for reflective samples

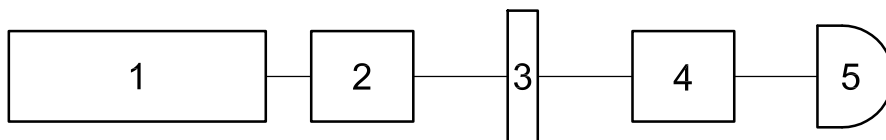

b) Optical path for transmissive samples

### Key

- 1 laser
- 2 polarizer (linear or circular)
- 3 sample under test
- 4 analyser
- 5 detector
- 6 alignment laser
- 7 positional sensitive detector

Figure 1 — Schematic drawing of the measuring set up



A laser and a polarizer generating linearly or circularly polarized radiation shall be used in combination with an analyser and a power detector. For measuring reflective samples an alignment laser in combination with a positional sensitive detector ensures a reproducible angle alignment of the sample under test.

## 6 Preparation of test sample and measuring arrangement

### 6.1 General

Storage, cleaning and the preparation of the test samples are carried out in accordance with the manufacturer's instructions for normal use.

The environment of the testing place consists of dust-free filtered air with less than 60 % relative humidity. The residual dust is reduced in accordance with, for example, the clean-room ISO class 7 as defined in ISO 14644-1:1999.

A linearly polarized laser shall be used as the radiation source. To keep errors as low as possible, the beam power stability should be as high as possible.

Wavelength, angle of incidence and state of polarization of the laser radiation used for the measurement shall correspond to the values specified by the manufacturer for the use of the test sample. If ranges are accepted for these three quantities, any combination of wavelength, angle of incidence and state of polarization may be chosen from these ranges.

### 6.2 Laser beam preparation

The accuracy of the measurement is strongly influenced by a clear definition of the state of polarization of the laser beam. Therefore it is necessary to prepare the polarization state of the probe beam (linearly or circularly) carefully.

If the expected phase retardation is near  $\pi/2$ , a linearly polarized beam shall be used. The quantity  $(1 - \rho)$ , where  $\rho$  is the degree of linear polarization, shall be less than  $10^{-3}$ . This shall be verified by using the analyser without the sample in the beam path.

NOTE 1 Such a state of polarization can be achieved by using a linearly polarized laser beam in combination with additional polarizing elements.

If the expected phase retardation is near zero, a circularly polarized beam shall be used. The degree of linear polarization  $\rho$  shall be less than  $10^{-3}$ . This shall be verified by using the analyser without the sample in the beam path.

NOTE 2 Such a state of polarization can be achieved by using a linearly polarized laser beam in combination with additional linearly polarizing elements and a  $\pi/2$  phase retarding element.

All optical elements shall not increase the quantity  $(1 - \rho)$  in the case of a linearly polarized beam and  $\rho$  in the case of a circularly polarized beam, by more than  $10^{-3}$ . For this reason the use of folding mirrors in the test setup is discouraged and all other optical elements shall be used under normal incidence.

### 6.3 Sample adjustment and system calibration

#### 6.3.1 Reflective samples

The sample shall be mounted very accurately at the angle of incidence according to the manufacturer's specification. The deviation from the intended angle of use shall be less than 2 mrad. For this purpose the component shall be mounted on a precision rotary stage. Back reflecting the laser beam into the laser cavity defines the normal incidence.

Additionally, in the case of a linearly polarized probe beam, the angle between the plane of vibration of the incoming laser beam and the plane of incidence shall be  $(\pi/4 \pm 2)$  mrad.

### 6.3.2 Possible alignment procedure

First, the laser beam shall be adjusted so that the beam propagation is parallel to the surface of the optical table. Second, the beam reflected from the sample shall be adjusted so that the propagation of the reflected beam is also parallel to the surface of the optical table for all angles of incidence. Third, in case of a linearly polarized incoming beam, the angle between the plane of vibration and the plane of the optical table shall be adjusted to be  $\pi/4$ . This can be achieved by adjusting the linear polarizer initially so that the plane of vibration is parallel to the optical table. This can be checked by using a Brewster window, the turning axis of which is perpendicular to the optical table. If under these conditions the reflected minimum power is propagating parallel to the optical table, then turning of the linear polarizer by  $\pi/4$  finally provides the desired angle of the linearly polarized beam.

When the alignment has been calibrated according to the procedure described above, the correct alignment of the additional samples can be simplified by using an additional laser with high pointing stability and a positional sensitive detector (see Figure 1). In this case the additional laser beam hits the component under near-normal incidence and the adjustment of the sample under test is performed so that the reflected laser beam hits the positional sensitive detector at the same position.

### 6.3.3 Transmissive samples

The sample shall be mounted under the angle of incidence according to the manufacturer's specification. The deviation from the intended angle of use shall be less than 2 mrad.

## 6.4 Detection system

### 6.4.1 General

The detection system consists of a polarization analyser and a power detector.

### 6.4.2 Polarization analyser

To determine the state of polarization of the laser beam after passing the test sample a polarization analyser mounted on a rotary stage is necessary.

The analyser shall be capable of characterizing the state of polarization of the laser beam after passing across the additional polarizer with the specified accuracy (see 6.2).

### 6.4.3 Power detector

To ensure that the entire beam hits the detector area, the detector width should be at least twice the beam diameter.

A high dynamic range of the signal to noise ratio is required for the low noise detector since this directly influences the resolution. Furthermore, the detector characteristics shall be linear over a wide signal range since this directly influences the accuracy of the measurements.

NOTE Silicon detectors for the visible and near infrared spectral range as well as pyroelectric detectors for the infrared spectral range may meet these specifications.

## 7 Test procedure

### 7.1 Test procedure for zero phase retardation

#### 7.1.1 General

If the expected phase retardation is near zero, the polarization of the probe beam shall be circularly polarized. This shall be achieved by using a linearly polarized laser in combination with a quarter-wave plate or similar means. Before the test the state and the degree of this circular polarization shall be measured and recorded. The initial state of polarization is characterized by (see also Annex A).

$$\cos \delta = \frac{E^2(45^\circ) - E^2(135^\circ)}{2\sqrt{E^2(90^\circ)E^2(0^\circ)}} \quad (1)$$

where  $E^2$  is the detector signal magnitude.

#### 7.1.2 Simple test procedure for zero absorptance difference

In the case of no absorptance difference, it is sufficient to measure the detector signals at two analyser positions,  $45^\circ$  and  $135^\circ$ . The phase difference is then given by

$$\cos \delta = \frac{\frac{E^2(45^\circ)}{E^2(135^\circ)} - 1}{\frac{E^2(45^\circ)}{E^2(135^\circ)} + 1} \quad (2)$$

#### 7.1.3 Test procedure for non zero absorptance difference

If there is a difference in the absorptance for the two polarization components it is sufficient to measure the detector signal at four analyser positions,  $0^\circ$ ,  $45^\circ$ ,  $90^\circ$  and  $135^\circ$ . The phase difference is given by Equation (1).

The relative difference in the absorptance is then given by

$$\frac{E^2(90^\circ)}{E^2(0^\circ)} = \left(\frac{a_2}{a_1}\right)^2 \quad \frac{a_2}{a_1} = \sqrt{\frac{1 - \alpha_y}{1 - \alpha_x}} \quad (3)$$

## 7.2 Test procedure for $\pi/2$ phase retardation

#### 7.2.1 General

If the expected phase retardation is near  $\pi/2$ , the polarization of the probe beam shall be linear. Before the test, the state and the degree of this linear polarization shall be measured and recorded. The initial state of polarization is characterized by a curve fit to the function given by Equation (A.4).

#### 7.2.2 Simple test procedure for zero absorptance difference

In the case of no absorptance difference, it is sufficient to measure the detector signals at two analyser positions,  $45^\circ$  and  $135^\circ$ . The phase difference is then given by Equation (2).

#### 7.2.3 Test procedure for non zero absorptance difference

If there is a difference in the absorptance for the two polarization components it is sufficient to measure the detector signal at four analyser positions,  $0^\circ$ ,  $45^\circ$ ,  $90^\circ$  and  $135^\circ$ . The phase difference is given by Equation (1).