

---

---

**Acoustics — Reference zero for the  
calibration of audiometric equipment —**

Part 7:

**Reference threshold of hearing under  
free-field and diffuse-field listening  
conditions**

iTeh STANDARD PREVIEW

(standards.iteh.ai)

*Acoustique — Zéro de référence pour l'étalonnage d'équipements  
audiométriques —*

*Partie 7: Niveau liminaire de référence dans des conditions d'écoute en  
champ libre et en champ diffus*

[https://standards.iteh.ai/catalog/standards/sist/969890bc-1c59-4097-b925-  
ba3e8979c317/iso-389-7-2005](https://standards.iteh.ai/catalog/standards/sist/969890bc-1c59-4097-b925-ba3e8979c317/iso-389-7-2005)



**PDF disclaimer**

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

[ISO 389-7:2005](https://standards.iteh.ai/catalog/standards/sist/969890be-1c59-4097-b925-ba3e8979c317/iso-389-7-2005)

<https://standards.iteh.ai/catalog/standards/sist/969890be-1c59-4097-b925-ba3e8979c317/iso-389-7-2005>

© ISO 2005

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Case postale 56 • CH-1211 Geneva 20  
Tel. + 41 22 749 01 11  
Fax + 41 22 749 09 47  
E-mail [copyright@iso.org](mailto:copyright@iso.org)  
Web [www.iso.org](http://www.iso.org)

Published in Switzerland

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 389-7 was prepared by Technical Committee ISO/TC 43, *Acoustics*.

This second edition cancels and replaces the first edition (ISO 389-7:1996), which has been technically revised.

ISO 389 consists of the following parts, under the general title *Acoustics — Reference zero for the calibration of audiometric equipment*:

- (standards.iteh.ai)
- ISO 389-7:2005
- <https://standards.iteh.ai/catalog/standards/sist/969890be-1c59-4097-b925-ba3e8979c317/iso-389-7-2005>
- *Part 1: Reference equivalent threshold sound pressure levels for pure tones and supra-aural earphones*
  - *Part 2: Reference equivalent threshold sound pressure levels for pure tones and insert earphones*
  - *Part 3: Reference equivalent threshold force levels for pure tones and bone vibrators*
  - *Part 4: Reference levels for narrow-band masking noise*
  - *Part 5: Reference equivalent threshold sound pressure levels for pure tones in the frequency range 8 kHz to 16 kHz*
  - *Part 6: Reference hearing threshold levels for test signals of short duration*
  - *Part 7: Reference threshold of hearing under free-field and diffuse-field listening conditions*
  - *Part 8: Reference equivalent threshold sound pressure levels for pure tones and circumaural earphones*

## Introduction

In some audiological applications the test signals are delivered by means of loudspeakers, either in a free sound field or in a diffuse sound field. This part of ISO 389 specifies the reference zero for the calibration of audiometric equipment used for sound field audiometry. Corresponding audiometric test methods are specified in ISO 8253-1 and ISO 8253-2.

In common with other subjective phenomena, the threshold of hearing varies in detail from person to person but, for a group of otologically normal persons within a restricted age range, values for the central tendency can be determined to characterize the group. This and other parts of ISO 389 specify threshold data applicable to otologically normal persons in the age range from 18 years to 25 years.

The data specified in this part of ISO 389 relate to

- a) pure tones heard under conditions of binaural listening in free progressive plane waves with the subject directly facing the source of sound (frontal incidence), and with the sound pressure level measured in the free progressive wave at the centre position of the listener's head with the listener absent;
- b) one-third-octave bands of (white or pink) noise heard under conditions of binaural listening in a diffuse sound field with the sound pressure level measured in the sound field at the centre position of the listener's head with the listener absent.

For frequencies up to 8 kHz, each set of data may be equally applied to any other bands of (white or pink) noise for which the bandwidth is less than the critical bandwidth.

The data are based on an assessment of technical information provided by laboratories in different countries representing the most reliable data available at the time. For information, a note on the derivation of the reference values and the origin of the data is given in Annex A.

# Acoustics — Reference zero for the calibration of audiometric equipment —

## Part 7: Reference threshold of hearing under free-field and diffuse-field listening conditions

### 1 Scope

This part of ISO 389 specifies a reference threshold of hearing for the calibration of audiometric equipment used under the following conditions.

- a) The sound field in the absence of the listener consists of either a free progressive plane wave (free field) or a diffuse sound field, as specified in ISO 8253-2. In the case of a free field, the source of sound is directly in front of the listener (frontal incidence).
- b) The sound signals are pure (sinusoidal) tones in the case of free-field conditions and one-third octave bands of (white or pink) noise in the case of diffuse-field conditions.
- c) The sound pressure level is measured in the absence of the listener at the position where the centre of the listener's head would be.
- d) Listening is binaural.

NOTE 1 Correction values for the threshold of hearing under free-field listening conditions and selected angles of sound incidence (45° and 90°) deviating from frontal incidence are given in ISO 8253-2 for information.

NOTE 2 Other conditions are given in Bibliographic Reference [1].

The data are given in numerical form for the preferred frequencies in the one-third-octave series from 20 Hz to 16 000 Hz inclusive in accordance with ISO 266 and, in addition, for some intermediate audiometric frequencies up to 18 000 Hz.

It should be emphasized that the threshold data differ from the audiometric zero specified in ISO 389-1, ISO 389-2, ISO/TR 389-5 and ISO 389-8, since the latter refer to monaural listening through earphones with sound pressure levels referred to specified couplers and ear simulators. Direct comparison between the data in the parts of ISO 389 mentioned above and in this part of ISO 389 is therefore not appropriate.

### 2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 8253-2, *Acoustics — Audiometric test methods — Part 2: Sound field audiometry with pure tone and narrow-band test signals*

### 3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

#### 3.1 threshold of hearing

level of a sound at which, under specified conditions, a person gives 50 % of correct detection responses on repeated trials

NOTE The results of threshold determination depend to a certain degree on the test procedure used. The data presented in the ISO 389 series are all based on the use of the threshold test procedures defined in ISO 8253-1. When a test procedure with other characteristics is used, differences of up to several decibels on average may be expected.

#### 3.2 otologically normal person

person in a normal state of health who is free from all signs or symptoms of ear disease and from obstructing wax in the ear canals, and who has no history of undue exposure to noise, exposure to potentially ototoxic drugs, or familial hearing loss

#### 3.3 reference threshold of hearing

at a specified frequency, the sound pressure level of a pure tone or a one-third-octave band of noise corresponding to the median value of the binaural thresholds of hearing of otologically normal persons within the age limits from 18 years to 25 years inclusive

#### 3.4 free sound field

sound field where the boundaries of the room exert a negligible effect on the sound waves

#### 3.5 diffuse sound field

sound field consisting of sound waves arriving at a given location more or less simultaneously from all directions with equal probability and level

iTeh STANDARD PREVIEW  
(standards.it-eh.at)

ISO 389-7:2005

<https://standards.it-eh.at/catalog/standards/sist/969890be-1c59-4097-b925-ba3e8979c317/iso-389-7-2005>


### 4 Specification

The reference thresholds of hearing for the listening conditions specified in Clause 1 are given in Table 1. This table also gives the differences between sound pressure levels of one-third-octave bands of noise in a diffuse sound field and the sound pressure levels of pure tones in a frontally incident free progressive wave for equal thresholds of hearing. A graphical illustration of the reference thresholds of hearing is given in Figure 1.

**Table 1 — Reference thresholds of hearing for the listening conditions specified in Clause 1 and differences between sound pressure levels in the two types of sound field**

Frequency <i>f</i> Hz	Reference threshold of hearing under the condition of		Difference $\Delta L = T_f - T'_f$ dB
	free-field listening (frontal incidence) $T_f$ (ref. 20 $\mu$ Pa) dB	diffuse-field listening $T'_f$ (ref. 20 $\mu$ Pa) dB	
20	78,5 <sup>a</sup>	78,5	0
25	68,7	68,7	0
31,5	59,5	59,5	0
40	51,1	51,1	0
50	44,0	44,0	0
63	37,5	37,5	0
80	31,5	31,5	0
100	26,5	26,5	0
125	22,1	22,1	0
160	17,9	17,9	0
200	14,4	14,4	0
250	11,4	11,4	0
315	8,6	8,4	0,2
400	6,2	5,8	0,4
500	4,4	3,8	0,6
630	3,0	2,1	0,9
750	2,4	1,2	1,2
800	2,2	1,0	1,2
1 000	2,4	0,8	1,6
1 250	3,5	1,9	1,6
1 500	2,4	1,0	1,4
1 600	1,7	0,5	1,2
2 000	-1,3	-1,5	0,2
2 500	-4,2	-3,1	-1,1
3 000	-5,8	-4,0	-1,8
3 150	-6,0	-4,0	-2,0
4 000	-5,4	-3,8	-1,6
5 000	-1,5	-1,8	0,3
6 000	4,3	1,4	2,9
6 300	6,0	2,5	3,5
8 000	12,6	6,8	5,8
9 000	13,9	8,4	5,5
10 000	13,9	9,8	4,1
11 200	13,0	11,5	1,5
12 500	12,3	14,4	-2,1
14 000	18,4	23,2	-4,8
16 000	40,2	43,7	-3,5 <sup>a</sup>
18 000	73,2 <sup>a</sup>	—	—

<sup>a</sup> At 20 Hz and 18 000 Hz, experimental data for  $T_f$  and at 16 000 Hz experimental data for  $\Delta L$ , respectively, were reported from one laboratory only.

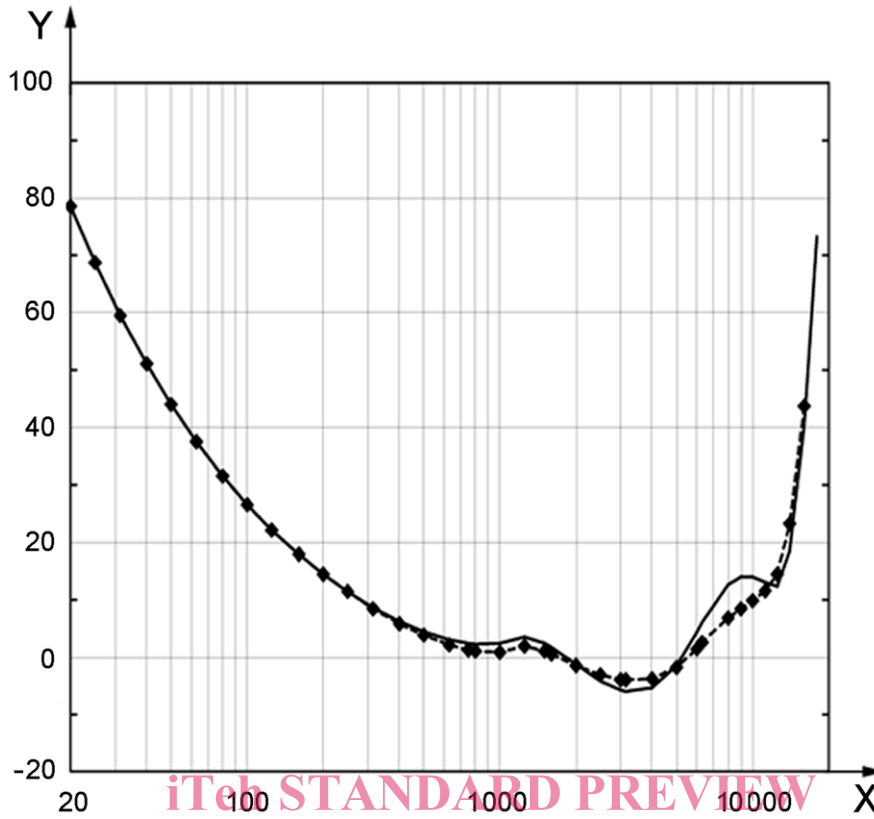

**Key**

X frequency, Hz  
 Y sound pressure level, dB

— free field  
 ---◆--- diffuse field

ISO 389-7:2005  
<https://standards.itech.ai/catalog/standards/sist/969890be-1c59-4097-b925-ba3e8979c317/iso-389-7-2005>

**Figure 1 — Reference thresholds of hearing for pure tones under binaural free-field listening conditions (frontal incidence) and for one-third-octave bands of noise under binaural diffuse-field listening conditions**

NOTE Contrary to other parts of ISO 389, the reference thresholds of hearing in Table 1 are given with a resolution of 0,1 dB. The reason is that the reference threshold of hearing for free-field listening was taken together with this resolution from ISO 226 in order to avoid having two standards containing free-field thresholds with different resolutions.




## Annex A (informative)

### Notes on the derivation of the reference thresholds of hearing

#### A.1 Under free-field listening conditions

From 20 Hz to 12 500 Hz, the reference thresholds of hearing under free-field listening conditions specified in this part of ISO 389 are taken from ISO 226. The values for the nine additional audiometric frequencies between 750 Hz and 18 000 Hz have been determined using the same fitting process as for the other threshold data given in ISO 226, using the 15 literature references given in that International Standard (see Figure A.1 below).

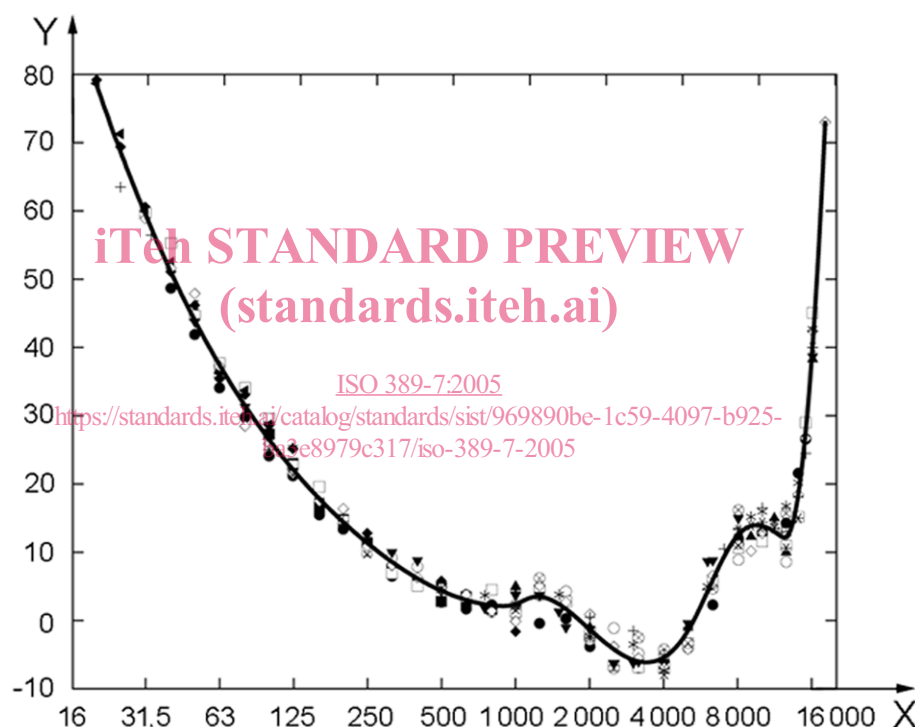

#### Key

X frequency, Hz

Y sound pressure level, dB

+ Robinson and Dadson (1956)

⋈ Teranishi (1965)

× Brinkmann (1973)

● Betke and Mellert (1989)

○ Suzuki et al. (1989)

■ Fastl et al. (1990)

◆ Watanabe and Møller (1990)

\* Vorländer (1991)

▲ Poulsen and Thøgersen (1994)

□ Takeshima et al. (1994)

▼ Lydolf and Møller (1997)

◀ Lydolf and Møller (1997) PF

\* Poulsen and Han (2000)

◇ Takeshima et al. (2001)

⊗ Takeshima et al. (2002)

**Figure A.1 — Experimental data used for the derivation of the reference thresholds of hearing under free-field listening conditions and the calculated curve giving best fit to these data**