



**SLOVENSKI STANDARD**  
**kSIST FprEN ISO 15548-1:2013**  
**01-november-2013**

---

**Neporušitveno preskušanje - Oprema za preskušanje z vrtinčnimi tokovi - 1. del:  
Značilnosti aparatov in preverjanje (ISO/FDIS 15548-1:2013)**

Non-destructive testing - Equipment for eddy current examination - Part 1: Instrument characteristics and verification (ISO/FDIS 15548-1:2013)

Zerstörungsfreie Prüfung - Technische Ausrüstung für die Wirbelstromprüfung - Teil 1:  
Kenngrößen von Prüfgeräten und deren Verifizierung (ISO/FDIS 15548-1:2013)

Essais non destructifs - Appareillage pour examen par courants de Foucault - Partie 1:  
Caractéristiques de l'appareil et vérifications (ISO/FDIS 15548-1:2013)

**Ta slovenski standard je istoveten z: FprEN ISO 15548-1**

---

**ICS:**

19.100          Neporušitveno preskušanje          Non-destructive testing

**kSIST FprEN ISO 15548-1:2013**          **en,fr,de**



FINAL  
DRAFTINTERNATIONAL  
STANDARDISO/FDIS  
15548-1

ISO/TC 135/SC 4

Secretariat: AFNOR

Voting begins on:  
2013-07-11Voting terminates on:  
2013-09-11**Non-destructive testing — Equipment  
for eddy current examination —****Part 1:  
Instrument characteristics and  
verification**

*Essais non destructifs — Appareillage pour examen par courants  
de Foucault —*  
*Partie 1: Caractéristiques de l'appareil et vérifications*

SIST EN ISO 15548-1:2014

<https://standards.iteh.ai/catalog/standards/sist/c23f487c-708e-4816-a67a-c6743ff2a706/sist-en-iso-15548-1-2014>

Please see the administrative notes on page iii

RECIPIENTS OF THIS DRAFT ARE INVITED TO SUBMIT, WITH THEIR COMMENTS, NOTIFICATION OF ANY RELEVANT PATENT RIGHTS OF WHICH THEY ARE AWARE AND TO PROVIDE SUPPORTING DOCUMENTATION.

IN ADDITION TO THEIR EVALUATION AS BEING ACCEPTABLE FOR INDUSTRIAL, TECHNOLOGICAL, COMMERCIAL AND USER PURPOSES, DRAFT INTERNATIONAL STANDARDS MAY ON OCCASION HAVE TO BE CONSIDERED IN THE LIGHT OF THEIR POTENTIAL TO BECOME STANDARDS TO WHICH REFERENCE MAY BE MADE IN NATIONAL REGULATIONS.



Reference number  
ISO/FDIS 15548-1:2013(E)

© ISO 2013

iTeh STANDARD PREVIEW  
(standards.iteh.ai)

SIST EN ISO 15548-1:2014

<https://standards.iteh.ai/catalog/standards/sist/c23f487c-708e-4816-a67a-c6743ff2a706/sist-en-iso-15548-1-2014>



**COPYRIGHT PROTECTED DOCUMENT**

© ISO 2013

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Case postale 56 • CH-1211 Geneva 20  
Tel. + 41 22 749 01 11  
Fax + 41 22 749 09 47  
E-mail [copyright@iso.org](mailto:copyright@iso.org)  
Web [www.iso.org](http://www.iso.org)

Published in Switzerland

## ISO/CEN PARALLEL PROCESSING

This final draft has been developed within the International Organization for Standardization (ISO), and processed under the **ISO-lead** mode of collaboration as defined in the Vienna Agreement. The final draft was established on the basis of comments received during a parallel enquiry on the draft.

This final draft is hereby submitted to the ISO member bodies and to the CEN member bodies for a parallel two-month approval vote in ISO and formal vote in CEN.

**Positive votes shall not be accompanied by comments.**

**Negative votes shall be accompanied by the relevant technical reasons.**

## iTeh STANDARD PREVIEW (standards.iteh.ai)

[SIST EN ISO 15548-1:2014](https://standards.iteh.ai/catalog/standards/sist/c23f487c-708e-4816-a67a-c6743ff2a706/sist-en-iso-15548-1-2014)

<https://standards.iteh.ai/catalog/standards/sist/c23f487c-708e-4816-a67a-c6743ff2a706/sist-en-iso-15548-1-2014>

## ISO/FDIS 15548-1:2013(E)

## Contents

Page

Foreword .....	v
<b>1 Scope</b> .....	<b>1</b>
<b>2 Normative references</b> .....	<b>1</b>
<b>3 Terms and definitions</b> .....	<b>1</b>
<b>4 Eddy current instrument characteristics</b> .....	<b>1</b>
4.1 General characteristics .....	1
4.2 Electrical characteristics .....	2
<b>5 Verification</b> .....	<b>7</b>
5.1 General .....	7
5.2 Levels of verification .....	7
5.3 Verification procedure .....	8
5.4 Corrective actions .....	8
<b>6 Measurement of electrical characteristics of instrument</b> .....	<b>8</b>
6.1 Measuring requirements .....	8
6.2 Generator unit .....	9
6.3 Input stage characteristics .....	12
6.4 Signal processing .....	14
6.5 Output .....	23
6.6 Digitisation .....	23
<b>Annex A (informative) Principle of frequency beat method</b> .....	<b>24</b>
<b>Annex B (informative) Method of measurement of linearity range between output and input</b> .....	<b>26</b>
<b>Annex C (normative) Alternative measurement of the input impedance</b> .....	<b>27</b>

SIST EN ISO 15548-1:2014

<https://standards.iteh.ai/catalog/standards/sist/c23f487c-708e-4816-a67a-c6743ff2a706/sist-en-iso-15548-1-2014>

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2. [www.iso.org/directives](http://www.iso.org/directives)

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received. [www.iso.org/patents](http://www.iso.org/patents)

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

The committee responsible for this document is ISO/TC 135, *Non-destructive Testing*, Subcommittee SC 4, *Eddy current methods*.

This second edition cancels and replaces the first edition (ISO 15548-1:2008), of which it constitutes a minor revision. It also incorporates the Correction ISO 15548-1:2008/Cor 1:2010.

ISO 15548 consists of the following parts, under the general title *Non-destructive testing — Equipment for eddy current examination*:

- *Part 1: Instrument characteristics and verification*
- *Part 2: Probe characteristics and verification*
- *Part 3: System characteristics and verification*





# Non-destructive testing — Equipment for eddy current examination —

## Part 1: Instrument characteristics and verification

### 1 Scope

This part of ISO 15548 identifies the functional characteristics of a general-purpose eddy current instrument and provides methods for their measurement and verification.

The evaluation of these characteristics permits a well-defined description and comparability of eddy current equipment.

By careful choice of the characteristics, a consistent and effective eddy current examination system can be designed for a specific application.

Where accessories are used, these are characterised using the principles of this part of ISO 15548.

This part of ISO 15548 gives neither the extent of verification nor acceptance criteria for the characteristics. They are given in the application documents.

### 2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 12718, *Non-destructive testing — Eddy current testing — Vocabulary*

ISO 15549, *Non-destructive testing — Eddy current testing — General principles*

### 3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 12718 apply.

## 4 Eddy current instrument characteristics

### 4.1 General characteristics

#### 4.1.1 Type of instrument

- a) An instrument has a general-purpose application when the relationship between the measured quantity and the display or output is established by the user. A range of probes can be connected to the instrument. The instrument manufacturer shall provide details of the internal electrical characteristics, in order that the user can design the examination system. The examination system shall be in accordance with ISO 15549. The user shall be able to vary the value of frequency, gain, balance (unless an automatic balance is used), phase, filters and gain and zero of the display.

## ISO/FDIS 15548-1:2013(E)

- b) An instrument is of specific application when the relationship between the measured quantity and the display or output is explicitly defined in the range of application. The probe is specific to the instrument. For this type of instrument, this part of ISO 15548 may be partially applied.

### 4.1.2 Power supply

The instrument can be powered by batteries or by the local AC power supply. The nominal values of voltage, frequency and power consumption shall be stated, together with the tolerance for correct operation.

### 4.1.3 Safety

The instrument and its accessories shall meet the applicable safety regulations, for example, electrical hazard, surface temperature, explosion, etc.

### 4.1.4 Technology

The instrument can be wholly analogue or partly analogue and partly digital.

The excitation can be single frequency, multifrequency, swept frequency or pulsed.

The instrument can be single or multichannel.

The instrument settings can be manual, remote controlled, stored or preset.

The instrument shall have component outputs and can be with or without a self-contained display.

### 4.1.5 Physical presentation

The instrument can be portable, cased or rack mounted, with the component parts integrated or modular.

The weight and size shall be specified for the instrument and its accessories.

The plugs and sockets shall be specified regarding type and pin interconnections.

The instrument model number and the serial number shall be clearly readable and located in a readily accessible place.

### 4.1.6 Environmental effects

The warm-up time necessary for the instrument to reach stable operating conditions within specified limits shall be stated.

The temperature, humidity and vibration ranges for normal use, storage and transport shall be specified for the instrument and its accessories.

The instrument shall conform to relevant electromagnetic compatibility (EMC) regulations.

## 4.2 Electrical characteristics

### 4.2.1 General

The electrical characteristics of an instrument shall be evaluated after the warm-up time has elapsed.


The electrical characteristics are only valid for the stated operating conditions.

When relevant, the stability of the specified values with time, for specified environmental conditions, shall be stated.

The electrical characteristics apply to various items of the functional block diagram of the instrument. Where applicable, they are provided by the manufacturer. Some of these characteristics can be verified according to the methodology described in [Clause 6](#).

#### 4.2.2 Functional block diagram

The functional block diagram of a typical general-purpose eddy current instrument is shown in [Figure 1](#).

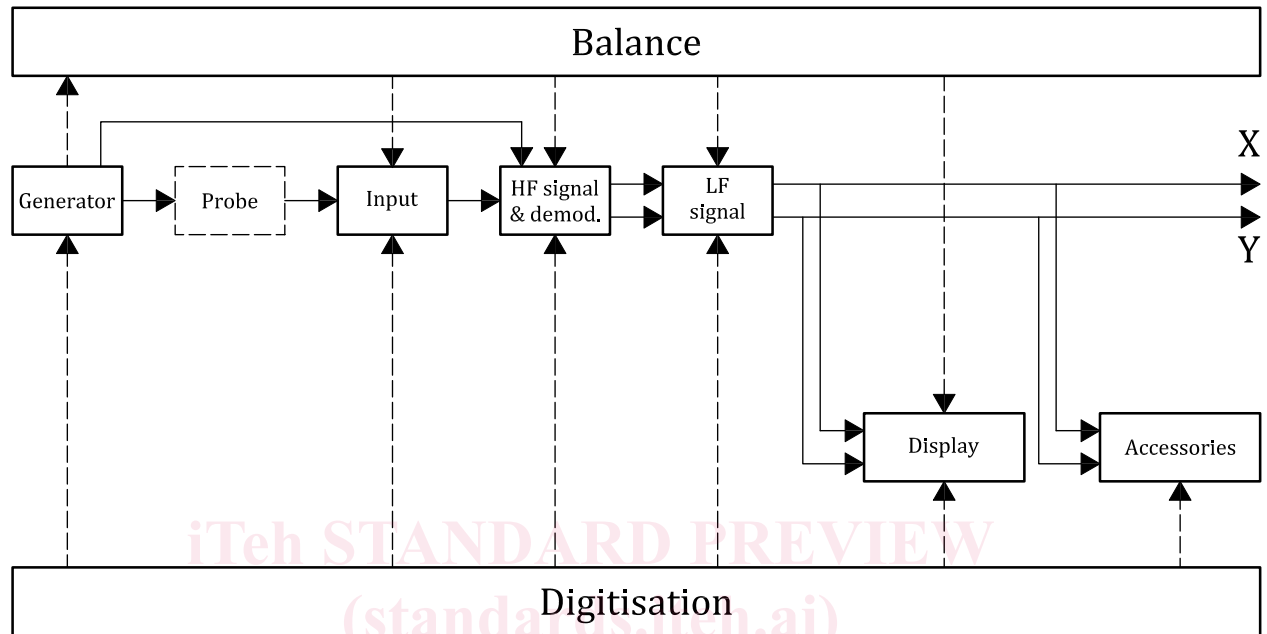

**Figure 1 — Functional block diagram of eddy current instrument**

#### 4.2.3 Generator unit

The source of excitation is the generator unit.

In the case of alternating excitation (sinusoidal, triangular, rectangular, etc.), the characteristics to be defined are as follows:

- type of generator: current or voltage;
- type of excitation: single or multifrequency;
- frequency setting: range, step size, deviation from nominal value;
- harmonic distortion;
- amplitude setting: range, step size, deviation from nominal value, maximum output voltage or current;
- source impedance with frequency dependence.

In the case of multifrequency excitation, it shall be stated whether frequencies are injected simultaneously or multiplexed, independent or related, and the multiplexing sequence shall be specified, when relevant.

#### 4.2.4 Input stage characteristics

The input stage interfaces the probe to the instrument. It provides impedance matching and amplification, as required.

## ISO/FDIS 15548-1:2013(E)

The characteristics to be defined are as follows:

- input impedance with frequency dependence;
- gain setting range, step size, deviation from nominal value;
- maximum input voltage;
- common-mode operating parameters, when relevant.

### 4.2.5 Balance

Balance is the compensation of the signal to achieve a predetermined operating point, e.g. zero. The compensation may be performed manually or automatically, at the input stage, or during HF signal processing, or during demodulated signal processing, or on the display.

The characteristics to be defined are as follows:

- maximum input range, which can be compensated;
- residual value at balance (expressed as a percentage of a specified range, e.g. full-scale output).

### 4.2.6 High-frequency signal processing

#### 4.2.6.1 HF filtering

Filters reduce the signal frequency content which can have an undesirable effect on the test result.

The filters used before demodulation are referred to as carrier frequency filters (HF filters). These are usually band-pass filters which suppress any signal frequencies which do not correspond to the excitation frequency.

The characteristics to be defined are as follows:

- gain;
- bandwidth at 3 dB attenuation;
- rate of attenuation;
- transient response.

#### 4.2.6.2 HF amplification

The characteristics to be defined are as follows:

- gain setting range, step size, deviation from nominal value;
- input signal range;
- bandwidth;
- output saturation level.

#### 4.2.6.3 Demodulation

Synchronous demodulation extracts the vector components from the HF signal.

For positive polarity of demodulation, a delay in the signal will cause the signal vector to rotate clockwise. The polarity of demodulation shall be positive and shall be confirmed.