



Designation: F 88 – 05

Standard Test Method for Seal Strength of Flexible Barrier Materials¹

This standard is issued under the fixed designation F 88; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This test method covers the measurement of the strength of seals in flexible barrier materials.

1.2 The test may be conducted on seals between a flexible material and a rigid material.

1.3 Seals tested in accordance with this test method may be from any source, laboratory or commercial.

1.4 This test method measures the force required to separate a test strip of material containing the seal. It also identifies the mode of specimen failure.

1.5 SI units are preferred. The values given in parentheses are for information only.

1.6 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 *ASTM Standards:*²

D 882 Test Method for Tensile Properties of Thin Plastic Sheeting

D 1898 Practice for Sampling of Plastics³

E 171 Specification for Atmospheres for Conditioning and Testing Flexible Barrier Materials

E 691 Practice for Conducting an Interlaboratory Study to Determine the Precision of a Test Method

3. Terminology

3.1 *Definitions:*

3.1.1 *average seal strength, n*—average force per unit width of seal required to separate progressively a flexible material from a rigid material or another flexible material, under the conditions of the test.

3.1.1.1 *Discussion*—The average force normally is calculated by the testing machine from the digitized plot of force versus grip travel. The plot starts from zero force after slack has been removed from the test strip. The initial ramp-up from zero to the force level required to peel the seal is not indicative of seal strength, and data from that part of the curve should not be included in the calculation of average strength, nor should the return to zero following complete failure of the specimen. The amount of data actually discarded on each end of the measured seal-profile curve must be the same for all tests within any set of comparisons of average seal strength (see 6.1.1 and 9.8.1).

3.1.2 *flexible, adj*—indicates a material with flexural strength and thickness permitting a turn back at an approximate 180 degree angle.

3.1.3 *maximum seal strength, n*—maximum force per unit width of seal required to separate progressively a flexible material from a rigid material or another flexible material, under the conditions of the test.

4. Significance and Use

4.1 Seal strength is a quantitative measure for use in process validation, process control and capability. Seal strength is not only relevant to opening force and package integrity, but to measuring the packaging processes' ability to produce consistent seals. Seal strength at some minimum level is a necessary package requirement, and at times it is desirable to limit the strength of the seal to facilitate opening.

4.1.1 The maximum seal force is important information, but for some applications, average force to open the seal may be useful, and in those cases also should be reported.

4.2 When a seal fails adhesively (peel seal) the value of the bond strength measured is reported. A cohesive failure of the bond, delamination, or failure elsewhere in the test strip indicates that the substrate, not the seal interface, would be the limiting factor in the strength of a package. In those cases seal strength may be reported as "no less than" the strength measured.

4.3 A portion of the force measured when testing materials may be a bending component and not seal strength alone. A number of fixtures and schemes have been devised to hold samples at various angles to the pull direction to control this bending force. Because the effect of each of these on test

¹ This test method is under the jurisdiction of ASTM Committee F02 on Flexible Barrier Materials and is the direct responsibility of Subcommittee F02.20 on Physical Properties.

Current edition approved April 1, 2005. Published April 2005. Originally approved in 1968. Last previous edition approved in 2000 as F 88 – 00.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

³ Withdrawn.

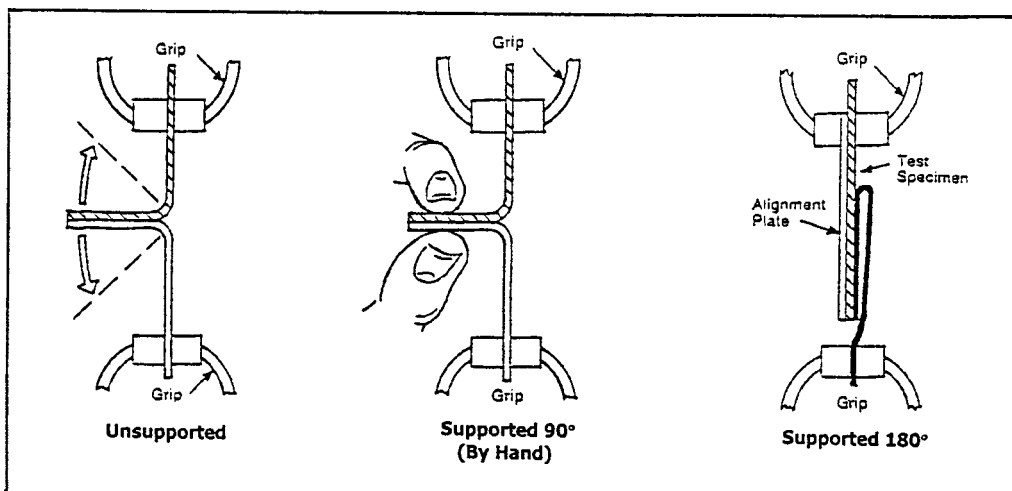


FIG. 1 Tail Holding Methods

results is varied, consistent use of one technique throughout a test series is recommended. Examples of fixtures and schemes are illustrated in Fig. 1.

5. Interferences

5.1 The value obtained for seal strength can be affected by properties of the specimen other than seal strength. These interferences are discussed in the annex.

6. Apparatus

6.1 *Tensile Testing Machine*—A testing machine of the constant rate-of-jaw-separation type. The machine shall be equipped with a weighing system that moves a maximum distance of 2 % of the specimen extension within the range being measured. The machine shall be equipped with a device for recording the tensile load and the amount of separation of the grips; both of these measuring systems shall be accurate to ±2 %. The rate of separation of the jaws shall be uniform and capable of adjustment from approximately 200 to 300 mm (8 to 12 in.)/min. The gripping system shall be capable of minimizing specimen slippage and applying an even stress distribution to the specimen.

6.1.1 If calculation of average seal strength is required, the testing machine system shall have the capability to calculate its value over a specified range of grip travel programmable by the operator. Preferably, the machine shall have the capability also to plot the curve of force versus grip travel.

6.2 *Specimen Cutter*, conforming to the requirements of 5.4 of Test Methods D 882, sized to cut specimens to a width of 25 mm (0.984 in.), 15 mm (0.591 in.), or 25.4 mm (1.00 in.). Tolerance shall be ±0.5 %.

7. Sampling

7.1 The number of test specimens shall be chosen to permit an adequate determination of representative performance. Practice D 1898 provides guidance for test specimen selection.

7.2 Testing of samples with visual defects or other deviations from normality may or may not be appropriate depending on the purpose of the investigation. Indiscriminate elimination of defects can bias results.

8. Aging and Conditioning

8.1 In the absence of information showing that heatseal strength stability of the materials under test is reached in shorter times, condition and test sealed materials in accordance with Specification E 171, with a minimum conditioning time of 40 h or longer if shown to be required to reach stability.

8.2 Heatseal conditioning periods may be shortened to times determined by experimentation as sufficient to achieve seal strength stability.

8.3 Modification of conditioning practices may be necessary to meet specific test objectives, such as the measurement of seal strength at specified storage or handling temperature.

9. Procedure

9.1 Calibrate the tensile machine in accordance with the manufacturer’s recommendations.

9.2 Prepare sealed test specimens for testing by cutting to the dimensions shown in Fig. 2. Edges shall be clean-cut and perpendicular to the direction of seal. Specimen legs may be shorter than shown, depending on the grip dimensions of the testing machine.

9.3 Clamp each leg of the test specimen in the tensile testing machine. The sealed area of the specimen shall be approximately equidistant between the grips. Recommended distance between grips (initial unconstrained specimen length) is:


Fin and Hot-Wire Seals		
Highly ^A extensible materials	10 mm	(0.39 in.)
Less ^A extensible materials	25 mm	(1.0 in.)
Lap Seals	X + 10 mm ^B	

^A Grip separation distance is recommended to be limited for highly extensible materials (100 + % elongation at seal failure) to minimize interferences (see annex).

^B Refer to Fig. 2 for definition of X.

9.4 Center the specimen laterally in the grips. Align the specimen in the grips so the seal line is perpendicular to the direction of pull, allowing sufficient slack so the seal is not stressed prior to initiation of the test.

9.5 A significant difference in measured seal strength has been shown to result, depending on the orientation of a fin-seal tail during the test. The test report should indicate the details of any method used to control tail orientation.

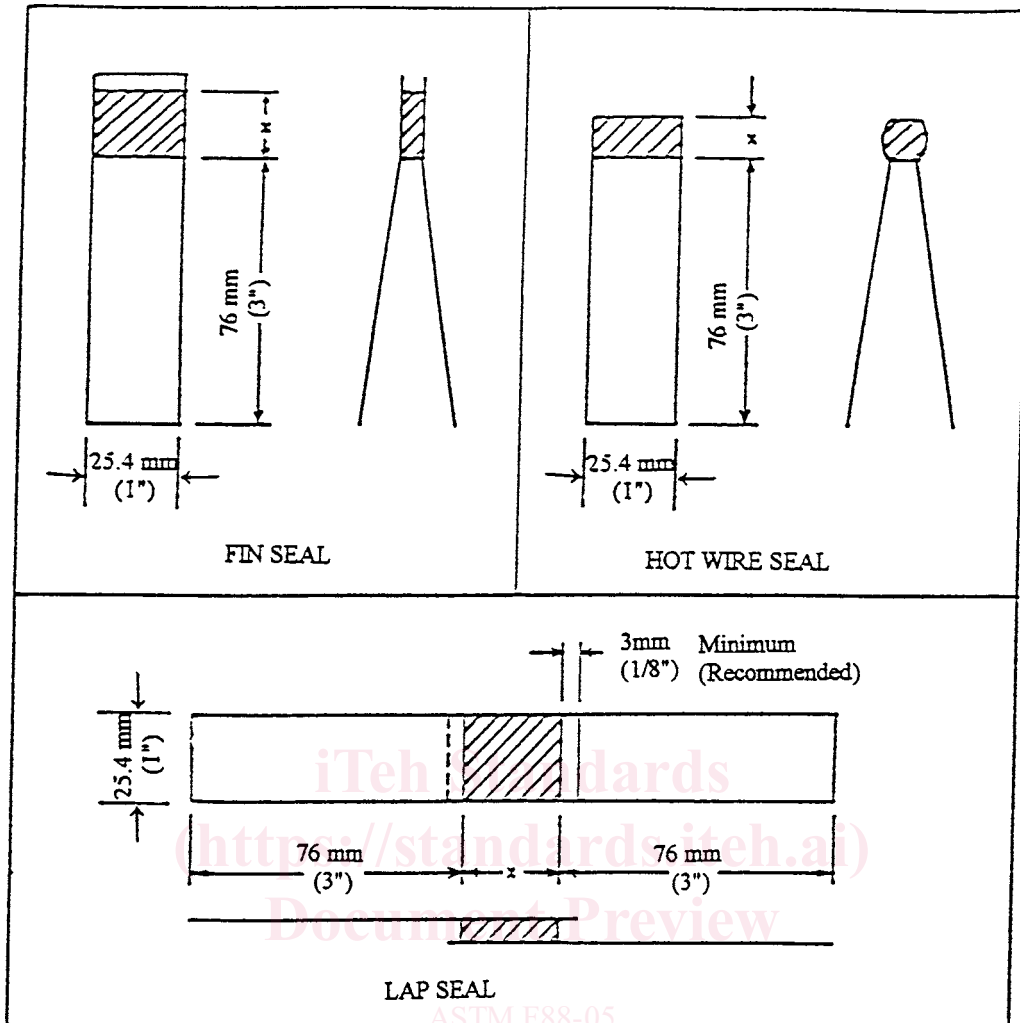

NOTE 1—Seal dimension marked X varies with sealer configuration.

FIG. 2 Recommended Specimen Dimensions

9.6 The seal shall be tested at a rate of grip separation of 200 to 300 mm/min. (8 to 12 ipm).

9.7 For each cycle, report the maximum force encountered as the specimen is stressed to failure and identify the mode of specimen failure.

9.8 If the test strip peels apart in the seal area, either by adhesive failure, cohesive failure, or delamination, the average peel force may be an important index of performance and should be measured by the testing machine as a part of the test cycle.

9.8.1 Follow the machine manufacturer's instructions to select the desired algorithm for calculating average seal strength. Fig. 3 illustrates the effect of an algorithm that uses data only from the central 80 % of the curve to calculate the average.

9.8.2 If the test strip does not peel significantly in the seal area and failure is largely by breaking, tearing, or elongation of the substrate material, average force to failure may have little significance in describing seal performance and should not be reported in such cases (see Annex A1.1).

9.9 A plot of force versus grip travel may be useful as an aid in interpretation of results. In those cases, the testing machine should be programmed to generate the plot.

9.10 Other properties, such as energy to cause seal separation, may be appropriate in cases where grip travel results only in peel. When other failure modes (delamination, elongation, break, tear or other) are present in addition to peel of the seal, energy, and other functions must be interpreted with caution.

10. Report

10.1 Report the following:

10.1.1 Complete identification of material being tested.

10.1.2 Equipment and test method or practice used to form seals, if known.


10.1.3 Equipment used to test seals.

10.1.4 Ambient conditions during tests; temperature and humidity.

10.1.5 Grip separation rate.

10.1.6 Initial grip separation distance.

10.1.7 Seal width.

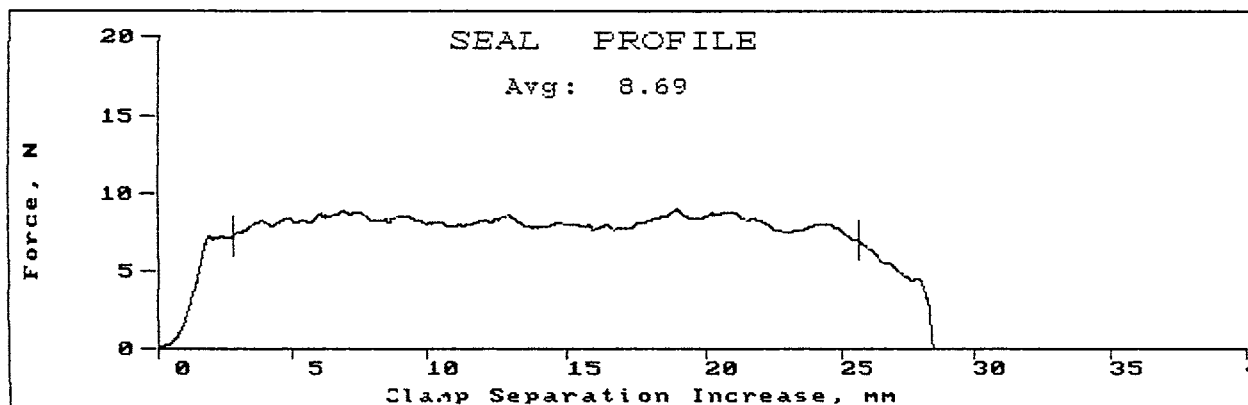

MARKERS ON SEAL PROFILE PLOT AT 10% AND 90% ESTABLISH DATA WINDOW OF 80% FOR CALCULATION

FIG. 3 Calculation of Average Seal Strength

TABLE 1

Test Series "A" (MAXIMUM Values)
Heat Seal Coated 50# Basis Weight Paper sealed to Film (48 ga. PET/2 mil LDPE) Supported 90° @ 12 in./min Unsupported @ 12 in./min Unsupported @ 8 in./min
Test Series "B" (Both MAXIMUM Values and AVERAGE Peel Values were reported)
Uncoated 1073B Tyvek® sealed to Film (48 ga. PET/2 mil LDPE) Supported 90° @ 12 in./min Unsupported @ 12 in./min Supported 180° @ 12 in./min Reverse direction of materials in grips @ 12 in./min
Test Series "C" (MAXIMUM Values)
Coex HDPE 3 mil film with peelable sealant layer sealed face-to-face Foil Composite 5 mil with same peelable sealant surface sealed face-to-face Unsupported @ 12 in./min Supported 180° @ 12 in./min

TABLE 2

Manufacturer	Models	Load Cell	
		N	lb
Dillon	AFG-50N	50	11.2
Instron	4464, 5500R, 5564,	5 kN, 500,	1124, 112.4,
	5565, S5R1123,	100, 50, 9	22.5, 11.2, 2
	4442, MN-44		
Lloyd Instruments	1300-36	100	22.4
MTS Sintech Renew	4204	111.2	25
Test Resources	2000ZR	111.2	25
Thwing Albert	EJA	50	11.2
Vinatoru Enterprises	CCT, HST	50	11.2

10.1.8 Machine direction of material in relation to direction of pull.

10.1.9 Force (strength) values to three significant figures.

10.1.10 Method of holding tail and any special fixtures used to hold specimens.

10.1.11 If the seal is made between two different materials, record which material is clamped in each grip.

10.1.12 Number of specimens tested and method of sampling.

10.1.13 Any other pertinent information that may affect test results.

10.1.14 Visual determination of mode of specimen failure. Frequently more than one mode will occur in the course of failure of an individual strip. Record all modes observed. A suggested classification of modes is (see Fig. 4):

- Adhesive failure of the seal; peel.
- Cohesive failure of the material.
- Break or tear of material in seal area or at seal edge.
- Delamination of surface layer(s) from substrate.
- Elongation of material.
- Break or tear of material remote from seal.

10.1.15 Maximum force encountered as each specimen is stressed to failure, expressed preferably in Newtons/meter or lbf/in. of original specimen width. Gmf/in. and lbf/in. are commonly used.

10.1.16 Average Peel Force, if applicable (see 9.8)—If this measurement is reported, a statement of the method or algorithm used to calculate the average should be included.



10.1.17 Plot of force versus grip travel, if deemed significant in interpretation of results.

10.1.18 Other data not compromised by interferences, if such data are relevant to the specific test purpose.

10.1.19 Any statistical calculation deemed appropriate (most commonly mean, range, and standard deviation).

11. Precision and Bias

11.1 Precision—A round robin was conducted using Practice E 691 as a guide, involving 18 laboratories measuring a total of 1980 samples distributed over 3 different test groups of 6 labs each. In order to maintain a focus on testing the method itself, laboratory samples were used to limit the amount of variation in the seals produced. Description of materials measured and methods used are listed in Table 1. Seven different brands of tensile testing equipment were used to collect information. The model identifications and load cell sizes are listed in Table 2. Statistical summaries of repeatability (within a laboratory) and reproducibility (between laboratories)

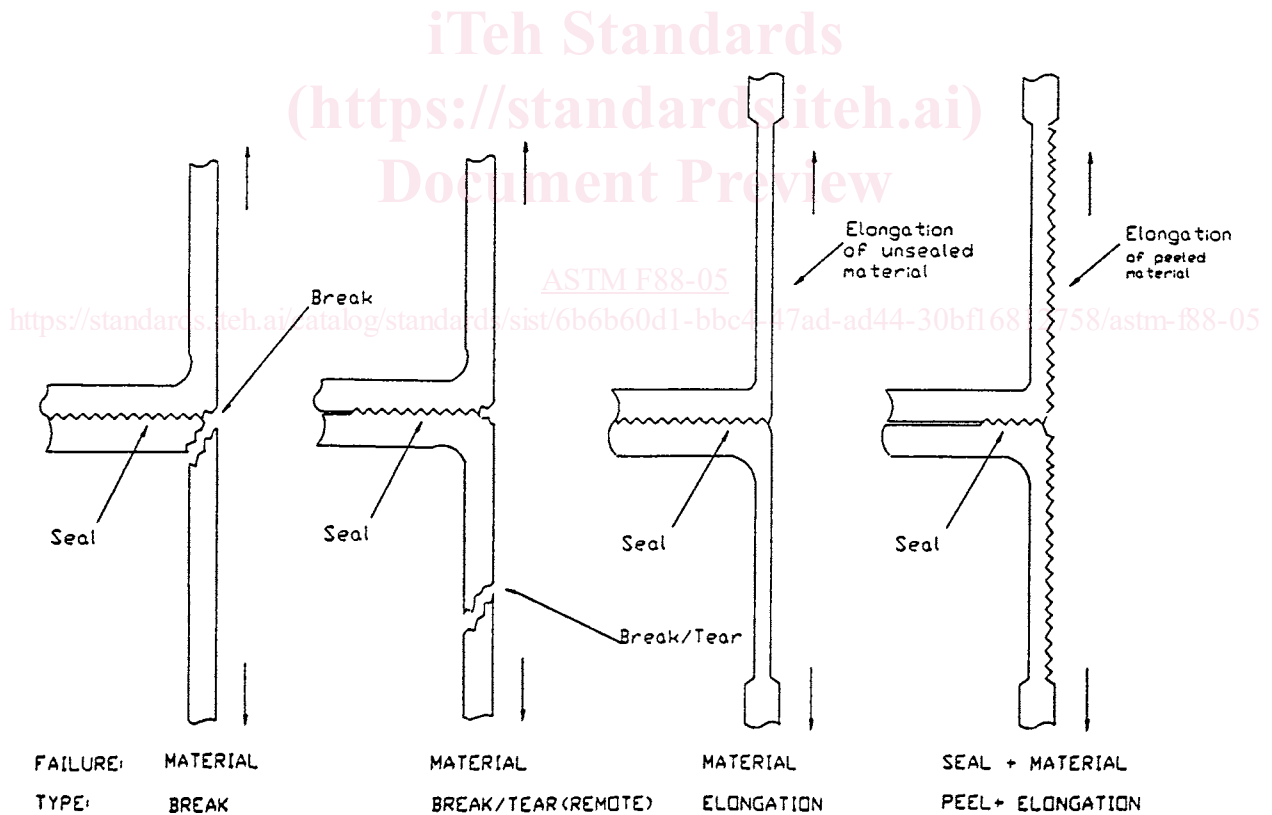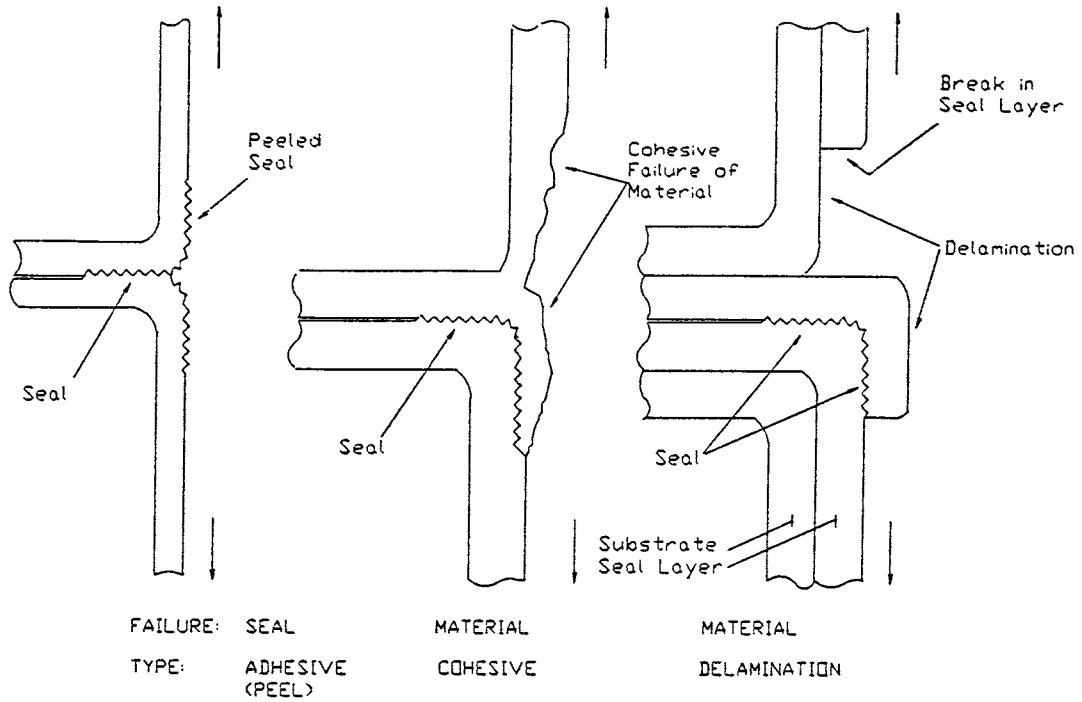

NOTE 1—Schematic representation of seal failure modes for seals between two webs. No diagram is included for systems including an adhesive as a third component.

FIG. 4 Test Strip Failure Modes

TABLE 3

Units: N/25.4 mm	s_r	s_R	r	R	$X_{2\bar{b}ar}$
A Supported 90°	0.1761	0.2103	0.4932	0.5889	4.2569
A Unsupported at 12 in./min	0.4132	0.5722	1.1568	1.6021	6.3343
A Unsupported at 8 in./min	0.4729	0.6618	1.3242	1.8529	6.3031
B PEAK 90°	1.1601	1.1200	3.2484	3.2484 ^A	4.1057
B AVG 90°	0.6882	0.6963	1.9269	1.9497	3.0426
B PEAK Unsupported	1.1936	1.1700	3.3421	3.3421 ^A	7.6020
B AVG Unsupported	1.1167	1.1084	3.1267	3.1267 ^A	6.4633
B PEAK 180°	1.3242	1.5135	3.7077	4.2378	14.4078
B AVG 180°	1.3656	1.5868	3.8236	4.4431	13.3002
B PEAK 180° Reverse	2.4625	2.6562	6.8950	7.4373	6.5122
B AVG 180° Reverse	1.1386	1.0901	3.1880	3.1880 ^A	4.1635
C 3 mil Film Unsupported	0.2693	0.4712	0.7539	1.3194	7.5397
C 3 mil Film 180°	0.7945	1.3357	2.2245	3.7400	15.4042
C 5 mil Foil Unsupported	0.1699	0.3203	0.4757	0.8968	5.3779
C 5 mil Foil 180°	1.4074	1.5460	3.9406	4.3287	20.3239

^A Per Practice E 691: "Enter the larger of the values obtained by the use of (equation for s_r) and (equation for s_R) as the final value of s_R to be used for precision statements."

TABLE 4

Units: lb/in.	s_r	s_R	r	R	$X_{2\bar{b}ar}$
A Supported 90°	0.0396	0.0473	0.1109	0.1324	0.957
A Unsupported at 12 in./min	0.0929	0.1286	0.2601	0.3602	1.424
A Unsupported at 8 in./min	0.1063	0.1488	0.2977	0.4166	1.417
B PEAK 90°	0.2608	0.2518	0.7303	0.7303 ^A	0.923
B AVG 90°	0.1547	0.1565	0.4332	0.4383	0.684
B PEAK Unsupported	0.2683	0.2630	0.7513	0.7513 ^A	1.709
B AVG Unsupported	0.2510	0.2492	0.7029	0.7029 ^A	1.453
B PEAK 180°	0.2977	0.3403	0.8335	0.9527	3.239
B AVG 180°	0.3070	0.3567	0.8596	0.9988	2.990
B PEAK 180° Reverse	0.5536	0.5971	1.5501	1.6720	1.464
B AVG 180° Reverse	0.2560	0.2451	0.7167	0.7167 ^A	0.936
C 3 mil Film Unsupported	0.0605	0.1059	0.1695	0.2966	1.695
C 3 mil Film 180°	0.1786	0.3003	0.5001	0.8408	3.463
C 5 mil Foil Unsupported	0.0382	0.0272	0.1069	0.2051	1.209
C 5 mil Foil 180°	0.3164	0.3476	0.8859	0.9731	4.569

^A Per Practice E 691: "Enter the larger of the values obtained by the use of (equation for s_r) and (equation for s_R) as the final value of s_R to be used for precision statements."

are listed in **Table 3** for SI units and **Table 4** in units of pounds per inch. **Fig. 5** and **Fig. 6** are graphical depictions of data.

11.2 *Concept of "r" and "R" in Tables 3 and 4*—If s_r and s_R have been calculated from a large enough body of data, and for test results that are averages from testing 10 specimens for each test result, then the following applies:

11.2.1 Repeatability "r" is the interval representing the critical difference between test results for the same material and method, obtained by the same operator using the same equipment on the same day in the same laboratory. Test results shall be deemed to be not equivalent if they differ by more than the "r" value for that material or method.

11.2.2 Reproducibility "R" is the interval representing the critical difference between test results for the same material and method, obtained by different operators using the different equipment in different laboratories, not necessarily on the same day. Test results shall be deemed to be not equivalent if they differ by more than the "R" value for that material or method.

11.3 Any judgment in accordance with 11.2.1 or 11.2.2 will have approximately 95 % (0.95) probability of being correct.

11.4 *Bias*—There are no recognized standards by which to estimate the bias of this test method.