
Natural gas — Energy determination

Gaz naturel — Détermination d'énergie

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[ISO 15112:2007](https://standards.iteh.ai/catalog/standards/sist/89bc8820-c609-40e4-99c5-0507b8bd1184/iso-15112-2007)

<https://standards.iteh.ai/catalog/standards/sist/89bc8820-c609-40e4-99c5-0507b8bd1184/iso-15112-2007>



PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 15112:2007

<https://standards.iteh.ai/catalog/standards/sist/89bc8820-c609-40e4-99c5-0507b8bd1184/iso-15112-2007>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2007

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

Page

Foreword.....	v
Introduction	vi
1 Scope	1
2 Normative references	1
3 Terms and definitions.....	1
4 Symbols and units.....	6
5 General principles.....	6
6 Gas measurement.....	8
6.1 General.....	8
6.2 Volume measurement.....	9
6.3 Calorific value measurement.....	9
6.4 Volume conversion.....	10
6.5 Calibration	11
6.6 Data storage and transmission	11
7 Energy determination.....	12
7.1 Interfaces	12
7.2 Methods of energy determination	14
8 Strategy and procedures	16
8.1 General.....	16
8.2 Strategies for energy determination.....	18
8.3 Plausibility checks.....	22
9 Assignment methods	23
9.1 Fixed assignment.....	23
9.2 Variable assignment	25
9.3 Determination of the representative calorific value	26
10 Calculation of energy quantities	28
10.1 General equations for energy	28
10.2 Calculation of averaged values — Calculation from average calorific values and cumulative volumes.....	29
10.3 Volume and volume-to-mass conversions	30
10.4 Energy determination on the basis of declared calorific values	30
11 Accuracy on calculated energy	31
11.1 Accuracy.....	31
11.2 Calculation of uncertainty.....	31
11.3 Bias.....	32
12 Quality control and quality assurance.....	33
12.1 General.....	33
12.2 Check of the course of the measuring data	33
12.3 Traceability	34
12.4 Substitute values	34
Annex A (informative) Main instruments and energy-determination techniques.....	36
Annex B (informative) Different possible patterns in the change of the calorific value	40
Annex C (informative) Volume conversion and volume-to-mass conversion	43
Annex D (informative) Incremental energy determination	44

Annex E (informative) Practical examples for volume conversion and energy quantity calculation	46
Annex F (informative) Practical examples for averaging the calorific value due to different delivery situations	50
Annex G (informative) Ways of determining substitute values	55
Annex H (informative) Plausibility check graphical example	57
Annex I (informative) Uncorrected data, bias correction and final result graphical example	58
Annex J (informative) Single-reservoir calorific value determination	60
Bibliography	61

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[ISO 15112:2007](https://standards.iteh.ai/catalog/standards/sist/89bc8820-c609-40e4-99c5-0507b8bd1184/iso-15112-2007)

<https://standards.iteh.ai/catalog/standards/sist/89bc8820-c609-40e4-99c5-0507b8bd1184/iso-15112-2007>

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 15112 was prepared by Technical Committee ISO/TC 193, *Natural gas*.

iTeh STANDARD PREVIEW (standards.iteh.ai)

[ISO 15112:2007](https://standards.iteh.ai/catalog/standards/sist/89bc8820-c609-40e4-99c5-0507b8bd1184/iso-15112-2007)

<https://standards.iteh.ai/catalog/standards/sist/89bc8820-c609-40e4-99c5-0507b8bd1184/iso-15112-2007>

Introduction

Since the early 1800s, it has been general practice for manufactured gas and, subsequently, natural gas to be bought and sold on a volumetric basis. Much time and effort has therefore been devoted to developing the means of flow measurement.

Because of the increasing value of energy and variations in gas quality, billing on the basis of thermal energy has now become essential between contracting partners and the need to determine calorific value by measurement or calculation has led to a number of techniques. However, the manner in which calorific value data are applied to flow volume data to produce the energy content of a given volume of natural gas has been far from a standardized procedure.

Energy determination is frequently a necessary factor wherever and whenever natural gas is metered, from production and processing operations through to end-user consumption. This International Standard has been developed to cover aspects related to production/transmission and distribution/end user. It provides guidance to users of how energy units for billing purposes are derived, based either on measurement or calculation or both, to increase confidence in results for contracting partners.

Other standards relating to natural gas, flow measurement, calorific value measurement, calculation procedures and data handling in regard to gas production, transmission and distribution involving purchase, sales or commodity transfer of natural gas may be relevant to this International Standard.

ISO 15112 contains ten informative annexes.

ITeH STANDARD PREVIEW
(standards.iteh.ai)
ISO 15112:2007
<https://standards.iteh.ai/catalog/standards/sist/89bc8820-c609-40e4-99c5-0507b8bd1184/iso-15112-2007>

Natural gas — Energy determination

1 Scope

This International Standard provides the means for energy determination of natural gas by measurement or by calculation, and describes the related techniques and measures that are necessary to take. The calculation of thermal energy is based on the separate measurement of the quantity, either by mass or by volume, of gas transferred and its measured or calculated calorific value. The general means of calculating uncertainties are also given.

Only systems currently in use are described.

NOTE Use of such systems in commercial or official trade can require approval of national authorization agencies, and compliance with legal regulations is required.

This International Standard applies to any gas-measuring station from domestic to very large high-pressure transmission.

New techniques are not excluded provided their proven performance is equivalent to, or better than, that of those techniques referred to in this International Standard.

Gas-measuring systems are not the subject of this International Standard.

<https://standards.iteh.ai/catalog/standards/sist/89bc8820-c609-40e4-99c5-0507b8bd1184/iso-15112-2007>

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 6976, *Natural gas — Calculation of calorific values, density, relative density and Wobbe index from composition*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

3.1 accuracy of measurement

closeness of the agreement between a measurement result and a true value of the measurand

[ISO 14532:2001]

**3.2
adjustment**

(of a measuring instrument) operation of bringing a measuring instrument into a state of performance suitable for its use

[VIM:1996, 4.30]

NOTE Adjustment may be automatic, semi-automatic or manual.

**3.3
assignment method**

(energy determination) method to derive a calorific value to be applied to the gas passing specified interfaces having only volume measurements

**3.4
availability**

probability, at any time, that the measuring system, or a measuring instrument forming part of the measuring system, is functioning according to specifications

[EN 1776]

**3.5
bias**

systematic difference between the true energy and the actual energy determined of the gas passing a gas-measuring station

**3.6
calibration**

set of operations that establish, under specified conditions, the relationship between values of quantities indicated by a measuring instrument or measuring system, or values represented by a material measure or a reference material, and the corresponding values obtained using working standards

[ISO 14532:2001, 2.5.2.2]

**3.7
superior calorific value**

energy released as heat by the complete combustion in air of a specified quantity of gas, in such a way that the pressure, p_1 , at which the reaction takes place remains constant, and all the products of combustion are returned to the same specified temperature, T_1 , as that of the reactants, all of these products being in the gaseous state except for water formed by combustion, which is condensed to the liquid state at T_1

[ISO 14532:2001, 2.6.4.1]

**3.8
inferior calorific value**

energy released as heat by the complete combustion in air of a specified quantity of gas, in such a way that the pressure, p_1 , at which the reaction takes place remains constant, and all the products of combustion are returned to the same specified temperature, T_1 , as that of the reactants, all of these products being in the gaseous state

[see ISO 14532:2001, 2.6.4.2]

**3.9
calorific value station**

installation comprising the equipment necessary for the determination of the calorific value of the natural gas in the pipeline

iTeh STANDARD PREVIEW
(standards.iteh.ai)

https://standards.iteh.ai/catalog/standards/sis/87bc8820-c009-40e4-99c5-0507b8bd1184/iso-15112-2007

3.10**adjusted calorific value**

calorific value measured at a measuring station compensated for the time taken for the gas to travel to the respective volume-measuring station

3.11**corrected calorific value**

result of correcting a measurement to compensate for systematic error

3.12**declared calorific value**

calorific value that is notified in advance of its application to interfaces for the purpose of energy determination

3.13**representative calorific value**

calorific value which is accepted to sufficiently approximate the actual calorific value at an interface

3.14**charging area**

set of interfaces where the same method of energy determination is used

3.15**conversion**

determination of the volume at reference conditions from the volume at operating conditions

3.16**correction**

value added algebraically to the uncorrected result of a measurement to compensate for systematic error

NOTE 1 The correction is equal to the negative of the estimated systematic error.

NOTE 2 Since the systematic error cannot be known perfectly, the correction cannot be complete (see Annex I).

3.17**correction factor**

numerical factor by which the uncorrected result of a measurement is multiplied to compensate for systematic error object

NOTE Since the systematic error cannot be known perfectly, the correction cannot be complete (see Annex I).

3.18**determination**

set of operations that are carried out on an object in order to provide a qualitative or quantitative information about this object

NOTE In this International Standard, the term "determination" is only used quantitatively.

3.19**direct measurement**

measurement of a property from quantities that, in principle, define the property

NOTE For example, the determination of the calorific value of a gas using the thermoelectric measurement of the energy released in the form of heat during the combustion of a known amount of gas.

[ISO 14532:2001, 2.2.1.2]

3.20**energy**

product of gas quantity (mass or volume) and calorific value at given conditions

NOTE 1 The energy may be called energy amount.

NOTE 2 Energy is usually expressed in units of megajoules.

**3.21
energy determination**

quantitative determination of the amount of energy of a quantity of gas based either on measurement or calculation using measured values

**3.22
energy flow rate**

energy of gas passing through a cross-section divided by time

NOTE Energy flow rate is usually expressed in units of megajoules per second.

**3.23
fixed assignment**

application without modification of the calorific value measured at one specific calorific-value-measuring station, or the calorific value declared in advance, to the gas passing one, or more, interfaces

**3.24
gas transporter**

company that conveys gas from one place to another through pipelines

**3.25
grid simulation**

calculation of a set of pressures and flow rates in a pipeline or a grid on the basis of given topology data, values of the flow rates at the inlet and outlet points and of the pressure and temperature at various points of the pipeline(s) by means of a mathematical model

NOTE The objective of any grid simulation is to yield information about a future state of gas pressures and flows. The result of the simulation is a more or less accurate estimation of the state of the gas flow.

**3.26
interface**

place on a pipe used for the transportation or supply of gas at which there is a change of ownership or physical custody of gas

NOTE Generally, an interface has an associated measuring station.

**3.27
local distribution company
LDC**

company that delivers gas to industrial, commercial and/or residential customers

**3.28
measuring station**

installation comprising all the equipment, including the inlet and outlet pipework as far as the isolating valves and structure within which the equipment is housed, used for gas measurement in custody transfer

[EN 1776]

**3.29
measuring system**

complete set of measuring instruments and auxiliary equipment assembled to carry out specified measurements

[VIM:1996, 4.5]

3.30**measuring instrument**

device intended to be used for measurements, alone or in conjunction with supplementary device(s)

[VIM:1996, 4.1]

3.31**plausibility**

property of a value to be within reasonable limits

3.32**producer**

company that extracts raw natural gas from reservoirs which, after processing and (fiscal) measurement, is supplied as dry natural gas to the transportation system

3.33**regional distributor**

company that delivers gas to local distribution companies and/or industrial, commercial or residential customers

3.34**residential customer**

person whose occupied premises are supplied with gas, wholly or in part, such gas not being used for any business purpose, commercial or industrial

3.35**systematic error**

mean that would result from an infinite number of measurements of the same measurand carried out under repeatability conditions minus a true value of the measurand

[VIM:1996, 3.14]

iTeh STANDARD PREVIEW
(standards.iteh.ai)
ISO 15112:2007
<https://standards.iteh.ai/catalog/standards/sist/89bc8820-c609-40e4-99c5-0507b8bd1184/iso-15112-2007>

3.36**traceability**

property of the result of a measurement or the value of a standard whereby it can be related to stated references, usually national or international standards, through an unbroken chain of comparisons all having stated uncertainties

[VIM:1996, 6.10]

NOTE This chain of comparisons is called a traceability chain.

3.37**uncertainty of measurement**

parameter, associated with the result of a measurement, that characterizes the dispersion of the values that could reasonably be attributed to the measurand

[VIM:1996, 3.9]

3.38**variable assignment**

application of a calorific value for an assignment procedure based on measurement(s) at calorific value station(s) to the gas passing one, or more, interfaces

NOTE That applied calorific value may take into account the time taken for the gas to travel from the calorific value station to the respective volume-measuring stations and other factors, to derive an average calorific value for a network, a state reconstruction of the variation of calorific values through a network, etc.

**3.39
zero floating point**

position in a grid conveying gas where there is a boundary with different gas qualities on either side

4 Symbols and units

Symbol	Meaning	SI unit	USC unit
<i>E</i>	energy	MJ	kWh
<i>e</i>	energy flow rate	MJ/s	kWh/h
<i>H</i>	calorific value	MJ/m ³ ; MJ/kg	kWh/m ³

NOTE 1 Where the calorific value is in megajoules per cubic metre and the gas volume is in cubic meters, or where the calorific value is in megajoules per kilogram and the gas mass is in kilograms, then the calculated energy is in megajoules.

Where the calorific value is in kilowatt-hours per cubic meter and the gas volume is in cubic meters, or where the calorific value is in kilowatt-hours per kilogram and the gas mass is in kilograms, then the calculated energy is in kilowatt-hours.

To convert the number of megajoules to the number of kilowatt-hours divide the number by 3,6.

<i>M</i>	mass	kg	t
<i>p</i>	pressure (absolute)	Pa, kPa	bar, mbar
<i>Q</i>	quantity of gas	m ³ , kg	t

NOTE 2 When the quantity is given in cubic metres, it should be qualified by temperature and pressure.

<i>q_v</i>	volume flow rate	m ³ /h, m ³ /s	
<i>q_m</i>	mass flow rate	kg/s, kg/h	
<i>T</i>	temperature (absolute)	K	
<i>t</i>	time	s, h, d	s, h, d
<i>V</i>	volume (gas)	m ³	
<i>Z</i>	compression factor		
<i>ρ</i>	density	kg/m ³	
<i>θ</i>	temperature	°C	°F

Subscripts:

<i>l</i>	inferior calorific value
<i>n</i>	number of time intervals
<i>nc</i>	normal reference conditions (273,15 K; 101,325 kPa)
<i>r</i>	ISO-recommended standard reference conditions (288,15 K; 101,325 kPa)
<i>S</i>	superior calorific value
<i>wa</i>	weighted average

5 General principles

The quantity of energy, *E*, contained in a given quantity of gas, *Q*, is given by the multiplication of the calorific value, *H*, by the respective quantity of gas.

Energy may be either measured directly (see Figure 1) or calculated from the quantity and the calorific value of the gas (see Figure 2).

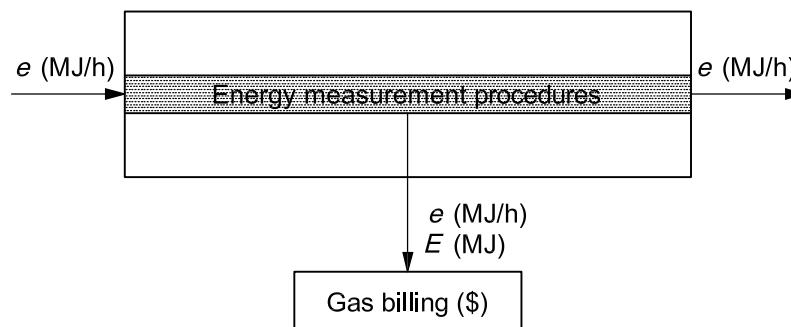


Figure 1 — Energy-measurement scheme

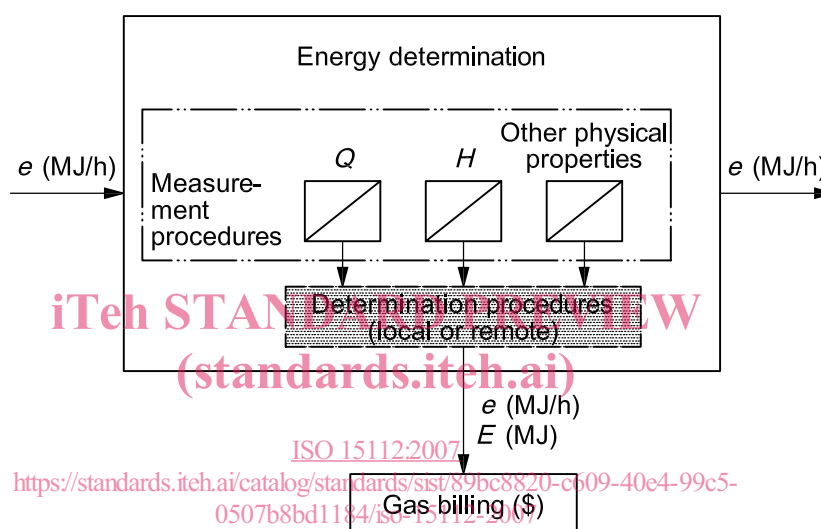


Figure 2 — Energy-determination scheme

Generally, the quantity of gas is expressed as a volume and the calorific value is on a volumetric basis. In order to achieve accurate determinations of energy, it is necessary that both the gas volume and calorific value be at the same reference conditions. The determination of energy is based either on the accumulation over time of calculation results from consecutive sets of calorific values and the concurrent flow rate values or on the multiplication of the total volume and the representative (assigned) calorific value for that period.

Especially in situations of varying calorific values and when flow rates are determined at a place different from that of the (representative) calorific value, the effect on the accuracy caused by the difference in time between the determination of the flow rate and the calorific value shall be considered (see Clause 11).

The gas volume may either be measured and reported as the volume at the ISO-recommended standard reference conditions or be measured at some other conditions and converted to an equivalent volume at the ISO-recommended standard reference conditions, using an appropriate method of volume conversion. The method of volume conversion used at a specific gas-volume-measuring station may require gas quality data determined at other places. For the purpose of this International Standard, the ISO-recommended standard reference conditions of 288,15 K and 101,325 kPa as defined in ISO 13443 should be used.

NOTE For gas supply, other conditions can be used, corresponding to national standards or laws. Methods for conversion between different conditions for dry natural gases are given in ISO 13443.

The calorific value may be measured at the gas-measuring station or at some other representative point and assigned to the gas-measuring station. It is also possible for the quantity of gas and the calorific value to be expressed on a mass basis.

This general principle of energy determination is extended in Clause 10 to those cases when the quantity of gas is expressed on either a volumetric or a mass basis.

To achieve the calculation of the quantity of energy of the gas passing a gas-measuring station over a period of time, the methods of energy determination in Clauses 7 to 10 are used. Such methods involve an integration over the time period; that integration may be

- of the energy flow, or
- of the gas flow rate over time to obtain the quantity of gas, which is then multiplied by the representative calorific value.

The method of integration may depend on contractual agreements or national legislation.

The general principles of energy determination in Clauses 7 to 10 are independent of the method with which the integrations are carried out. The method of integration influences the uncertainty of the determined energy; these effects are considered in Clause 11.

6 Gas measurement

6.1 General

iTeh STANDARD PREVIEW
(standards.iteh.ai)

The type of measuring devices and methods used in real measuring stations depends among other things on

- the respective national requirements, [ISO 15112:2007](https://standards.iteh.ai/catalog/standards/sist/89bc8820-c609-40e4-99c5-0507b8bd1184/iso-15112-2007)
- the flow rate,
- the commercial value of the gas,
- the gas quality variations,
- the need for redundancy, and
- the instrument specification.

Only proven methods and measuring devices/products used at the respective interfaces should be used. An overview of the techniques and procedures currently used in different countries is shown in Annex A.

Methods used for flow and calorific value measurement shall be in accordance with standards, contractual agreements and/or national legislation, as appropriate.

Action should be taken to identify and reconcile systematic effects. For example, use of different national standards, regulations and/or operating procedures can introduce systematic differences; contract partners should determine the appropriate means to overcome these differences.

The quality of the measurement results in general depends on the following factors:

- operating conditions;
- maintenance frequency and quality;
- calibration standards;

- sampling and clean-up;
- changes in gas composition;
- ageing of measurement devices.

A high accuracy can be achieved if the requirements fixed by the manufacturers and by officials are met and all operating procedures for operating, calibration and maintenance are strictly observed.

6.2 Volume measurement

The volume flow-metering system of a natural-gas-measuring station consists of one or more meter runs. Generally, the meters measure the gas volume flow at actual operating conditions. Standards for orifice meters (ISO 5167-1) and turbine meters (ISO 9951) exist.

The selection of a flow-metering system for a specific application depends as a minimum on the following:

- conditions of flow;
- flow-measuring range;
- operating conditions, especially operating pressure;
- acceptable pressure loss;
- required accuracy.

iTeh STANDARD PREVIEW
(standards.iteh.ai)

For natural-gas volume flow measurement, the instruments mostly used at the interfaces 1 to 6 (see 7.1) are shown in Annex A.

[ISO 15112:2007](https://standards.iteh.ai/catalog/standards/sist/89bc8820-c609-40e4-99c5-9307b8bd1184/iso-15112-2007)

<https://standards.iteh.ai/catalog/standards/sist/89bc8820-c609-40e4-99c5-9307b8bd1184/iso-15112-2007>

6.3 Calorific value measurement

6.3.1 Measurement techniques and sampling

A calorific-value measuring system consists of a sampling system and a measurement device taken from one of the following groups:

- direct measurement (e.g. by combustion calorimeters);
- inferential measurement [e.g. by a gas chromatograph (GC)];
- correlation techniques.

To achieve a high accuracy of calorific value measurement, representative sampling is required. Guidelines are given in ISO 10715.

Depending on

- the measuring system,
- the operating procedures,
- the fluctuation of composition of the gas, and/or
- the quantity of gas delivered,

one of the following sampling techniques can be used: