

---

---

**Corrugating medium — Determination of  
the flat crush resistance after laboratory  
fluting**

*Papier cannelure pour carton ondulé — Détermination de la résistance  
à la compression à plat après cannelage en laboratoire*

**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

[ISO 7263:2008](https://standards.iteh.ai/catalog/standards/sist/e80defb1-a7d1-499c-8b52-23435a8cfbb9/iso-7263-2008)

[https://standards.iteh.ai/catalog/standards/sist/e80defb1-a7d1-499c-8b52-  
23435a8cfbb9/iso-7263-2008](https://standards.iteh.ai/catalog/standards/sist/e80defb1-a7d1-499c-8b52-23435a8cfbb9/iso-7263-2008)



**PDF disclaimer**

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

ISO 7263:2008

<https://standards.iteh.ai/catalog/standards/sist/e80defb1-a7d1-499c-8b52-23435a8cfbb9/iso-7263-2008>



**COPYRIGHT PROTECTED DOCUMENT**

© ISO 2008

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Case postale 56 • CH-1211 Geneva 20  
Tel. + 41 22 749 01 11  
Fax + 41 22 749 09 47  
E-mail [copyright@iso.org](mailto:copyright@iso.org)  
Web [www.iso.org](http://www.iso.org)

Published in Switzerland

**Contents**

Page

<b>Foreword</b> .....	<b>iv</b>
<b>Introduction</b> .....	<b>v</b>
<b>1 Scope</b> .....	<b>1</b>
<b>2 Normative references</b> .....	<b>1</b>
<b>3 Terms and definitions</b> .....	<b>1</b>
<b>4 Principle</b> .....	<b>1</b>
<b>5 Apparatus</b> .....	<b>1</b>
<b>6 Sampling</b> .....	<b>4</b>
<b>7 Conditioning</b> .....	<b>4</b>
<b>8 Preparation of test pieces</b> .....	<b>4</b>
<b>9 Procedure</b> .....	<b>4</b>
<b>10 Expression of results</b> .....	<b>5</b>
<b>11 Precision</b> .....	<b>6</b>
<b>12 Test report</b> .....	<b>6</b>
<b>Annex A (informative) Maintenance of fluting rolls (horizontal type)</b> .....	<b>7</b>
<b>Bibliography</b> .....	<b>8</b>

iTeh STANDARD PREVIEW

(standards.iteh.ai)

ISO 7263:2008

<https://standards.iteh.ai/catalog/standards/sist/e80defb1-a7d1-499c-8b52-23435a8cfbb9/iso-7263-2008>

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 7263 was prepared by Technical Committee ISO/TC 6, *Paper, board and pulps*, Subcommittee SC 2, *Test methods and quality specifications for paper and board*.

This third edition cancels and replaces the second edition (ISO 7263:1994), which has been technically revised. The major revision is the change in how the time between fluting and compression testing is expressed. Description and calibration of the compression testing equipment have been eliminated and the appropriate International Standard is referenced. Precision statements for the rigid platen instrument and for the procedure involving conditioning prior to testing have been added. An annex describing steps to be taken for fluter maintenance is included.

iTeh STANDARD PREVIEW

(standards.iteh.ai)

ISO 7263:2008

[https://standards.iteh.ai/catalog/standards/sist/e80defb1-a7d1-499c-8b52-](https://standards.iteh.ai/catalog/standards/sist/e80defb1-a7d1-499c-8b52-23435a8cfbb9/iso-7263-2008)

[23435a8cfbb9/iso-7263-2008](https://standards.iteh.ai/catalog/standards/sist/e80defb1-a7d1-499c-8b52-23435a8cfbb9/iso-7263-2008)

## Introduction

The flat crush resistance of laboratory-fluted corrugating medium is regarded as an important property because it is an indication of the potential flat crush resistance of corrugated fibreboard made from that medium. The corrugated medium is fluted by passing it between heated rollers. Two different test procedures are then widely used:

- a) the fluted corrugating medium is compressed immediately after fluting (i.e. 5 s to 8 s after fluting);
- b) the fluted corrugating medium is conditioned for 30 min to 35 min under standard laboratory test conditions before being compressed.

Procedure a) generally gives considerably higher results than those obtained with procedure b). The differences in results are claimed to be caused by

- the lower moisture content (and thus higher stiffness) of the unconditioned fluted corrugating medium,
- the change in flute profile which occurs during the conditioning period.

Since considerable advantages are claimed for both procedures and both are widely used, this International Standard describes both procedures.

A method of determining the flat crush resistance of manufactured corrugated fibreboard is given in ISO 3035:1982, *Single-faced and single-wall corrugated fibreboard — Determination of flat crush resistance*.

[ISO 7263:2008](https://standards.iteh.ai/catalog/standards/sist/e80defb1-a7d1-499c-8b52-23435a8cfbb9/iso-7263-2008)

<https://standards.iteh.ai/catalog/standards/sist/e80defb1-a7d1-499c-8b52-23435a8cfbb9/iso-7263-2008>

**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

ISO 7263:2008

<https://standards.iteh.ai/catalog/standards/sist/e80defb1-a7d1-499c-8b52-23435a8cfbb9/iso-7263-2008>

# Corrugating medium — Determination of the flat crush resistance after laboratory fluting

## 1 Scope

This International Standard specifies two methods for the determination of the flat crush resistance of corrugating medium after laboratory fluting.

The procedures are applicable to any corrugating medium intended to be used, after fluting, in the manufacture of corrugated board.

## 2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 186, *Paper and board — Sampling to determine average quality*

ISO 187, *Paper, board and pulps — Standard atmosphere for conditioning and testing and procedure for monitoring the atmosphere and conditioning of samples*

ISO 13820, *Paper, board and corrugated fibreboard — Description and calibration of compression-testing equipment*

## 3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

### 3.1

#### **flat crush resistance**

maximum force that a corrugated test piece will withstand before the flutes collapse under an increasing force applied perpendicular to its surface

## 4 Principle

Fluting of the corrugating medium by passing it between heated rollers, and its formation into single-faced corrugated board using pressure-sensitive adhesive tape as the facing. Application of a crushing force, in the direction perpendicular to the plane of the flutes, and determination of the flat crush resistance.

## 5 Apparatus

**5.1 Cutting device**, for cutting the test pieces to the dimensions required.

**5.2 Fluter**, consisting of a pair of matched steel corrugating rolls.

The roll temperature shall be maintained at  $175\text{ °C} \pm 8\text{ °C}$ . The temperature is controlled by any suitable method. Check the temperature when the rolls are in motion.

One roll is motor-driven at  $4,5\text{ r/min} \pm 1,0\text{ r/min}$  and the rolls are held in mesh by a force of  $100 \pm 10\text{ N}$  exerted between the rolls and distributed evenly across the teeth, under test conditions. In some instruments, the force between the rolls is applied by a spring acting in a slide. In such instruments, friction in this device can result in the force which acts upon the test piece being considerably less than the force required to displace the rolls initially. When verifying that an instrument conforms to the requirements given in 5.2, it is therefore necessary to measure the force required to just prevent the undriven roll from moving towards the driven roll, from a position about  $200\text{ }\mu\text{m}$  away.

The essential characteristics of each roll are the following (see also Figure 1):

Roll diameter	$228,5\text{ mm} \pm 0,5\text{ mm}$
Roll face width	$16\text{ mm} \pm 1\text{ mm}$
Number of teeth	84 (see Note)
Radius of teeth at peak	$1,5\text{ mm} \pm 0,1\text{ mm}$
Radius of teeth at base	$2,0\text{ mm} \pm 0,1\text{ mm}$
Depth of teeth	$4,75\text{ mm} \pm 0,05\text{ mm}$
Distance between teeth (peak to peak around the arc)	$8,55\text{ mm} \pm 0,05\text{ mm}$

**iTeh STANDARD PREVIEW**

(standards.iteh.ai)

In order to optimize the matching of pairs of rolls, pairs of rolls should be selected in which the differences in dimensions between the two are substantially less than the tolerances shown. A difference of  $\pm 0,1\text{ mm}$  or better is recommended. Prior to first use, the rolls should be run at the operating temperature for about 6 h with a mild abrasive on the teeth. The two rolls should then be marked in some way so that, after removal for cleaning or maintenance, they can be reassembled with exactly the same teeth in mesh.

NOTE In some fluters, a full roll is not used.

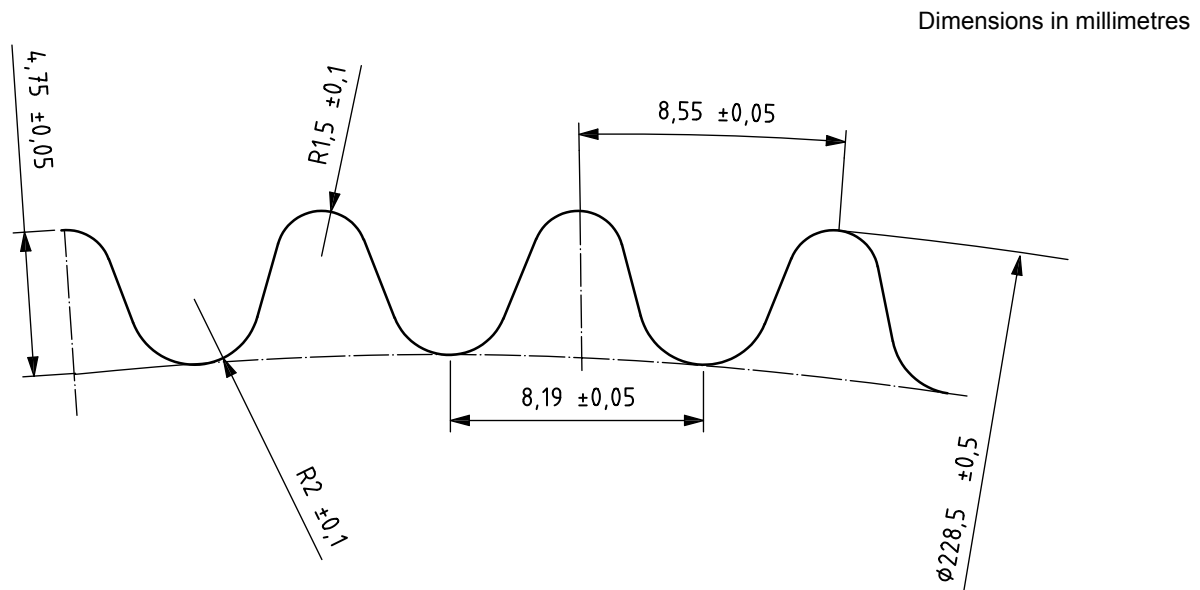


Figure 1 — Profile of corrugating rolls




### 5.3 Rack and comb

**5.3.1 Rack**, at least 19 mm wide with a profile corresponding to the teeth of the corrugating rolls.

It has nine full teeth and one incomplete tooth at each end so as to form 10 valleys. The tooth spacing is  $8,50 \text{ mm} \pm 0,05 \text{ mm}$  and the height of the teeth is  $4,75 \text{ mm} \pm 0,05 \text{ mm}$ . (See 2 in Figures 2 and 3.)

**5.3.2 Comb**, at least 19 mm wide with 10 prongs,  $3,4 \text{ mm} \pm 0,1 \text{ mm}$  high. (See 1 in Figures 2 and 3.)

The rack (5.3.1) and comb (5.3.2) may be replaced with an automatic device, provided it can be demonstrated that this device will produce the same results.

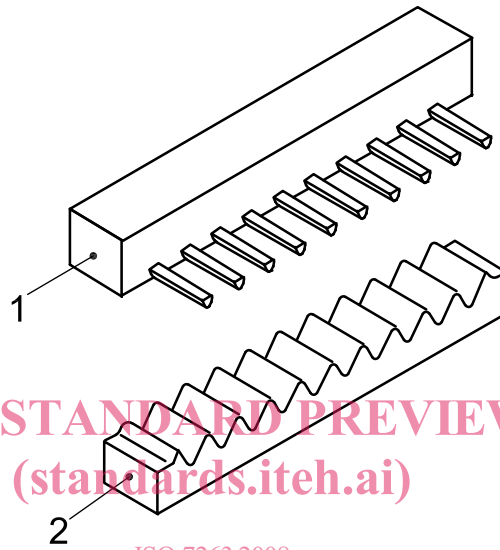


#### Key

- 1 comb
- 2 rack

ISO 7263:2008  
<https://standards.iteh.ai/catalog/standards/sist/e80defb1-a7d1-499c-8b52-23435a8cfbb9/iso-7263-2008>

**Figure 2 — Profile of comb and rack**

Dimensions in millimetres

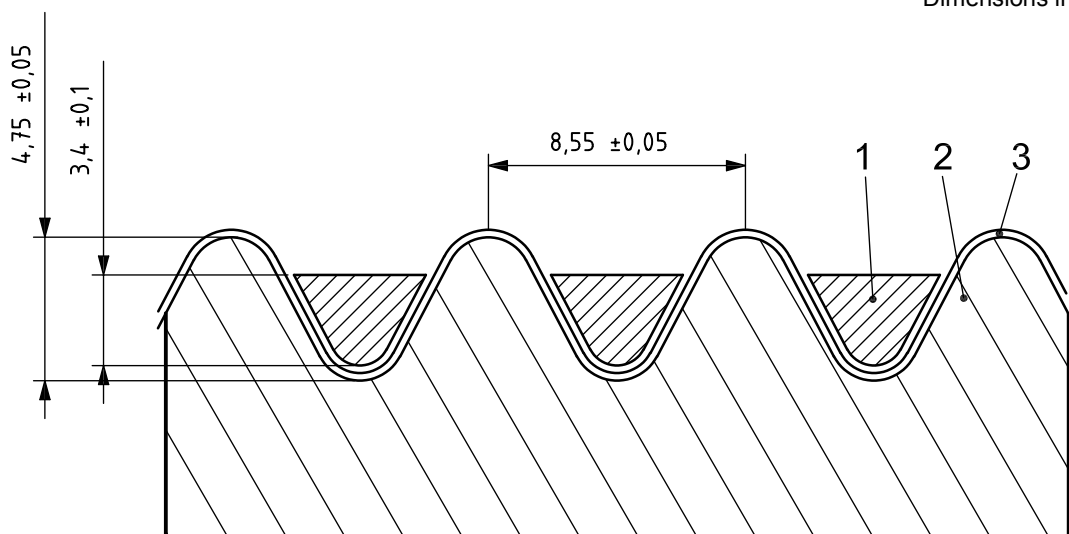

#### Key

- 1 comb
- 2 rack
- 3 paper

**Figure 3 — Dimensions of comb and rack**