



Designation: D4329 – 05

# Standard Practice for Fluorescent UV Exposure of Plastics<sup>1</sup>

This standard is issued under the fixed designation D4329; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

## 1. Scope\*

1.1 This practice covers specific procedures and test conditions that are applicable for fluorescent UV exposure of plastics conducted in accordance with Practices [G151](#) and [G154](#). This practice also covers the preparation of test specimens, the test conditions best suited for plastics, and the evaluation of test results.

1.2 The values stated in SI units are to be regarded as standard. The values given in brackets are for information only.

1.3 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

NOTE 1—This practice is technically similar to ISO 4892-3.

## 2. Referenced Documents

2.1 *ASTM Standards:*<sup>2</sup>

[D3980 Practice for Interlaboratory Testing of Paint and Related Materials](#) (Withdrawn 1998)<sup>3</sup>

[D5870 Practice for Calculating Property Retention Index of Plastics](#)

[E691 Practice for Conducting an Interlaboratory Study to Determine the Precision of a Test Method](#)

[G113 Terminology Relating to Natural and Artificial Weathering Tests of Nonmetallic Materials](#)

[G141 Guide for Addressing Variability in Exposure Testing of Nonmetallic Materials](#)

[G147 Practice for Conditioning and Handling of Nonmetallic Materials for Natural and Artificial Weathering Tests](#)

[G151 Practice for Exposing Nonmetallic Materials in Accelerated Test Devices that Use Laboratory Light Sources](#)

<sup>1</sup> This practice is under the jurisdiction of ASTM Committee [D20](#) on Plastics and is the direct responsibility of Subcommittee [D20.50](#) on Durability of Plastics.

Current edition approved July 15, 2005. Published August 2005. Originally approved in 1984. Last previous edition approved in 1999 as D4329 - 99. DOI: 10.1520/D4329-05.

<sup>2</sup> For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

<sup>3</sup> The last approved version of this historical standard is referenced on www.astm.org.

[G154 Practice for Operating Fluorescent Light Apparatus for UV Exposure of Nonmetallic Materials](#)

[G169 Guide for Application of Basic Statistical Methods to Weathering Tests](#)

[G177 Tables for Reference Solar Ultraviolet Spectral Distributions: Hemispherical on 37° Tilted Surface](#)

2.2 *ISO Standard:*<sup>4</sup>

[ISO 4892-3 Plastics—Methods of Exposure to Laboratory Light Sources—Part 3, Fluorescent UV Lamps](#)

2.3 *SAE Standard:*<sup>5</sup>

[SAE J2020 Accelerated Exposure of Automotive Exterior Materials Using a Fluorescent UV and Condensation Apparatus](#)

## 3. Terminology

3.1 The definitions in Terminology [G113](#) are applicable to this practice.

## 4. Significance and Use

4.1 The ability of a plastic material to resist deterioration of its electrical, mechanical, and optical properties caused by exposure to light, heat, and water can be very significant for many applications. This practice is intended to induce property changes associated with end-use conditions, including the effects of sunlight, moisture, and heat. The exposure used in this practice is not intended to simulate the deterioration caused by localized weather phenomena, such as, atmospheric pollution, biological attack, and saltwater exposure. (**Warning**—Variation in results may be expected when operating conditions are varied within the accepted limits of this practice. Therefore, no reference to the use of this practice should be made unless accompanied by a report prepared in accordance with Section [8](#) that describes the specific operating conditions used. Refer to Practice [G151](#) for detailed information on the caveats applicable to use of results obtained in accordance with this practice.)

NOTE 2—Additional information on sources of variability and on strategies for addressing variability in the design, execution, and data analysis of laboratory-accelerated exposure tests is found in Guide [G141](#).

<sup>4</sup> Available from American National Standards Institute (ANSI), 25 W. 43rd St., 4th Floor, New York, NY 10036.

<sup>5</sup> Available from Society of Automotive Engineers (SAE), 400 Commonwealth Dr., Warrendale, PA 15096-0001.

\*A Summary of Changes section appears at the end of this standard

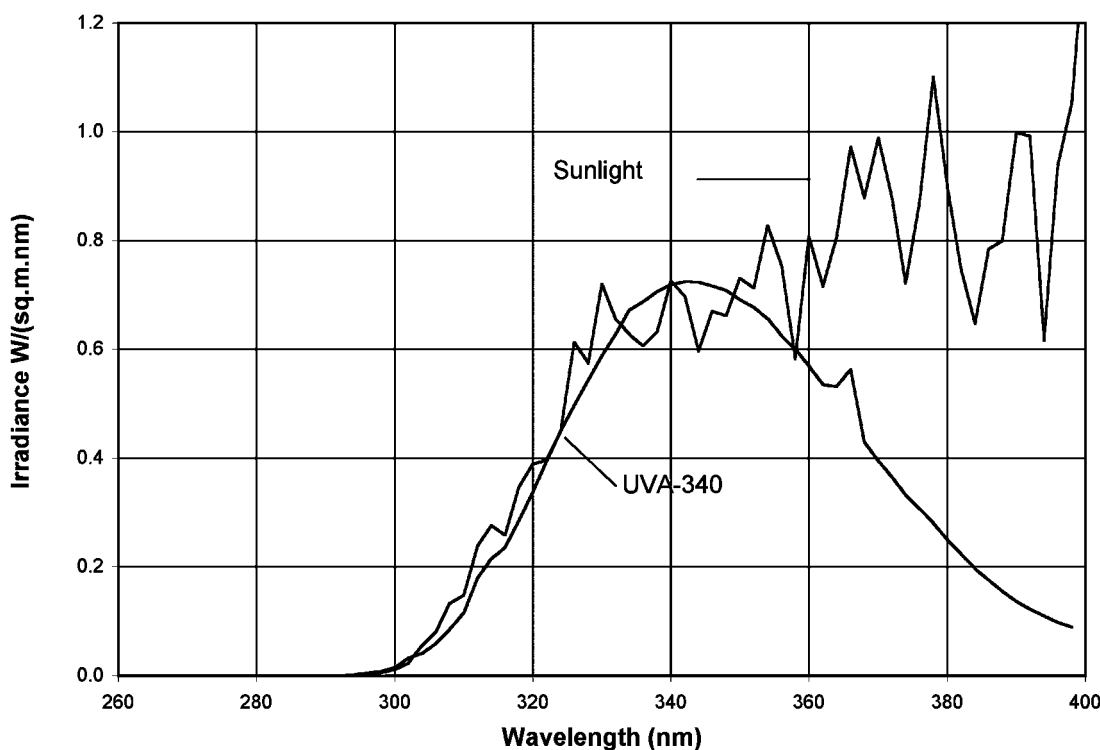


FIG. 1 Representative Spectral Power Distribution of UVA-340 Fluorescent Lamps

4.2 Reproducibility of test results between laboratories has been shown to be good when the stability of materials is evaluated in terms of performance ranking compared to other materials or to a control.<sup>6,7</sup> Therefore, exposure of a similar material of known performance (a control) at the same time as the test materials is strongly recommended. It is recommended that at least three replicates of each material be exposed to allow for statistical evaluation of results.

4.3 Test results will depend upon the care that is taken to operate the equipment in accordance with Practice G154. Significant factors include regulation of line voltage, temperature of the room in which the device operates, temperature control, and condition and age of the lamp.

## 5. Apparatus

5.1 Use of fluorescent UV apparatus that conforms to the requirements defined in Practices G151 and G154 is required to conform to this practice.

5.2 Unless otherwise specified, the spectral power distribution of the fluorescent UV lamp shall conform to the requirements in Practice G154 for a UVA 340 lamp. Fig. 1 is a spectral

irradiance plot for a typical UVA-340 lamp and benchmark solar radiation.

NOTE 3—The source of the sunlight data in Fig. 1 is from Standard G177 standard solar spectrum.

### 5.3 Test Chamber Location:

5.3.1 Locate the apparatus in an area maintained between 18 and 27°C [65 and 80°F]. Measure ambient temperature at a maximum distance of 150 mm [6 in.] from the plane door of the apparatus. Control of ambient temperature is particularly critical when one apparatus is stacked above another, because the heat generated from the lower unit can interfere with the operation of the units above.

5.3.2 Place the apparatus at least 300 mm from walls or other apparatus. Do not place the apparatus near a heat source such as an oven.

5.3.3 Ventilate the room in which the apparatus is located to remove heat and moisture.

## 6. Test Specimen

6.1 The size and shape of specimens to be exposed will be determined by the specifications of the particular test method used to evaluate the effects of the exposure on the specimens; the test method shall be determined by the parties concerned. Where practical, it is recommended that specimens be sized to fit specimen holders and racks supplied with the exposure apparatus. Unless supplied with a specific backing as an integral part of the test, specimens shall be mounted so that only the minimum specimen area required for support by the

<sup>6</sup> Fischer, R., "Results of Round Robin Studies of Light- and Water-Exposure Standard Practices," *Accelerated and Outdoor Durability Testing of Organic Materials*, ASTM STP 1202, Warren D. Ketola and Douglas Grossman, eds., American Society for Testing and Materials, Philadelphia, 1993.

<sup>7</sup> Ketola, W., and Fischer, R., "Characterization and Use of Reference Materials in Accelerated Durability Tests," *VAMAS Technical Report No. 30*, available from NIST, Gaithersburg, MD.

holder shall be covered. This unexposed surface must not be used as part of the test area.

6.2 For specimens of insulating materials, such as foams, maximum specimen thickness is 20 mm in order to allow for adequate heat transfer for condensation.

6.3 To provide rigidity, attach flexible specimens to a backing panel made of aluminum, 0.635 mm [0.025 in.] thick. Suggested aluminum alloys are 5052, 6061, or 3003.

6.4 Seal any holes in specimens larger than 2 mm and any openings larger than 1 mm around irregularly shaped specimens to prevent loss of water vapor. Attach porous specimens to a solid backing such as aluminum that can act as a vapor barrier.

6.5 Unless otherwise specified, expose at least three replicate specimens of each test and control material.

6.6 Follow the procedures described in Practice G147 for identification, conditioning, and handling of specimens of test, control, and reference materials prior to, during, and after exposure.

6.7 Do not mask the face of a specimen for the purpose of showing on one panel the effects of various exposure times. Misleading results may be obtained by this method, since the masked portion of the specimen is still exposed to temperature and humidity cycles that in many cases will affect results.

6.8 Since the thickness of a specimen may markedly affect the results, thickness of test and control specimens shall be within  $\pm 10\%$  of the nominal dimensions.

NOTE 4—This is especially important when mechanical properties are being investigated.

6.9 Retain a supply of unexposed file specimens of all materials evaluated.

6.9.1 When destructive tests are run, ensure that sufficient file specimens are retained so that the property of interest can be determined on unexposed file specimens each time exposed materials are evaluated.

6.10 Specimens should not be removed from the exposure apparatus for more than 24 h and then returned for additional tests, since this does not produce the same results on all materials as tests run without this type of interruption. When specimens are removed from the exposure apparatus for 24 h or more and then returned for additional exposure, report the elapsed time as noted in accordance with Section 9.

NOTE 5—Since the stability of the file specimen may also be time-dependent, users are cautioned that over prolonged exposure periods, or where small differences in the order of acceptable limits are anticipated, comparison of exposed specimens with the file specimen may not be valid. Instrumental measurements are recommended whenever possible.

## 7. Procedure

7.1 When the test and control specimens do not completely fill the specimen racks, fill all empty spaces with blank panels to maintain the test conditions within the chamber.

7.2 Unless otherwise specified, program the device to one of the following test cycles. Operate the device continuously.

### 7.2.1 Cycle A:

8 h UV with uninsulated black panel temperature controlled at  $60 \pm 3^\circ\text{C}$   
 4 h condensation with uninsulated black panel temperature controlled at  $50 \pm 3^\circ\text{C}$   
 (Used for most general applications)

### 7.2.2 Cycle B:

8 h UV with uninsulated black panel temperature controlled at  $70 \pm 3^\circ\text{C}$   
 4 h condensation with uninsulated black panel temperature controlled at  $50 \pm 3^\circ\text{C}$   
 (Typically used for automotive applications) Note: Cycle B is equivalent to the exposure test cycle specified in SAE J2020.

### 7.2.3 Cycle C:

8 h UV with uninsulated black panel temperature controlled at  $50 \pm 3^\circ\text{C}$   
 4 h condensation with uninsulated black panel temperature controlled at  $50 \pm 3^\circ\text{C}$   
 (Typically used for some plastic building products)

7.3 Practice G154 lists several other exposure cycles that are used for fluorescent UV exposures of nonmetallic materials. Obtain mutual agreement between all concerned parties for the specific exposure cycle used.

7.4 In order to minimize any effects from temperature or UV light variation, reposition the specimens as follows. Fig. 2 shows a diagram of the specimen repositioning.

7.4.1 Reposition the specimens horizontally to ensure that each specimen spends the same amount of exposure time in each horizontal position within the specimen holder by (1) moving the two extreme right-hand holders to the far left of the exposure area, and (2) sliding the remaining holders to the right.

7.4.2 Reposition the specimens vertically so that each specimen spends the same amount of exposure time in each vertical position within the specimen holder. For instance, if two specimens are stacked vertically in each holder, then the top and bottom specimens should switch places halfway through the test. If four specimens are stacked vertically, then the specimens should be repositioned vertically three times during the test.

7.5 *Water Purity*—The purity of water used for specimen spray is very important. Follow the purity requirements in Practice G151 for water sprayed on specimen surfaces. It is recommended that deionized water be used for water used to produce condensation.

7.6 It is recommended that a control material be exposed at the same time as the test specimens for comparison purposes, if performance comparisons are not being made between the test materials themselves. All concerned parties must agree on the control material used.

7.6.1 Identification of any control specimen used shall accompany the report.

## 8. Periods of Exposure and Evaluation of Test Results

8.1 In most cases, periodic evaluation of test and control materials is necessary to determine the variation in magnitude and direction of property change as a function of exposure time or radiant exposure.

8.2 The time or radiant exposure necessary to produce a defined change in a material property can be used to evaluate