

Third edition
2006-04-15

Corrected version
2006-08-01

**Injection equipment for medical use —
Part 1:
Ampoules for injectables**

Matériel d'injection à usage médical —

Partie 1: Ampoules pour produits injectables

**iTeh STANDARD PREVIEW
(standards.iteh.ai)**

ISO 9187-1:2006

<https://standards.iteh.ai/catalog/standards/sist/bf4b76e3-fef7-49de-8ea9-4ab466e9716e/iso-9187-1-2006>



Reference number
ISO 9187-1:2006(E)

© ISO 2006

PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 9187-1:2006

<https://standards.iteh.ai/catalog/standards/sist/bf4b76e3-fef7-49de-8ea9-4ab466e9716e/iso-9187-1-2006>

© ISO 2006

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 9187-1 was prepared by Technical Committee ISO/TC 76, *Transfusion, infusion and injection equipment for medical and pharmaceutical use*.

This third edition cancels and replaces the second edition (ISO 9187-1:2000), which has undergone a minor revision with the addition of footnote a) in Table 1.

ISO 9187 consists of the following parts, under the general title *Injection equipment for medical use*:

- Part 1: Ampoules for injectables
- Part 2: One-point-cut (OPC) ampoules

This corrected version of ISO 9187-1:2006 incorporates the correction of Table 1 on page 4.

Introduction

Ampoules are suitable packaging materials for storing pharmaceutical products until they are administered to the patient. Owing to the direct contact between injectables and the primary container over extended storage periods, possible interactions are avoided in order to guarantee patient safety. Adequate means to achieve this objective include proper selection of primary packaging materials, the choice of suitable package design and the availability of specific requirements and methods for testing individual container systems.

In the past, four standardized forms of ampoule (forms A, B, C and D) have been in widespread use. However, form A is no longer used in the pharmaceutical industry and consequently has not been included in this part of ISO 9187. To avoid any confusion among manufacturers and users, it was decided to retain the same designation letters (i.e. B, C and D) for the forms of ampoules in current use, and to disregard the letter A.

iTeh STANDARD PREVIEW (standards.iteh.ai)

ISO 9187-1:2006

<https://standards.iteh.ai/catalog/standards/sist/bf4b76e3-fef7-49de-8ea9-4ab466e9716e/iso-9187-1-2006>

Injection equipment for medical use —

Part 1: Ampoules for injectables

1 Scope

This part of ISO 9187 specifies materials, dimensions, capacities, performance and packaging requirements for three forms of glass ampoule (forms B, C and D) for injectable pharmaceutical products.

It is applicable to ampoules with and without a colour break-ring.

The provision of ampoules with a colour break-ring, and the choice of colour of the break-ring, is subject to agreement between the manufacturer and user.

Ampoules complying with this part of ISO 9187 are intended for single use only.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 720, *Glass — Hydrolytic resistance of glass grains at 121 °C — Method of test and classification*

ISO 1101, *Geometrical Product Specifications (GPS) — Geometrical tolerancing — Tolerances of form, orientation, location and run-out*

ISO 2859-1, *Sampling procedures for inspection by attributes — Part 1: Sampling schemes indexed by acceptance quality limit (AQL) for lot-by-lot inspection*

ISO 4802-1, *Glassware — Hydrolytic resistance of the interior surfaces of glass containers — Part 1: Determination by titration method and classification*

ISO 4802-2, *Glassware — Hydrolytic resistance of the interior surfaces of glass containers — Part 2: Determination by flame spectrometry and classification*

ISO 7500-1, *Metallic materials — Verification of static uniaxial testing machines — Part 1: Tension/compression testing machines — Verification and calibration of the force-measuring system*

3 Dimensions and designation

3.1 Dimensions

The dimensions of ampoules shall be as shown in Figures 1, 2 and 3 (forms B, C and D respectively) and as given in Table 1.

3.2 Designation

Designation of ampoules shall consist of the descriptor word "ampoule", followed by a reference to this part of ISO 9187, followed by the ampoule form, the nominal volume, the colour of the glass and, if applicable, mention of a colour break-ring.

EXAMPLE 1 Designation of a form B ampoule without colour break-ring with a nominal volume of 10 ml, made of colourless glass (cl) complying with the requirements of this part of ISO 9187:

Ampoule ISO 9187-1 – B – 10 – cl

EXAMPLE 2 Designation of a form B ampoule with a colour break-ring (cbr) with a nominal volume of 10 ml, made of colourless glass (cl) complying with the requirements of this part of ISO 9187:

Ampoule ISO 9187-1 – B – 10 – cl – cbr

4 Material

Colourless (cl) or amber (br) glass of hydrolytic resistance grain class ISO 720 – HGA 1 shall be used.

A change in the chemical composition of the glass material should be notified by the tube manufacturer to the user at least nine months in advance.

5 Requirements

iTeh STANDARD PREVIEW
(standards.iteh.ai)

5.1 Hydrolytic resistance

When tested in accordance with ISO 4802-1 and ISO 4802-2, the hydrolytic resistance of the internal surface of ampoules shall comply with the requirements specified for hydrolytic resistance container class ISO 4802-HC 1.


5.2 Annealing quality

Ampoules shall be annealed; the maximum residual stress of uncoloured ampoules after annealing shall not produce an optical retardation exceeding 50 nm per millimetre of glass thickness.

5.3 Breaking force

It is presumed that the ampoules to be tested are provided with a predetermined breaking point, such as a ceramic ring, at the constriction.

When tested in accordance with Clause 6, the breaking force shall be as specified in Table 2.

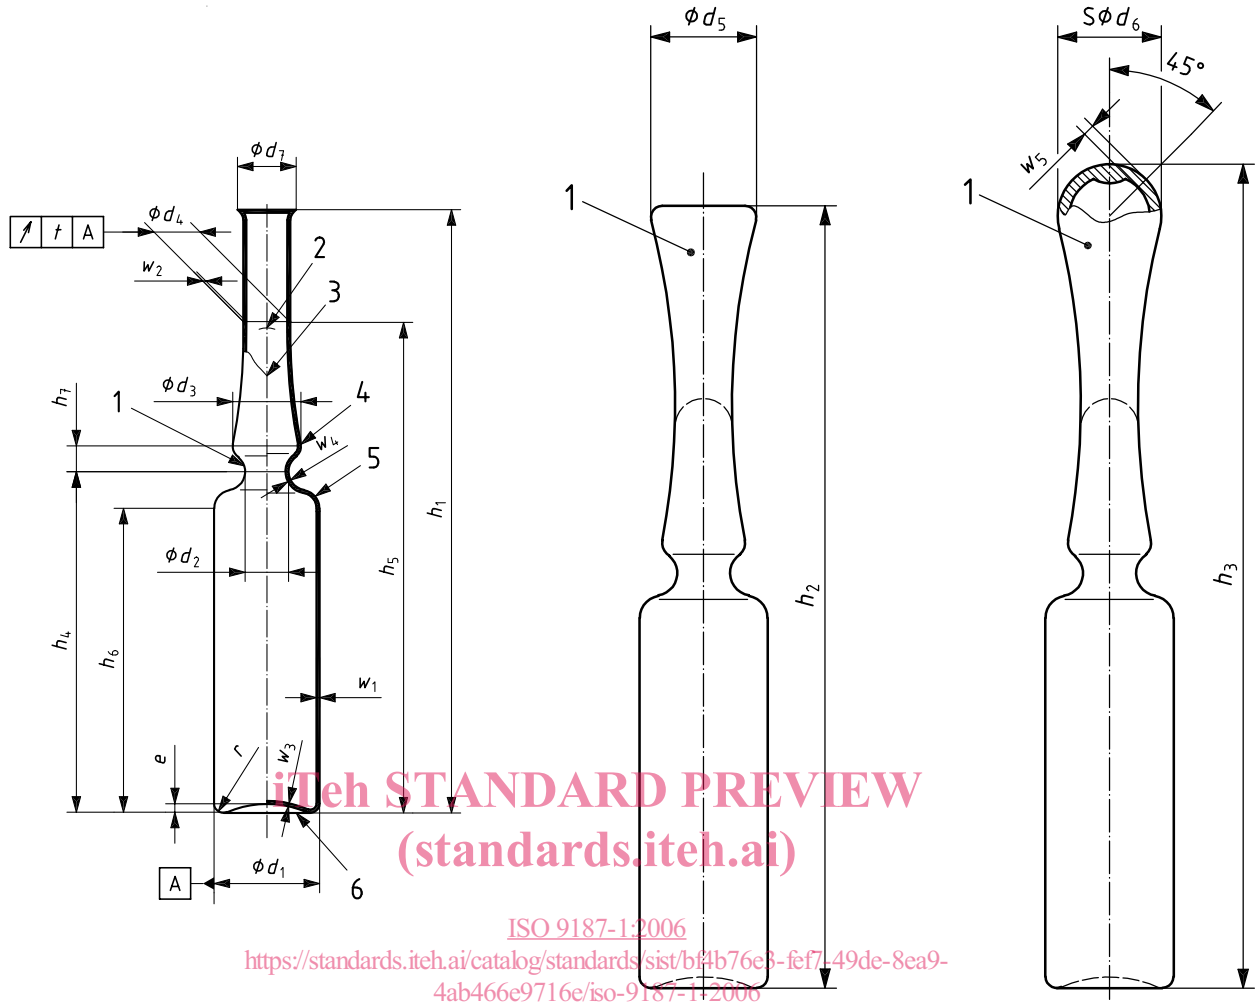

- Key**
- 1 constriction
 - 2 sealing point
 - 3 stem
 - 4 bulb
 - 5 shoulder
 - 6 base or bottom

- Key**
- 1 funnel

- Key**
- 1 dome

NOTE For other dimensions, see Figure 1.

NOTE For other dimensions, see Figure 1.

NOTE For dimensions of parameters, see Table 1.

Figure 1 — Form B: stem, cut ampoule with constriction

Figure 2 — Form C: stem, open-funnel ampoule with constriction

Figure 3 — Form D: stem, sealed ampoule with constriction

Table 1 – Dimensions of ampoules

Dimensions in millimetres

Dimension		Nominal volume ml								
		1	2	3	5	10	20	25	30	
External diameter	Body d_1^a	tol.	10,75	10,75	12,75	14,75	17,75	22,5	22,5	22,5
			± 0,15	± 0,15	± 0,15	± 0,15	± 0,20	± 0,25	± 0,25	± 0,25
	Constriction d_2^b	tol.	6,5	6,5	6,5	7	7,5	8,5	8,5	8,5
			± 0,5	± 0,5	± 0,5	± 0,5	± 0,5	± 0,5	± 0,5	± 0,5
	Bulb d_3	tol.	8,5	8,5	8,5	9	9,5	12	12	12
			± 0,5	± 0,5	± 0,5	± 0,5	± 0,5	± 1	± 1	± 1
	Stem d_4	tol.	6	6	6	7	7,1	7,8	7,8	7,8
		± 0,35	± 0,35	± 0,35	± 0,35	± 0,35	± 0,5	± 0,5	± 0,5	
Funnel d_5^c	tol.	9	9	10,7	12,2	13	14	14	14	
		± 0,8	± 0,8	± 0,8	± 1	± 1	± 1	± 1	± 1	
Dome d_6^c	tol.	10	10	10,5	12	13,5	13,5	13,5	13,5	
		± 1	± 1	± 1	± 1	± 1	± 1	± 1	± 1	
Flared end d_7	tol.	8	8	8	9	9,5	11	11	11	
		± 1	± 1	± 1	± 1	± 1	± 1	± 1	± 1	
Overall height	Form B h_1	tol.	60	72	75	83	102	113	128	143
			± 1	± 1	± 1	± 1	± 1	± 1	± 1	± 1
	Form C h_2	tol.	67	79	82	90	109	120	135	150
		± 1	± 1	± 1	± 1	± 1	± 1,5	± 1,5	± 1,5	
Form D h_3	tol.	70	83	89	95	112	126	141	156	
		± 1	± 1	± 1	± 1	± 1	± 1	± 1	± 1	
Height	Height to constriction h_4	tol.	25,5	37,5	39,5	46,5	62	76	91	106
			± 0,5	± 0,5	± 0,5	± 0,5	± 1	± 1,3	± 1,3	± 1,3
	Height to gauging point h_5	tol.	47	57	62	68	87	100	115	130
			± 2	± 2	± 2	± 2	± 2	± 2	± 2	± 2
Body height h_6	min.	21	33	35	41	55	65	80	95	
Centre of constriction to bulb h_7	max.	4,5	4,5	5	5,5	6	6,5	6,5	6,5	
Base	Radius r	tol.	1	1	1,5	1,5	2	2,5	2,5	2,5
			± 0,5	± 0,5	± 0,5	± 0,5	± 0,5	± 0,5	± 0,5	± 0,5
	Depth of the base e	tol.	1	1	1	1	1,25	1,5	1,5	1,5
			± 0,5	± 0,5	± 0,5	± 0,5	± 0,75	± 1	± 1	± 1
Wall thickness	Glass thickness of body w_1	tol.	0,5	0,5	0,5	0,55	0,6	0,7	0,7	0,7
			± 0,03	± 0,03	± 0,03	± 0,03	± 0,04	± 0,04	± 0,04	± 0,04
	Glass thickness of stem at gauging w_2	tol.	0,37	0,37	0,37	0,40	0,47	0,50	0,50	0,50
			± 0,05	± 0,05	± 0,05	± 0,05	± 0,05	± 0,05	± 0,05	± 0,05
	Glass thickness at base w_3	min.	0,3	0,3	0,3	0,4	0,4	0,5	0,5	0,5
	Glass thickness of constriction w_4	tol.	0,7	0,7	0,7	0,7	0,8	1	1	1
			± 0,1	± 0,1	± 0,1	± 0,15	± 0,15	± 0,2	± 0,2	± 0,2
Glass thickness of dome w_5		0,1 to 0,25					0,1 to 0,30			
Circular run-out tolerance t^d		0,6	0,6	0,8	1	1	1,2	1,2	1,2	
Volume to centre of constriction V	ml ≈	1,5	2,3	3,5	5,5	11,5	23,5	28,5	33,5	

^a The deviation from the perpendicularity between bottom and length axis at the body outside diameter shall not exceed an angle of 2°.
^b If there is a need to reduce the constriction diameter, e.g. due to reducing of particles, it shall be agreed between manufacturer and purchaser.
^c No point of the funnel and the dome shall be outside of the body diameter.
^d The run-out tolerance shall be measured at the sealing point (according to ISO 1101).

Table 2 — Breaking force

Nominal volume	Length $l (= l_1 + l_2)$ mm	Breaking force	
		$F_{\min.}$ N	$F_{\max.}$ N
1	36 (= 18 + 18)	30	80
2			
3			
5			
10	60 (= 22 + 38)	30	90
20			
25			
30			100

6 Test for breaking force

6.1 Principle

The test is suitable for determining the force required to separate the ampoule stem from the body and for assessing whether a clean break is obtained.

6.2 Apparatus

6.2.1 Tensile testing machine

The tensile testing machine shall be in accordance with ISO 7500-1 and have the following characteristics:

- a test speed, v , of 10 mm/min, and
- a measuring range for force of 200 N.

NOTE Other test procedures, e.g. with a power increase of 20 N/s, are admissible if equivalent results can be obtained.

An example of the test set-up is illustrated in Figure 4.

6.3 Sampling

6.3.1 Number of samples

Random sampling in accordance with ISO 2859-1 (inspection level S-4) is recommended.

6.3.2 Conditioning of samples

The temperature of the samples shall be $20\text{ °C} \pm 5\text{ °C}$.

6.4 Procedure

Set the distance between the metal bars, as shown in Figure 4, so that the force is imparted on the middle of the bars at an angle of 90° to the axis of the ampoule.

Apply the force using the tensile testing machine to rupture. Record the breaking force.