

---

---

**Anaesthetic vaporizers — Agent-specific  
filling systems**

*Évaporateurs d'anesthésie — Systèmes de remplissage spécifiques à  
l'agent*

**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

[ISO 5360:2006](https://standards.iteh.ai/catalog/standards/sist/c6280d74-4623-4d08-82a5-e92ce3c120ed/iso-5360-2006)

[https://standards.iteh.ai/catalog/standards/sist/c6280d74-4623-4d08-82a5-  
e92ce3c120ed/iso-5360-2006](https://standards.iteh.ai/catalog/standards/sist/c6280d74-4623-4d08-82a5-e92ce3c120ed/iso-5360-2006)



**PDF disclaimer**

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

[ISO 5360:2006](#)

<https://standards.iteh.ai/catalog/standards/sist/c6280d74-4623-4d08-82a5-e92ce3c120ed/iso-5360-2006>

© ISO 2006

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Case postale 56 • CH-1211 Geneva 20  
Tel. + 41 22 749 01 11  
Fax + 41 22 749 09 47  
E-mail [copyright@iso.org](mailto:copyright@iso.org)  
Web [www.iso.org](http://www.iso.org)

Published in Switzerland

## Contents

Page

Foreword.....	iv
<b>1 Scope .....</b>	<b>1</b>
<b>2 Normative references .....</b>	<b>1</b>
<b>3 Terms and definitions.....</b>	<b>1</b>
<b>4 Bottle .....</b>	<b>2</b>
<b>5 Bottle collar .....</b>	<b>4</b>
<b>6 Bottle adaptor.....</b>	<b>8</b>
<b>7 Filler receptacle.....</b>	<b>12</b>
<b>8 Filling rate .....</b>	<b>14</b>
<b>9 Leakage.....</b>	<b>16</b>
<b>10 Overfilling protection.....</b>	<b>16</b>
<b>11 Colour coding.....</b>	<b>16</b>
<b>12 Information provided by the manufacturer.....</b>	<b>16</b>
<b>Annex A (informative) Types of agent-specific filling systems.....</b>	<b>18</b>
<b>Annex B (normative) Determination of total leakage into atmosphere of anaesthetic agent during filling.....</b>	<b>19</b>
<b>Bibliography .....</b>	<b>21</b>

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 5360 was prepared by Technical Committee ISO/TC 121, *Anaesthetic and respiratory equipment*, Subcommittee SC 1, *Breathing attachments and anaesthetic machines*.

This second edition cancels and replaces the first edition (ISO 5360:1993) which has been technically revised by virtue of incorporation of Technical Corrigendum 1:1998, inclusion of the changes presented and approved for ISO 5360:1993/Amd 1 (not published) and the need to update cross-references and other factual matters due to the passage of time.

[ISO 5360:2006](https://standards.iteh.ai/catalog/standards/sist/c6280d74-4623-4d08-82a5-e92ce3c120ed/iso-5360-2006)

<https://standards.iteh.ai/catalog/standards/sist/c6280d74-4623-4d08-82a5-e92ce3c120ed/iso-5360-2006>

# Anaesthetic vaporizers — Agent-specific filling systems

## 1 Scope

This International Standard specifies the dimensions of agent-specific filling systems for agent-specific anaesthetic vaporizers.

This International Standard does not specify construction materials. Materials used for the parts of filling systems which come into contact with liquid anaesthetic agent should be selected with regard to:

- a) toxicity;
- b) compatibility with anaesthetic agents;
- c) minimization of health risks due to substances leached from the materials.

Because of the unique properties of desflurane, dimensions for this agent have not been specified in this International Standard.

NOTE Designs of connection systems are encouraged which only permit engagement of the agent-specific bottle adaptor to the bottle when the bottle collar is in place.

[ISO 5360:2006](https://standards.iteh.ai/catalog/standards/sist/c6280d74-4623-4d08-82a5-e92ce3c120ed/iso-5360-2006)

<https://standards.iteh.ai/catalog/standards/sist/c6280d74-4623-4d08-82a5-e92ce3c120ed/iso-5360-2006>

## 2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 1101:2004, *Geometrical Product Specifications (GPS) — Geometrical tolerancing — Tolerances of form, orientation, location and run-out*

## 3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

### 3.1

#### **agent-specific**

having both a prescribed configuration and prescribed dimensions, which are specific for a prescribed liquid anaesthetic agent

### 3.2

#### **agent-specific filling system**

functional system of agent-specific coded connections between an anaesthetic bottle and an agent-specific anaesthetic vaporizer, consisting of, for example, a threaded bottle neck with collar, bottle connector, male adaptor and filler receptacle

NOTE Different types of agent-specific filling systems are shown in Annex A.

- 3.3 anaesthetic vaporizer**  
device designed to facilitate the change of an anaesthetic agent from a liquid to a vapour
- 3.4 bottle adaptor**  
assembly that is intended to connect a bottle for liquid anaesthetic agent to an agent-specific anaesthetic vaporizer
- 3.5 bottle collar**  
agent-specific component on the neck of a bottle causing it to be agent-specific
- 3.6 bottle connector**  
agent-specific component that fits the thread on the bottle neck and mates with the agent-specific bottle collar
- 3.7 bottle neck**  
external threaded part of the bottle and the adjacent contour over which an agent-specific collar is fitted
- 3.8 filler receptacle**  
receptacle for a bottle or a bottle adaptor on an agent-specific anaesthetic vaporizer
- 3.9 male adaptor**  
part of a bottle adaptor that mates with a filler receptacle on an agent-specific vaporizer


iTeh STANDARD PREVIEW  
(standards.iteh.ai)

## 4 Bottle

ISO 5360:2006  
<https://standards.iteh.ai/catalog/standards/sist/c6280d74-4623-4d08-82a5-e92ce3c120ed/iso-5360-2006>

Each bottle shall have:

- a) the name of the anaesthetic agent, with which it is intended to be used, marked on it;
- b) either a bottle collar complying with Clause 5 and a threaded neck complying with Figure 1 and Table 1, or a permanently attached bottle adaptor complying with 6.2.

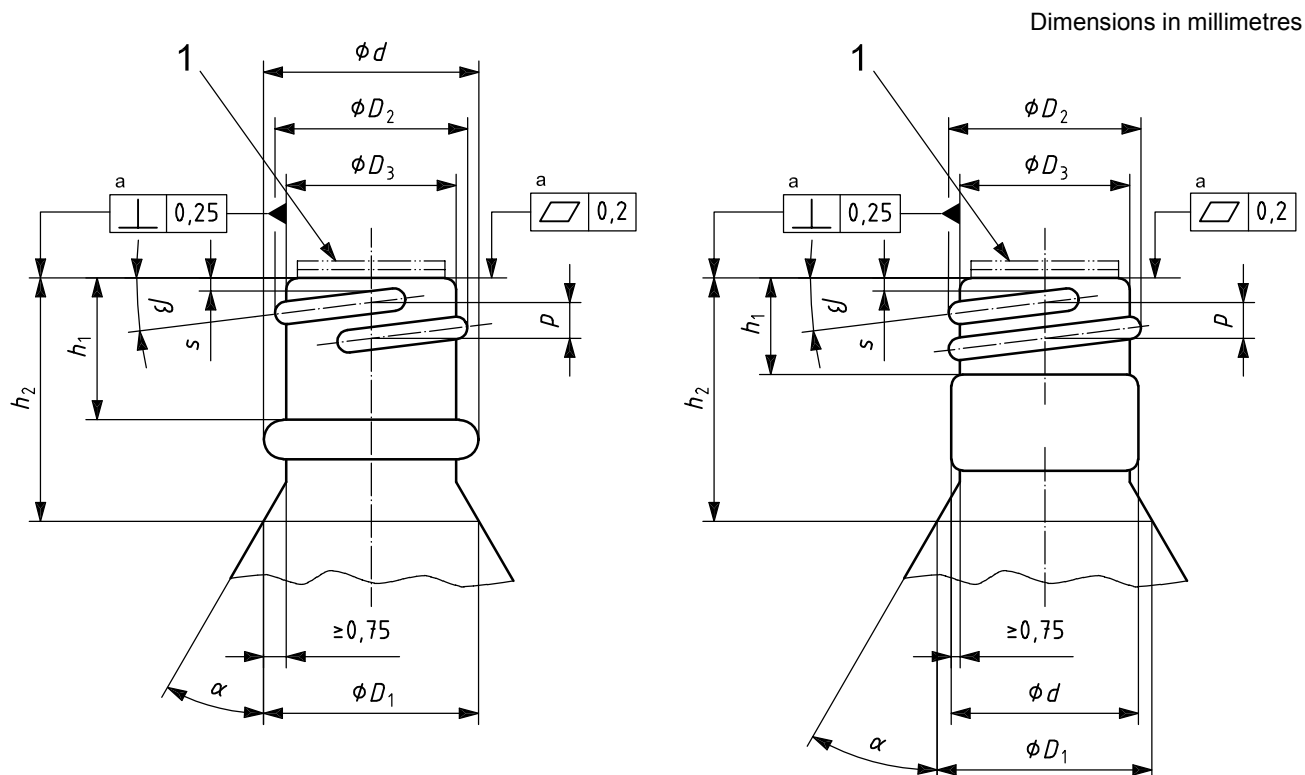

**Key**

1 optional pouring lip (not dimensioned)

a Flatness and perpendicularity tolerances in accordance with ISO 1101.

NOTE The dimensions shown form part of this International Standard. Other features are for illustrative purposes only. See also Table 1.

**Figure 1 — Two examples of threaded necks of bottles for anaesthetic agents**

**Table 1 — Dimensions of threaded necks of bottles for anaesthetic agents (see also Figure 1)**

Bottle type	Anaesthetic agent	$h_1$ $\pm 0,3$ mm	$h_2^a$ min. mm	$s$ $\pm 0,45$ mm	$\beta$	$\alpha$ min. at $\phi D_1$	$p$ mm	Thread turns min.	$D_1^a$ nom. mm	$D_2^b$ $\pm 0,3$ mm	$D_3^b$ $\pm 0,3$ mm	$d$ max. mm.
1	Isoflurane Enflurane	9,75	23	1,2	2° 35'	30°	3,2	1	28	23,6	21,5	28
2	Halothane	6,8	18,7	1,2	2° 15'	30°	2,54	1,25	24	21,45	19,7	28
3	Halothane (North America)	15	26,3	1	2° 50'	30°	3,2	1,75	24	21,7	19,5	28
4	Spare	9,05	20	1,15	3° 30'	30°	3,2	1,25	20	17,65	15,5	28
5	Spare	9,05	20	1,15	3° 7'	30°	3,2	1,25	22	19,65	17,5	28
6	Methoxy-flurane	9,8	20	1,15	2° 57'	30°	4,25	1,25	30	27,3	24,9	32
7	Spare	9,85	20	1,15	2° 31'	30°	4,25	1,25	34	31,8	29,4	32
8	Sevoflurane	8,9	23,9	1,3	2° 56'	30°	3,63	1,25	23,9	23,5	21,5	28

<sup>a</sup> Recommended values.

<sup>b</sup> Summation of the tolerances of measures  $D_2$  and  $D_3$  shall be avoided. A maximum tolerance of  $\pm 0,3$  mm for  $(D_2 - D_3)$  should be required to avoid problems with the fitting of any bottle connector.


**5 Bottle collar**

5.1 Bottle collars shall comply with the configuration and dimensions shown in Figure 2 and angle  $\theta$  specified in Table 2 for the anaesthetic agent with which it is intended to be used.

5.2 The position of the bottle collar relative to the screw thread of the bottle shall be as shown in Figure 3.

5.3 The bottle collar shall be attached to the bottle and shall be rotatable by hand.


Dimensions in millimetres

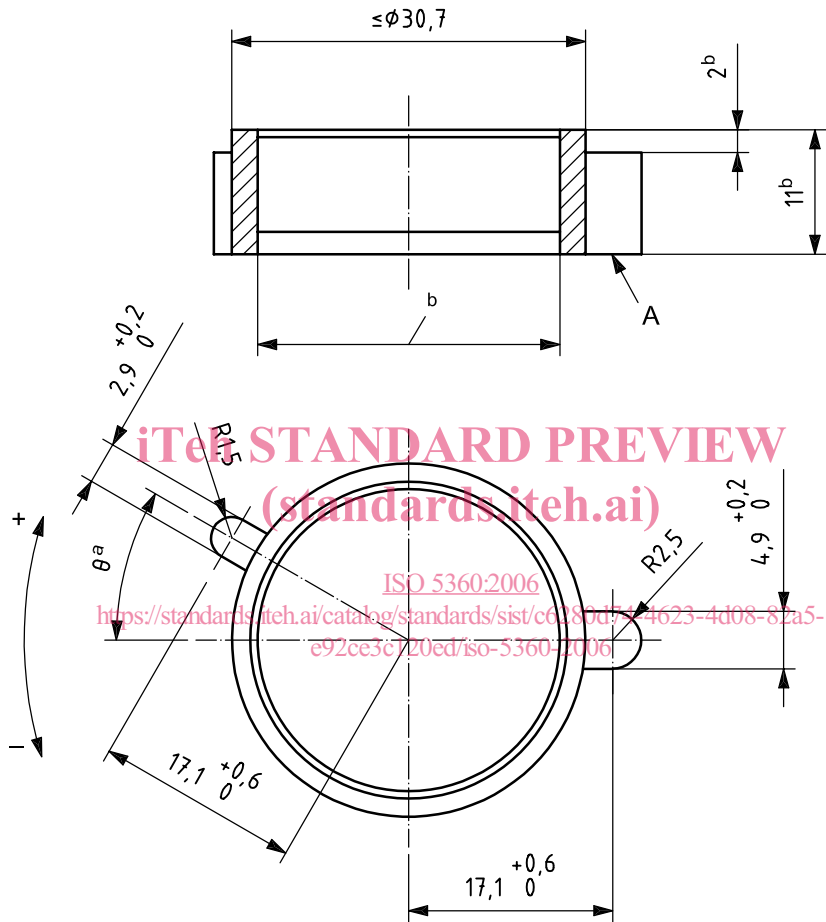

a) Bottle collar for small bottles, i.e. types 1 to 5 and 8



Dimensions in millimetres

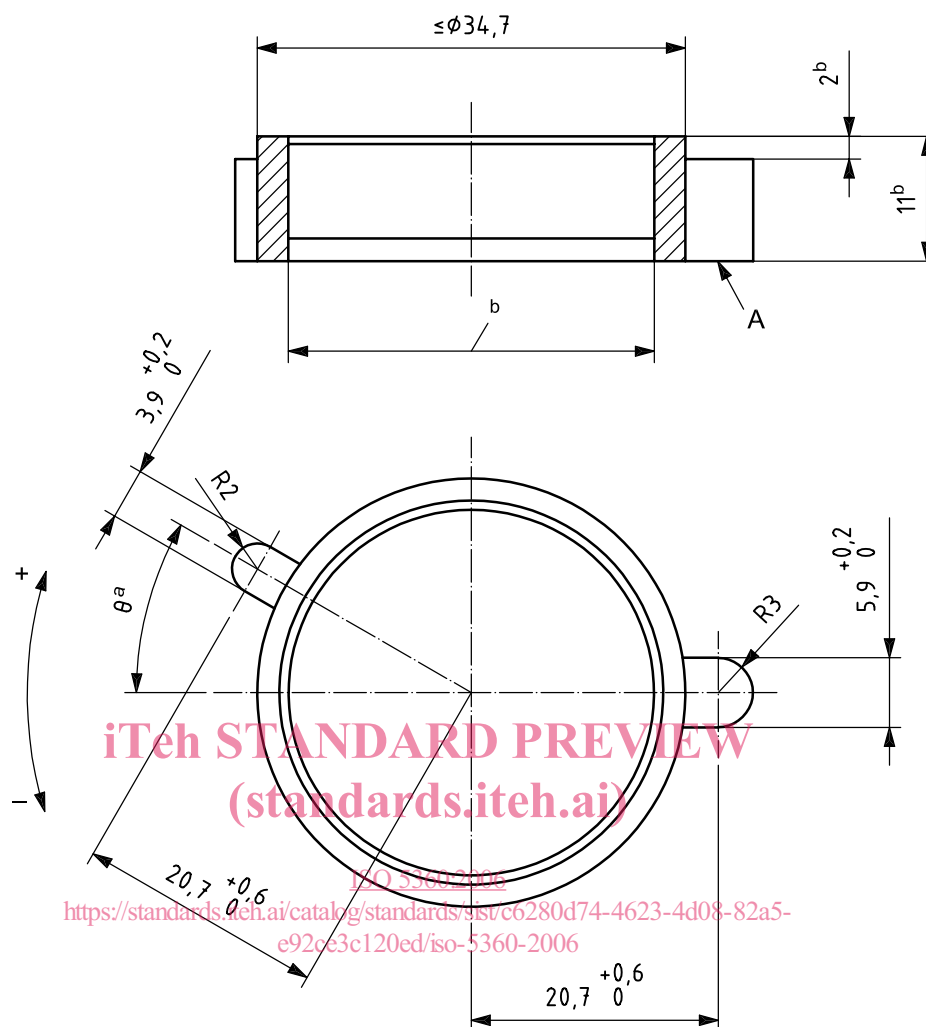

b) Bottle collar for large bottles, i.e. types 6 and 7

A = Face A

<sup>a</sup> See Table 2.

<sup>b</sup> May vary to suit bottle.

Figure 2 — Configuration of agent-specific bottle collars

Table 2 — Dimensions and colours of agent-specific bottle collars and connectors

Anaesthetic agent	$\theta^a$ $\pm 0^\circ 30'$	Specified colour <sup>b</sup>	Example of colour samples					
			Federal Standard 595:1994 colour	BS 5252 colour	Pantone colour	SS 01 91 02: 2004 colour	Munsell colour <sup>c</sup>	DIN 6164 colour
Halothane	- 20°	Red	11 105	04 E 56	200 C	NCS S 1080 R	5R4/14	8:7:2
Enflurane	+ 20°	Orange	22 510	06 E 55	151 C	NCS S 0585-Y50R	2,5YR 6/16	5:5:1
Methoxy-flurane	0°	Green	14 187	14 E 53	334 C	NCS S 2060-B90G	10G 5/10	21:6:3
Desflurane	N.S. <sup>d</sup>	Blue	n.a. <sup>e</sup>	18 E 53	3015 C	NCS S 3060 B	10B 4/10	18:4:3
Not for agent identification		White	37 875	18 B 15	5455 C	NCS S 0502-B	10B 9/1	N:0:0.5
Not for agent identification		Black	15 042	00 E 53	Process black C	NCS S 9000-N	N 0,5	N:0:9
Sevoflurane	+ 50°	Yellow	n.a. <sup>e</sup>	10 E 53	108 C	NCS S 0570-Y	6,25Y 8,5/12	2:6:1
Isoflurane	- 40°	Purple	n.a. <sup>e</sup>	24 E 53	254 C	NCS S 3055-R50B	7,5P4/12	11:4:4
Spare		Grey	16 251	00 A 09	Cool grey 9 C	NCS S 5502 B	5PB 5/1	N:0:4

<sup>a</sup> Sign "+" means clockwise rotation and sign "-" means anticlockwise rotation, when viewed from the top.


<sup>b</sup> If a colour is used on a vaporizer, bottle or package label to facilitate correct identification, it is important that only the colour for the appropriate anaesthetic agent be used.

<sup>c</sup> Munsell colour is the original. Other colour systems show nearest available colour sample.


<sup>d</sup> N.S. = not specified.

<sup>e</sup> n.a. = not available.

Dimensions in millimetres

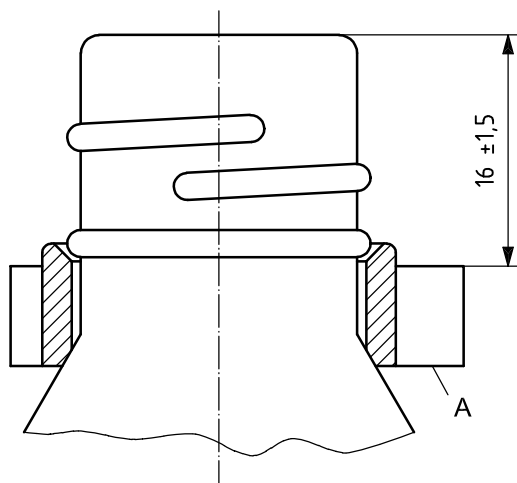

a) Position without clearance between collar and transfer ring

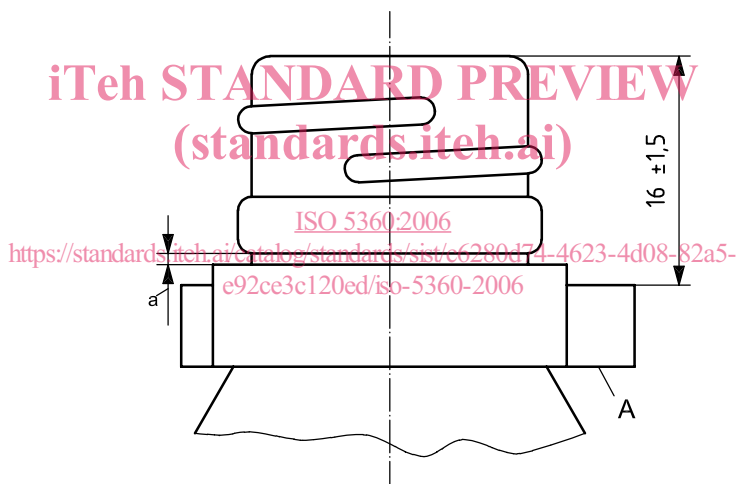

b) Position with clearance between collar and transfer ring

A = Face A (see Figure 2)

<sup>a</sup> Clearance to suit bottle.

Figure 3 — Alternative positions of agent-specific bottle collar