



SLOVENSKI STANDARD

SIST EN 50147-1:1997

01-marec-1997

Gluhe sobe - 1. del: Meritev dušenja oklopa

Anechoic chambers - Part 1: Shield attenuation measurement

Absorberräume - Teil 1: Schirmdämpfungsmessung

Chambres anéchoïques - Partie 1: Mesure d'atténuation de blindage

Ta slovenski standard je istoveten z: EN 50147-1:1996

[SIST EN 50147-1:1997](https://standards.iteh.ai/catalog/standards/sist/ea5f2ef2-e944-435b-9252-2ba3e9194f09/sist-en-50147-1-1997)

<https://standards.iteh.ai/catalog/standards/sist/ea5f2ef2-e944-435b-9252-2ba3e9194f09/sist-en-50147-1-1997>

ICS:

| | | |
|-----------|--|--|
| 17.220.01 | Elektrika. Magnetizem. Splošni vidiki | Electricity. Magnetism. General aspects |
| 29.020 | Elektrotehnika na splošno | Electrical engineering in general |

SIST EN 50147-1:1997

en

iTeh STANDARD PREVIEW
(standards.iteh.ai)

SIST EN 50147-1:1997

<https://standards.iteh.ai/catalog/standards/sist/ea5f2ef2-e944-435b-9252-2ba3e9194f09/sist-en-50147-1-1997>

EUROPEAN STANDARD
NORME EUROPÉENNE
EUROPÄISCHE NORM

EN 50147-1

March 1996

ICS 17.220.00; 29.020

Descriptors: Electromagnetic compatibility, measurements, tests, anechoic chambers, specifications

English version

Anechoic chambers
Part 1: Shield attenuation measurement

Chambres anéchoïques
Partie 1: Mesure d'atténuation
de blindage

Absorberräume
Teil 1: Schirmdämpfungsmessung

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[SIST EN 50147-1:1997](https://standards.iteh.ai/catalog/standards/sist/ea5f2ef2-e944-435b-9252-2ba3e9194f09/sist-en-50147-1-1997)

<https://standards.iteh.ai/catalog/standards/sist/ea5f2ef2-e944-435b-9252-2ba3e9194f09/sist-en-50147-1-1997>

This European Standard was approved by CENELEC on 1995-07-04. CENELEC members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration.

Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the Central Secretariat or to any CENELEC member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CENELEC member into its own language and notified to the Central Secretariat has the same status as the official versions.

CENELEC members are the national electrotechnical committees of Austria, Belgium, Denmark, Finland, France, Germany, Greece, Iceland, Ireland, Italy, Luxembourg, Netherlands, Norway, Portugal, Spain, Sweden, Switzerland and United Kingdom.

CENELEC

European Committee for Electrotechnical Standardization
Comité Européen de Normalisation Electrotechnique
Europäisches Komitee für Elektrotechnische Normung

Central Secretariat: rue de Stassart 35, B - 1050 Brussels

Foreword

This European Standard was prepared by working group WG 4 of CENELEC Technical Committee TC 210, EMC.

It was submitted to the CENELEC Unique Acceptance procedure (UAP) in August 1994 and was approved by CENELEC as EN 50147-1 on 1995-07-04.

The following dates were fixed:

- latest date by which the EN has to be implemented
at national level by publication of an identical
national standard or by endorsement (dop) 1996-09-01
- latest date by which national standards
conflicting with the EN have to be withdrawn (dow) 1996-09-01

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[SIST EN 50147-1:1997](https://standards.iteh.ai/catalog/standards/sist/ea5f2ef2-e944-435b-9252-2ba3e9194f09/sist-en-50147-1-1997)

<https://standards.iteh.ai/catalog/standards/sist/ea5f2ef2-e944-435b-9252-2ba3e9194f09/sist-en-50147-1-1997>

Contents

| | Page |
|--|------|
| Foreword | 2 |
| 1 Scope | 4 |
| 2 Normative references | 4 |
| 3 Definitions | 4 |
| 4 General points relating to shielding effectiveness | 4 |
| 4.1 Shielding | 4 |
| 4.2 Shield attenuation | 4 |
| 5 Shield attenuation measurement | 6 |
| 5.1 Test equipment | 6 |
| 5.2 Acceptance test | 7 |
| 5.3 Reference level | 9 |

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[SIST EN 50147-1:1997](https://standards.iteh.ai/catalog/standards/sist/ea5f2ef2-e944-435b-9252-2ba3e9194f09/sist-en-50147-1-1997)

<https://standards.iteh.ai/catalog/standards/sist/ea5f2ef2-e944-435b-9252-2ba3e9194f09/sist-en-50147-1-1997>

1 Scope

This standard applies to measurements of shielding attenuation of shielded enclosures (chambers, rooms) in the frequency range 9 kHz - 40 GHz. The object of this standard is to establish a common measurement procedure for validating the shielding effectiveness of a shielded enclosure.

2 Normative references

This European Standard incorporates by dated or undated reference, provisions from other publications. These normative references are cited at the appropriate places in the text and the publications listed hereafter. Dated references, subsequent amendments to or revisions of any of these publications apply to this European Standard only when incorporated in it by amendment or revision. For undated references the latest edition of the publication referred to applies.

| | | |
|-------------|------|---|
| IEC 50(161) | 1990 | International Electrotechnical Vocabulary (IEV) Chapter 161: Electromagnetic Compatibility |
|-------------|------|---|

3 Definitions

For the purposes of this standard the definitions contained in IEC 50(161) apply.

4 General points relating to shielding effectiveness

4.1 Shielding

Shield attenuation can be calculated only in ideal cases. The most significant factor is that the shielded enclosure should be homogeneous and consist of materials whose properties are defined in every respect. In practice, deviations from these conditions may be so great that the calculation results only in approximate values.

4.2 Shield attenuation

The shield attenuation is given by (see figure 1)

$$a_s = 20 \log(E_0 / E_1) \text{ for the electric field}$$

$$a_s = 20 \log(H_0 / H_1) \text{ for the magnetic field}$$



where:

a_s is the shield attenuation in dB.

E_0 and H_0 are the E and H field strengths at a location without shielding between the transmitting and receiving antennas (reference level).

E_1 and H_1 are the E and H field strengths at the same location as above with shielding between the transmitting and receiving antennas.

Figure 2 shows typical shield attenuation values of a state of the art shielded enclosure.

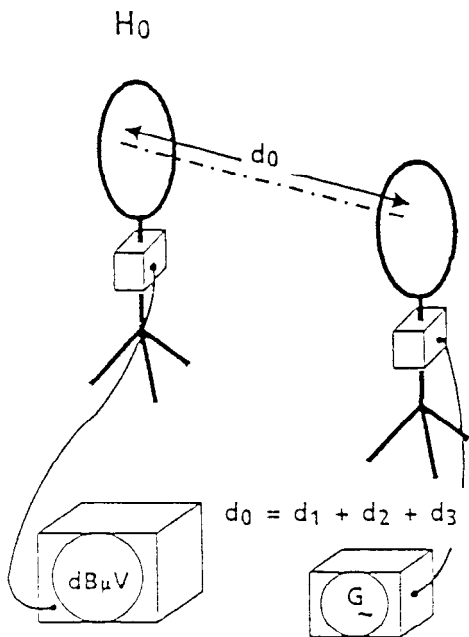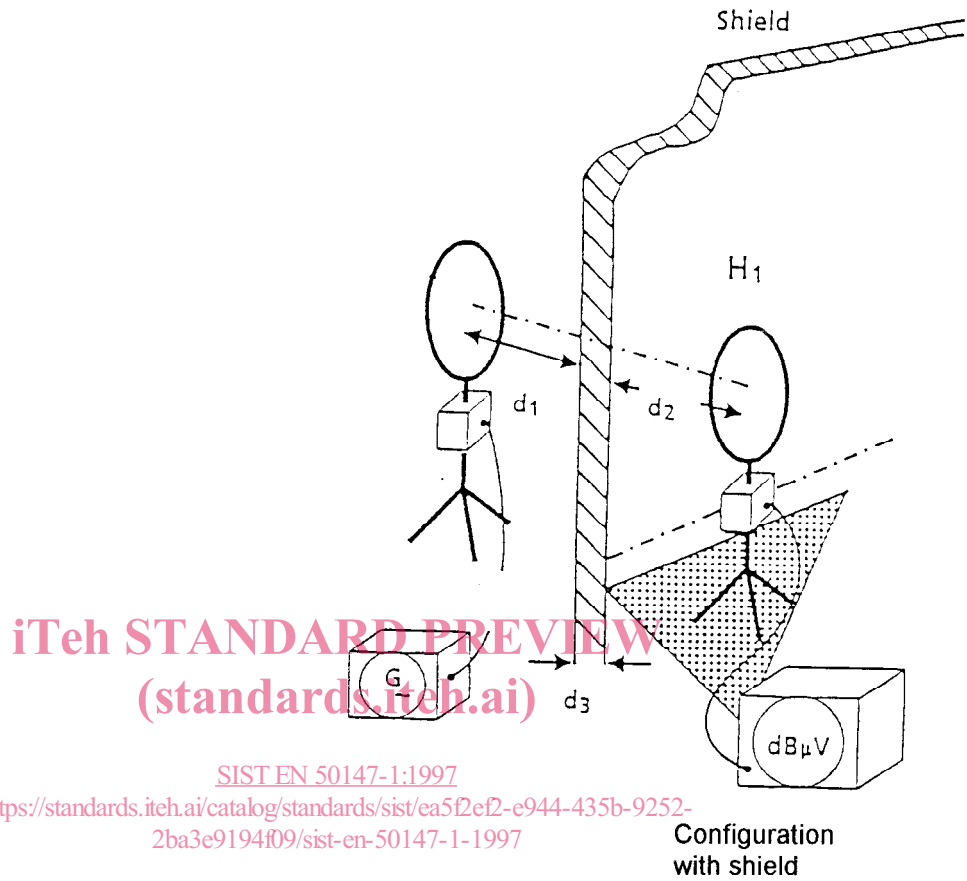


Reference configuration

$$a_s = 20 \log(H_0 / H_1)$$

analog

$$a_s = 20 \log(E_0 / E_1)$$

Figure 1: Shield attenuation

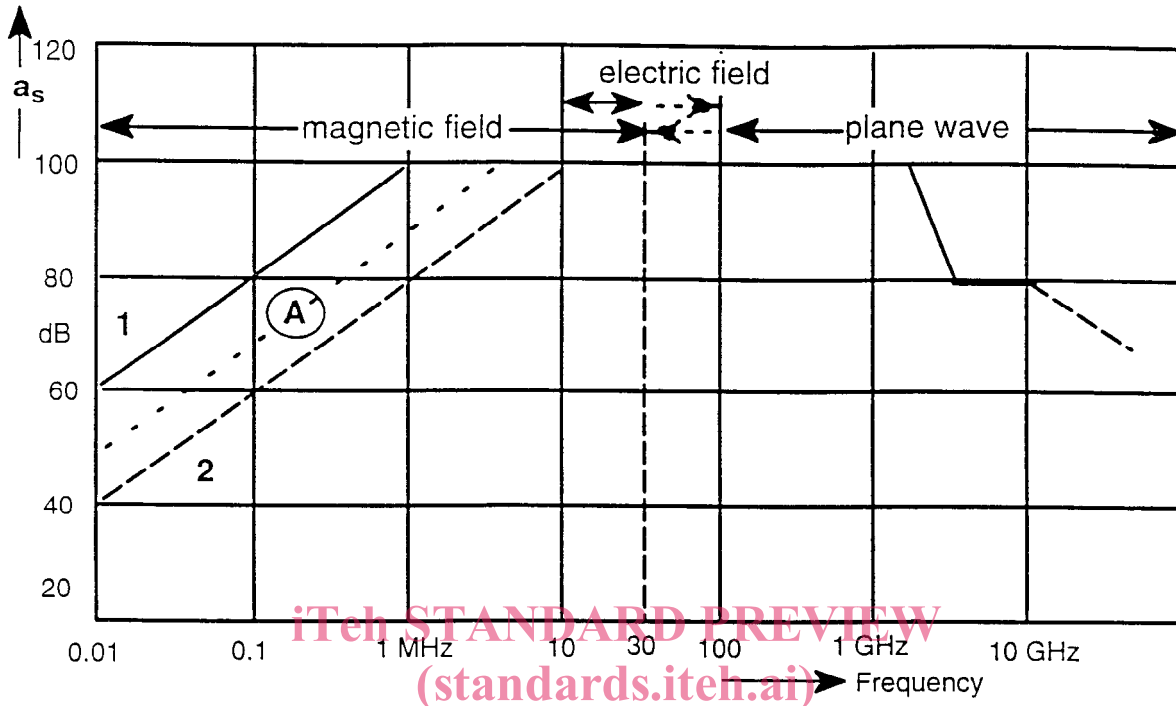

SIST EN 50147-1:1997
<https://standards.iteh.ai/catalog/standards/sist/ea5f2ef2-e944-435b-9252-2ba3e9194f09/sist-en-50147-1-1997>

a_s = shield attenuation in dB
 curve A = tolerated performance of the door seams for high performance shielded enclosure
 curve 1 = high performance of a shielded enclosure
 curve 2 = standard performance of a shielded enclosure

Figure 2: Typical shield attenuation values

5 Shield attenuation measurement

The measurement is normally carried out with all the shielding components in place and, in the case of filters, with all wires and cables connected.

NOTE: The procedure is derived from NSA 65-6-October 1964; National Security Agency Specification for R.F. Shielded Enclosures for Communication Equipment

5.1 Test equipment

The following types of equipment shall be used in performing the shield attenuation test, depending on the frequency range given in the specification of the enclosure. The measurement equipment shall have sufficient dynamic range to enable the test to be performed:

- a) CW signal sources covering 9 kHz to 40 GHz with adequate frequency stability. If unavailable in the microwave region (1 - 40 GHz), pulsed sources may be substituted;

NOTE: The starting frequency for shield attenuation measurements may be 10 kHz if the measurement equipment offers no other alternative.

- b) loop antennas for magnetic field measurements;
- c) tunable or broadband dipoles, monopoles with ground planes for electric field and plane wave measurements, and horn antennas for plane waves at microwave frequencies;
- d) probes for joint leakage tests;
- e) receivers with adequate sensitivity;

5.2 Acceptance tests

Acceptance tests shall be performed in accordance with the procedures described below and illustrated in figures 3 and 4.

Measurements shall be taken at several positions around the enclosure as given in the specification of the enclosure. In general, these measurements are made before absorber installation.

If the ambient noise level is low enough, all tests should be run with the receiver outside and the transmitter inside the enclosure.

5.2.1 Leakage test

Prior to acceptance tests leakage tests should be made all around the door frame, through accessible joints, around the filters and all around the air ducts. In addition, the magnitude and location of the maximum signal level emanating from the enclosure should be found by moving the antennas to at least four locations, preferably on different walls.

5.2.2 Electric and magnetic field measurements

Electric and magnetic field attenuation tests (reference measurements) shall be made with the antennas located directly opposite each other and separated by a distance shown in figures 3 and 4 plus the wall thickness.

Magnetic fields shall be measured with the loops parallel to a wall panel directly opposite each other.

Recommended test frequencies for magnetic fields are 10 kHz, 100 kHz, 1 MHz, 10 MHz and 30 MHz and 10 MHz and 30 MHz for electric field.

5.2.3 Plane wave measurements

Measurements shall be taken at the frequencies 100 MHz, 400 MHz, 1 GHz, 10 GHz and 40 GHz at least, depending on the frequency range given in the specification of the enclosure.

The test set-up is shown in figure 4.