



Designation: C408 – 88 (Reapproved 2006)

## Standard Test Method for Thermal Conductivity of Whiteware Ceramics<sup>1</sup>

This standard is issued under the fixed designation C408; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

*This standard has been approved for use by agencies of the Department of Defense.*

### 1. Scope

1.1 This test method covers a general procedure<sup>2</sup> for determining the thermal conductivity of whiteware ceramics over the temperature range from 100 to 300°F (40 to 150°C).

1.2 The values stated in inch-pound units are to be regarded as the standard. The SI (metric) units given in parentheses are for information purposes only.

1.3 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

### 2. Significance and Use

2.1 This test method provides information useful in understanding and quantifying such parameters as thermal shock resistance and ability to conduct or dissipate heat.

### 3. Apparatus

3.1 Essentially, the apparatus<sup>3</sup> shall consist of a heating unit, upper and lower copper “thermodes” (bars that serve to introduce heat) to which the ceramic test specimen is soldered, and a cooling jacket. The foregoing set of parts shall be enclosed by a 5-in. (127-mm) diameter brass cylinder, 12 in. (305 mm) long, which is sealed to the base with a rubber gasket. With the exception of the copper thermodes and the copper cooling jackets, the instrument shall be made entirely of brass with all joints silver soldered. During operation, the system shall be evacuated to a pressure of approximately 1  $\mu$ m

<sup>1</sup> This test method is under the jurisdiction of ASTM Committee C21 on Ceramic Whitewares and Related Products and is the direct responsibility of Subcommittee C21.03 on Methods for Whitewares and Environmental Concerns.

Current edition approved Feb. 15, 2006. Published February 2006. Originally approved in 1957. Last previous edition approved in 1999 as C408 – 88 (1999). DOI: 10.1520/C0408-88R06.

<sup>2</sup> This work was done under the sponsorship of the U.S. Signal Corps., Squier Signal Laboratory, Ft. Monmouth, NJ, and the U.S. Air Force, Wright-Patterson Air Development Center, OH.

<sup>3</sup> A suitable type of apparatus is described by Edwin Ruh in “Improved Method of Measuring Thermal Conductivity of Dense Ceramics,” *Journal, Am. Ceramic Society*, Vol 37, 1954, No. 5, pp. 224–229.

of mercury with an oil-diffusion pump which is backed up with a mechanical vacuum pump.

3.1.1 *Heating Unit*—The heating unit, shown in detail in Fig. 1, shall consist of a 500-W Nichrome element helically supported by ceramic insulators inside a 2-in. (50.8-mm) diameter brass cylinder. This brass cylinder shall be highly polished to serve also as a reflector, since heat transmission to the upper thermode is primarily by radiation. Line voltage to the heater circuit shall be held constant to within  $\pm 0.1\%$  by means of an electronic voltage regulator, and power input to the heater shall be controlled by a variable transformer.

3.1.2 *Thermodes*—The thermodes to which the ceramic test specimen is soldered shall be machined from electrolytically deposited pure copper to tolerances of  $\pm 0.001$  in. (0.03 mm) on diameters. Thermodes of diameters from 0.250 to 0.500 in. (6.50 to 12.70 mm) may be used, but in all cases the diameters of the specimen, and that portion of the upper and lower thermodes incorporating the thermocouple shall be equal in diameter to within  $\pm 0.001$  in. (0.03 mm). The section of the upper thermode above the upper cooling jacket shall be coated with carbon black to increase its emissivity.

3.1.3 *Cooling Jackets*—Details of the lower cooling jacket are shown in Fig. 1. The lower thermode makes contact with the lower cooling jacket by means of a tapered fit. The upper  $\frac{1}{8}$ -in. (3.2-mm) brass plate which supports the heating unit shall also be water-cooled for the purpose of eliminating radiation from the heating unit to the thermodes and test specimen below. In addition, the upper thermode shall be fitted with a copper reflecting shield to prohibit any direct radiation from striking the thermodes and specimen in the chamber below. A water-circulating system shall be provided for supplying the cooling jackets with water at constant pressure and temperature. The water temperatures shall not vary at a rate greater than 1°F (0.5°C)/h.

3.1.4 *Thermocouples*—Calibrated glass-asbestos insulated iron-constantan thermocouples shall be permanently attached to the thermodes in positions 1.75 in. (44.4 mm) apart as noted in Fig. 2. The diameter of the thermocouple wires used shall not exceed the diameter of No. 28 AWG (0.321 mm). The thermocouple wires shall be permanently attached to the thermode by silver-soldering each wire of the thermocouple

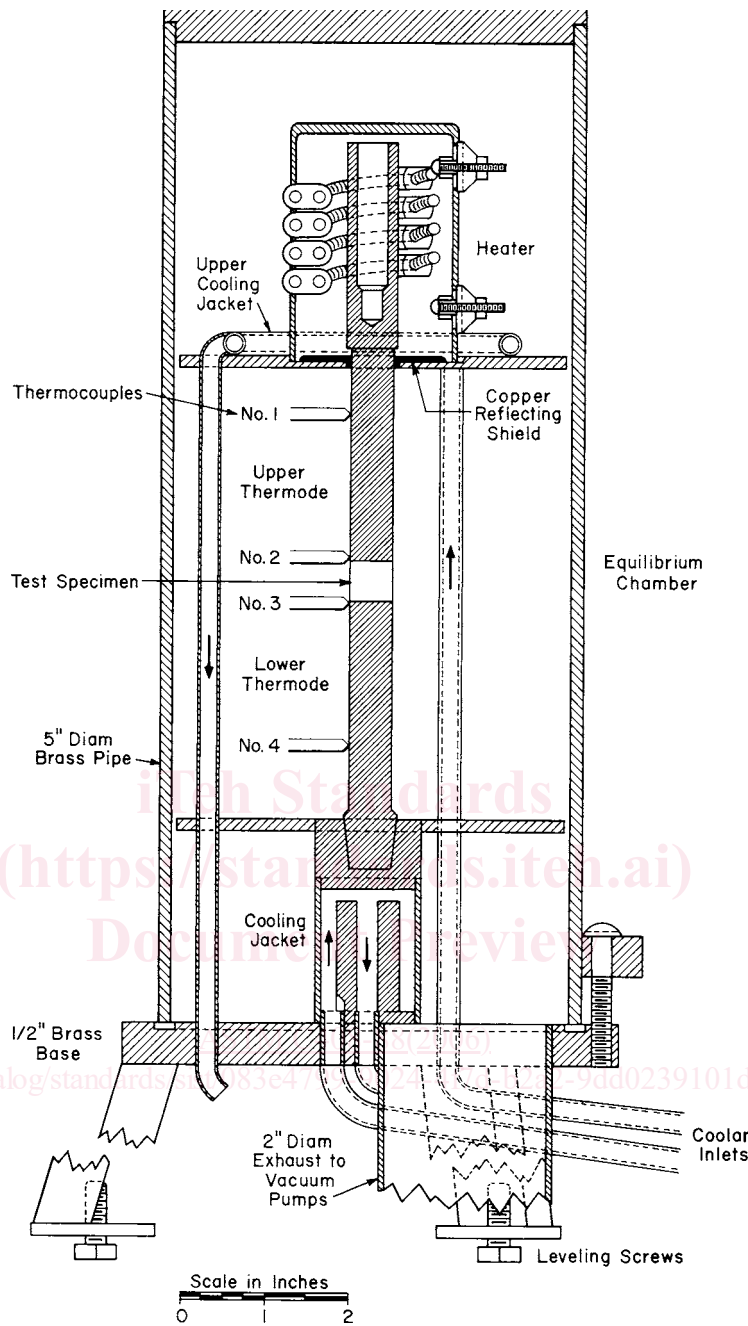


FIG. 1 Thermal Conductivity Apparatus

into No. 70 (0.028-in. diameter) (0.71-mm) holes drilled in the thermode to a depth of  $\frac{1}{32}$  in. (0.8 mm) on opposite ends of a diameter. All thermocouple wires shall be taken through the base plate without any break in the continuity of the wire. An ice-water bath shall be used for cold junction reference. The instrument for measuring emf shall not have an instrument error greater than  $\pm 0.001$  mV.

**4. Test Specimens**

4.1 The ceramic test specimens used in the thermal conductivity instrument shall be accurately ground cylinders. The specimens may be formed using normal ceramic procedures of slip-casting, dry-pressing, or extrusion. After firing to maturity,

the specimens shall be ground to within  $\pm 0.001$  in. (0.03 mm) of the diameter of the thermodes being used. The bases shall be perpendicular to the axis of the cylinder within  $\pm 15$  min. The length of the cylinder shall be equal to its diameter within  $\pm 1$  %.

**5. Preparation of Test Specimens**

5.1 Metallize the plane faces of the specimen to be evaluated with a fired-on platinum alloy, silver, or other metallic glaze that may be readily soft soldered. Then soft solder the metallized specimen into position between the upper and lower thermodes by placing solder preforms between the specimen and thermode and applying heat to the thermode. Upon