
Dentistry — Hose connectors for air driven dental handpieces

*Art dentaire — Connexions pour pièces à main dentaires à air
comprimé*

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 9168:2009

<https://standards.iteh.ai/catalog/standards/sist/93371250-b2fe-4885-88e0-c608c5ae94b1/iso-9168-2009>



PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 9168:2009

<https://standards.iteh.ai/catalog/standards/sist/93371250-b2fe-4885-88e0-c608c5ae94b1/iso-9168-2009>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2009

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 9168 was prepared by Technical Committee ISO/TC 106, *Dentistry*, Subcommittee SC 4, *Dental instruments*.

This third edition cancels and replaces the second edition (ISO 9168:1991), which has been technically revised. The following changes were made:

- a) requirement resistance to sterilization has been replaced by reprocessing requirement;
- b) language-independent figures;
- c) introduction of definition for “hose connector” and updated references and Bibliography.

iTeh STANDARD PREVIEW **(standards.iteh.ai)**

ISO 9168:2009

<https://standards.iteh.ai/catalog/standards/sist/93371250-b2fe-4885-88e0-c608c5ae94b1/iso-9168-2009>

Dentistry — Hose connectors for air driven dental handpieces

1 Scope

This International Standard is applicable for achieving reliable interchangeability between hoses from dental units and dental handpieces.

This International Standard specifies four types of hose connector for use between air driven dental handpieces and the flexible hoses of the dental unit which supply the handpieces with water, air and light, and provide for exhaust.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 261, *ISO general purpose metric screw threads — General plan*

ISO 1942, *Dentistry — Vocabulary*

ISO 7494-1, *Dentistry — Dental units — Part 1: General requirements and test methods*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 1942 and the following apply.

3.1

hose connector

connector at the dental handpiece to enable one to connect the hose with the handpiece

4 Classification

For the purpose of this International Standard, hose connectors for air driven dental handpieces are classified into the following four types:

- Type 1: connector with two or three outlets and connection thread 9/16 – 40 UNS;
- Type 2: connector with four or five outlets and connection thread 0,555 – 36 UNS;
- Type 3: connector with four outlets and electrical contacts and connection thread 0,555 – 36 UNS;
- Type 4: connector with three outlets and connection thread M12 × 0,5, in accordance with ISO 261.

5 Requirements

5.1 General

Hose connectors for air driven dental handpieces are specific parts of dental handpieces. Requirements for dental handpieces are specified in the relevant product standards.

NOTE Relevant product standards for dental handpieces are e.g. ISO 7785-1, ISO 13294 and ISO 15606.

5.2 Dimensions

The dimensions, the outlet configuration and the use of the outlets shall be as specified in Figure 1, Figure 2, Figure 3 and Figure 4.

The thread characteristics for Type 1, Type 2 and Type 3 shall be as specified in Table 1. The thread characteristics for Type 4 (M12 × 0,5) shall be in accordance with ISO 261.

Testing shall be carried out in accordance with 7.1.

5.3 Resistance to reprocessing

Hose connectors shall be capable of withstanding a minimum of 250 reprocessing cycles as defined in the manufacturer's instructions for use without deterioration in appearance or performance.

Quick connectors with and without lights supply, which are not permanently fixed to the instrument, shall be capable of withstanding the reprocessing procedure as given in the manufacturer's instructions. In this case the requirements of ISO 7494-1 are applicable.

Testing shall be carried out in accordance with 7.2. [ISO 9168:2009](https://standards.iteh.ai/catalog/standards/sist/93371250-b2fe-4885-88e0-c608c5ae94b1/iso-9168-2009)

<https://standards.iteh.ai/catalog/standards/sist/93371250-b2fe-4885-88e0-c608c5ae94b1/iso-9168-2009>

Dimensions in millimetres



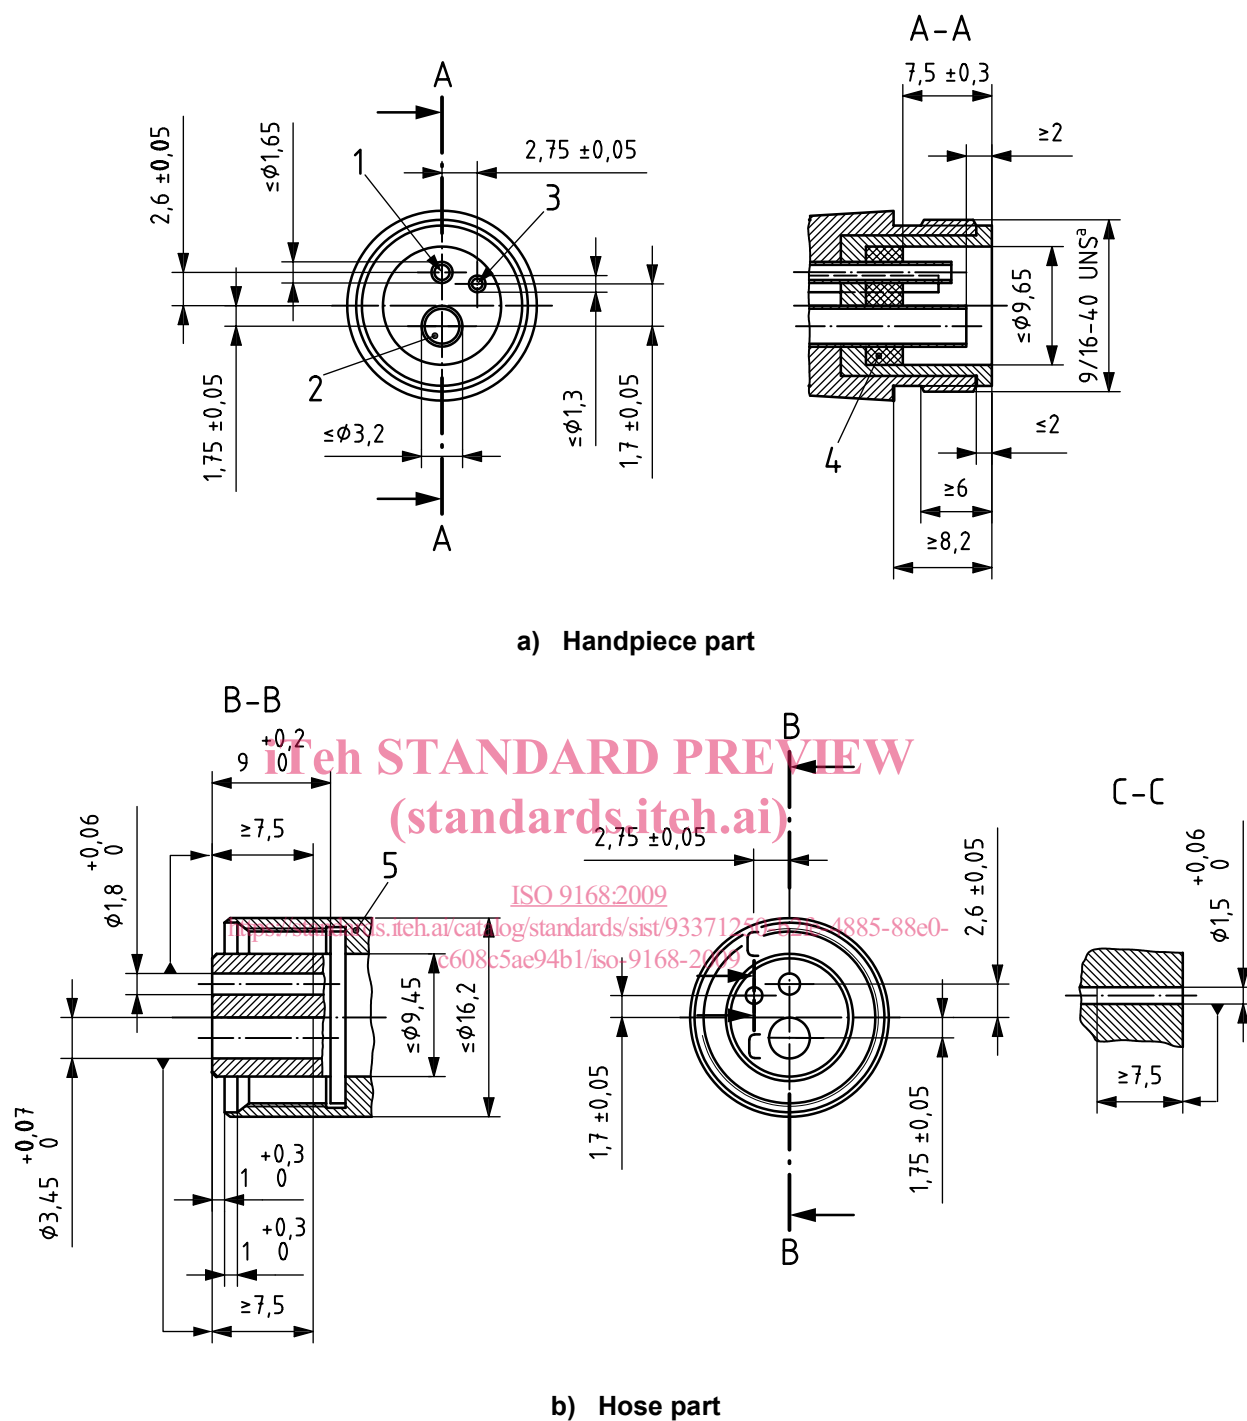


Figure 1 — Type 1 connector

Dimensions in millimetres

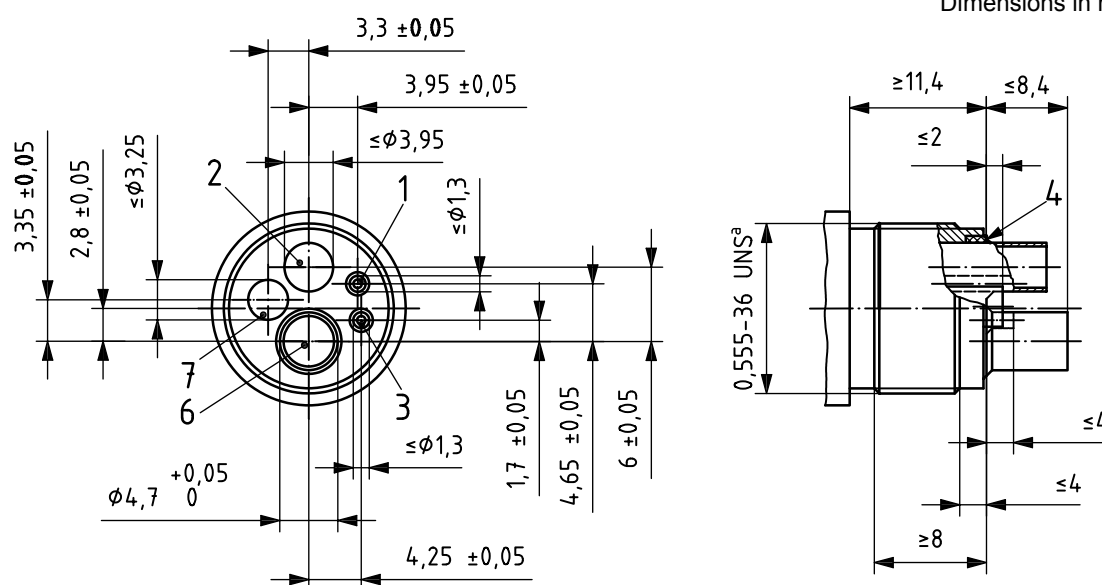

a) Handpiece part

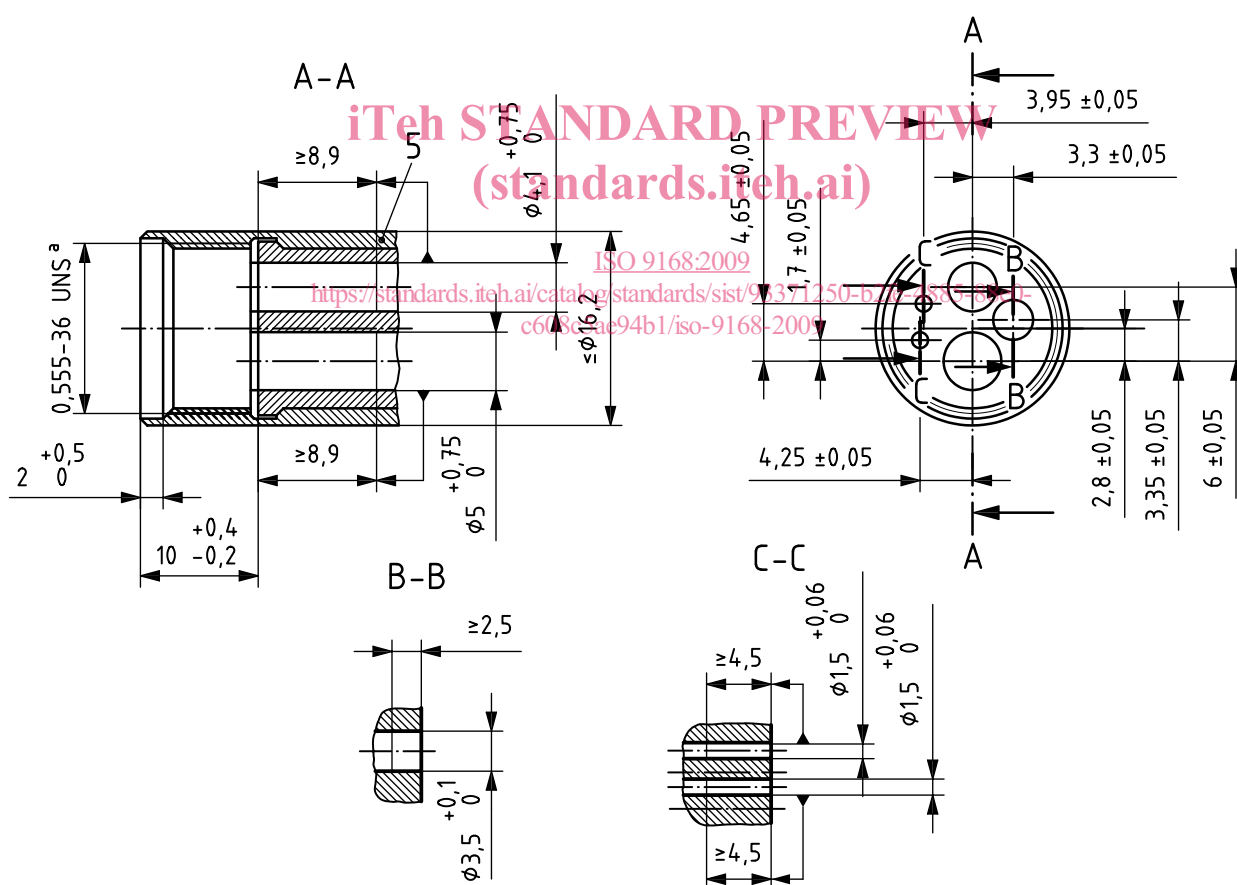

b) Hose part


Key

- | | | | | | |
|---|-----------|---|---------|---|-------------|
| 1 | water | 4 | gasket | 7 | fibre optic |
| 2 | drive air | 5 | nut | | |
| 3 | spray air | 6 | exhaust | a | See Table |

^a See Table 1 for thread characteristics.

Figure 2 — Type 2 connector

Dimensions in millimetres

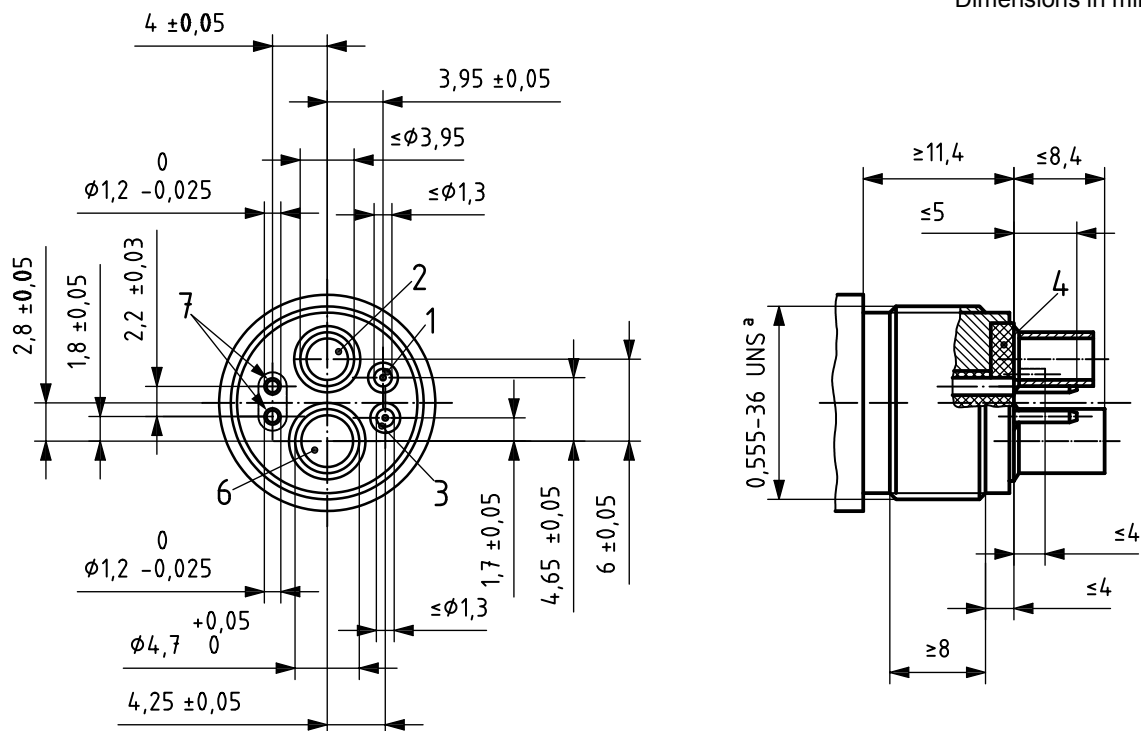

iTeh STANDARD PREVIEW
a) Handpiece part
(standards.itih.ai)

Figure 3 — Type 3 connector (continued)

<https://standards.itih.ai/catalog/standards/sist/93371250-b2fe-4885-88e0-c608c5ae94b1/iso-9168-2009>