



**SLOVENSKI STANDARD**  
**SIST EN 27963:1996**  
**01-januar-1996**

---

**Zvari v jeklu - Kalibracijski blok št. 2 za ultrazvočno preiskavo zvarov**

Welds in steel - Calibration block No. 2 for ultrasonic examination of welds (ISO 7963:1985)

Schweißverbindungen in Stahl - Kalibrierkörper Nr. 2 zur Ultraschallprüfung von Schweißverbindungen (ISO 7963:1985)

Soudures sur acier - Bloc d'étalonnage no 2 pour l'examen par ultrasons des soudures (ISO 7963:1985)

**iTeh STANDARD PREVIEW**  
(standards.itteh.ai)

[SIST EN 27963:1996](#)

**Ta slovenski standard je istoveten z: EN 27963:1992**

<https://standards.itteh.ai/catalog/standards/sist/47770549-48e2-4742-9649-57cad7b515c4/sist-en-27963-1996>

---

**ICS:**

25.160.40      Varjeni spoji in vari      Welded joints

**SIST EN 27963:1996**      **en**

**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

SIST EN 27963:1996

<https://standards.iteh.ai/catalog/standards/sist/47770549-48e2-4742-9649-57cad7b515c4/sist-en-27963-1996>

EUROPEAN STANDARD

EN 27963:1992

NORME EUROPÉENNE

EUROPÄISCHE NORM

April 1992

UDC 621.791.053:669.14:620.179.16

Descriptors: Steels, welding, welded joints, ultrasonic tests, calibration, reference sample, dimensions

English version

**Welds in steel - Calibration block No. 2 for  
ultrasonic examination of welds (ISO 7963:1985)**

Soudures sur acier - Bloc d'étallonnage no 2  
pour l'examen par ultrasons des soudures (ISO  
7963:1985)

Schweißverbindungen in Stahl - Kalibrierkörper  
Nr. 2 zur Ultraschallprüfung von  
Schweißverbindungen (ISO 7963:1985)

**iTeh STANDARD PREVIEW  
(standards.iteh.ai)**SIST EN 27963:1996

<https://standards.iteh.ai/catalog/standards/sist/47770549-48e2-4742-9649-57cad7b515c4/sist-en-27963-1996>

This European Standard was approved by CEN on 1992-03-27. CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration.

Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the Central Secretariat or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the Central Secretariat has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Denmark, Finland, France, Germany, Greece, Iceland, Ireland, Italy, Luxembourg, Netherlands, Norway, Portugal, Spain, Sweden, Switzerland and United Kingdom.

**CEN**

European Committee for Standardization  
Comité Européen de Normalisation  
Europäisches Komitee für Normung

Central Secretariat: rue de Stassart, 36 B-1050 Brussels

Page 2  
EN 27963:1992

### Foreword

In 1990, ISO 7963:1985 was submitted to the CEN Primary Questionnaire procedure.

Following the positive result of this procedure, the CEN Technical Board, agreed to submit ISO 7963:1985, without modifications, to Formal Vote. The result of the Formal Vote was positive.

National Standards identical to this European Standard shall be published at the latest by 92-10-31 and conflicting national standards shall be withdrawn at the latest by 92-10-31.

In accordance with the CEN/CENELEC Common Rules, the following countries are bound to implement this European Standard :

Austria, Belgium, Denmark, Finland, France, Germany, Greece, Iceland, Ireland, Italy, Luxembourg, Netherlands, Norway, Portugal, Spain, Sweden, Switzerland and United Kingdom.

[SIST EN 27963:1996](https://standards.iteh.ai/catalog/standards/sist/47770549-48e2-4742-9649-57cad7b515c4/sist-en-27963-1996)

<https://standards.iteh.ai/catalog/standards/sist/47770549-48e2-4742-9649-57cad7b515c4/sist-en-27963-1996>

Endorsement notice

The text of the International Standard ISO 7963:1985 was approved by CEN as a European Standard without any modification.

# International Standard



# 7963

INTERNATIONAL ORGANIZATION FOR STANDARDIZATION • МЕЖДУНАРОДНАЯ ОРГАНИЗАЦИЯ ПО СТАНДАРТИЗАЦИИ • ORGANISATION INTERNATIONALE DE NORMALISATION

## Welds in steel — Calibration block No. 2 for ultrasonic examination of welds

*Soudures sur acier — Bloc d'étalonnage n° 2 pour l'examen par ultrasons des soudures*

First edition — 1985-09-15

**ITeH STANDARD PREVIEW**  
**(standards.iteh.ai)**

[SIST EN 27963:1996](#)

<https://standards.iteh.ai/catalog/standards/sist/47770549-48e2-4742-9649-57cad7b515c4/sist-en-27963-1996>

UDC 620.179.16 : 53.089.6 : 621.791.053

Ref. No. ISO 7963-1985 (E)

**Descriptors:** steels, welding, welded joints, tests, ultrasonic tests, calibration, reference sample, dimensions.

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work.

Draft International Standards adopted by the technical committees are circulated to the member bodies for approval before their acceptance as International Standards by the ISO Council. They are approved in accordance with ISO procedures requiring at least 75 % approval by the member bodies voting.

International Standard ISO 7963 was prepared by Technical Committee ISO/TC 44, *Welding and allied processes*.

**iTeh STANDARD PREVIEW**  
(standards.iteh.ai)

SIST EN 27963:1996

<https://standards.iteh.ai/catalog/standards/sist/47770549-48e2-4742-9649-57cad7b515c4/sist-en-27963-1996>

# Welds in steel — Calibration block No. 2 for ultrasonic examination of welds

## 0 Introduction

This calibration block differs in size and shape from the block described in ISO 2400.

It is very much smaller and therefore lighter, and its geometry is much simpler.

It does not offer as much scope as the larger block; in particular it is not meant to check an ultrasonic flaw detector completely.

Its easy handling, however, makes it possible, during practical examination, to check simply, from time to time, the setting of the time base and the sensitivity of the ultrasonic equipment. Moreover, it is suited to checking the beam angle and the probe index of miniature shear wave probes.

## 1 Scope and field of application

This International Standard lays down the dimensions, type of steel and directives for the use of block No. 2 for the calibration of ultrasonic equipment for the examination of welds in steel.

## 2 References

ISO 468, *Surface roughness — Parameters, their values and general rules for specifying requirements.*

ISO 2400, *Welds in steel — Reference block for the calibration of equipment for ultrasonic examination.*

ISO 2604/4, *Steel products for pressure purposes — Quality requirements — Part 4: Plates.*<sup>1)</sup>

## 3 Dimensions

The dimensions of the block, in millimetres, are given in figure 1.

The tolerances are  $\pm 0,1$  mm, except on the length of the engraved scale where it is  $\pm 0,5$  mm.

### NOTES

- 1 The thickness of the block can be greater (see the annex).
- 2 In figure 1,  $R_a$  indicates the average roughness.  $R_a$  is not very different from  $R_z$ ; both are defined in ISO 468.

## 4 Material

The calibration block is made of steel of composition corresponding to P 18 of ISO 2604/4.

## 5 Preparation

The calibration block shall be homogeneous and free from defects revealed by ultrasonic examination (see the annex).

In order to obtain a fine structure and good homogeneity, the block, before final machining, shall be heat treated as follows:

- a) heating for 30 min at 920 °C and water-quenching;
- b) re-heating for 2 h at 650 °C and cooling in still air.

The thickness to be removed from all surfaces by machining after heat treatment shall be at least 2 mm.

After the heat treatment, and without waiting for machining to end, the blocks shall undergo a further ultrasonic examination from two different directions at right angles to each other and in the direction of rolling.

All surfaces shall be machined lengthwise except the echo side, which shall be ground.

In order to prevent parasitic effects, the depth of the marks of the engraved scale shall be  $0,1 \pm 0,05$  mm. The length of the marks shall be 6 mm and the tolerance on the positioning of the marks shall be  $\pm 0,2$  mm. On completion of machining, a final ultrasonic examination shall be carried out.

## 6 Method of use

### 6.1 Setting of the time base

To set the time base, the leading edge (left side) of successive echoes shall be made to coincide with the appropriate scale markings on the screen of the equipment.

The pulse-travel time depends on the velocity of ultrasonic waves in the material examined.

For the steel composition given in clause 4, the velocities of longitudinal and shear waves are  $(5\,920 \pm 30) \text{ m}\cdot\text{s}^{-1}$  and  $(3\,255 \pm 15) \text{ m}\cdot\text{s}^{-1}$ , respectively.

1) At present at the stage of draft. (Revision of ISO 2604/4-1975.)

## ISO 7963-1985 (E)

### 6.1.1 Calibration of time base up to 250 mm with a longitudinal wave probe

The position of the probe on the calibration block is indicated in figure 2a). Figure 2b) is a schematic representation of the screen appearance for calibration of a distance of 50 mm.

NOTE — Depending on the probe and frequency used, difficulties may arise when calibrating distances greater than 10 times the thickness of the block.

### 6.1.2 Calibration of distance of 100 or 125 mm with a miniature shear wave probe

The position of the miniature shear wave probe on the calibration block is shown in figure 3a) for a distance of 125 mm and in figure 3b) for a distance of 100 mm. In figures 3a) and 3b) the screen appearances for the calibration of the two distances are also shown schematically.

NOTE — Calibration of the distance of 125 mm is, however, preferable, since the linearity of the time base is better.

## 6.2 Checking during examination

A large number of factors exercise an influence on sensitivity setting (see the annex).

### 6.2.1 Longitudinal wave probes — Sensitivity setting

The probe can be placed in position "a" as indicated in figure 4.

The oscillogram representing the successive echoes can be used as a reference for setting sensitivity.

It is also possible to use the reflection from the 5 mm diameter hole, position "b" in figure 4, the probe being placed so that the corresponding echo amplitude is at its maximum.

### 6.2.2 Miniature shear wave probes

#### 6.2.2.1 Sensitivity setting

In this case, the maximum echo from the 5 mm diameter hole can also be used (see figure 5, position "a") as a reference for setting sensitivity.

Similarly, it is possible to make use of the reflections from the cylindrical surfaces of radii of 50 mm and 25 mm respectively.

In this case there are two possibilities.

- In the first, by using a calibrated gain control, the amplitude of the echo from the cylindrical surface is initially set to 80 % of screen height and subsequently adjusted to the level desired (see figure 5, position "b").
- In the second, without the use of a calibrated gain control, the successive echoes from the cylindrical surfaces can be used for the adjustment of sensitivity (see figure 6).

When checking probes, the acoustic coupling is an important factor and, when probes are compared, the same coupling medium shall be used.

#### 6.2.2.2 Determination of the position of the probe index

The miniature shear wave probe is, as shown in figures 3a) and 3b), moved parallel to the main faces of the calibration block until the amplitude of the echo from the cylindrical surface has reached its maximum.

The probe index then coincides with the centre mark of the millimetre scale.

#### 6.2.2.3 Determination of beam angle

In this case, use is made of the echo obtained from the 5 mm diameter hole.

The miniature shear wave probe is, as before, moved parallel to the main faces of the calibration block until the amplitude of the echo from the 5 mm diameter hole has reached its maximum.

The beam angle is obtained either by direct reading of the scale engraved on the calibration block, as shown in figure 7, or by interpolation if the position found does not coincide with one of the scale lines.

The positions shown in figure 7 make it possible to check beam angles of 45°, 60° and 70° probes.



Dimensions in millimetres

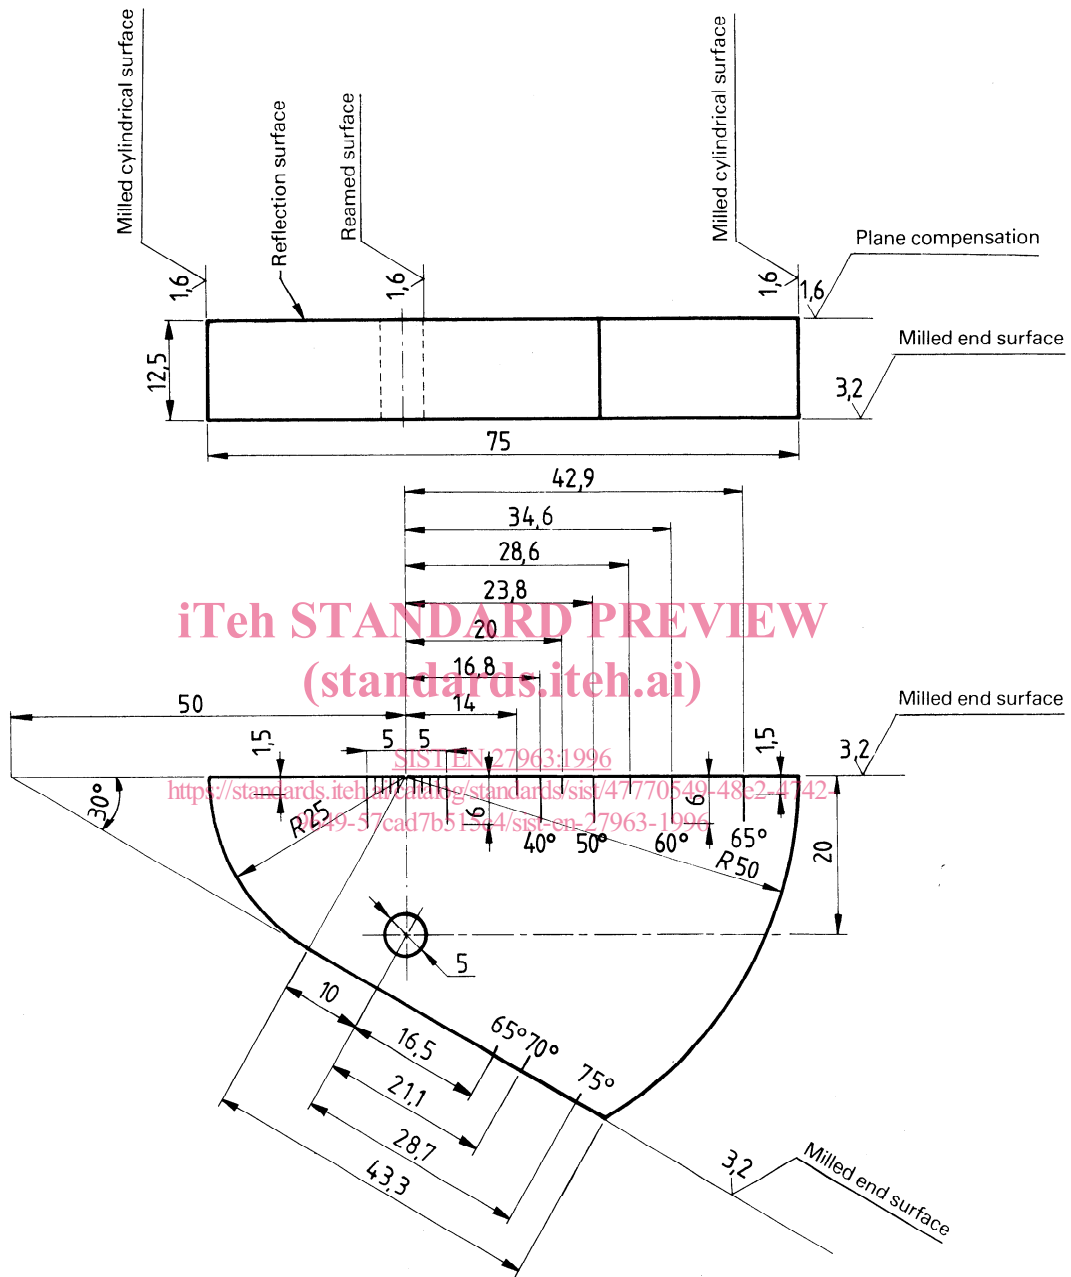


Figure 1