



SLOVENSKI STANDARD SIST EN ISO 9934-3:2004

01-marec-2004

**Neporušitveno preskušanje – Preskušanje z magnetnimi delci – 3. del: Naprave
(ISO 9934-3:2002)**

Non-destructive testing - Magnetic particle testing - Part 3: Equipment (ISO 9934-3:2002)

Zerstörungsfreie Prüfung - Magnetpulverprüfung - Teil 3: Geräte (ISO 9934-3:2002)

Essais non destructifs - Magnétoscopie - Partie 3: Equipement (ISO 9934-3:2002)

STANDARD PREVIEW
(standards.iteh.ai)

Ta slovenski standard je istoveten z: EN ISO 9934-3:2002

<https://standards.iteh.ai/catalog/standards/sist/4f430c8c-205e-46b1-8b32-296381ae812e/sist-en-iso-9934-3-2004>

ICS:

19.100 Neporušitveno preskušanje Non-destructive testing

SIST EN ISO 9934-3:2004

en

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[SIST EN ISO 9934-3:2004](https://standards.iteh.ai/catalog/standards/sist/4f430c8c-205e-46b1-8b32-296381ae812e/sist-en-iso-9934-3-2004)

<https://standards.iteh.ai/catalog/standards/sist/4f430c8c-205e-46b1-8b32-296381ae812e/sist-en-iso-9934-3-2004>

EUROPEAN STANDARD
NORME EUROPÉENNE
EUROPÄISCHE NORM

EN ISO 9934-3

July 2002

ICS 19.100

English version

**Non-destructive testing - Magnetic particle testing - Part 3:
Equipment (ISO 9934-3:2002)**

Essais non destructifs - Magnétoscopie - Partie 3:
Equipement (ISO 9934-3:2002)

Zerstörungsfreie Prüfung - Magnetpulverprüfung - Teil 3:
Geräte (ISO 9934-3:2002)

This European Standard was approved by CEN on 4 August 2001.

CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration. Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the Management Centre or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the Management Centre has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Czech Republic, Denmark, Finland, France, Germany, Greece, Iceland, Ireland, Italy, Luxembourg, Malta, Netherlands, Norway, Portugal, Spain, Sweden, Switzerland and United Kingdom.

[SIST EN ISO 9934-3:2004](https://standards.iteh.ai/catalog/standards/sist/4f430c8c-205e-46b1-8b32-296381ae812e/sist-en-iso-9934-3-2004)

<https://standards.iteh.ai/catalog/standards/sist/4f430c8c-205e-46b1-8b32-296381ae812e/sist-en-iso-9934-3-2004>



EUROPEAN COMMITTEE FOR STANDARDIZATION
COMITÉ EUROPÉEN DE NORMALISATION
EUROPÄISCHES KOMITEE FÜR NORMUNG

Management Centre: rue de Stassart, 36 B-1050 Brussels

Contents

Foreword.....	3
1 Scope	4
2 Normative references	4
3 Safety requirements	4
4 Types of devices	4
4.1 Portable electromagnets (AC)	4
4.2 Current generators	6
4.3 Magnetic benches	8
4.4 Specialized testing systems	10
5 UV-A sources.....	11
5.1 Generals.....	11
5.2 Technical data	11
5.3 Minimum requirements	11
6 Detection media system.....	12
6.1 General.....	12
6.2 Technical data	12
6.3 Minimum requirements	12
7 Inspection booth	12
7.1 General.....	12
7.2 Technical data	12
7.3 Minimum requirements	13
8 Demagnetization	13
8.1 General.....	13
8.2 Technical data	13
8.3 Minimum requirements	13
9 Measurements	13
9.1 General.....	13
9.2 Current measurement.....	14
9.3 Magnetic field measurement.....	14
9.4 Visible light measurement	14
9.5 UV-A irradiance measurement.....	15
9.6 Verification and calibration of instruments.....	15
Bibliography	16

iTech STANDARD PREVIEW
(standards.itech.ai)

SIST EN ISO 9934-3:2004

<https://standards.itech.ai/catalog/standards/sist/4f430c8c-205e-46b1-8b32-296381ae812e/sist-en-iso-9934-3-2004>

Foreword

This document (ISO 9934-3:2002) has been prepared by Technical Committee ISO/TC 135 "Non-destructive testing" in collaboration with Technical Committee CEN/TC 138, "Non-destructive testing", the secretariat of which is held by AFNOR.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by January 2003, and conflicting national standards shall be withdrawn at the latest by January 2003.

This Standard consists of the following parts :

EN ISO 9934-1	Non destructive testing - Magnetic particle testing - Part 1 : General rules
prEN ISO 9934-2	Non destructive testing - Magnetic particle testing - Part 2 : Detection media
EN ISO 9934-3	Non destructive testing - Magnetic particle testing - Part 3 : Equipment

According to the CEN/CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Czech Republic, Denmark, Finland, France, Germany, Greece, Iceland, Ireland, Italy, Luxembourg, Malta, Netherlands, Norway, Portugal, Spain, Sweden, Switzerland and the United Kingdom.

[SIST EN ISO 9934-3:2004](https://standards.iteh.ai/catalog/standards/sist/4f430c8c-205e-46b1-8b32-296381ae812e/sist-en-iso-9934-3-2004)

<https://standards.iteh.ai/catalog/standards/sist/4f430c8c-205e-46b1-8b32-296381ae812e/sist-en-iso-9934-3-2004>

EN ISO 9934-3:2002 (E)**1 Scope**

This European Standard describes three types of equipment for magnetic particle testing :

- portable or transportable equipment ;
- fixed installations ;
- specialized testing systems for testing components on a continuous basis, comprising a series of processing stations placed in sequence to form a process line.

Equipment for magnetizing, demagnetizing, illumination, metering and monitoring are also described.

This standard specifies the properties to be provided by the equipment supplier, minimum requirements for application and the method of measuring certain parameters. Where appropriate, measuring and calibration requirements and in-service checks are also specified.

2 Normative references

This European Standard incorporates by dated or undated reference, provisions from other publications. These normative references are cited at the appropriate places in the text and the publications are listed hereafter. For dated references, subsequent amendments to or revisions of any of these publications apply to this European Standard only when incorporated in it by amendment or revision. For undated references the latest edition of the publication referred to applies (including amendments).

EN 10084 *Case hardening steels - Technical delivery conditions*

EN ISO 3059:2001 *Non-destructive testing - Penetrant testing and magnetic particle testing - Viewing conditions (ISO 3059:2001)*

EN ISO 9934-1:2001 *Non-destructive testing - Magnetic particle testing - Part 1 : General rules (ISO 9934-1:2001)*

EN 60529 *Degrees of protection provides by enclosures (IP Code) (IEC 60529:1989)*

3 Safety requirements

The equipment design shall take into account of all European, national and local regulations which include health, safety, electrical and environmental requirements.

4 Types of devices**4.1 Portable electromagnets (AC¹⁾)****4.1.1 General**


Hand-held portable electromagnets (yokes) produce a magnetic field between the two poles. (When testing according to EN ISO 9934-1, DC electromagnets should only be used if agreed at enquiry and order stages).

Magnetization shall be determined by measuring the tangential field strength H_t at the centre of a line joining the centres of the pole faces of the electromagnet with pole extenders where used. The electromagnet with a pole spacing s is placed on a steel plate as shown in Figure 1. The plate shall have the dimensions (500 ± 25) mm x (250 ± 13) mm x (10 ± 0.5) mm and shall be of steel conforming to C 22 (EN 10084)..

1) AC = alternative current, and DC = rectified current

Periodic functional checks may be carried out either by the method described above or by a lift test. The electromagnet shall be capable of supporting a steel plate or rectangular bar conforming to C 22 (EN 10084) and having a minimum mass of 4,5 kg, with the magnet poles set at their recommended spacing. The major dimension of the plate or bar shall be greater than the pole spacing s of the electromagnet

NOTE : To lift a steel plate with a mass of 4,5 kg requires a lifting force of 44 N.

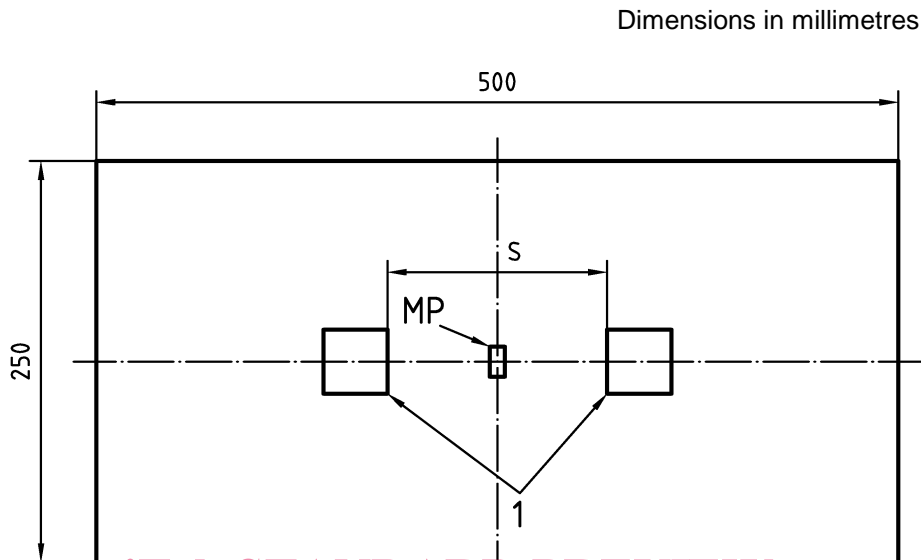

iTech STANDARD PREVIEW
(standards.iteh.ai)

Key

MP Measuring point for the tangential field strength

s Pole spacing

1 Poles

SIST EN ISO 9934-3:2004

<https://standards.iteh.ai/catalog/standards/sist/4f430c8c-205e-46b1-8b32-296381ae812e/sist-en-iso-9934-3-2004>

Figure 1 — Determination of the characteristics of portable electromagnets

4.1.2 Technical data

The following data shall be provided by the equipment supplier:

- recommended pole spacing (maximum and minimum pole spacing) (s_{\max} , s_{\min});
- cross sectional dimensions of the poles;
- electrical supply (voltage, current and frequency);
- current wave forms available;
- method of current control and effect on waveform (e.g. : thyristor);
- duty cycle at maximum output (ratio of current 'ON' to 'Total' time expressed as a percentage);
- maximum current 'ON' time;
- tangential field strength H_t at s_{\max} and s_{\min} (following 4.1);
- overall dimensions of the equipment;
- equipment mass, in kilograms;
- specified electrical protection degree (IP) see EN 60529.

EN ISO 9934-3:2002 (E)

4.1.3 Minimum requirements

The following requirements shall be satisfied at an ambient temperature of 30 °C and at maximum output :

- duty cycle $\geq 10 \%$
- current 'ON' time $\geq 5 \text{ s}$
- surface temperature of handle $\leq 40 \text{ °C}$
- tangential field strength at s_{max} (see 4.1) $\geq 2 \text{ kA/m (RMS)}$
- lifting force $\geq 44 \text{ N}$

4.1.4 Additional requirements

The electromagnet shall be supplied with a power ON/OFF switch preferably mounted on the handle.


Generally electromagnets should be usable with one hand.

4.2 Current generators

Current generators are used to supply current for magnetizing equipment. A current generator is characterized by the open circuit voltage U_0 , the short circuit current I_k and the rated current I_r (RMS-values).

The rated current I_r is defined as the maximum current for which the generator is rated at the duty cycle of 10 % and for a current 'ON' time of 5 s if not otherwise specified.

The open circuit voltage U_0 and the short circuit current I_k are derived from the load-characteristic of the generator at maximum power (with any feed back controls disconnected). The load line of the generator may be derived by connecting two widely different loads, such as different lengths of cable, in turn to the generator. For the first cable, the current I_1 through the cable and voltage U_1 across the output terminals are measured and plotted, to give point P_1 on Figure 2. The process is repeated with a second load to give point P_2 . The load line is constructed by drawing a straight line between P_1 and P_2 . The open circuit voltage U_0 and short circuit current I_k are then given by the intercepts on the axes, as shown in Figure 2.

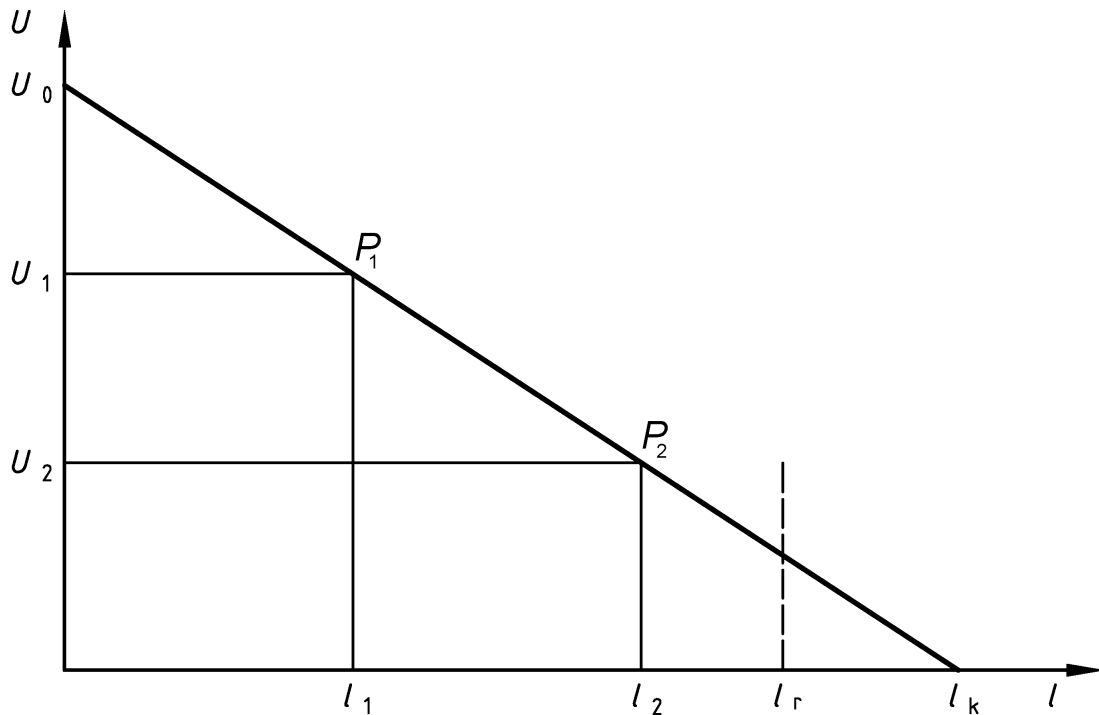**Key**

P_1, P_2 Measuring points for determination of the load characteristics

iTeh STANDARD PREVIEW
(standards.iteh.ai)

Figure 2 — Load characteristics of the current generator

SIST EN ISO 9934-3:2004

4.2.1 Technical data <https://standards.iteh.ai/catalog/standards/sist/4f430c8c-205e-46b1-8b32-296381ae812e/sist-en-iso-9934-3-2004>

The following data shall be provided by the equipment supplier:

- open circuit voltage U_0 (RMS);
- short circuit current I_k (RMS);
- rated current I_r (RMS);
- duty cycle at maximum output (if other than as specified in 4.2);
- maximum current 'ON' time (if other than specified in 4.2);
- current wave forms available;
- method of current regulation and effect on waveform;
- working range and incremental setting steps;
- method of constant current control if available;
- type of meter (digital, analog);
- resolution and accuracy of current output meter;
- electrical supply requirements at maximum current output (voltage, phases, frequency and current);
- specified electrical protection degree (IP) see EN 60529;