



SLOVENSKI STANDARD SIST EN 829:2000

01-januar-2000

8]U[bcgh] b]g]ghYa]]b`j]]fc`!`HfUbgdcfHbU`Ya VU`Uj`UnUa YX]W]bg_Y`]b`V]c`cý_Y
j ncfWY`!`NU` hYj YždfYg_i g]

In vitro diagnostic systems - Transport packages for medical and biological specimens - Requirements, tests

In-vitro-Diagnostik/Diagnostika - Transportverpackungen für medizinisches und biologisches Untersuchungsgut - Anforderungen, Prüfung

Systemes d'analyses médicales in vitro - Emballages de transport pour échantillons médicaux et biologiques - Exigences, essais

<https://standards.iteh.ai/catalog/standards/sist/77a27dd4-f975-4cb2-8369-2c3897d7440e/sist-en-829-2000>

Ta slovenski standard je istoveten z: EN 829:1996

ICS:

11.100.10	Öäë } [• ä } ä ^ • \ • } ä • ä c ^ { ä ä Ä ä [In vitro diagnostic test systems
55.020	Pakiranje in distribucija blaga na splošno	Packaging and distribution of goods in general

SIST EN 829:2000

en

iTeh STANDARD PREVIEW
(standards.iteh.ai)

SIST EN 829:2000

<https://standards.iteh.ai/catalog/standards/sist/77a27dd4-f975-4cb2-8369-2c3897d7440e/sist-en-829-2000>

EUROPEAN STANDARD

EN 829

NORME EUROPÉENNE

EUROPÄISCHE NORM

May 1996

ICS 11.100; 55.020

Descriptors: medicine, biology, samples, packing, transport packing, freight transport, specifications, tests, marking, graphic symbols

English version

**In vitro diagnostic systems - Transport packages
for medical and biological specimens -
Requirements, tests**

iTeh STANDARD PREVIEW

Systèmes d'analyses médicales in vitro -
Emballages de transport pour échantillons
médicaux et biologiques - Exigences, essais

In-vitro-Diagnostik/Diagnostika -
Transportverpackungen für medizinisches und
biologisches Untersuchungsgut - Anforderungen,
Prüfung

standards.iteh.ai
SIST EN 829:2000

<https://standards.iteh.ai/catalog/standards/sist/77a27dd4-f975-4cb2-8369-2c3897d7440e/sist-en-829-2000>

This European Standard was approved by CEN on 1996-02-29. CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration.

Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the Central Secretariat or to any CEN member.

The European Standards exist in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the Central Secretariat has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Denmark, Finland, France, Germany, Greece, Iceland, Ireland, Italy, Luxembourg, Netherlands, Norway, Portugal, Spain, Sweden, Switzerland and United Kingdom.

CEN

European Committee for Standardization
Comité Européen de Normalisation
Europäisches Komitee für Normung

Central Secretariat: rue de Stassart, 36 B-1050 Brussels

Foreword

This European Standard has been prepared by the Technical Committee CEN/TC 140 "In vitro diagnostic systems", the secretariat of which is held by DIN.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by November 1996, and conflicting national standards shall be withdrawn at the latest by November 1996.

The international agreements of the Universal Postal Union, the committee of experts of the United Nations, as well as of the World Health Organization (WHO) were taken into consideration when establishing graphical symbols.

According to the CEN/CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Denmark, Finland, France, Germany, Greece, Iceland, Ireland, Italy, Luxembourg, Netherlands, Norway, Portugal, Spain, Sweden, Switzerland, United Kingdom.

iTeh STANDARD PREVIEW (standards.iteh.ai)

SIST EN 829:2000

<https://standards.iteh.ai/catalog/standards/sist/77a27dd4-f975-4cb2-8369-2e3897d7440c/sist-en-829-2000>



1 Scope

This European Standard applies to packages for transport of medical and biological specimens, referred to in this European Standard as specimens, provided that

- the nominal volume of the specimen container(s) does not exceed 100 ml;
- in the case of multiple specimens, the total volume of specimens in the protecting container does not exceed 500 ml;
- no infectious substances are present in the specimen or a relatively low probability exists that infectious substances are present, e.g. medical and biological specimens to undergo routine screening tests or for the purpose of initial diagnosis.

NOTE 1: "Transport" is defined as the movement of specimens outside the premises of either the sender or the receiver of the specimen.

NOTE 2: Transport packages used for specimens which contain or are likely to contain infectious substances of risk group II to IV as defined by WHO are subject to the provisions on the transport of dangerous goods. In this case the provisions of the agreements [1] to [5] quoted in annex A apply as appropriate.

This European Standard does not apply to packages for transport of disinfected microscopic slides or sterilized specimens for pathological examinations.

The purpose of this standard is to lay down standardised definitions, requirements and tests for transport packages for medical and biological specimens in order to minimise risk for man, animals and the environment.

2 Normative references

This European Standard incorporates, by dated or undated reference, provisions from other publications. These normative references are cited at the appropriate places in the text and the publications are listed hereafter. For dated references, subsequent amendments to or revisions of any of these publications apply to this European Standard only when incorporated in it by amendment or revision. For undated references the latest edition of the publication referred to applies.

ISO 2758	Paper – Determination of bursting strength
ISO 2859-1	Sampling procedures for inspection by attributes – Part 1: Sampling plans indexed by acceptable quality level (AQL) for lot-by-lot inspection
ISO 6710	Single-use containers for venous blood specimen collection
Pharmacopoea Europaea	

3 Definitions

For the purposes of this standard, the following definitions apply:

3.1 Medical and biological specimens

Materials derived from man, animal or plant, destined by the sender for examination.

NOTE: Infected living animals are not included.

3.2 Transport package for medical and biological specimens

An assembled package consisting of:

- a) one or more specimen container(s);
- b) absorbent material,
- c) a protecting container,
- d) a box or mailing bag.

4 Requirements

4.1 General

Ecological and waste disposal considerations should be observed when designing the transport package.

4.2 Assembled transport package

The assembled transport package shall be leakproof and resist mechanical stress, temperature change and a decrease in outer pressure.

The transport package, when tested in accordance with clause 5, shall not show any evidence of leakage from either the specimen or the protecting container.

4.3 Specimen container

The specimen container shall be leakproof when tested in accordance with 5.3.2.1 a), b), d), f) and g) last dash, and should, where appropriate, conform to existing International Standards, e.g. ISO 6710.

4.4 Absorbent material

Absorbent material shall be sufficient to absorb any potential leakage. The maximum volume which can be absorbed shall be given in the product information.

4.5 Protecting container

4.5.1 If intended for multiple use, the protecting container shall be washable and able to withstand sterilisation.

4.5.2 Unprotected accompanying papers should not be put in the protecting container.

4.6 Mailing bag

The box or mailing bag shall be sufficiently strong to withstand usual stress during transport.

These requirements are considered to be fulfilled if the mailing bag corresponds to the specifications of clauses 4.6.1 and 4.6.2.

4.6.1 Bursting strength

When tested according to ISO 2758, the applied paper shall resist a bursting strength of 230 kPa.

4.6.2 Breaking length

The average breaking length of the applied paper shall be at least 4800 m.

NOTE: Testing procedures are given in ISO 1924-1 and ISO 1924-2.

4.7 Use of coolants

The use of coolant demands special features of the transport package as are for example given in the UN Recommendations on Transport of Dangerous Goods (see 6.13.2) and in the Convention of the Universal Postal Union, article 120.

5 Test

5.1 Instruments and accessories

For a test according to this standard, the following instruments and accessories are needed:

- thermostated freezer capable of maintaining a temperature at or below $-20\text{ }^{\circ}\text{C}$,
- steel cylinder (mass 500 g, diameter 30 mm),
- device for a drop test from a height of 500 mm, carried out by means of a steel cylinder according to b),
- vacuum pump, pressure gauge and chamber capable of maintaining an absolute pressure of 5 kPa,
- UV lamp, e.g. a mercury lamp, emitting spectrum lines 365 nm and 405 nm,

f) spectro-fluorometer (optional).

5.2 Reagents

5.2.1 Water

The water shall meet the requirements in accordance with the monograph "Aqua Purificata" of Pharmacopoea Europaea.

5.2.2 Immersing alkaline buffer

50 mmol · l⁻¹ sodium phosphate buffer; pH = 8,5.

5.2.3 Fluorescein solution

25 g disodium salt of fluorescein (C₂₀H₁₀O₅Na₂)

9 g NaCl

60 g Dextran 70

Water ad 1000 ml

NOTE: The intense fluorescence of the dye is still visible when diluting the solution by adding 10⁶ parts by volume of water to 1 part by volume of the solution.

5.3 Test method and test plan

5.3.1 General

A set of assembled transport packages including appropriate specimen containers(s) shall be tested using sampling schemes in accordance with ISO 2859-1 to determine resistance to transport conditions, that is for

- a change in temperature,
- a mechanical stress,
- a decrease in outer pressure.

Each transport package is tested in that order.

The test shall be performed in two stages; the first with the specimen container closed and the second with the specimen container intentionally allowed to leak.

5.3.2 Performance of the test

5.3.2.1 Performance of the first stage of the test

- a) Fill the specimen container with fluorescein solution to the nominal volume specified by the manufacturer.
- b) Immerse the specimen container in 100 ml of buffer according to 5.2.2 and inspect for contamination. If contaminated, wash container to eliminate contamination.
- c) Assemble transport package with specimen container(s) enclosed according to the instruction of the manufacturer.
- d) Heat the transport package to 50 °C, then cool to -18 °C and heat once more to 50 °C and cool to room temperature. Every step shall be monitored to ensure equilibrium of temperature in the specimen container.
- e) Expose the transport package to mechanical stress by dropping a guided steel cylinder with a diameter of 30 mm and a mass of 500 g from a height of 500 mm onto the transport package. The height of the drop shall be measured from the underside of the cylinder to the upper side of the transport package. The transport package shall be placed on a rigid, non-elastic, plane and horizontal bearing surface made of steel. Each transport package shall be tested so that the weight impacts on the transport package in three different planes, ensuring that the specimen container is in the line of impact.
- f) Place the transport package, with the closure of the specimen container oriented downwards, in a chamber and evacuate down to 5 kPa at room temperature for 4 h.

g) Examine the transport package as follows

- visually inspect the protecting container for external contamination,
- open the protecting container,
- visually inspect the absorbent material,
- visually inspect the specimen container,
- immerse the specimen container in 100 ml buffer in accordance with 5.2.2 and inspect for contamination.

5.3.2.2 Performance of the second stage of the test

- a) Fill the specimen container with fluorescein solution to nominal volume specified by the manufacturer and close in such a way as to ensure that contents will leak. The means of ensuring that the specimen container leaks shall be recorded.
- b) Proceed as in 5.3.2.1 c)
- c) Proceed as in 5.3.2.1 d)
- d) Proceed as in 5.3.2.1 e)
- e) Proceed as in 5.3.2.1 f)
- f) Examine the transport package as follows
 - visually inspect the protecting container for external contamination,
 - immerse the transport package in 1 l of buffer in accordance with 5.2.2 and inspect for contamination.

5.3.3 Test evaluation criteria

The first stage of the test is considered passed if, after the testing procedure, the transport package shows no evidence of leakage from either the specimen container or the protecting container.

The second stage of the test is considered passed if, after the testing procedure, the transport package shows no evidence of leakage from the protecting container.

The fluorescein solution that has possibly leaked out is detected visually by the occurrence of a yellow-green fluorescence under UV light (see 5.1 e) or, better, measured by means of a spectro-fluorometer.

6 Marking**6.1 Marking of the specimen container**

The marking of the specimen container shall, where appropriate, conform to existing International Standards. It is a minimum requirement that the specimen container shall carry the manufacturer's name or logo.

6.2 Marking of the protecting container

Protecting containers shall be provided with the year of manufacture and the manufacturer's name or logo.

Protecting containers shall be provided with the graphical symbol according to figure 1. Its size and colour need not meet the requirements specified under 6.3., it shall be well recognizable, however.

6.3 Marking of the assembled transport package

The box or mailing bag mentioned in 3.2 d) shall carry the symbol according to figure 1 on a violet background in the dimensions of 62 mm x 44 mm.

NOTE: For transport inside a country, the lettering should be in a language of the country. For international transport, according to the specifications of the Universal Postal Union regulations, the lettering in French applies: "Matières Médicales Périssables" or "Matières Biologiques Périssables".

Dimensions in millimetres

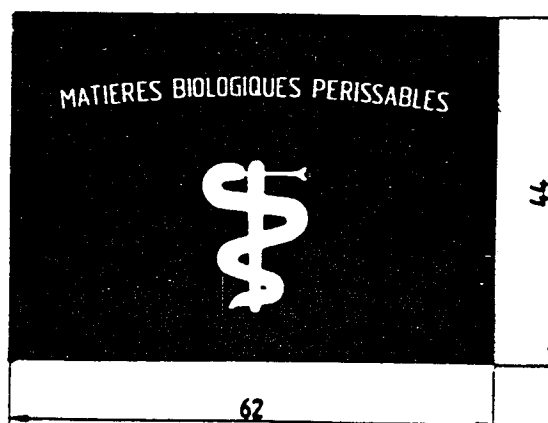


Figure 1

7 Instructions for use

A manufacturer shall supply instructions for use. These shall include details of compatibility between specimen containers and protecting containers.

(standards.iteh.ai)

SIST EN 829:2000

<https://standards.iteh.ai/catalog/standards/sist/77a27dd4-f975-4cb2-8369-2c3897d7440e/sist-en-829-2000>