
**Paper and board — Determination
of roughness/smoothness (air leak
methods) —**

**Part 2:
Bendtsen method**

iTeh STANDARD PREVIEW
*Papier et carton — Détermination de la rugosité/du lissé (méthodes
du débit d'air) —*
(standards.iteh.ai)
Partie 2: Méthode Bendtsen

[ISO 8791-2:2013](https://standards.iteh.ai/catalog/standards/sist/d1b4b93d-c009-4339-a947-2c7c79ac0723/iso-8791-2-2013)

[https://standards.iteh.ai/catalog/standards/sist/d1b4b93d-c009-4339-a947-
2c7c79ac0723/iso-8791-2-2013](https://standards.iteh.ai/catalog/standards/sist/d1b4b93d-c009-4339-a947-2c7c79ac0723/iso-8791-2-2013)



iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 8791-2:2013

<https://standards.iteh.ai/catalog/standards/sist/d1b4b93d-c009-4339-a947-2c7c79ac0723/iso-8791-2-2013>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2013

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

	Page
Foreword.....	iv
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Principle	1
5 Apparatus	2
5.1 Bendtsen tester (two types).....	2
5.2 Variable-area flowmeter type.....	2
5.3 Electronic flowmeter type.....	3
6 Sampling	5
7 Conditioning	5
8 Preparation of test pieces	5
9 Calibration and verification	5
9.1 Variable-area flowmeter type tester.....	5
9.2 Electronic flowmeter type tester.....	5
10 Procedure	5
10.1 Test atmosphere.....	5
10.2 Determination using variable-area flowmeter type tester.....	5
10.3 Determination using electronic flowmeter type tester.....	6
11 Expression of results	6
12 Test report	6
Annex A (normative) Care and maintenance of variable-area flowmeter-type Bendtsen testers	8
Annex B (normative) Calibration of capillary tubes and variable-area and electronic flowmeters	10
Annex C (informative) Precision	14
Bibliography	16

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2. www.iso.org/directives

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received. www.iso.org/patents

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

The committee responsible for this document is ISO/TC 6, *Paper, board and pulps*, Subcommittee SC 2, *Test methods and quality specifications for paper and board*.

This second edition cancels and replaces the first edition (ISO 8791-2:1990), which has been technically revised. In this second edition mainly editorial changes have been made to include the electronic version of the test apparatus and also precision data has been added as an informative Annex.

ISO 8791 consists of the following parts, under the general title *Paper and board — Determination of roughness/smoothness (air leak methods)*: www.iso.org/standard/59077.html

- *Part 1: General method*
- *Part 2: Bendtsen method*
- *Part 3: Sheffield method*
- *Part 4: Print-surf method*

NOTE *Part 1: General method* is considered to be redundant and will be withdrawn after Parts 2, 3 and 4 have been revised and published.

Paper and board — Determination of roughness/ smoothness (air leak methods) —

Part 2: Bendtsen method

1 Scope

This part of ISO 8791 specifies a method for the determination of the roughness of paper and board using the Bendtsen apparatus.

This part of ISO 8791 is applicable to paper and board which have Bendtsen roughness values between about 5 ml/min and 3 000 ml/min when measured with variable-area type testers and between about 50 ml/min and 5 000 ml/min when measured with electronic type testers. It is not suitable for soft papers which allow the land to make a significant impression on the surface or for high-air-permeance papers which allow a significant flow of air to pass through the sheet, or for papers which will not lie flat under the measuring head.

2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 186, *Paper and board — Sampling to determine average quality*

ISO 187, *Paper, board and pulps — Standard atmosphere for conditioning and testing and procedure for monitoring the atmosphere and conditioning of samples*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

3.1

Bendtsen roughness

a measure of the rate at which air will pass between a flat circular land and a sheet of paper or board when tested under specified conditions and at operating pressure

Note 1 to entry: Bendtsen roughness is expressed in millilitres per minute.

4 Principle

Clamping a test piece between a flat plate and a circular metal land. Supplying air at a nominal pressure of 1,47 kPa to the space enclosed inside the land and measuring the rate of air flow between the land and the test piece.

5 Apparatus

5.1 Bendtsen tester (two types)

Bendtsen tester, which operates according to one of the following principles of measurement of air flow rate:


- variable-area flowmeter type (see 5.2).
- electronic flowmeter type (see 5.3).

For variable-area flowmeter type testers, the pressure between the flowmeter and the measuring head is known to decrease at high air flow rates (see 10.2.2) which can reduce the accuracy of the flowmeter reading. For electronic flowmeter type testers, the pressure between the flowmeter and the measuring head is automatically controlled.

5.2 Variable-area flowmeter type

A standard pressure difference is created across the measuring land and the air flow rate is measured on a variable-area flowmeter. The apparatus, see Figure 1, consists of a compressor (5.2.1) and pressure stabilizing reservoir (5.2.2) to supply air, a flowmeter (5.2.4) with a pressure controlling device (5.2.3), and a measuring head (5.2.5).

Annex A gives details of care and maintenance of this type of Bendtsen tester.

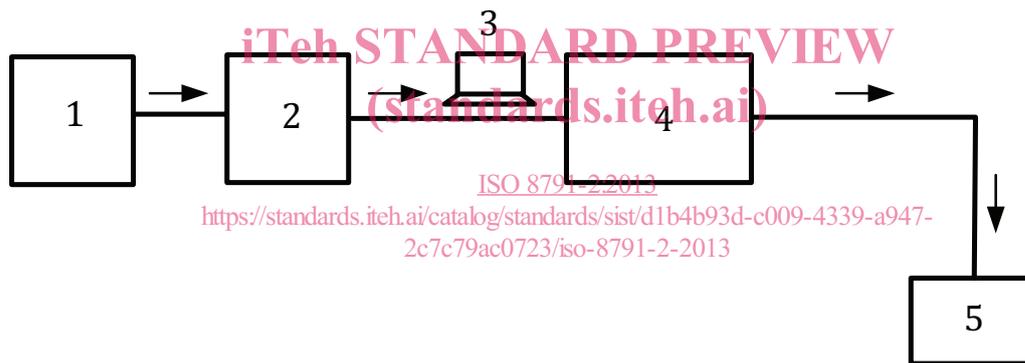

Key

- 1 compressor
- 2 pressure stabilizing reservoir
- 3 pressure controlling device
- 4 flowmeter
- 5 measuring head

Figure 1 — Circuit diagram of variable-area flowmeter type test apparatus

5.2.1 Compressor, capable of generating air at a pressure of about 127 kPa. If necessary, filters shall be provided to ensure that the air is clean and free from oil.

NOTE It is advisable to have the compressor located in a laboratory having the standard atmosphere for conditioning and testing.

5.2.2 Pressure stabilizing reservoir, having a volume of not less than 10 litres, installed between the compressor and the pressure controlling device.

5.2.3 Pressure controlling device to control the air pressure at the inlet of the flowmeter. This shall comprise a manostat weight, a pressure regulator or some means of creating a steady nominal air pressure of $(1,47 \pm 0,02)$ kPa measured at the manostat.

NOTE Most Bendtsen apparatus are provided with three interchangeable manostat weights but only the 1,47 kPa manostat meets the requirement of this part of ISO 8791.

5.2.4 Flowmeter. The flow rate shall be measured by variable-area flowmeters which offer optional flow rate measurements in the ranges 5 ml/min to 150 ml/min, 50 ml/min to 500 ml/min and, on some instruments, 300 ml/min to 3 000 ml/min. These three variable-area flowmeters shall be capable of being read to within 2 ml/min, 5 ml/min and 20 ml/min respectively. The variable area flowmeter may be replaced by another kind of air flowmeter having a measuring range suitable for the material measured that allows the air flow to be determined with an error of less than ± 5 ml/min or $\pm 5\%$ whichever is greater.

One capillary tube shall be provided for verifying the calibration of each variable-area flowmeter. The capillary tubes shall be within the working range of the relevant flowmeter and shall themselves be accurately calibrated against a reliable standard (e.g. a soap-bubble meter) under the same pressure difference as that in the measuring head ([Annex B](#) gives details of the calibration of capillary tubes and variable-area flowmeters).

5.2.5 Measuring head, consisting of a circular land with an enclosed area preferably corrosion-resistant with an optically flat lower surface of $31,5 \text{ mm} \pm 0,2 \text{ mm}$ internal diameter and $0,150 \text{ mm} \pm 0,002 \text{ mm}$ width, and with a mass of $267 \text{ g} \pm 2 \text{ g}$. The tubing used to connect the head to the flowmeter shall be of rubber or plastic, 5 mm internal diameter and not more than 700 mm long.

NOTE 1 A longer length of tubing will result in a significant pressure drop between the flowmeter and the measuring head.

NOTE 2 On most commercial instruments the valve at the outlet of the flowmeter has two outlets. For roughness measurement the tubing is connected to the smaller diameter outlet.

Because the measuring head shall be placed on the test piece in such a manner as to avoid any indentation of the surface, it is advisable to provide a mechanical device to lower and raise the head.¹⁾


5.2.6 Flat plate, polished flat plate, preferably glass used to check for air leaks and upon which the test piece is placed for testing. The leakage between the measuring head land and the flat plate shall not exceed 5 ml/min.

5.2.7 Heavy metal weight, heavy metal annulus, or other suitably shaped weight, for keeping the test piece flat around the measuring head.

5.3 Electronic flowmeter type

A standard pressure difference is created across the measuring land and the air flow rate is measured on an electronic flowmeter. The apparatus, see [Figure 2](#), consists of a compressed air supply system ([5.3.1](#)), a pressure regulator ([5.3.2](#)), an electronic flowmeter ([5.3.3](#)) with a pressure controlling device ([5.3.4](#)), and a measuring [head](#) ([5.3.5](#)).

1) A suitable device is described by Zubryn, E. And Hook, G.L. in Appita 23(4): 279-290 (January 1970).

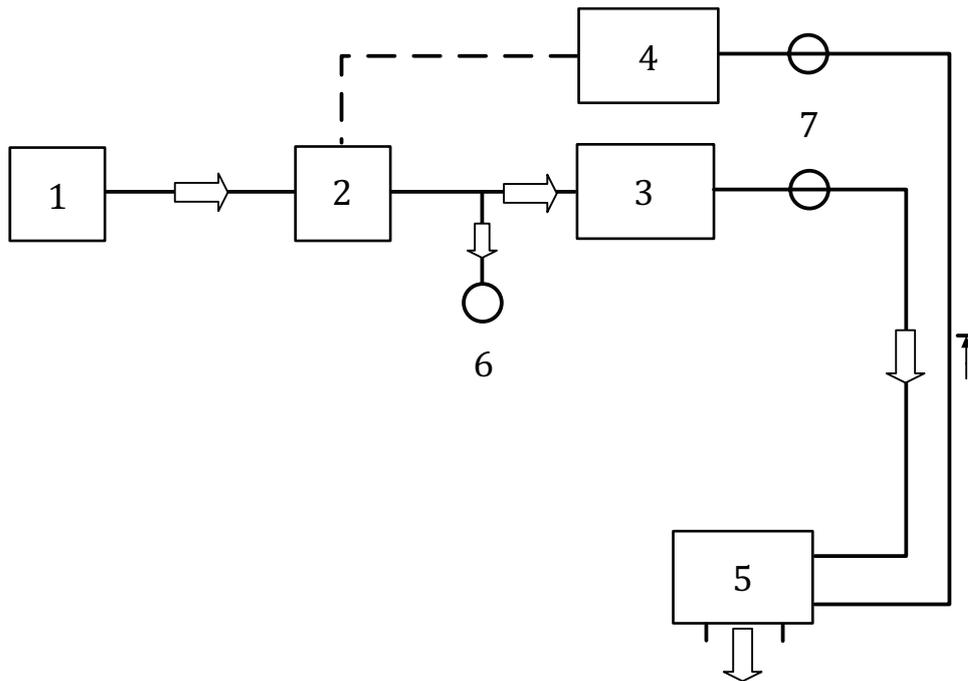

Key

- 1 air supplying device
- 2 pressure controlling device
- 3 flow sensor
- 4 pressure sensor
- 5 measuring head
- 6 permanent air leak
- 7 connectors

iTeh STANDARD PREVIEW
(standards.iteh.ai)

<https://standards.iteh.ai/catalog/standards/sist/d1b4b93d-c009-4339-a947-2c7c79ac0723/iso-8791-2-2013>

Figure 2 — Circuit diagram of electronic flowmeter type test apparatus

5.3.1 Compressed air supply system, capable of generating air at a pressure of about 127 kPa. If necessary, filters shall be provided to ensure that the air is clean and free from oil.

NOTE It is advisable to have the compressor located in a laboratory having the standard atmosphere for conditioning and testing.

5.3.2 Pressure regulator, or other means of creating a steady nominal air pressure of $1,47 \pm 0,02$ kPa.

5.3.3 Flowmeter, having a measuring range of 50 ml/min to 5 000 ml/min that allows the air flow to be determined with an error of less than ± 5 ml/min or ± 5 % of actual value whichever is greater.

5.3.4 Differential air pressure meter, that allows the differential air pressure over the test piece to be determined with an error of less than 3 % of the actual pressure.

5.3.5 Measuring head, consisting of an enclosed metal land preferably corrosion-resistant with an optically flat lower surface of $31,5 \text{ mm} \pm 0,2 \text{ mm}$ internal diameter and $0,150 \text{ mm} \pm 0,002 \text{ mm}$ width, and with a mass of $267 \text{ g} \pm 2 \text{ g}$.

5.3.6 Flat plate, polished flat plate, preferably glass used to check for air leaks and upon which the test piece is placed for testing. The leakage between the measuring head land and the flat plate shall not exceed 5 ml/min.

5.3.7 Heavy metal weight, heavy metal annulus, or other suitably shaped weight, for keeping the test piece flat around the measuring head

6 Sampling

If the tests are being made to evaluate a lot, the sample shall be selected in accordance with ISO 186. If the tests are made on another type of sample, make sure that the specimens taken are representative of the sample received.

7 Conditioning

Samples shall be conditioned in accordance with ISO 187.

8 Preparation of test pieces

Cut at least 10 test pieces for each side to be tested. The minimum size of each test piece shall be 75 mm x 75 mm and its surfaces shall be identified, e.g. top side and wire side.

The test area shall be free from folds, wrinkles, holes, watermarks or defects normally not inherent in the paper or board. Do not handle that part of the test piece which will become part of the test area.

9 Calibration and verification

9.1 Variable-area flowmeter type tester

Calibrate the instrument as described in [10.2.4](#) and [Annex B](#).
ISO 8791-2:2013

9.2 Electronic flowmeter type tester

Calibrate the instrument as described in Annex B.2 (as well as according to the instructions of the manufacturer).

10 Procedure

10.1 Test atmosphere

Carry out the testing under the same atmospheric conditions as those used to condition the test pieces. Test each side of the test pieces separately.

10.2 Determination using variable-area flowmeter type tester

10.2.1 Place the instrument on a rigid level bench. Level the instrument, ensure that no vibration can cause erroneous readings, and turn on the air supply.

10.2.2 Decide which variable-area flowmeter will be used for the test, selecting, where possible, the variable-area flowmeter which will give a reading in the upper 80 % of the range with the 1,47 kPa manostat weight. Do not use air flows above 1 200 ml/min because at high air flows the pressure drop between the flowmeter and the measuring head can be sufficient to render the calibration of the variable-area flowmeter invalid.

Set the valves at the bottom of the variable-area flowmeters so that air flows through the selected variable-area flowmeter. When the air flow has started, gently place the 1,47 kPa manostat weight on the shaft and start it spinning. It should continue to spin smoothly.

The manostat weight shall not be placed on the shaft until after the air flow has started and shall be removed before the air flow is stopped.

10.2.3 Set the valve at the outlet of the flowmeter so that air flows through the smaller (lower) outlet.

10.2.4 Verify the calibration of the variable-area flowmeter by temporarily replacing the measuring head with the appropriate capillary tube. The air flow reading should agree with the correct reading for that capillary tube to within $\pm 5\%$.

10.2.5 With the head connected to the flowmeter, lower the land on to the flat plate (5.2.6) and ensure that the float comes to rest at the bottom of the flowmeter. If not, check the system for air leaks as described in [Annex A](#), Clause A.1.

10.2.6 Place the test piece on the flat plate, with the side to be tested uppermost. Gently lower the measuring head on to the test piece, taking particular care to ensure that the land does not make an impression on the surface of the test piece. If the test piece will not lie flat, use the metal annulus (5.2.7) to hold it down. Record the flowmeter reading at the top of the float at least 5 s after lowering the head, with the reading accuracy indicated in 5.2.4.

10.2.7 Repeat 10.2.6 for the remaining test pieces for each side to be tested.

10.2.8 After completing the tests, remove the manostat weight and then turn off the air supply.

10.3 Determination using electronic flowmeter type tester (standards.iteh.ai)

10.3.1 Place the instrument on a rigid level bench. Level the instrument, ensure that no vibration can cause erroneous readings, and turn on the air supply.

10.3.2 Lower the land on to the flat plate (5.3.6) and check that the flowmeter reading does not exceed 5 ml/min.

10.3.3 Place the test piece on the flat plate, with the side to be tested uppermost and perform the test according to the instructions of the instrument manufacturer. If the test piece will not lie flat, use the metal annulus (5.3.7) to hold it down. Record the flowmeter reading of the instrument, with the reading accuracy indicated in 5.3.3.

10.3.4 Repeat 10.3.3 for the remaining test pieces for each side to be tested.

10.3.5 After completing the tests, turn off the air supply.

11 Expression of results

11.1 For each side tested, calculate and report the mean of the air flow readings, in ml/min, to three significant figures.

11.2 For each side tested, calculate the standard deviation or coefficient of variation to two significant figures for values less than 10 ml/min and to the nearest whole number for values equal to or greater than 10 ml/min.

12 Test report

The test report shall include the following information:

- a) a reference to this part of ISO 8791;

- b) date and place of testing;
- c) all the information necessary for complete identification of the sample;
- d) the type of instrument used;
- e) the conditioning atmosphere used;
- f) the number of test pieces tested;
- g) the pressure difference used, in kilopascals;
- h) the flowmeter range used;
- i) the mean Bendtsen roughness, in ml/min, as calculated in [11.1](#);
- j) the standard deviation or coefficient of variation, as calculated in [11.2](#);
- k) any deviations from the procedure described in this part of ISO 8791, that may have influenced the results.

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[ISO 8791-2:2013](#)

<https://standards.iteh.ai/catalog/standards/sist/d1b4b93d-c009-4339-a947-2c7c79ac0723/iso-8791-2-2013>