

---

---

**Measurement of radioactivity in the  
environment — Air: radon-222 —**

Part 2:

**Integrated measurement method for  
determining average potential alpha  
energy concentration of its short-lived  
decay products**

iTeh STANDARD PREVIEW  
(standards.iteh.ai)

*Mesurage de la radioactivité dans l'environnement — Air: radon 222 —*

*Partie 2: Méthode de mesure intégrée pour la détermination de l'énergie  
alpha potentielle volumique moyenne de ses descendants à vie courte*

<https://standards.iteh.ai/catalog/standards/sist/12ca04c-1d02-4a00-9679-51df7185bcfd/iso-11665-2-2012>



**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

ISO 11665-2:2012

<https://standards.iteh.ai/catalog/standards/sist/f2eac4e-f90d-4a6d-9679-51df7185bcfd/iso-11665-2-2012>



**COPYRIGHT PROTECTED DOCUMENT**

© ISO 2012

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Case postale 56 • CH-1211 Geneva 20  
Tel. + 41 22 749 01 11  
Fax + 41 22 749 09 47  
E-mail [copyright@iso.org](mailto:copyright@iso.org)  
Web [www.iso.org](http://www.iso.org)

Published in Switzerland

# Contents

Page

Foreword .....	iv
Introduction .....	v
1 Scope .....	1
2 Normative references .....	1
3 Terms, definitions and symbols .....	1
3.1 Terms and definitions .....	1
3.2 Symbols .....	2
4 Principle of the measurement method .....	3
5 Equipment .....	3
5.1 General .....	3
5.2 Measuring device .....	3
5.3 Counting system .....	4
6 Sampling .....	4
6.1 Sampling objective .....	4
6.2 Sampling characteristics .....	4
6.3 Sampling conditions .....	5
7 Detection method .....	6
8 Measurement .....	6
8.1 Procedure .....	6
8.2 Influence quantities .....	6
8.3 Calibration .....	7
9 Expression of results .....	7
9.1 Average potential alpha energy concentration .....	7
9.2 Standard uncertainty .....	8
9.3 Decision threshold and detection limit .....	8
9.4 Limits of the confidence interval .....	9
10 Test report .....	9
Annex A (informative) Example of a method meeting the requirements of this part of ISO 11665 .....	11
Bibliography .....	13

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 11665-2 was prepared by Technical Committee ISO/TC 85, *Nuclear energy, nuclear technologies, and radiological protection*, Subcommittee SC 2, *Radiological protection*.

ISO 11665 consists of the following parts, under the general title *Measurement of radioactivity in the environment — Air: radon-222*:

- *Part 1: Origins of radon and its short-lived decay products and associated measurement methods*
- *Part 2: Integrated measurement method for determining average potential alpha energy concentration of its short-lived decay products*
- *Part 3: Spot measurement method of the potential alpha energy concentration of its short-lived decay products*
- *Part 4: Integrated measurement method for determining average activity concentration using passive sampling and delayed analysis*
- *Part 5: Continuous measurement method of the activity concentration*
- *Part 6: Spot measurement method of the activity concentration*
- *Part 7: Accumulation method for estimating surface exhalation rate*
- *Part 8: Methodologies for initial and additional investigations in buildings*

The following parts are under preparation:

- *Part 9: Method for determining exhalation rate of dense building materials*
- *Part 10: Determination of diffusion coefficient in waterproof materials using activity concentration measurement*

## Introduction

Radon isotopes 222, 220 and 219 are radioactive gases produced by the disintegration of radium isotopes 226, 224 and 223, which are decay products of uranium-238, thorium-232 and uranium-235 respectively, and are all found in the earth's crust. Solid elements, also radioactive, followed by stable lead are produced by radon disintegration<sup>[1]</sup>.

When disintegrating, radon emits alpha particles and generates solid decay products, which are also radioactive (polonium, bismuth, lead, etc.). The potential effects on human health of radon lie in its solid decay products rather than the gas itself. Whether or not they are attached to atmospheric aerosols, radon decay products can be inhaled and deposited in the bronchopulmonary tree to varying depths according to their size.

Radon is today considered to be the main source of human exposure to natural radiation. The UNSCEAR (2006) report<sup>[2]</sup> suggests that, at the worldwide level, radon accounts for around 52 % of global average exposure to natural radiation. The radiological impact of isotope 222 (48 %) is far more significant than isotope 220 (4 %), while isotope 219 is considered negligible. For this reason, references to radon in this part of ISO 11665 refer only to radon-222.

Radon activity concentration can vary by one to multiple orders of magnitude over time and space. Exposure to radon and its decay products varies tremendously from one area to another, as it depends firstly on the amount of radon emitted by the soil and the building materials in each area and, secondly, on the degree of containment and weather conditions in the areas where individuals are exposed.

Variations of a few nanojoules per cubic metre to several thousand nanojoules per cubic metre are observed in the potential alpha energy concentration of short-lived radon decay products.

The potential alpha energy concentration of short-lived radon-222 decay products in the atmosphere can be measured by spot and integrated measurement methods (see ISO 11665-1). This part of ISO 11665 deals with integrated measurement methods. Integrated measuring methods are applicable in assessing human exposure to radiation<sup>[3]</sup>.

[ISO 11665-2:2012](https://standards.iteh.ai/catalog/standards/sist/f2eaac4e-f90d-4a6d-9679-1d7183684a5e/iso-11665-2-2012)

NOTE The origin of radon-222 and its short-lived decay products in the atmospheric environment and other measurement methods are described generally in ISO 11665-1.

**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

[ISO 11665-2:2012](https://standards.iteh.ai/catalog/standards/sist/f2eaac4e-f90d-4a6d-9679-51df7185bcfd/iso-11665-2-2012)

<https://standards.iteh.ai/catalog/standards/sist/f2eaac4e-f90d-4a6d-9679-51df7185bcfd/iso-11665-2-2012>

# Measurement of radioactivity in the environment — Air: radon-222 —

## Part 2:

# Integrated measurement method for determining average potential alpha energy concentration of its short-lived decay products

## 1 Scope

This part of ISO 11665 describes integrated measurement methods for short-lived radon-222 decay products<sup>[4]</sup>. It gives indications for measuring the average potential alpha energy concentration of short-lived radon-222 decay products in the air and the conditions of use for the measuring devices.

This part of ISO 11665 covers samples taken over periods varying from a few weeks to one year. This part of ISO 11665 is not applicable to systems with a maximum sampling duration of less than one week.

The measurement method described is applicable to air samples with potential alpha energy concentration of short-lived radon-222 decay products greater than 10 nJ/m<sup>3</sup> and lower than 1 000 nJ/m<sup>3</sup>.

NOTE For informative purposes only, this document also addresses the case of radon-220 decay products, given the similarity in behaviour of the radon isotopes 222 and 220.

## 2 Normative references

[ISO 11665-2:2012](https://standards.iteh.ai/catalog/standards/sist/f2eaac4e-f90d-4a6d-9679-31df2185bcd/iso-11665-2-2012)

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 11665-1, *Measurement of radioactivity in the environment — Air: radon-222 — Part 1: Origins of radon and its short-lived decay products and associated measurement methods*

ISO/IEC 17025, *General requirements for the competence of testing and calibration laboratories*

IEC 61577-1, *Radiation protection instrumentation — Radon and radon decay product measuring instruments — Part 1: General principles*

IEC 61577-3, *Radiation protection instrumentation — Radon and radon decay product measuring instruments — Part 3: Specific requirements for radon decay product measuring instruments*

## 3 Terms, definitions and symbols

### 3.1 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 11665-1 apply.

### 3.2 Symbols

For the purposes of this document, the symbols given in ISO 11665-1 and the following apply.

$a$	attenuation coefficient relating to the $^{222}\text{Rn}$ found in the collimators corresponding to the range $P_1$ (established theoretically and provided by the manufacturer)
$b$	attenuation coefficient relating to the $^{222}\text{Rn}$ found in the collimators corresponding to the range $P_2$ (established theoretically and provided by the manufacturer)
$E_{\text{AE},i}$	alpha particle energy produced by the disintegration of the nuclide $i$ , in joules
$\bar{E}_{\text{PAEC},i}$	average potential alpha energy concentration of the nuclide $i$ , in joules per cubic metre
$\bar{E}_{\text{PAEC},i}^*$	decision threshold of the average potential alpha energy concentration of the nuclide $i$ , in joules per cubic metre
$\bar{E}_{\text{PAEC},i}^\#$	detection limit of the average potential alpha energy concentration of the nuclide $i$ , in joules per cubic metre
$\bar{E}_{\text{PAEC},i}^{\triangleleft}$	lower limit of the confidence interval of the average potential alpha energy concentration of the nuclide $i$ , in joules per cubic metre
$\bar{E}_{\text{PAEC},i}^{\triangleright}$	upper limit of the confidence interval of the average potential alpha energy concentration of the nuclide $i$ , in joules per cubic metre
$n$	counting number of each range $P_i$
$P_i$	range recording alpha particles for $i = 1, 2, 3, 4$
$R_{P_i,j}$	$j^{\text{th}}$ number of net count of range $P_i$ with deduced background for $i = 1, 2, 3, 4$
$\bar{R}_{P_i}$	mean number of net count of range $P_i$ with deduced background for $i = 1, 2, 3, 4$
$\bar{R}_0$	mean number of count due to background
$r$	ratio between the number of alpha particles emitted by $^{212}\text{Bi}$ ( $\alpha$ emitter at 36 %) and the number of alpha particles emitted by $^{212}\text{Po}$ (produced by $\beta$ disintegration at 64 % of $^{212}\text{Bi}$ ); 0,56
$U$	expanded uncertainty calculated by $U = k \cdot u( )$ with $k = 2$
$u( )$	standard uncertainty associated with the measurement result
$u_{\text{rel}}( )$	relative standard uncertainty
$V$	sampled volume, in cubic metres
$\varepsilon_{\text{gd}}$	geometric detection efficiency (established theoretically), i.e. the ratio between the number of tracks counted and the number of alpha particles emitted by the deposit collected on the filter
$\varepsilon_{\text{hc}}$	collection efficiency (established experimentally), i.e. the ratio between the number of atoms of short-lived decay products collected per unit of sampled volume of air and the number of atoms per unit of volume of air present in the detection system environment

STANDARD PREVIEW

(standards.iteh.ai)

ISO 11665-2:2012

<https://standards.iteh.ai/catalog/standards/sist/124ae4c1-b0d1-4add-9679-51df7185bcfd/iso-11665-2-2012>

51df7185bcfd/iso-11665-2-2012



## 4 Principle of the measurement method

Integrated measurement of potential alpha energy concentration of short-lived radon decay products is based on the following elements:

- a) continuous sampling of short-lived radon decay products contained in an air volume representative of the atmosphere under investigation, using a high-efficiency filtering membrane;
- b) counting, and discriminating over four energy ranges, the alpha particles emitted by the collected short-lived radon-222 decay products (alpha particles with an energy  $E_{AE,218Po}$  and  $E_{AE,214Po}$  produced by the disintegration of  $^{218}Po$  and  $^{214}Po$ , and the disintegration of  $^{214}Pb$  and  $^{214}Bi$  potential emitters of alpha particles of this type), using a solid-state nuclear track detector;
- c) calculation of the potential alpha energy concentration of the short-lived radon-222 decay products.

NOTE For the radon-220 decay products, this involves distinguishing between, and counting, the alpha particles, with an energy  $E_{AE,212Bi}$  and  $E_{AE,212Po}$ , released through disintegration of  $^{216}Po$  and  $^{212}Po$ , and disintegration of  $^{212}Pb$  and  $^{212}Bi$  potential emitters of alpha particles of this type.

## 5 Equipment

### 5.1 General

The apparatus shall include a measuring device, composed of a sampling system and a detection system (see Figure 1), and a counting system. The measuring device shall be in accordance with IEC 61577-1 and IEC 61577-3.

### 5.2 Measuring device

[ISO 11665-2:2012](https://standards.iteh.ai/catalog/standards/sist/f2eac4e-f90d-4a6d-9679-51df7185bcfd/iso-11665-2-2012)

[https://standards.iteh.ai/catalog/standards/sist/f2eac4e-f90d-4a6d-9679-](https://standards.iteh.ai/catalog/standards/sist/f2eac4e-f90d-4a6d-9679-51df7185bcfd/iso-11665-2-2012)

#### 5.2.1 Sampling system

[51df7185bcfd/iso-11665-2-2012](https://standards.iteh.ai/catalog/standards/sist/f2eac4e-f90d-4a6d-9679-51df7185bcfd/iso-11665-2-2012)

The sampling system shall include the following components:


- a) a high-efficiency filtering membrane in cellulose acetate to collect the radon decay products;
- b) a sampling pump which provides a volume rate compatible with the air and metrological characteristics of the detection system;
- c) a mass flow-meter which measures the flow-rate of air sampled throughout the sampling duration.

The sampling system is located downstream of the detection system.

#### 5.2.2 Detection system

The detection system shall include the following components:

- a) three boPET screens of different thickness placed at one end of the collimators are used to discriminate between the particles over three energy ranges. This geometry is used to mitigate the initial energy of each alpha particle emitted by the collected radionuclides in an energy range compatible with the characteristics of the sensor (SSNTD) used;
- b) a solid-state nuclear track detector (SSNTD).

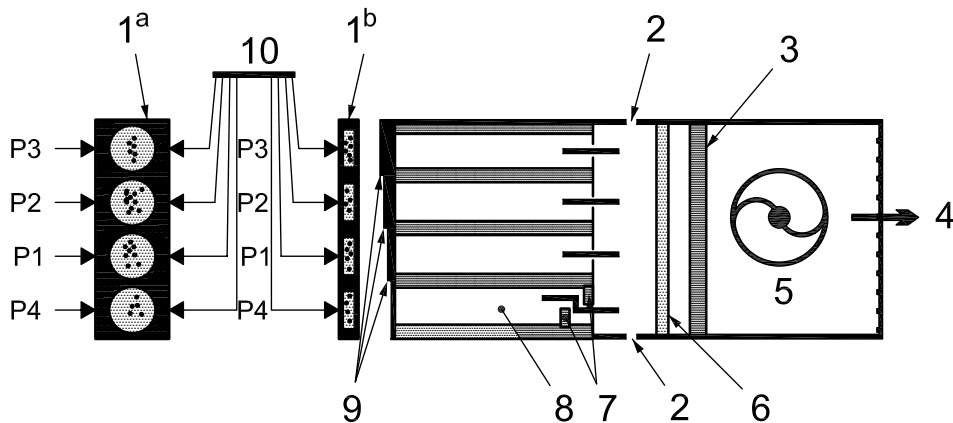

- Key**
- 1 solid state nuclear track detector (SSNTD)
  - 2 air inlet
  - 3 mass flow-meter
  - 4 air outlet
  - 5 vacuum pump
  - 6 high-efficiency filter
  - 7 baffles (diffusion barrier)
  - 8 collimator
  - 9 boPET (biaxially oriented polyethylene terephthalate) screen
  - 10 scanning range
  - a Front view.
  - b Side view.

ITIH STANDARD PREVIEW  
(standards.iteh.ai)

ISO 11665-2:2012

Figure 1 — Example set-up of a measuring device for determination over four energy ranges of average potential alpha energy concentration of short-lived radon-222 decay products

**5.3 Counting system**

The counting system shall include the following components:

- a) equipment and suitable chemical reagents for etching the detector (SSNTD);
- b) an optical microscope and associated equipment for scanning and counting the etched tracks.

**6 Sampling**

**6.1 Sampling objective**

The sampling objective is to collect, without interruption, all the aerosols carrying short-lived radon decay products, regardless of size (unattached and attached fractions), that are contained in the ambient air during a given sampling duration (at least one week).

**6.2 Sampling characteristics**

Sampling shall be carried out under the conditions specified in ISO 11665-1.

The short-lived radon decay products shall be sampled continuously and directly in the atmosphere under investigation by pumping and filtering a known volume of air through a high-efficiency collection membrane. The air sample shall be omni-directional.

The filtering membrane shall be as close as possible to the sampler inlet section, so as to collect the ambient decay products with the maximum efficiency.

In order to count the emitted alpha particles correctly, the sampling system shall conduct to the surface deposit of the radionuclides on the filter and shall prevent the aerosols from being buried.

The sampling system shall be used in conditions that preclude clogging of the filtering membrane, which would cause self-absorption of the alpha emissions of particles collected on the filter or a reduction in the sampling flow-rate over time.

The sampling flow-rate shall be stable (no more than 10 % variation from the average value) in order for the sampling to remain representative throughout the sampling duration. This can be achieved by using a flow-rate controller (sonic throat, servo-controlled valve, etc.).

### 6.3 Sampling conditions

#### 6.3.1 General

Sampling shall be carried out as specified in ISO 11665-1.

#### 6.3.2 Installation of sampling system

Installation of the sampling system shall be carried out as specified in ISO 11665-1.

In the specific case of an indoor measurement, the sampling system shall be installed as follows:

- a) in an area not directly exposed to solar radiation;
- b) away from a heat source (radiator, picture windows, electrical equipment, etc.);
- c) away from traffic areas, doors and windows, walls and ventilation sources (it could, for example, be sited on an item of furniture like a shelf or sideboard).

#### 6.3.3 Sampling duration

The sampling duration is equal to the time interval between installation and removal of the sampling system at a given point.

Time (date and hour) of installation and time of removal of the sampling system shall be recorded.

Sampling duration shall be determined according to the intended use of the measurement results and the phenomenon under investigation.

A sampling duration of at least one week is required in order to obtain a measurement result above the detection limit.

It is recommended that measurements be performed with a sampling duration of several months when assessing the annual human exposure.

Users should be aware of the saturation characteristics of the sensor (SSNTD) and should perform their sampling regime so as to ensure that saturation does not occur.

#### 6.3.4 Volume of air sampled

The volume of air sampled shall be ascertained by measuring the flow-rate or volume during sampling with a calibrated system (for example, a sonic nozzle) (see IEC 61577-3).

The total volume of air sampled throughout the sampling duration shall be recorded.