



Designation: E355 – 96(Reapproved 2007)

Standard Practice for Gas Chromatography Terms and Relationships¹

This standard is issued under the fixed designation E355; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

This standard has been approved for use by agencies of the Department of Defense.

1. Scope

1.1 This practice covers primarily the terms and relationships used in gas elution chromatography. However, most of the terms should also apply to other kinds of gas chromatography and are also valid in the various liquid column chromatographic techniques, although at this time they are not standardized for the latter usage.

2. Names of Techniques

2.1 *Gas Chromatography*, abbreviated as GC, comprises all chromatographic methods in which the moving phase is gaseous. The stationary phase may be either a dry granular solid or a liquid supported by the granules or by the wall of the column, or both. Separation is achieved by differences in the distribution of the components of a sample between the mobile and stationary phases, causing them to move through the column at different rates and from it at different times. In this recommended practice gas elution chromatography is implied.

2.2 *Gas-Liquid Chromatography*, abbreviated as GLC, utilizes a liquid as the stationary phase, which acts as a solvent for the sample components.

2.3 *Gas-Solid Chromatography*, abbreviated as GSC, utilizes an active solid (adsorbent) as the stationary phase.

2.4 *Gas Elution Chromatography* utilizes a continuous inert gas flow as the carrier gas and the sample is introduced as a gas or a liquid with a finite volume into the carrier gas stream. If the sample is introduced as a liquid, it is vaporized in the system prior to or during passage through the separation column.

2.5 *Gas-Frontal Chromatography* is a technique in which a continuous stream of carrier gas mixed with sample vapor is instantaneously replaced by a continuous stream of carrier gas containing sample vapor at a different concentration. The concentration profile is therefore step-shaped at the column inlet.

2.6 *Gas-Displacement Chromatography* employs a desorbent as the carrier gas or in the carrier gas to displace a less strongly held solute from the stationary phase which in turn displaces the next less strongly held one etc., causing the components to emerge in the normal order, that is, least-to-most strongly absorbed.

2.7 *Isothermal Gas Chromatography* is the version of the technique in which the column temperature is held constant during the passage of the sample components through the separation column.

2.8 *Programmed Temperature Gas Chromatography* (PTGC), is the version of the technique in which the column temperature is changed with time during the passage of the sample components through the separation column. In linear PTGC the program rate is constant during analysis. Isothermal intervals may be included in the temperature program.

2.9 *Programmed Flow, Pressure, or Velocity Gas Chromatography* is the version of the technique in which the carrier gas flow, pressure, or velocity is changed during analysis.

2.10 *Reaction Gas Chromatography* is the version of the technique in which the composition of the sample is changed between sample introduction and the detector. The reaction can take place upstream of the column when the chemical composition of the individual components passing through the column differs from that of the original sample, or between the column and the detector when the original sample components are separated in the column but their chemical composition is changed prior to entering the detection device.

2.11 *Pyrolysis Gas Chromatography* is the version of reaction gas chromatography in which the original sample is decomposed by heat to more volatile components prior to passage through the separation column.

3. Apparatus

3.1 *Sample Inlet Systems*, represent the means for introducing samples into the separation column, including the heated zones permitting the vaporization of the introduced liquid samples prior to their passage through the column. Sample introduction can be carried out by introduction of a liquid, solid, or gas into the carrier-gas stream. The sample may be vaporized before or after introduction into the column.

¹ This practice is under the jurisdiction of ASTM Committee E13 on Molecular Spectroscopy and Separation Science and is the direct responsibility of Subcommittee E13.19 on Separation Science.

Current edition approved March 1, 2007. Published March 2007. Originally approved in 1968. Last previous edition approved in 2001 as E355 – 96 (2001). DOI: 10.1520/E0355-96R07.

3.1.1 *Direct Inlets*, rapidly vaporize the sample prior to entering the column. All of the sample vapor enters the column.

3.1.2 *On-Column Inlets*, introduce a liquid sample into the column. The sample vaporizes as the column section containing the liquid heats up after injection.

3.1.3 *Split Inlets*, rapidly vaporize the sample prior to entering the column. A defined fraction of the sample vapor enters the column; the remainder leaves the inlet through a vent at a flow rate F_v . The ratio of the total inlet flow ($F_v + F_c$) to the column flow (F_c) is called the split ratio (s):

$$s = \frac{F_v + F_c}{F_c} \quad (1)$$

3.1.4 *Splitless Injection*, utilizes a split inlet wherein the split vent flow is blocked during the injection period such that most of the sample vapor enters the column. The injection period is typically one minute. The split vent flow is reestablished afterward usually for the remainder of the run.

3.1.5 *Programmed-Temperature Vaporizers (PTV)*, accept a liquid sample that vaporizes as the inlet system heats up after injection. A PTV may operate in either a split, splitless, on-column, or direct mode.

3.1.6 A *Retention Gap*, is a section of tubing inserted between the inlet and the analytical column proper. The retention gap may have an inner diameter different than the analytical column. The retention gap has significantly lower retaining power than the analytical column; in practice the retention gap is deactivated but not coated.

3.2 *Columns*, consist of tubes that contain the stationary phase and through which the gaseous mobile phase flows.

3.2.1 *Packed Columns*, are filled with granular packing that is kept in place by gas-permeable plugs at both ends.

3.2.2 *Open-Tubular Columns*, have unobstructed central gasflow channels.

3.2.2.1 *Wall-Coated Open-Tubular Columns*, abbreviated WCOT columns, have the liquid phase coated directly on the inside, relatively smooth wall of the column tubing.

3.2.2.2 *Porous-Layer Open-Tubular Columns*, abbreviated PLOT columns, have a solid porous layer present on the tube wall but still maintain the unobstructed central gas-flow channel. This porous solid layer can either act as an adsorbent or a support which in turn is coated with a thin film of the liquid phase, or both. The solid layer can either be deposited on the inside tube wall or formed by chemical means from the wall.

3.2.2.3 *Support-Coated Open-Tubular Columns*, abbreviated SCOT columns, refer to those PLOT Columns where the solid layer consists of the particles of a solid support which were deposited on the inside tube wall.

3.3 *Detectors*, are devices that indicate the presence of eluted components in the carrier gas emerging from the column.

3.3.1 *Differential Concentration Detectors*, measure the instantaneous proportion of eluted sample components in the carrier gas passing through the detector.

3.3.2 *Differential Mass Detectors*, measure the instantaneous rate of arrival of sample components at the detector.

3.3.3 *Integral Detectors*, measure the accumulated quantity of sample component(s) reaching the detector.

3.3.4 *Spectrometric Detectors*, measure and record spectra of eluting components, such as the mass spectrum of the infrared spectrum.

3.4 *Traps*, are devices for recovering sample components from the mobile phase eluting from GC columns.

4. Reagents

4.1 *Carrier Gas* is the *Mobile Phase* used to sweep or elute the sample components through and from the column.

4.2 The *Stationary Phase* is composed of the active immobile materials within the column that selectively delay the passage of sample components by dissolving or adsorbing them, or both. Inert materials that merely provide physical support for the stationary phase or occupy space within the column are not part of the stationary phase.

4.2.1 *Liquid Stationary Phase* is one type of stationary phase which is dispersed on the solid support or the inner column wall and causes the separation of the sample components by differences in the partitioning of the sample components between the mobile and liquid phases.

4.2.2 An *Active Solid* is one that has ab- or adsorptive properties by means of which chromatographic separations may be achieved.

4.3 The *Solid Support* is the inert material that holds the stationary (liquid) phase in intimate contact with the carrier gas flowing through it. It may consist of porous or impenetrable particles or granules which hold the liquid phase and between which the carrier gas flows, or the interior wall of the column itself, or a combination of these.

4.4 The *Column Packing* consists of all the material used to fill packed columns, including the solid support and the liquid phase or the active solid.

4.4.1 The *Liquid-Phase Loading* describes the relative amount of liquid phase present in a packed column when the column packing consists only of the liquid phase plus the solid support. It is usually expressed as weight percent of liquid phase present in the column packing:

$$\begin{aligned} \text{Liquid - phase loading, wt\%} & \quad (2) \\ & = \frac{(\text{amount of liquid phase}) \times 100}{(\text{amount of liquid phase} + \text{amount of solid support})} \end{aligned}$$

4.5 *Solutes* are the introduced sample components that are delayed by the column as they are eluted through it by the carrier gas.

4.6 *Unretained Substances* are not delayed by the column packing.

5. Gas Chromatographic Data

5.1 A *Chromatogram* is a plot of detector response against time or effluent volume. Idealized chromatograms obtained with differential and integral detectors for an unretained substance and one other component are shown in Fig. 1.

5.2 The definitions in this paragraph apply to chromatograms obtained directly by means of differential detectors or by

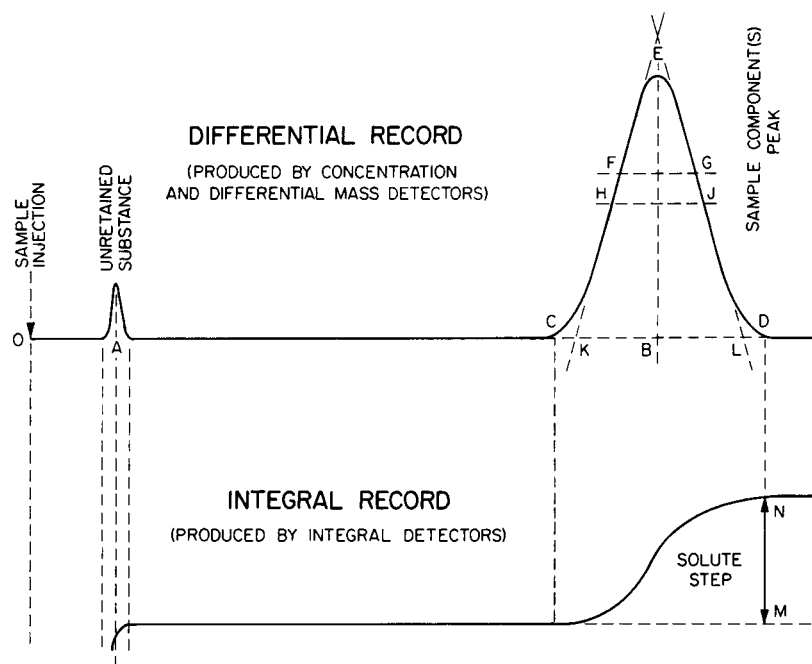


FIG. 1 Typical Chromatogram.

differentiating the records obtained by means of integral detectors. The *Baseline* is the portion of the chromatogram recording the detector response in the absence of solute or solvent emerging from the column. A *Peak* is the portion of the chromatogram recording the detector response while a single component is eluted from the column. If two or more sample components emerge together, they appear as a single peak. The *Peak Base*, *CD* in Fig. 1, is an interpolation of the baseline between the extremities of the peak. The area enclosed between the peak and the peak base, *CHFEGJD* in Fig. 1, is the *Peak Area*. The dimension *BE* from the peak maximum to the peak base measured in the direction of detector response is the *Peak Height*. Retention dimensions parallel to the baseline are termed as the peak widths. The retention dimension of a line parallel to the peak base bisecting the peak height and terminating at the inflexion points *FG* of the tangents drawn to the inflexion points (= 60.7 % of peak height) is the *Peak Width at Inflexion Points*, w_i . The retention dimension of a line parallel to the peak base drawn to 50 % of the peak height and terminating at the sides *HJ* of the peak is the *Peak Width at Half Height*, w_h . The retention dimension of the segment of the peak base *KL* intercepted by the tangents drawn to the inflection points on both sides of the peak is the *Peak Width at Base* or *Base Width*, w_b .

5.3 The following definitions apply to chromatograms obtained with integral detectors, or by integration of the records obtained by means of differential detectors. As sample components pass through the detector the baseline is displaced cumulatively. The change in baseline position as a single sample component is eluted is a *Step*. The difference between

straight line extensions of the baselines on both sides of the step, measured in the direction of detector response, is the *Step Height*, *NM*.

6. Retention Parameters

6.1 Retention parameters are listed in Table 1. The interrelations shown apply only to gas elution chromatography columns operated under constant conditions and for which the partition coefficients are independent of concentration. Fig. 1 can be used to illustrate some of these parameters:

Gas holdup time	=	OA
Retention time	=	OB
Adjusted retention time	=	AB
Partition (capacity) ratio	=	AB/OA
Peak width at half height	=	HJ
Peak width at base	=	KL
Number of theoretical plates	=	$16 (OB/KL)^2 = v 5.54 (OB/HJ)^2$
Relative retention	=	$(AB)/(AB)_i$ or $(AB)/(AB)_s$
Peak resolution	=	$\frac{2[(OB)_j - (OB)_i]}{(KL)_i + (KL)_j} = \frac{(OB)_j - (OB)_i}{(KL)_j}$

Subscripts *i*, *j*, and *s* refer to any earlier peak, any later peak, and a reference peak, respectively.

7. Presentation of Isothermal Retention Data

7.1 Retention values should be reported in a form that can be applied for a specific stationary phase composition in different apparatus and for different conditions of column length, diameter, and inlet and outlet pressures, and for different carrier gases and flow rate. When the solid support is inert, its particle-size range and distribution, and (within limits)