
**Laboratory glass and plastics ware —
Tubes for the measurement of the
erythrocyte sedimentation rate by the
Westergren method**

*Matériel de laboratoire en verre et en plastique — Tubes pour le
mesurage de la vitesse de sédimentation des érythrocytes par la
méthode Westergren*

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 13079:2011

<https://standards.iteh.ai/catalog/standards/sist/de9f8db9-21ac-4f51-813b-b0b04984e35f/iso-13079-2011>



iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 13079:2011

<https://standards.iteh.ai/catalog/standards/sist/de9f8db9-21ac-4f51-813b-b0b04984e35f/iso-13079-2011>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2011

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

Page

Foreword	iv
1 Scope	1
2 Normative references	1
3 Material	1
3.1 General	1
3.2 Glass	1
3.3 Plastics	2
4 Single-use Westergren tubes	2
4.1 General design	2
4.2 Straightness	2
4.3 Finish	2
4.4 Dimensions	2
4.5 Graduation and figuring	3
4.6 Inscriptions	3
4.7 Labelling	3
5 Re-usable Westergren tubes	3
5.1 General design	3
5.2 Straightness	4
5.3 Finish	4
5.4 Dimensions	4
5.5 Graduation and figuring	4
5.6 Inscriptions	4
5.7 Labelling	4
6 Support for Westergren tubes	5
6.1 Construction	5
6.2 Graduation and figuring	6
6.3 Inscriptions	6
7 Graduation and figuring	6
7.1 Graduation	6
7.2 Figuring of graduation lines	7
8 Marking	7
9 Labelling	7
9.1 Single-use Westergren tubes	7
9.2 Re-usable Westergren tubes	7
Annex A (normative) Type test for rigidity of Westergren tubes	9
Annex B (normative) Type test for contamination and interfering substances	10
Annex C (normative) Type test for straightness of Westergren tubes	11
Annex D (informative) Measurement of the erythrocyte sedimentation rate by the Westergren reference method	13
Bibliography	15

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 13079 was prepared by Technical Committee ISO/TC 48, *Laboratory equipment*, Subcommittee SC 6, *Glass and plastics ware including volumetric instruments*.

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[ISO 13079:2011](https://standards.iteh.ai/catalog/standards/sist/de9f8db9-21ac-4f51-813b-b0b04984e35f/iso-13079-2011)

<https://standards.iteh.ai/catalog/standards/sist/de9f8db9-21ac-4f51-813b-b0b04984e35f/iso-13079-2011>

Laboratory glass and plastics ware — Tubes for the measurement of the erythrocyte sedimentation rate by the Westergren method

1 Scope

This International Standard specifies requirements for single-use and re-usable glass and plastics tubes for measuring the erythrocyte sedimentation rate (ESR) by the Westergren method, and for a support to hold tubes during the performance of the test. These so-called “Westergren tubes” are also sometimes designated as “Westergren pipettes”. A procedure for measuring the erythrocyte sedimentation rate by the Westergren method is given in informative Annex D.

This International Standard does not apply to single-use containers for human venous blood specimen collection and their accessories for which other standards apply. It also does not apply for devices where the Westergren method has been used as basis to develop other, similar methods or equipment for the erythrocyte sedimentation rate determination.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 719, *Glass — Hydrolytic resistance of glass grains at 98 °C — Method of test and classification*

3 Material

3.1 General

3.1.1 Westergren tubes shall be made from rigid, transparent plastics or from glass of Class HGB 1, HGB 2 or HGB 3 in accordance with ISO 719 so that:

- a) the rigidity, when tested according to Annex A, shall be such that the distortion does not exceed 1 mm for re-usable Westergren tubes and 1,5 mm for single-use Westergren tubes;
- b) the transparency shall be sufficient to permit the top of the column of blood and the top of the red cell layer to be seen clearly in relation to the scale.

3.1.2 Westergren tubes shall be free from defects which impair observation of the top of the column of blood and of the top of the red cell layer.

3.2 Glass

The manufacturer of the glass tubes should ensure that the glass tubes are as free as possible from visible defects and reasonably free from internal stress.

3.3 Plastics

3.3.1 The material of which plastics tubes are made shall not affect the ESR value, when tested in accordance with the method described in Annex B, by more than 6 mm.

3.3.2 The manufacturer of the plastics tubes shall ensure the following:

- a) they shall not show adhesive properties towards blood cells;
- b) they shall not release plasticizers that might alter sedimentation;
- c) if a mould-release agent is used in the manufacturing process, it shall not alter sedimentation.

3.3.3 The user should also check the validity of a batch of plastics tubes by comparing the ESR obtained when the test is performed using some of these with the results when glass reference tubes are used.

4 Single-use Westergren tubes

4.1 General design

The general design of the single-use Westergren tube shall be as shown in Figure 1.

4.2 Straightness

The tube shall be straight when tested in accordance with the method described in Annex C.

4.3 Finish

4.3.1 The glass tube shall be cut square (within 10°) with the axis of the tube, and shall be lightly fire polished at each end. The ends may be slightly narrowed within or close to the tolerance given in Table 1, due to the finishing process.

4.3.2 The plastics tube should be cut square (within 10°) with the axis of the tube. The ends should be smooth and may be slightly bevelled. Other ends are acceptable if they comply with the dimensional requirements as specified in Table 1.

4.3.3 The tube shall be supplied free from any contamination which would affect the ESR value when tested in accordance with the method described in Annex B.

4.3.4 The tube, by itself or in association with its support, shall have a mechanism which ensures that the tube remains filled with blood, from its lower end to the zero mark on the scale, during the 60 min required to determine the ESR.

4.4 Dimensions

The measuring part of the tube shall conform to the dimensions given in Table 1.

Table 1 — Essential dimensions of single-use Westergren tubes

Dimensions in millimetres

Internal diameter	2,55 ± 0,15
Length of measuring part	200 ± 2

4.5 Graduation and figuring


Graduation or figuring shall be in accordance with Clause 7.

4.6 Inscriptions

Inscriptions on the Westergren tube shall be in accordance with Clause 8.

4.7 Labelling

Inscriptions on the packaging shall be in accordance with 9.1.

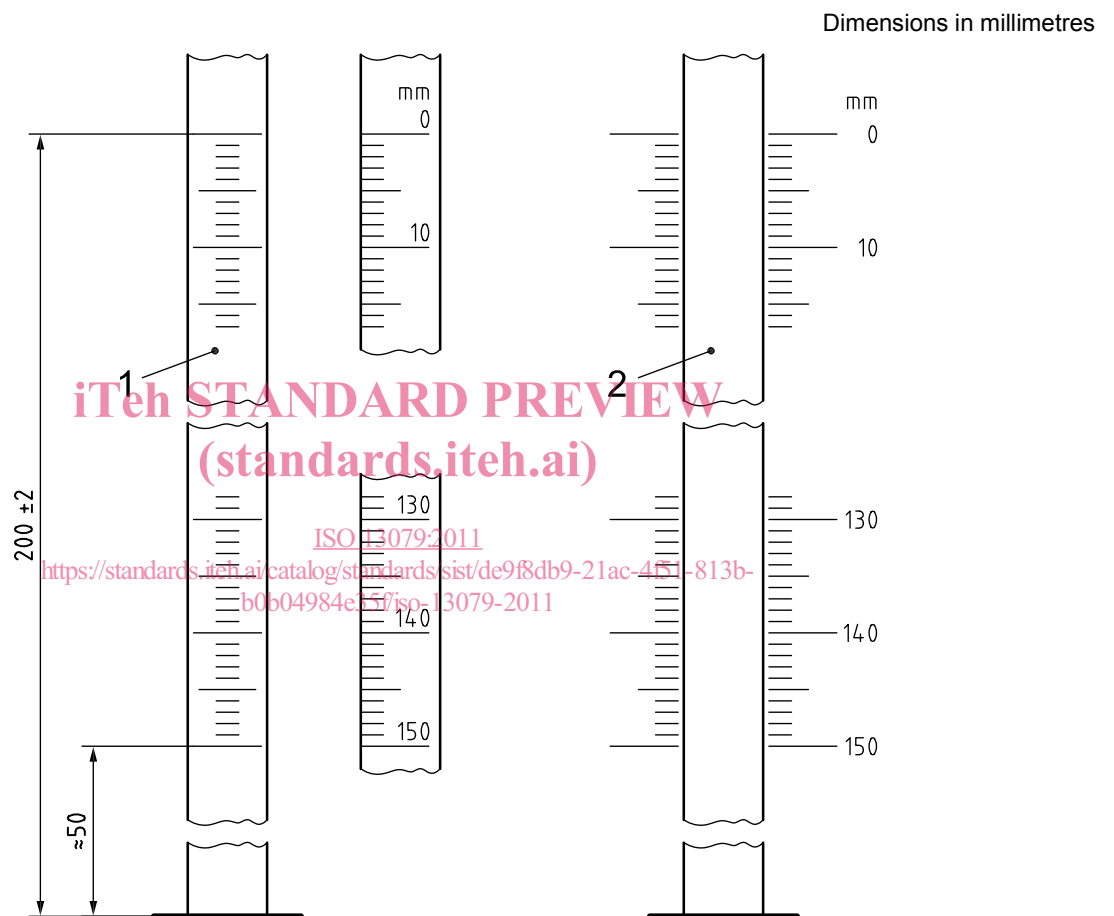

5 Re-usable Westergren tubes

5.1 General design

The general design of a re-usable Westergren tube shall be as shown in Figure 2.

5.2 Straightness

The tube shall be straight when tested in accordance with the method described in Annex C.

5.3 Finish

5.3.1 The upper end of the tube shall be ground smooth and cut square with the axis of the tube, and shall be slightly bevelled, finely ground, polished or hot calendered.

5.3.2 The lower end of the tube shall be tapered as shown in Figure 2; the tapered portion shall be cut square with the axis of the tube and shall be finely ground, polished or hot calendered.

5.3.3 The specified bore of the tube shall be maintained throughout, and shall not be drawn down to form the jet. If jet and upper end of the tube are calendered, they may slightly narrow.

5.4 Dimensions

The tube shall conform to the dimensions given in Table 2.

Table 2 — Dimensions of re-usable Westergren tubes

Dimensions in millimetres

Overall length	300 ± 2
External diameter	6,5 ± 0,5
Internal diameter (bore)	2,55 ± 0,15
Length of measuring part	200 ± 2
Length of tapering portion	6 ± 2
Wall thickness of orifice	at least 0,5

5.5 Graduation and figuring


Graduation and figuring shall be in accordance with Clause 7. All graduation and markings on re-usable Westergren tubes shall be clean and permanent.

5.6 Inscriptions

Inscriptions on the re-usable Westergren tube shall be in accordance with Clause 8. Additionally, the inscription “re-usable Westergren ESR tube” may be inscribed.

5.7 Labelling

Inscriptions on the packaging shall be in accordance with 9.2.

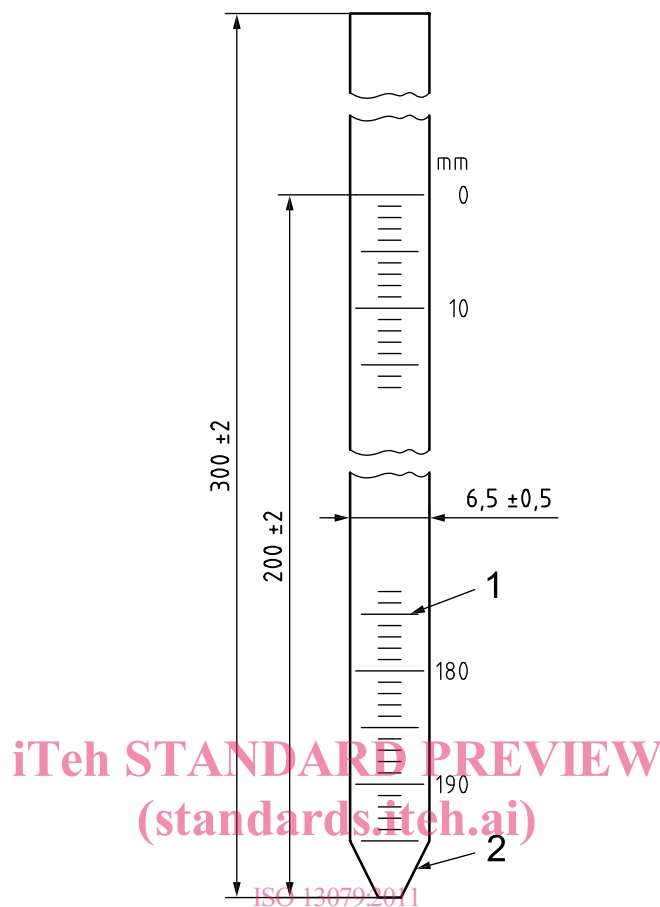**Key**

- 1 scale graduated every millimetre, numbered downwards every centimetre
 2 length of taper 4 mm to 8 mm, wall at orifice minimum 0,5 mm

<https://standards.iteh.ai/catalog/standards/sist/de9f8db9-21ac-4f51-813b-b0b04984e35f/iso-13079-2011>

Figure 2 — Re-usable Westergren tubes

6 Support for Westergren tubes

6.1 Construction

6.1.1 The support shall be a rigid structure having clips or holes to hold rigidly one or several Westergren tubes in vertical position. The support shall stand on at least three feet, at the least two of which shall be adjustable.

NOTE The adjustable feet and an optional plumb-line or spirit-level permit adjustment that the tubes are held in vertical position. Vibration-free positioning of the support enables correct measurements.

6.1.2 When erythrocyte sedimentation rates are to be measured against scales marked on the support, the scales shall be marked on a surface fixed vertically behind the tubes and not more than 10 mm from each tube.

6.1.3 The support may be supplied with an automatic reading of the ESR value.

6.1.4 The support shall be constructed of such materials, and in such a way, that it is able to withstand repeated disinfection in the laboratory.

6.2 Graduation and figuring

6.2.1 Scales, figuring and inscriptions shall be provided on the support, if not marked on the tubes, and shall conform to Clause 7.

NOTE A re-usable tube is intended for use with an appropriate support forming a system. The distribution of markings between tube and support can differ between one system and another.

6.2.2 Markings on the support shall be permanent.

6.2.3 When scales are provided on a support, they shall be fixed behind every tube, within 10 mm of the tube, as shown in Figure 1.

6.3 Inscriptions

Inscriptions shall be permanent and shall conform to Clause 8. The following additional inscriptions shall be marked:

- a) the recommended method for the disinfection of the support after use;
- b) the inscription "Westergren ESR – ISO 13079".

Alternatively, this information may be given in an accompanying product manual or product data sheet.

7 Graduation and figuring

iTeh STANDARD PREVIEW
(standards.iteh.ai)

7.1 Graduation

7.1.1 Graduation lines <https://standards.iteh.ai/catalog/standards/sist/de9f8db9-21ac-4f51-813b-b0b04984e35f/iso-13079-2011>
ISO 13079:2011

Graduation lines shall be clean and of uniform thickness not greater than 0,4 mm.

Graduation lines shall lie in planes at right angles to the axis of each tube, and shall be without irregularity in their spacing.

7.1.2 Scale

A scale, graduated in millimetres, shall run downwards for at least 150 mm from a zero mark situated 200 mm above the lower end of each tube.

There shall be a distance of 1 mm between the centres of adjacent graduation lines.

The lengths of the graduation lines shall be varied so as to distinguish clearly every tenth line and every intermediate fifth line as follows.

- a) The length of the short lines shall be not less than 10 % and not more than 20 % of the circumference of the tube.
- b) The length of the medium lines shall be approximately 1,5 times the length of the short lines. They shall either extend symmetrically at each end beyond the ends of the short lines or they shall be right-aligned or left-aligned to the short lines.
- c) The length of the long lines shall be approximately twice the length of the short lines. They shall either extend symmetrically at each end beyond the ends of the short and medium lines or they shall be right-aligned or left-aligned to the short and medium lines.

7.2 Figuring of graduation lines

Every tenth (long) graduation line shall be figured.

Figures shall be at least 2 mm high and shall be placed immediately above or next to the long lines.

8 Marking

8.1 The following inscription shall be marked on the tube or on the support, or both:

— the symbol “mm” above “0” on the scale.

8.2 The following inscriptions shall be labelled on the packaging and in the user information and can optionally be marked on the tube or on the support, or both:

- a) the temperature “(20 ± 3) °C” or “(27 ± 2) °C”¹⁾;
- b) the maker's and/or vendor's mark or name;
- c) the number and date of this International Standard.

The inscriptions shall be positioned so that they are visible to the operator when the tube is put in the support for which it is intended.

iTeh STANDARD PREVIEW
(standards.iteh.ai)

9 Labelling

9.1 Single-use Westergren tubes ISO 13079:2011

<https://standards.iteh.ai/catalog/standards/sist/de9f8db9-21ac-4f51-813b->

Each package of single-use Westergren tubes shall be clearly labelled with at least the following information:

- a) the words “Single-use Westergren ESR tubes”;
- b) the words “Ready for use”;
- c) the temperature “(20 ± 3) °C” or “(27 ± 2) °C”;
- d) the maker's and/or vendor's name or mark;
- e) an identifying reference to the batch of manufacture;
- f) the number of this International Standard.

Symbols in accordance with ISO 15223-1 may be used.

9.2 Re-usable Westergren tubes

Each package of re-usable Westergren tubes shall provide the following information:

- a) the words “Re-usable Westergren ESR tubes”;
- b) the maker's and/or vendor's name or mark;

1) Some countries in tropical regions have adopted a standard reference temperature of 27 °C instead of 20 °C.