

---

---

**Water quality — Measurement of  
polonium 210 activity concentration in  
water by alpha spectrometry**

*Qualité de l'eau — Mesurage de l'activité du polonium 210 dans l'eau  
par spectrométrie alpha*

**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

ISO 13161:2011

<https://standards.iteh.ai/catalog/standards/sist/af59a693-29bd-4c0e-8476-6398d92c2b98/iso-13161-2011>



## iTeh STANDARD PREVIEW (standards.iteh.ai)

ISO 13161:2011

<https://standards.iteh.ai/catalog/standards/sist/af59a693-29bd-4c0e-8476-6398d92c2b98/iso-13161-2011>



### **COPYRIGHT PROTECTED DOCUMENT**

© ISO 2011

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Case postale 56 • CH-1211 Geneva 20  
Tel. + 41 22 749 01 11  
Fax + 41 22 749 09 47  
E-mail [copyright@iso.org](mailto:copyright@iso.org)  
Web [www.iso.org](http://www.iso.org)

Published in Switzerland

# Contents

Page

Foreword .....	iv
Introduction .....	v
1 Scope .....	1
2 Normative references .....	1
3 Terms, definitions, symbols and units .....	1
3.1 Terms and definitions .....	2
3.2 Symbols, definitions and units .....	2
4 Principle .....	2
4.1 General .....	2
4.2 Treatment .....	3
4.3 Principle of alpha spectrometry .....	3
5 Reagents and equipment .....	3
5.1 Reagents .....	3
5.2 Preparation material and treatment .....	4
5.3 Alpha spectrometry measuring equipment .....	4
6 Sampling and samples .....	4
7 Chemical treatment and deposit process .....	4
7.1 General .....	4
7.2 Chemical treatment .....	5
7.3 Disc cleaning .....	5
7.4 Deposition phase .....	5
8 Measurement by alpha spectrometry .....	6
8.1 General .....	6
8.2 Quality control .....	6
8.3 Measurement .....	6
9 Expression of results .....	6
9.1 General .....	6
9.2 Total yield .....	7
9.3 Activity concentration of $^{210}\text{Po}$ in the sample .....	7
9.4 Combined uncertainties .....	8
9.5 Decision threshold .....	8
9.6 Detection limit .....	8
9.7 Confidence limits .....	9
10 Test report .....	9
Annex A (informative) Cell deposit examples .....	11
Annex B (informative) Spectrum examples .....	13
Bibliography .....	15

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 13161 was prepared by Technical Committee ISO/TC 147, *Water quality*, Subcommittee SC 3, *Radiological methods*.

## iTeh STANDARD PREVIEW (standards.iteh.ai)

ISO 13161:2011

<https://standards.iteh.ai/catalog/standards/sist/af59a693-29bd-4c0e-8476-6398d92c2b98/iso-13161-2011>

## Introduction

There are different techniques to measure  $^{210}\text{Po}$  activity concentration in water: alpha spectrometry, liquid scintillation counting, alpha proportional counting.


This International Standard describes a method for measuring  $^{210}\text{Po}$  activity concentration in natural waters by alpha spectrometry.

Polonium 210 ( $^{210}\text{Po}$ ) is a natural alpha-emitting radionuclide with a half-life of 138 d. It appears in the natural chain of uranium 238 ( $^{238}\text{U}$ ) (see Figure 1). It is a long-life decay product of radon 222 ( $^{222}\text{Rn}$ ) through lead 210 ( $^{210}\text{Pb}$ ) (see References [5] to [9]).

Precautions are required when manipulating radioactive materials such as polonium isotopes.

The activity concentration ranges of  $^{210}\text{Po}$ , in drinking waters for example, are generally very low, usually ranging from  $1 \text{ mBq l}^{-1}$  to  $30 \text{ mBq l}^{-1}$ .

This International Standard is applicable to all types of water, including sea water, and usually allows the measurement of  $^{210}\text{Po}$  activity concentrations greater or equal to  $5 \text{ mBq l}^{-1}$ .

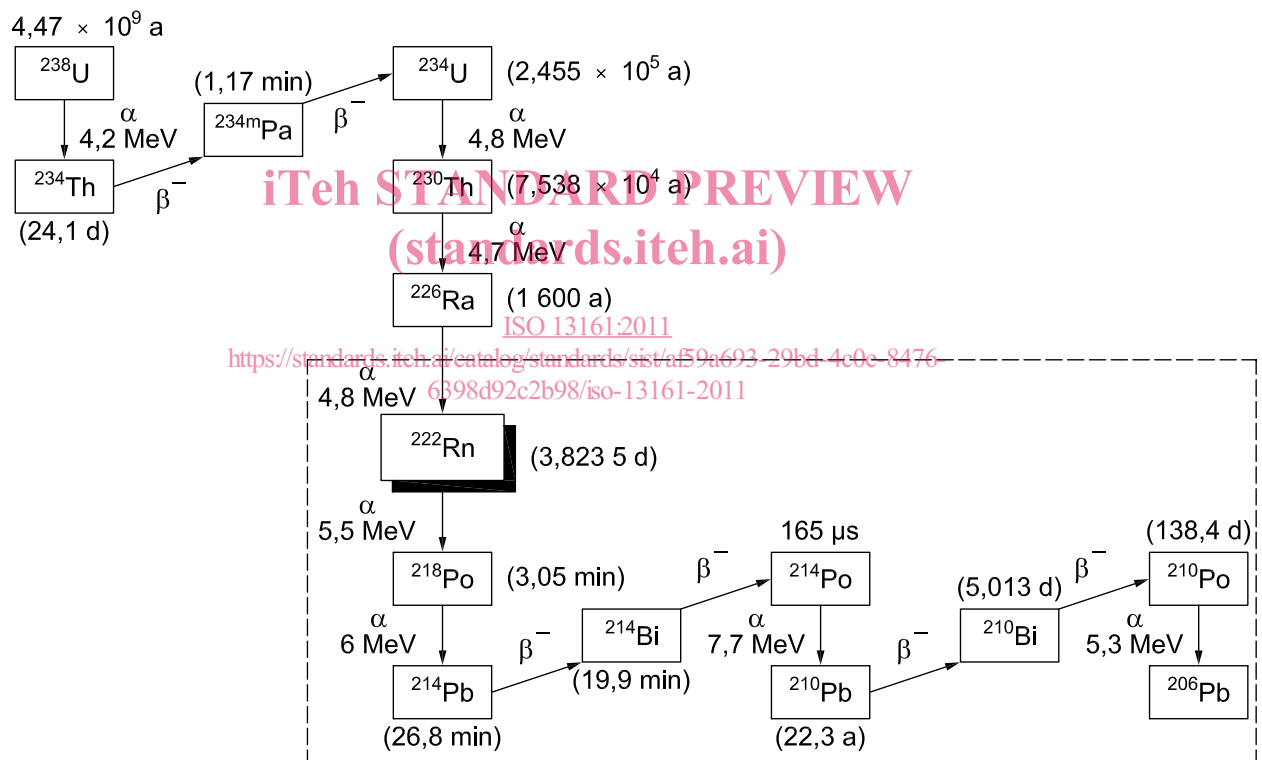

NOTE  $^{206}\text{Pb}$  is stable.

Figure 1 — Uranium 238 and its decay products

**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

ISO 13161:2011

<https://standards.iteh.ai/catalog/standards/sist/af59a693-29bd-4c0e-8476-6398d92c2b98/iso-13161-2011>

# Water quality — Measurement of polonium 210 activity concentration in water by alpha spectrometry

**WARNING** — Persons using this International Standard should be familiar with normal laboratory practice. This International Standard does not purport to address all of the safety problems, if any, associated with its use. It is the responsibility of the user to establish appropriate safety and health practices and to ensure compliance with any national regulatory conditions.

**IMPORTANT** — It is absolutely essential that tests conducted according to this International Standard be carried out by suitably trained staff.

## 1 Scope

This International Standard specifies the measurement of  $^{210}\text{Po}$  activity concentration by alpha spectrometry in all kinds of natural waters.

The detection limit of this method depends on the volume of the sample, the counting time, the background count rate and the detection efficiency. In the case of drinking water, the analysis is usually carried out on the raw sample, without filtration or other pretreatment.

If suspended material has to be removed or analysed, filtration at 0.45  $\mu\text{m}$  is recommended. The analysis of the insoluble fraction requires a mineralization step that is not covered by this International Standard (see NF M 60-790-4<sup>[4]</sup>). In this case, the measurement is made on the different phases obtained. The final activity is the sum of all the measured activity concentrations.

## 2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 3696, *Water for analytical laboratory use — Specification and test methods*

ISO 5667-1, *Water quality — Sampling — Part 1: Guidance on the design of sampling programmes and sampling techniques*

ISO 5667-3, *Water quality — Sampling — Part 3: Preservation and handling of water samples*

ISO 11929, *Determination of the characteristic limits (decision threshold, detection limit and limits of the confidence interval) for measurements of ionizing radiation — Fundamentals and application*

ISO 80000-10, *Quantities and units — Part 10: Atomic and nuclear physics*

ISO/IEC 17025, *General requirements for the competence of testing and calibration laboratories*

ISO/IEC Guide 98-3, *Uncertainty of measurement — Part 3: Guide to the expression of uncertainty in measurement (GUM:1995)*

## 3 Terms, definitions, symbols and units

For the purposes of this document, the terms, definitions, symbols and abbreviations given in ISO 80000-10 and the following apply.

3.1 Terms and definitions

3.1.1

**certified reference solution**

solution of known concentration traceable to primary or secondary certified reference solution standards of radioactivity

3.1.2

**tracer solution**

usually a secondary standard or reference material, such as <sup>208</sup>Po or <sup>209</sup>Po, employed to determine the chemical yield of the analysis

3.1.3

**quality control standard**

radioactive source used to demonstrate that the measurement equipment employed performs within defined limits

NOTE Quality control is usually carried out by the regular measurement of a suitable radioactive source in accordance with ISO 7870-1<sup>[1]</sup>, ISO 7870-2<sup>[2]</sup>, and ISO 7871<sup>[3]</sup>.

3.2 Symbols, definitions and units

$A$	activity of the tracer added	Bq
$c_A$	activity concentration of <sup>210</sup> Po	Bq l <sup>-1</sup>
$c_A^*$	decision threshold	Bq l <sup>-1</sup>
$c_A^\#$	detection limit	Bq l <sup>-1</sup>
$c_A^\triangleleft, c_A^\triangleright$	lower and upper limits of the confidence interval	Bq l <sup>-1</sup>
$R_C$	chemical yield	1
$R_T$	total yield	1
$r_0$	background count rate in the <sup>210</sup> Po region of interest	s <sup>-1</sup>
$r_{0T}$	background count rate in the tracer region of interest	s <sup>-1</sup>
$r_g$	gross count rate of the sample in the <sup>210</sup> Po region of interest	s <sup>-1</sup>
$r_T$	gross count rate in the tracer region of interest	s <sup>-1</sup>
$t_0$	background counting time	s
$t_g$	sample counting time	s
$U$	expanded uncertainty calculated by $U = k \cdot u(c_A)$ with $k = 1, 2 \dots$	Bq l <sup>-1</sup>
$u(c_A)$	standard uncertainty associated with the initial measurement result	Bq l <sup>-1</sup>
$V$	volume of the test sample aliquot	l
$\varepsilon$	counting efficiency	1

iTeH STANDARD PREVIEW  
(standards.iteh.ai)

<https://standards.iteh.ai/catalog/standards/sist/af59a693-29bd-4c0e-8476-6398d92c2b98/iso-13161-2011>

4 Principle

4.1 General

After sampling, the test sample undergoes a treatment which leads to an extremely thin deposit of the polonium on a metal disc, for measurement by alpha spectrometry.



$^{210}\text{Po}$  has a half-life of  $138,376 \text{ d} \pm 0,002 \text{ d}$  (see Reference [11]).

The sample shall be analysed as soon as possible to give an activity concentration on the sampling date. If the time elapsed between sampling and measurement is long, the activity concentration measured requires correction and it is then necessary to know the  $^{210}\text{Pb}$  and  $^{210}\text{Bi}$  activity concentrations of the sample to adjust the  $^{210}\text{Po}$  activity concentration on the sampling date.

## 4.2 Treatment

The main steps of the sample treatment are:

- filtration if necessary;
- acidification with concentrated hydrochloric acid or nitric acid and addition of a polonium tracer ( $^{208}\text{Po}$  or  $^{209}\text{Po}$ ) solution;

NOTE The polonium isotopes  $^{208}\text{Po}$  (5,11 MeV alpha emission) or  $^{209}\text{Po}$  (4,88 MeV alpha emission) can be used as tracers since interference with  $^{210}\text{Po}$  (5,31 MeV alpha emission) is minimal for sources displaying good resolution (<50 keV FWHM);  $^{209}\text{Po}$  is preferred, but  $^{208}\text{Po}$  is acceptable.

- addition of a reducing agent (e.g. ascorbic acid);
- spontaneous deposition of a thin layer on to a metal disc.

The activity concentration measurement as well as the determination of the total yield is carried out by alpha spectrometry.

**iTeh STANDARD PREVIEW**  
(standards.iteh.ai)

## 4.3 Principle of alpha spectrometry

The thin layer deposited on the metal disc allows the detection of alpha particles. The interaction of alpha particles and detector results in a change in (bias) current that is proportional to the energy of the particles.

The electronic pulses generated by the detector are amplified, and displayed as an energy spectrum using an analogue-digital converter, multiple channel analyser, and computer processing. The spectrum display enables the radionuclides present in the source to be identified and integration of counts enables the determination of activity concentration of the test sample, taking into account the background counting rates and/or the blank test and the total yield.

A blank test should be carried out with the same reagents replacing the water sample by water complying with ISO 3696, grade 3 previously used for the preparation of the reagents without tracer.

To ensure the acceptable performance of the detector system, a quality control standard shall be measured.

The chemical yield of  $^{210}\text{Po}$  measurement is determined by adding a radioactive tracer. The total yield is a product of the chemical yield and the detection efficiency.

## 5 Reagents and equipment

### 5.1 Reagents

During chemical treatment and cleaning of the metal disc, use only reagents of recognized analytical grade. Use only reagents with no measurable  $^{210}\text{Po}$  concentration.

**5.1.1 Water**, complying with ISO 3696, grade 3.

**5.1.2 Tracer solution.**

$^{208}\text{Po}$  ( $T_{1/2} = 1\,058,5 \text{ d} \pm 0,7 \text{ d}$ ) or  $^{209}\text{Po}$  ( $T_{1/2} = 37\,300 \text{ d} \pm 1\,800 \text{ d}$ ) tracer solution of known activity; the spike is adjusted to the  $^{210}\text{Po}$  activity concentration expected in the test sample (References [12][13]).

When  $^{208}\text{Po}$  is used, its decay shall be taken into account in accordance with the information given on the calibration certificate.

NOTE The half-life of  $^{209}\text{Po}$  and its associated uncertainty commonly used was subjected to a recent investigation that suggests an uncertainty of  $\pm 25\%$  instead of  $4,8\%$  (Reference [14]).

**5.1.3 Concentrated hydrochloric acid**, 37 % mass fraction, or **concentrated nitric acid**.

**5.1.4 Dilute hydrochloric acid** or **dilute nitric acid**, to adjust the pH at the beginning of the treatment.

**5.1.5 Ascorbic acid** or **hydroxylamine hydrochloride**.

**5.1.6 Ethanol**.

## 5.2 Preparation material and treatment

The preparation material should be appropriate for the operating method used (Clause 7).

**5.2.1 Standard laboratory equipment**, including filtration material, hot plate, pH meter or pH paper.

**5.2.2 Analytical precision scale**.

**5.2.3 Stirrer**.

**5.2.4 Equipment for the preparation of the thin layer deposit**.

**5.2.5 Metal disc**, of a metal that allows reductive deposition of polonium (e.g. stainless steel [304L type], silver, nickel or another metal displaying this property).

## 5.3 Alpha spectrometry measuring equipment

The alpha spectrometry counting can be carried out using either gridded ionization chambers or thin semiconductor detectors.

A spectrum display is essential.

## 6 Sampling and samples

It is important that the laboratory receives the test sample as soon as possible.

Carry out sampling, handling, and storage as specified in ISO 5667-1 and ISO 5667-3.

## 7 Chemical treatment and deposit process

### 7.1 General

The volume of the test sample is variable; the usual quantity is between 150 ml and 2 000 ml.

Where necessary, the test sample can be filtered on a filter of  $0,45\ \mu\text{m}$  porosity (the use of a single-use filtering device is recommended).

Acidify the filtrate, preferably with dilute hydrochloric acid (5.1.4), to ensure that the pH of the test sample is below 1,5.

All reasonable precautions should be taken during handling and storage of the test sample to avoid contamination or degradation.

The verification that any contamination of reagents and residual contamination in the analytical equipment are below the detection limit for the analysis shall be carried out and documented (blank analysis).

The analysis shall be carried out under a fume-extracting hood.

NOTE If large test samples are used, or if a special study is being carried out, it is possible that a preliminary concentration prior to the first step of chemical treatment is necessary, e.g. co-precipitation of  $\text{Fe}(\text{OH})_3$  adding  $\text{Fe}^{3+}$  can be used. If this co-precipitation is used, the volume of analysed sample can be large and the detection limit decreases in the same proportion.

## 7.2 Chemical treatment

Take an aliquot of volume  $V$  from the test sample, e.g. 500 ml.

Adjust the pH with concentrated hydrochloric acid or concentrated nitric acid (5.1.3) in order to reduce the pH below 1,5. Add a known quantity of tracer solution (5.1.2) in order to enable the determination of the chemical yield without introducing large measurement uncertainties and avoiding contamination of the laboratory equipment. Ideally the  $^{210}\text{Po}$  and the tracer peaks should be of the same magnitude (an ideal aim is the acquisition of between 400 counts and 10 000 counts in the tracer peak).

At this stage, a concentration step [dry evaporation and addition of dilute hydrochloric acid (5.1.4)] can be carried out by slow evaporation at a temperature lower than 80 °C (to avoid losses of Po) to dryness and then add, for example, 20 ml of 6 mol/l HCl.

Adjust the volume of the solution to approximately 100 ml with water (5.1.1).

A final HCl concentration between 0,1 mol/l and 3 mol/l and consistent use of the same concentration in order to maintain the repeatability level are recommended. The final volume can vary from 50 ml to 100 ml.

## 7.3 Disc cleaning

The disc shall be thoroughly cleaned in order to remove deposits of organic impurities, e.g. using ethanol; it may also be necessary to remove surface oxide deposits with dilute hydrochloric acid.

NOTE In the case of unprotected silver discs, the oxide and sulfur deposits present on the surface can be eliminated by polishing or by washing with dilute ammonia solution.

Rinse the disc with water.

## 7.4 Deposition phase

Transfer the solution to the deposition equipment (Annex A) and add an excess of the reducing agent, e.g. 0,1 g of ascorbic acid or hydroxylamine hydrochloride (5.1.5).

During the deposition phase, the metal disc catalyses the reduction of the polonium from  $\text{Po}^{4+}$  or  $\text{Po}^{2+}$  to metallic polonium. The addition of a reducing agent in the solution prevents the reoxidation (and therefore redissolution) of the deposited polonium on the disc by any oxidants that may be present in the solution, e.g.  $\text{Fe}^{3+}$ .

Stir the solution continuously using an automatic stirrer during the entire deposition phase.

The reduction kinetics of  $\text{Po}^{4+}$  or  $\text{Po}^{2+}$  to metallic polonium are slow at room temperature. The deposition rate can be accelerated by heating the solution to a maximum of 90 °C, making sure that the solution is in permanent contact with the metal disc, without excessive bubbling. Therefore, it is advisable to limit evaporation losses by keeping the acidity of the solution low. This phase shall be long enough to allow a good deposition yield and in normal circumstances is complete within 3 h.

Add ascorbic acid carefully as it can interfere with the spectral resolution. The quantity needed depends on the amount of Fe present in the sample, especially when an  $\text{Fe}(\text{OH})_3$  co-precipitation has been used.

On completion, polonium is deposited as a thin source on the disc. Rinse the disc with water (5.1.1) and wait until it is dry before measuring it by alpha spectrometry.