



SLOVENSKI STANDARD

SIST ISO 13161:2013

01-januar-2013

Kakovost vode - Merjenje koncentracije aktivnosti polonija Po-210 v vodi z alfa spektrometrijo

Water quality - Measurement of polonium 210 activity concentration in water by alpha spectrometry

iTeh STANDARD PREVIEW

Qualité de l'eau - Mesurage de l'activité du polonium 210 dans l'eau par spectrométrie alpha

[SIST ISO 13161:2013](https://standards.itih.ai/catalog/standards/sist/30a1fcb6-094c-459e-bd0c-0d1fc300d54ac/sist-iso-13161-2013)

Ta slovenski standard je istoveten z: **ISO 13161:2011**

ICS:

| | | |
|-----------|-------------------------------------|---|
| 13.060.60 | Preiskava fizikalnih lastnosti vode | Examination of physical properties of water |
| 17.240 | Merjenje sevanja | Radiation measurements |

SIST ISO 13161:2013

en,fr

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[SIST ISO 13161:2013](#)

<https://standards.iteh.ai/catalog/standards/sist/30a1fcb6-094c-459e-bd0c-6d1e300d54ac/sist-iso-13161-2013>

**Water quality — Measurement of
polonium 210 activity concentration in
water by alpha spectrometry**

*Qualité de l'eau — Mesurage de l'activité du polonium 210 dans l'eau
par spectrométrie alpha*

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[SIST ISO 13161:2013](https://standards.iteh.ai/catalog/standards/sist/30a1fcb6-094c-459e-bd0c-6d1e300d54ac/sist-iso-13161-2013)

<https://standards.iteh.ai/catalog/standards/sist/30a1fcb6-094c-459e-bd0c-6d1e300d54ac/sist-iso-13161-2013>



iTeh STANDARD PREVIEW (standards.iteh.ai)

SIST ISO 13161:2013

<https://standards.iteh.ai/catalog/standards/sist/30a1fcb6-094c-459e-bd0c-6d1e300d54ac/sist-iso-13161-2013>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2011

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

| Contents | Page |
|---|-------------|
| Foreword | iv |
| Introduction | v |
| 1 Scope | 1 |
| 2 Normative references | 1 |
| 3 Terms, definitions, symbols and units | 1 |
| 3.1 Terms and definitions | 2 |
| 3.2 Symbols, definitions and units | 2 |
| 4 Principle | 2 |
| 4.1 General | 2 |
| 4.2 Treatment | 3 |
| 4.3 Principle of alpha spectrometry | 3 |
| 5 Reagents and equipment | 3 |
| 5.1 Reagents | 3 |
| 5.2 Preparation material and treatment | 4 |
| 5.3 Alpha spectrometry measuring equipment | 4 |
| 6 Sampling and samples | 4 |
| 7 Chemical treatment and deposit process | 4 |
| 7.1 General | 4 |
| 7.2 Chemical treatment | 5 |
| 7.3 Disc cleaning | 5 |
| 7.4 Deposition phase | 5 |
| 8 Measurement by alpha spectrometry | 6 |
| 8.1 General | 6 |
| 8.2 Quality control | 6 |
| 8.3 Measurement | 6 |
| 9 Expression of results | 6 |
| 9.1 General | 6 |
| 9.2 Total yield | 7 |
| 9.3 Activity concentration of ²¹⁰Po in the sample | 7 |
| 9.4 Combined uncertainties | 8 |
| 9.5 Decision threshold | 8 |
| 9.6 Detection limit | 8 |
| 9.7 Confidence limits | 9 |
| 10 Test report | 9 |
| Annex A (informative) Cell deposit examples | 11 |
| Annex B (informative) Spectrum examples | 13 |
| Bibliography | 15 |

ISO 13161:2011(E)

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 13161 was prepared by Technical Committee ISO/TC 147, *Water quality*, Subcommittee SC 3, *Radiological methods*.

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[SIST ISO 13161:2013](https://standards.iteh.ai/catalog/standards/sist/30a1fcb6-094c-459e-bd0c-6d1e300d54ac/sist-iso-13161-2013)

<https://standards.iteh.ai/catalog/standards/sist/30a1fcb6-094c-459e-bd0c-6d1e300d54ac/sist-iso-13161-2013>

Introduction

There are different techniques to measure ^{210}Po activity concentration in water: alpha spectrometry, liquid scintillation counting, alpha proportional counting.

This International Standard describes a method for measuring ^{210}Po activity concentration in natural waters by alpha spectrometry.

Polonium 210 (^{210}Po) is a natural alpha-emitting radionuclide with a half-life of 138 d. It appears in the natural chain of uranium 238 (^{238}U) (see Figure 1). It is a long-life decay product of radon 222 (^{222}Rn) through lead 210 (^{210}Pb) (see References [5] to [9]).

Precautions are required when manipulating radioactive materials such as polonium isotopes.

The activity concentration ranges of ^{210}Po , in drinking waters for example, are generally very low, usually ranging from 1 mBq l^{-1} to 30 mBq l^{-1} .

This International Standard is applicable to all types of water, including sea water, and usually allows the measurement of ^{210}Po activity concentrations greater or equal to 5 mBq l^{-1} .

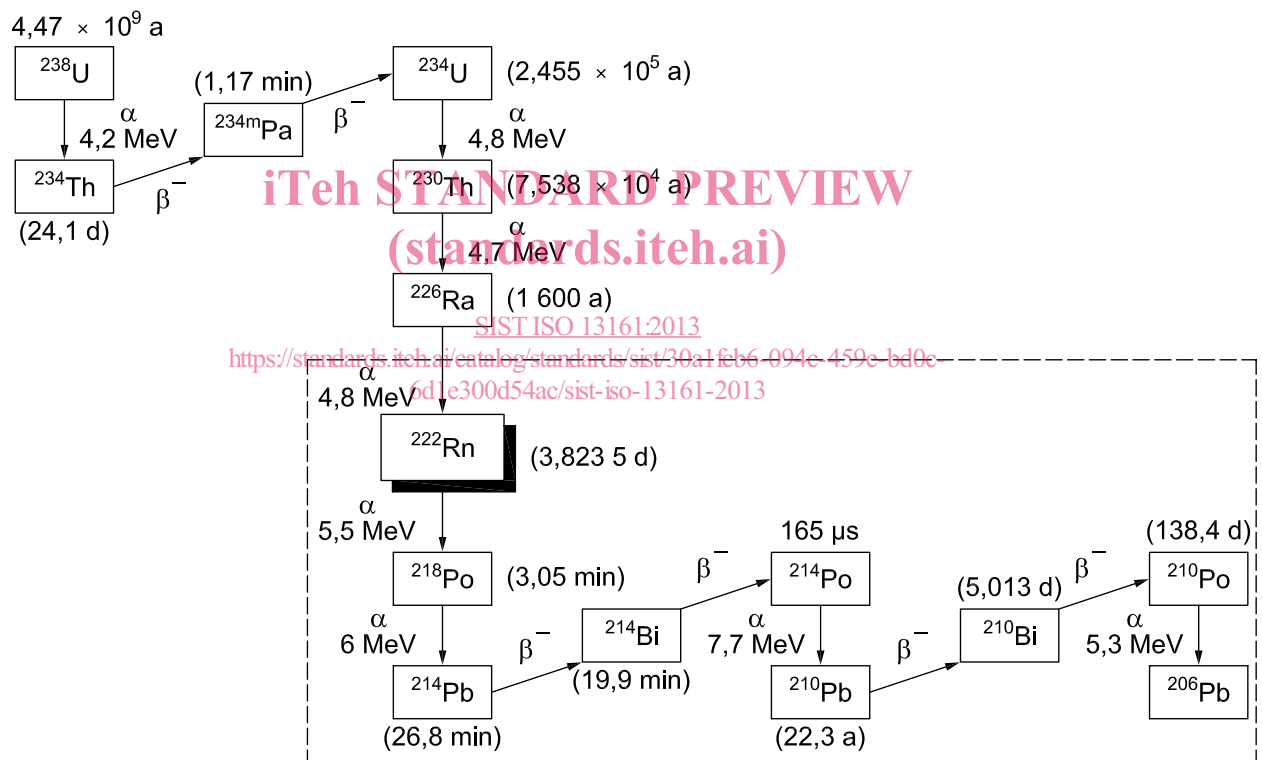


Figure 1 — Uranium 238 and its decay products

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[SIST ISO 13161:2013](#)

<https://standards.iteh.ai/catalog/standards/sist/30a1fcb6-094c-459e-bd0c-6d1e300d54ac/sist-iso-13161-2013>

Water quality — Measurement of polonium 210 activity concentration in water by alpha spectrometry

WARNING — Persons using this International Standard should be familiar with normal laboratory practice. This International Standard does not purport to address all of the safety problems, if any, associated with its use. It is the responsibility of the user to establish appropriate safety and health practices and to ensure compliance with any national regulatory conditions.

IMPORTANT — It is absolutely essential that tests conducted according to this International Standard be carried out by suitably trained staff.

1 Scope

This International Standard specifies the measurement of ^{210}Po activity concentration by alpha spectrometry in all kinds of natural waters.

The detection limit of this method depends on the volume of the sample, the counting time, the background count rate and the detection efficiency. In the case of drinking water, the analysis is usually carried out on the raw sample, without filtration or other pretreatment.

If suspended material has to be removed or analysed, filtration at 0.45 μm is recommended. The analysis of the insoluble fraction requires a mineralization step that is not covered by this International Standard (see NF M 60-790-4^[4]). In this case, the measurement is made on the different phases obtained. The final activity is the sum of all the measured activity concentrations.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 3696, *Water for analytical laboratory use — Specification and test methods*

ISO 5667-1, *Water quality — Sampling — Part 1: Guidance on the design of sampling programmes and sampling techniques*

ISO 5667-3, *Water quality — Sampling — Part 3: Preservation and handling of water samples*

ISO 11929, *Determination of the characteristic limits (decision threshold, detection limit and limits of the confidence interval) for measurements of ionizing radiation — Fundamentals and application*

ISO 80000-10, *Quantities and units — Part 10: Atomic and nuclear physics*

ISO/IEC 17025, *General requirements for the competence of testing and calibration laboratories*

ISO/IEC Guide 98-3, *Uncertainty of measurement — Part 3: Guide to the expression of uncertainty in measurement (GUM:1995)*

3 Terms, definitions, symbols and units

For the purposes of this document, the terms, definitions, symbols and abbreviations given in ISO 80000-10 and the following apply.

ISO 13161:2011(E)

3.1 Terms and definitions

3.1.1

certified reference solution

solution of known concentration traceable to primary or secondary certified reference solution standards of radioactivity

3.1.2

tracer solution

usually a secondary standard or reference material, such as ^{208}Po or ^{209}Po , employed to determine the chemical yield of the analysis

3.1.3

quality control standard

radioactive source used to demonstrate that the measurement equipment employed performs within defined limits

NOTE Quality control is usually carried out by the regular measurement of a suitable radioactive source in accordance with ISO 7870-1^[1], ISO 7870-2^[2], and ISO 7871^[3].

3.2 Symbols, definitions and units

| | | |
|----------------|---|--------------------|
| A | activity of the tracer added | Bq |
| c_A | activity concentration of ^{210}Po | Bq l ⁻¹ |
| c_A^* | decision threshold | Bq l ⁻¹ |
| $c_A^\#$ | detection limit | Bq l ⁻¹ |
| $c_A^<, c_A^>$ | lower and upper limits of the confidence interval | Bq l ⁻¹ |
| R_C | chemical yield | 1 |
| R_T | total yield | 1 |
| r_0 | background count rate in the ^{210}Po region of interest | s ⁻¹ |
| r_{0T} | background count rate in the tracer region of interest | s ⁻¹ |
| r_g | gross count rate of the sample in the ^{210}Po region of interest | s ⁻¹ |
| r_T | gross count rate in the tracer region of interest | s ⁻¹ |
| t_0 | background counting time | s |
| t_g | sample counting time | s |
| U | expanded uncertainty calculated by $U = k \cdot u(c_A)$ with $k = 1, 2 \dots$ | Bq l ⁻¹ |
| $u(c_A)$ | standard uncertainty associated with the initial measurement result | Bq l ⁻¹ |
| V | volume of the test sample aliquot | l |
| ε | counting efficiency | 1 |

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[SIST ISO 13161:2013](https://standards.iteh.ai/catalog/standards/sist/30a1fcb6-094c-459e-bd0c-6d1e300d54ac/sist-iso-13161-2013)

<https://standards.iteh.ai/catalog/standards/sist/30a1fcb6-094c-459e-bd0c-6d1e300d54ac/sist-iso-13161-2013>

4 Principle

4.1 General

After sampling, the test sample undergoes a treatment which leads to an extremely thin deposit of the polonium on a metal disc, for measurement by alpha spectrometry.

^{210}Po has a half-life of $138,376 \text{ d} \pm 0,002 \text{ d}$ (see Reference [11]).

The sample shall be analysed as soon as possible to give an activity concentration on the sampling date. If the time elapsed between sampling and measurement is long, the activity concentration measured requires correction and it is then necessary to know the ^{210}Pb and ^{210}Bi activity concentrations of the sample to adjust the ^{210}Po activity concentration on the sampling date.

4.2 Treatment

The main steps of the sample treatment are:

- filtration if necessary;
- acidification with concentrated hydrochloric acid or nitric acid and addition of a polonium tracer (^{208}Po or ^{209}Po) solution;

NOTE The polonium isotopes ^{208}Po (5,11 MeV alpha emission) or ^{209}Po (4,88 MeV alpha emission) can be used as tracers since interference with ^{210}Po (5,31 MeV alpha emission) is minimal for sources displaying good resolution (<50 keV FWHM); ^{209}Po is preferred, but ^{208}Po is acceptable.

- addition of a reducing agent (e.g. ascorbic acid);
- spontaneous deposition of a thin layer on to a metal disc.

The activity concentration measurement as well as the determination of the total yield is carried out by alpha spectrometry.

iTeh STANDARD PREVIEW

4.3 Principle of alpha spectrometry

The thin layer deposited on the metal disc allows the detection of alpha particles. The interaction of alpha particles and detector results in a change in (bias) current that is proportional to the energy of the particles.

The electronic pulses generated by the detector are amplified and displayed as an energy spectrum using an analogue-digital converter, multiple channel analyser, and computer processing. The spectrum display enables the radionuclides present in the source to be identified and integration of counts enables the determination of activity concentration of the test sample, taking into account the background counting rates and/or the blank test and the total yield.

A blank test should be carried out with the same reagents replacing the water sample by water complying with ISO 3696, grade 3 previously used for the preparation of the reagents without tracer.

To ensure the acceptable performance of the detector system, a quality control standard shall be measured.

The chemical yield of ^{210}Po measurement is determined by adding a radioactive tracer. The total yield is a product of the chemical yield and the detection efficiency.

5 Reagents and equipment

5.1 Reagents

During chemical treatment and cleaning of the metal disc, use only reagents of recognized analytical grade. Use only reagents with no measurable ^{210}Po concentration.

5.1.1 Water, complying with ISO 3696, grade 3.

5.1.2 Tracer solution.

^{208}Po ($T_{1/2} = 1\,058,5 \text{ d} \pm 0,7 \text{ d}$) or ^{209}Po ($T_{1/2} = 37\,300 \text{ d} \pm 1\,800 \text{ d}$) tracer solution of known activity; the spike is adjusted to the ^{210}Po activity concentration expected in the test sample (References [12][13]).