

SLOVENSKI STANDARD

SIST ISO 13271:2013

01-april-2013

Emisije nepremičnih virov - Določevanje masne koncentracije PM10/PM2,5 v odpadnih plinih - Meritve pri večjih koncentracijah z uporabo impaktorjev

Stationary source emissions - Determination of PM10/PM2,5 mass concentration in flue gas - Measurement at higher concentrations by use of virtual impactors

iTeh STANDARD PREVIEW

Émissions de sources fixes - Détermination de la concentration en masse de PM10/PM2,5 dans les effluents gazeux - Mesurage à des hautes concentrations à l'aide des impacteurs virtuels

[SIST ISO 13271:2013](#)

<https://standards.iteh.ai/catalog/standards/sist/dfbe9038-2fd5-4281-bea4-71a59800118/sist-iso-13271-2013>

Ta slovenski standard je istoveten z: [**ISO 13271:2012**](#)

ICS:

13.040.40 Emisije nepremičnih virov Stationary source emissions

SIST ISO 13271:2013

en,fr

iTeh STANDARD PREVIEW (standards.iteh.ai)

[SIST ISO 13271:2013](#)

<https://standards.iteh.ai/catalog/standards/sist/dfbe9038-2fd5-4281-bea4-71a59800118/sist-iso-13271-2013>

INTERNATIONAL STANDARD

ISO
13271

First edition
2012-06-15

Stationary source emissions — Determination of PM₁₀/PM_{2,5} mass concentration in flue gas — Measurement at higher concentrations by use of virtual impactors

Émissions de sources fixes — Détermination de la concentration en
masse de PM₁₀/PM_{2,5} dans les effluents gazeux — Mesurage à des
hautes concentrations à l'aide des impacteurs virtuels
iTeh STANDARD REVIEW
(standards.iteh.ai)

[SIST ISO 13271:2013](#)
<https://standards.iteh.ai/catalog/standards/sist/dfbe9038-2fd5-4281-bea4-71a59800118/sist-iso-13271-2013>



Reference number
ISO 13271:2012(E)

iTeh STANDARD PREVIEW (standards.iteh.ai)

[SIST ISO 13271:2013](#)

<https://standards.iteh.ai/catalog/standards/sist/dfbe9038-2fd5-4281-bea4-71a59800118/sist-iso-13271-2013>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2012

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

Page

Foreword	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Symbols and abbreviated terms	4
4.1 Symbols	4
4.2 Abbreviated terms	5
5 Principle	6
5.1 General	6
5.2 Theory of virtual impactor	6
6 Specification of the two-stage virtual impactor	8
6.1 General	8
6.2 Separation curves	8
6.3 Verification of the separation curves	9
6.4 Operating conditions	9
7 Sampling train	12
7.1 Measuring setup	12
7.2 Equipment and working materials	13
8 Preparation, measurement procedure and post-treatment	15
8.1 General	15
8.2 Pre-treatment	15
8.3 Measurement procedure	16
8.4 Weighing procedure	17
8.5 Post-sampling treatment of weighed parts	18
9 Calculation of the results	18
10 Performance characteristics	19
10.1 Virtual impactor load	19
10.2 Detection limit	19
10.3 Measurement uncertainty	19
10.4 Particle losses	19
11 Test report	20
Annex A (informative) Physical property estimation for the calculation of sample volume flow rate	21
Annex B (informative) Errors by deviations from isokinetic sampling	25
Annex C (informative) Example of a two-stage virtual impactor	27
Annex D (informative) Influence of variations in the flue gas temperature and flue gas composition on the Reynolds number	31
Annex E (informative) Entry nozzle	34
Annex F (informative) Equipment list	35
Annex G (normative) Determination of a representative sampling point	37
Annex H (informative) Generation of standard aerosol for virtual impactor calibration	39
Bibliography	40

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 13271 was prepared by Technical Committee ISO/TC 146, *Air quality*, Subcommittee SC 1, *Stationary source emissions*.

iTeh STANDARD PREVIEW (standards.iteh.ai)

[SIST ISO 13271:2013](#)

<https://standards.iteh.ai/catalog/standards/sist/dfbe9038-2fd5-4281-bea4-71a59800118/sist-iso-13271-2013>

Introduction

In order to quantify the amount of PM₁₀ and PM_{2,5} particles in stationary source emissions or to identify the contribution sources of PM₁₀ and PM_{2,5} in ambient air, it is necessary to measure fine particulate matter in the flue gas of industrial sources.

This International Standard describes a measurement method for determination of mass concentrations of PM₁₀ and PM_{2,5} emissions, which realizes the same separation curves as those specified in ISO 7708^[1] for PM₁₀ and PM_{2,5} in ambient air. The method is based on the principle of gas stream separation using two-stage virtual impactors. This is applicable to higher dust concentrations than the concentrations used for cascade impactors with impaction plates.

The measurement method allows the simultaneous determination of concentrations of PM₁₀ and PM_{2,5} emissions. The method is designed for in-stack measurements at stationary emission sources with possible reactive gases and/or high water vapour.

The contribution of stationary source emissions to PM₁₀ and PM_{2,5} concentrations in ambient air is classified as primary and secondary. Those emissions that exist as particulate matter within the stack gas and that are emitted directly to air can be considered "primary". Secondary particulate consists of those emissions that form in ambient air due to atmospheric chemical reactions. The measurement technique in this International Standard does not measure the contribution of stack emissions to the formation of secondary particulate matter in ambient air.

iTeh STANDARD PREVIEW (standards.iteh.ai)

[SIST ISO 13271:2013](#)

<https://standards.iteh.ai/catalog/standards/sist/dfbe9038-2fd5-4281-bea4-71a59800118/sist-iso-13271-2013>

iTeh STANDARD PREVIEW (standards.iteh.ai)

[SIST ISO 13271:2013](#)

<https://standards.iteh.ai/catalog/standards/sist/dfbe9038-2fd5-4281-bea4-71a59800118/sist-iso-13271-2013>

Stationary source emissions — Determination of PM₁₀/PM_{2,5} mass concentration in flue gas — Measurement at higher concentrations by use of virtual impactors

1 Scope

This International Standard specifies a standard reference method for the determination of PM₁₀ and PM_{2,5} mass concentrations at stationary emission sources by use of two-stage virtual impactors. The measurement method is especially suitable for in-stack measurements of particle mass concentrations in flue gas. The method can also be used for flue gas which contains highly reactive compounds (e.g. sulfur, chlorine, nitric acid) at high temperature or in the presence of high humidity.

The International Standard is applicable to higher dust concentrations. Coarse particles are separated into the nozzles with negligible rebound and entrainment phenomena of collected coarse particulates. For the same reason, the artefacts due to high concentrations in gases or emissions are quite limited.

This International Standard is not applicable to the determination of the total mass concentration of dust.

2 Normative references

iTeh STANDARD PREVIEW

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 12141, *Stationary source emissions — Determination of mass concentration of particulate matter (dust) at low concentrations — Manual gravimetric method* SIST ISO 13271:2013
<https://standards.teh.ai/catalog/standards/sist/dibe9038-2fd5-4281-bea4-71a59800118/sist-iso-13271-2013>

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

3.1

aerodynamic diameter

diameter of a sphere of density 1 g/cm³ with the same terminal velocity due to gravitational force in calm air as the particle under prevailing conditions of temperature, pressure, and relative humidity

NOTE Adapted from ISO 7708:1995,^[1] 2.2.

3.2

backup filter

plane filter used for collection of the PM_{2,5} particle fraction

[ISO 23210:2009,^[7] 3.2.3]

3.3

collection filter

plane filter used for coarse particle collection

3.4

Cunningham factor

correction factor taking into account the change in the interaction between particles and the gas phase

[ISO 23210:2009,^[7] 3.1.7]

NOTE See A.2.

ISO 13271:2012(E)

3.5**cut-off diameter**

aerodynamic diameter where the separation efficiency of the impactor stage is 50 %

[ISO 23210:2009,^[7] 3.1.2]

NOTE Particle separation with real impactors is not ideal and exhibits separation curves similar to the example shown in Figure 1.

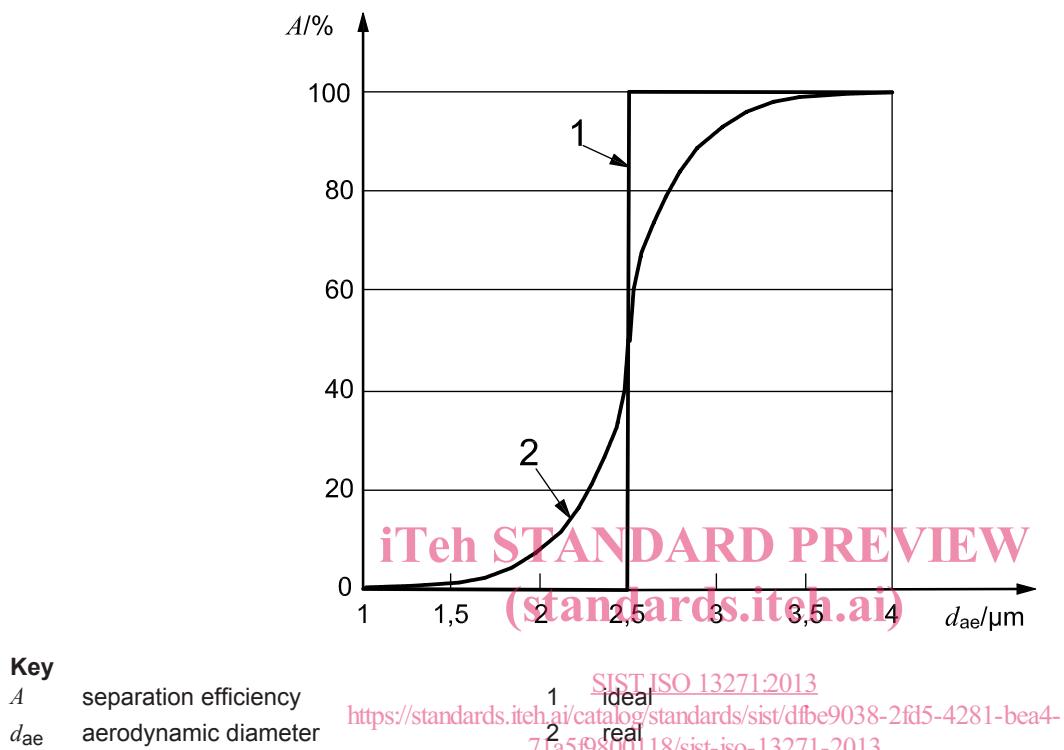


Figure 1 — Separation efficiency A of an impactor as a function of aerodynamic diameter d_{ae} (adapted from ISO 23210:2009,^[7] Figure 2)

3.6**filter holder**

substrate holder designed to hold a filter and for which only the filter deposit is analysed (weighed)

[ISO 15767:2009,^[4] 2.4]

3.7**measurement plane****sampling plane**

plane normal to the centreline of the duct at the sampling position

[ISO 23210:2009,^[7] 3.3.3]

3.8**measurement section**

region of the waste gas duct which includes the measurement plane(s) and the inlet and outlet sections

[ISO 23210:2009,^[7] 3.3.2]

3.9**measurement site****sampling site**

place on the flue gas duct in the area of the measurement plane(s) consisting of structures and technical equipment

NOTE The measurement site consists, for example, of working platforms, measurement ports and energy supply.

[ISO 23210:2009,^[7] 3.3.1]

3.10**PM_{2,5}**

particles which pass through size-selective nozzles with 50 % efficiency cut-off at 2,5 µm aerodynamic diameter

NOTE PM_{2,5} corresponds to the “high risk respirable convention” as defined in ISO 7708:1995,^[1] 7.1.

[ISO 23210:2009,^[7] 3.1.4]

3.11**PM₁₀**

particles which pass through size-selective nozzles with 50 % efficiency cut-off at 10 µm aerodynamic diameter

NOTE PM₁₀ corresponds to the “thoracic convention” as defined in ISO 7708:1995,^[1] Clause 6.

[ISO 23210:2009,^[7] 3.1.3]

3.12**Reynolds number**

Re

iTeh STANDARD PREVIEW (standards.iteh.ai)

where

[SIST ISO 13271:2013](#)

<https://standards.iteh.ai/catalog/standards/sist/dfbe9038-2fd5-4281-bea4-71a59800118/sist-iso-13271-2013>

ρ is the mass density;

v is the gas velocity in the particle acceleration nozzle;

l is the length;

η is the dynamic viscosity.

NOTE 1 Adapted from ISO 80000-11:2008,^[8] 11-4.1.

NOTE 2 “Dimensionless” parameter (parameter of dimension 1) describing flow conditions.

3.13**Stokes's number**

St

$$St = \frac{\rho_{0,P} d_{ae}^2 C_m v}{9\eta D_0}$$

where

ISO 13271:2012(E)

$\rho_{0,P}$ is the particle density (1 g/cm^3);
 d_{ae} is the aerodynamic diameter (m);
 C_m is the Cunningham factor;
 v is the gas velocity in the particle acceleration nozzle (m/s);
 η is the dynamic viscosity of the gas (Pa s);
 D_0 is the particle acceleration nozzle diameter (m).

NOTE 1 Adapted from ISO 23210:2009,^[7] B.2.

NOTE 2 An instrument-specific “dimensionless” parameter (parameter of dimension 1) describing a measure of the inertial movement of a particle in gas stream near an obstacle.

3.14**particle acceleration nozzle**

acceleration nozzle used for accelerating particle-laden gas before separation takes place in the particle collection nozzle

3.15**particle collection nozzle**

collection nozzle used for coarse-particle separation

4 Symbols and abbreviated terms iTeh STANDARD PREVIEW (standards.iteh.ai)

4.1 Symbols

A	separation efficiency	SIST ISO 13271:2013 https://standards.iteh.ai/catalog/standards/sist/dfbe9038-2fd5-4281-bea4-71a59800118/sist-iso-13271-2013
C_m	Cunningham factor	71a59800118/sist-iso-13271-2013
D_0	particle acceleration nozzle diameter	
D_1	particle collection nozzle diameter	
d_{ae}	aerodynamic diameter	
d_{entry}	internal diameter of the entry nozzle	
d_{50}	cut-off diameter	
i	series element number, $i = 1,2,3,\dots,m$, or a subscript to identify the particle fraction ($i = 2,5 \mu\text{m}, 10 \mu\text{m}$)	
j	series element number, $j = 1,2,3,\dots,n$	
l_0	impactor nozzle length	
m_{BF}	particle mass on the backup filter	
m_{CF2}	particle mass on the collection filter of the second separation stage	
N	number of impactor nozzles	
n	number of measurement pairs	
p_{amb}	ambient pressure at the measurement site	
p_n	standard pressure	

p_{st}	difference between the static pressure in the measurement cross-section and the atmospheric pressure at the measurement site
q_V	volume flow rate at operating conditions
q_{Vn}	volume flow rate under standard conditions and for dry gas
q_{v0}	volume flow rates per nozzle at operating conditions for total flow
q_{v1}	volume flow rates per nozzle at operating conditions for minor flow
q_{v2}	volume flow rates per nozzle at operating conditions for major flow
Re	Reynolds number
St_{50}	Stokes's number in relation to the cut-off diameter d_{50}
s	distance between the end of the particle acceleration nozzle and the top of the particle collection nozzle
T	gas temperature
T_n	standard temperature
$u(\gamma)$	standard uncertainty of paired measurements
v	gas velocity at particle acceleration nozzle
v_{fg}	flue gas velocity
V_n	sample volume under standard conditions and for dry gas
$\gamma_{n,H_2O,v}$	mass concentration of water vapour under standard conditions and with dry gas https://standards.iteh.ai/catalog/standards/sist/dfbe9038-2fd5-4281-bea4-71a5d9800118/sist-iso-13271-2013
$\gamma_{(PM_{2,5})}$	concentration of $PM_{2,5}$
$\gamma_{(PM_{10})}$	concentration of PM_{10}
$\gamma_{1,i}$	i th concentration value of the first measuring system
$\gamma_{2,i}$	i th concentration value of the second measuring system
η	dynamic viscosity of the gas
$\rho_{n,H_2O,v}$	density of water vapour under standard conditions
$\rho_{0,P}$	particle density (1 g/cm^3)
ξ	minor flow ratio at impactor stage

4.2 Abbreviated terms

BF	backup filter
CF1	collection filter of the first separation stage
CF2	collection filter of the second separation stage