
**Geometrical product specifications
(GPS) — Coordinate measuring machines
(CMM): Technique for determining the
uncertainty of measurement —**

Part 3:

**Use of calibrated workpieces or
measurement standards**

(standards.iteh.ai)

*Spécification géométrique des produits (GPS) — Machines à mesurer
tridimensionnelles (MMT): Technique pour la détermination de
l'incertitude de mesure —*

[https://standards.iteh.ai/catalog/standards/sist/9ddfd480-647c-4c4b-9516-](https://standards.iteh.ai/catalog/standards/sist/9ddfd480-647c-4c4b-9516-480000000000/iso-15530-3-2011)

4 Partie 3: Utilisation de pièces étalonnées ou d'étalons de mesure



iTeh STANDARD PREVIEW (standards.iteh.ai)

ISO 15530-3:2011

<https://standards.iteh.ai/catalog/standards/sist/9ddf480-647c-4c4b-9516-43a58d5a7581/iso-15530-3-2011>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2011

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

Page

Foreword	iv
Introduction.....	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Symbols.....	2
5 Requirements.....	3
5.1 Operating conditions	3
5.2 Similarity conditions	3
6 Principle of the uncertainty evaluation using calibrated workpieces.....	4
7 Procedure	4
7.1 Measuring equipment	4
7.2 Execution	4
7.3 Calculation of the uncertainty.....	5
7.4 Applying the substitution method: special considerations.....	9
8 Reverification of the measurement uncertainty.....	9
9 Interim check of the measurement uncertainty	10
Annex A (informative) Examples of application.....	11
Annex B (informative) Relation to the GPS matrix model.....	16
Bibliography.....	18

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 15530-3 was prepared by Technical Committee ISO/TC 213, *Dimensional and geometrical product specifications and verification*.

This first edition of ISO 15530-3 cancels and replaces ISO/TS 15530-3:2004, which has been technically revised.

ISO 15530 consists of the following parts, under the general title *Geometrical product specifications (GPS) — Coordinate measuring machines (CMM): Technique for determining the uncertainty of measurement*:

- *Part 1: Overview and metrological characteristics* [Technical Specification]
- *Part 3: Use of calibrated workpieces or measurement standards*
- *Part 4: Evaluating task-specific measurement uncertainty using simulation* [Technical Specification]

Introduction

This part of ISO 15530 is a Geometrical Product Specification (GPS) and is to be regarded as a general GPS document (see ISO/TR 14638). It influences chain link 6 of the chain of standards on size, distance, radius, angle, form, orientation, location, run-out and datums.

The ISO/GPS Masterplan given in ISO/TR 14638 gives an overview of the ISO/GPS system of which this standard is a part. The fundamental rules of ISO/GPS given in ISO 8015 apply to this document and the default decision rules given in ISO 14253-1 apply to specifications made in accordance with this document, unless otherwise indicated.

For more detailed information on the relation of this standard to the GPS matrix model, see Annex B.

Coordinate measuring machines (CMMs) have become essential for the verification of geometry in industry. According to the ISO 9000 series of standards, in a quality management system, the relevant measuring equipment is required to be calibrated against certified equipment having a known and valid relationship to internationally or nationally recognized standards in order to establish traceability. According to the *International vocabulary of basic and general terms in metrology* (VIM), a calibration comprises — besides the establishment of the relationship between the measured and the correct values of a quantity — the uncertainty evaluation in the final results (measurands) of the measurement task. However, uncertainty evaluation methods covering the errors arising in the innumerable measurement tasks a CMM can actually perform are often very complex. In these cases, the risk of an unrealistic estimation of task-related uncertainty is likely to arise.

The aim of this part of ISO 15530 is to provide an experimental technique for simplifying the uncertainty evaluation of CMM measurements. In this experimental approach, measurements are carried out in the same way as actual measurements, but with calibrated workpieces or measurement standards of similar dimension and geometry instead of the unknown objects to be measured. The description of this experimental technique to evaluate measurement uncertainty is the key element of this part of ISO 15530. The standardization of such procedures for the uncertainty evaluation serves the worldwide mutual recognition of calibrations and other measurement results.

This part of ISO 15530 is applicable for non-substitution measurement of workpieces or measurement standards, where the measurement result is given by the indication of the CMM. Furthermore, this part of ISO 15530 is applicable for substitution measurement, where, in opposition to the non-substitution measurement, a check standard is used to correct for the systematic errors of the CMM. The latter will generally decrease the measurement uncertainty and is often used, especially in the field of gauge calibration.

This part of ISO 15530 describes one of several methods of uncertainty evaluation, which will be outlined in later ISO documents. Because of the experimental approach, it is simple to perform, and it provides realistic statements of measurement uncertainties.

The limitations of this method can be summarized as: the availability of artefacts with sufficiently defined geometrical characteristics, stability, reasonable costs, and the possibility of being calibrated with sufficiently small uncertainty.

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 15530-3:2011

<https://standards.iteh.ai/catalog/standards/sist/9ddf480-647c-4c4b-9516-43a58d5a7581/iso-15530-3-2011>

Geometrical product specifications (GPS) — Coordinate measuring machines (CMM): Technique for determining the uncertainty of measurement —

Part 3: Use of calibrated workpieces or measurement standards

1 Scope

This part of ISO 15530 specifies the evaluation of measurement uncertainty for results of measurements obtained by a CMM (coordinate measuring machine) and by using calibrated workpieces or measurement standards. It provides an experimental technique for simplifying the uncertainty evaluation of CMM measurements, whose approach (substitution measurements) leads to measurements being carried out in the same way as actual measurements, but with calibrated workpieces of similar dimension and geometry instead of the unknown workpieces to be measured.

Non-substitution measurements on CMMs are also covered, as are the requirements of the uncertainty evaluation procedure, the measurement equipment needed, and the reverification and interim check of the measurement uncertainty.

NOTE The evaluation of measurement uncertainty is always related to a specific measuring task.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 10360-1:2000, *Geometrical Product Specifications (GPS) — Acceptance and reverification tests for coordinate measuring machines (CMM) — Part 1: Vocabulary*

ISO/IEC Guide 98-3:2008, *Uncertainty of measurement — Part 3: Guide to the expression of uncertainty in measurement (GUM:1995)*

ISO/IEC Guide 99:2007, *International vocabulary of metrology — Basic and general concepts and associated terms (VIM)*

ISO 14978:2006, *Geometrical product specification (GPS) — General concepts and requirements for GPS measuring equipment*

3 Terms and definitions

For the purpose of this part of ISO 15530, the terms and definitions given in ISO 10360-1, ISO/IEC Guide 98-3, ISO/IEC Guide 99 and the following apply.

- 3.1 non-substitution measurement**
measurement where the uncorrected indication of the CMM is used as a result
- 3.2 substitution measurement**
measurement where both a workpiece and a check standard are measured in order to provide additional corrections for systematic errors of the CMM

4 Symbols

For the purpose of this part of ISO 15530, the symbols given in Table 1 apply.

Table 1 — Symbols

Symbol	Interpretation
b	Systematic error observed during the evaluation of the measurement uncertainty
Δ_i	Difference between the measured and calibrated values of the check standard when applying the substitution method
k	Coverage factor
l	Measured dimension
n	Number of repeated measurements
T	Average temperature of the workpiece or measurement standard
u_{cal}	Standard uncertainty of the parameter of the calibrated workpiece or measurement standard
u_p	Standard uncertainty of the measurement procedure
u_b	Standard uncertainty of the systematic error
u_w	Standard uncertainty associated with the variations in the uncalibrated workpieces
u_{wp}	Standard uncertainty associated with the variations in the mechanical properties of the uncalibrated workpieces
u_{wt}	Standard uncertainty associated with the variations in the CTEs (thermal expansion coefficients) of the uncalibrated workpieces
u_α	Standard uncertainty of the thermal expansion coefficient
U	Expanded measurement uncertainty
U_{cal}	Expanded uncertainty of the calibrated workpiece parameter or measurement standard
x_{cal}	Value of the parameter of the calibrated workpiece or measurement standard
y	Measurement result
y_i	Measurement results during evaluation of measurement uncertainty
y_i^*	Uncorrected indications of the CMM during evaluation of measurement uncertainty when applying the substitution method
\bar{y}	Mean value of the measurement result

5 Requirements

5.1 Operating conditions

Before starting the measurements, initialize the CMM and perform procedures such as probe configuration and probe qualification according to the conditions specified in the manufacturer's operating manual. In particular, an adequate thermal equilibrium of the (calibrated) workpiece or measurement standard and the CMM should exist.

For the measurements given in 7.2, the environmental and operational conditions quoted by the CMM manufacturer and conditions quoted in the user's quality manual shall apply. In particular, existing error compensating functions (such as corrections applied via the software of the CMM's computer) shall be active if this is prescribed in the quality manual.

The CMM shall fulfil the specifications of the manufacturer, or — if different — the specifications laid down in the procedural instructions for the measurement task (task-related calibration, see ISO 14978); therefore, it is not necessary to calibrate all the metrological characteristics of a CMM (global calibration, see ISO 14978).

5.2 Similarity conditions

The method requires similarity of the following.

- a) The dimension and geometry of the workpiece or measurement standard used in the actual measurements (see 7.2.2) and the calibrated workpiece or measurement standard used in the evaluation of measurement uncertainty (see 7.2.3).

NOTE Conditions to be repeated are, for example, positions and orientations.

- b) The measurement procedure of the evaluation of measurement uncertainty and the actual measurement.

NOTE Conditions to be repeated are, for example, handling, exchange and clamping, time elapsed between probing points, loading and unloading procedures, measuring force and speed.

- c) The environmental conditions (including all variations) during evaluation of measurement uncertainty and actual measurement.

NOTE Conditions to be repeated are, for example, temperature, temperature stabilization time and temperature corrections (if used).

In Table 2, the similarity requirements are given.

Table 2 — Similarity requirements for workpieces or standard to be measured and the calibrated workpieces or standard used during evaluation of measurement uncertainty

Subject	Requirements	
Dimensional characteristics	Dimensions	Identical within: — 10 % beyond 250 mm — 25 mm below 250 mm
	Angles	Identical within $\pm 5^\circ$
Form error and surface texture	Similar due to functional properties	
Material (e.g. thermal expansion, elasticity, hardness)	Similar due to functional properties	
Measuring strategy	Identical	
Probe configuration	Identical	

The similarity of the thermal conditions are considered to be assured if the above requirements are met. The evaluation of measurement uncertainty using the calibrated workpiece shall cover, in particular, the range of temperatures which will prevail during the measurements of the uncalibrated workpieces. If the variation of the thermal expansion coefficient of the measured workpieces or standards is assumed to be significant, this uncertainty contribution has to be taken into account (see 7.3.3 and 7.3.4).

For some CMMs, errors associated with dynamic effects may become significant with a decreasing probe approach distance. For small internal features, e.g. a hole, the probe approach distance may be limited by the feature size. Consequently, care shall be taken to ensure that the probe approach distance is identical.

6 Principle of the uncertainty evaluation using calibrated workpieces

The evaluation of measurement uncertainty is a sequence of measurements, performed in the same way and under the same conditions as the actual measurements. The only difference is that, instead of the workpieces to be measured, one or more calibrated workpieces are measured. The differences between the results obtained by the measurement and the known calibration values of these calibrated workpieces are used to estimate the uncertainty of the measurements.

The uncertainty of the measurement consists of uncertainty contributions

- a) due to the measurement procedure,
- b) from the calibration of the calibrated workpiece,
- c) due to the variations of the measured workpieces (changing form deviations, expansion coefficient and surface texture).

The full effect of all variation in environmental conditions should be included to perform a comprehensive evaluation of the measurement uncertainty.

<https://standards.iteh.ai/catalog/standards/sist/9ddfd480-647c-4c4b-9516-43a58d5a7581/iso-15530-3-2011>

7 Procedure

7.1 Measuring equipment

The uncertainty evaluation on a CMM using calibrated workpieces requires the following equipment:

- a) a task-related stylus set-up;
- b) at least one calibrated workpiece.

The metrological characteristics of the calibrated workpieces shall be calibrated with a known and sufficiently low uncertainty to fulfil the requirements of the measurement task.

The probe shall be re-qualified for each calibration.

The uncertainty stated for the calibration of the calibrated workpieces should be valid for the measurement strategy employed during the actual measurements and the uncertainty evaluation, i.e. the measurand of the calibrated workpiece shall be the same as the measurand evaluated in the measurement uncertainty process.

7.2 Execution

7.2.1 General

The user of the CMM has a high degree of freedom to design the measurement procedure (i.e. the measurement strategy) according to the technical requirements. This is possible because the procedure and conditions of actual measurements and those during the uncertainty evaluation shall be the same.

7.2.2 Actual measurement

One cycle of an actual measurement consists of the handling of the workpieces and one or more measurements of the workpieces (see Figure 1).

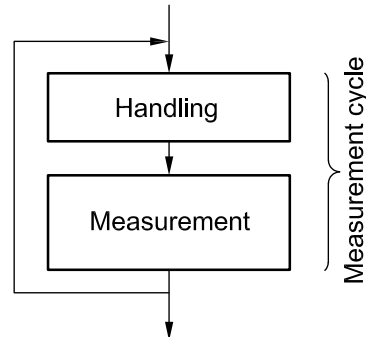


Figure 1 — Procedure of non-substitution measurement — Measurement cycle

The position and the orientation of the measured workpieces are free within the range covered by the uncertainty evaluation.

7.2.3 Uncertainty evaluation

The uncertainty evaluation shall be as follows.

Calibrated workpieces are measured instead of the workpieces. Calibrated workpieces and workpieces shall fulfil the similarity conditions outlined in 5.2. Special loading and unloading procedures shall be performed during the uncertainty evaluation.

To obtain a sufficient number of samples for the uncertainty evaluation, at least 10 measurement cycles and a total of at least 20 measurements on calibrated workpieces shall be carried out. For example, a total of 20 cycles is the minimum, if only one calibrated workpiece per cycle is measured.

During the uncertainty evaluation, the position and orientation of the calibrated workpieces are systematically varied within the limits given by the procedure of the actual measurements.

As specified in 7.2.2, a measurement cycle shall contain all actions involved in a real measurement to ensure the similarity of thermal conditions. This implies, for example, that the CMM has to move through the same positions as if a complete measurement were being carried out, even though during the uncertainty evaluation not all workpieces might be present (dummy measurements).

7.3 Calculation of the uncertainty

7.3.1 General

In a calibration certificate or measurement report, the measurement result, y , and its expanded uncertainty, U , shall be expressed in the form $y \pm U$, where U is determined with a coverage factor $k = 2$ for an approximated coverage probability of 95 %.

When performing the measurements, four uncertainty contributions shall basically be taken into account, described by the following standard uncertainties:

- u_{cal} standard uncertainty associated with the uncertainty of the calibration of the calibrated workpiece stated in the calibration certificate;
- u_{p} standard uncertainty associated with the measurement procedure as assessed below;