

---

---

**Dentistry — Torsion test of implant  
body/connecting part joints of  
endosseous dental implant systems**

*Médecine bucco-dentaire — Essai de torsion sur l'interface corps  
d'implant/élément de connexion des systèmes d'implants dentaires  
endo-osseux*

**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

[ISO/TS 13498:2011](https://standards.iteh.ai/catalog/standards/sist/a23cb1d1-c851-4814-af95-f942d1573233/iso-ts-13498-2011)

[https://standards.iteh.ai/catalog/standards/sist/a23cb1d1-c851-4814-af95-  
f942d1573233/iso-ts-13498-2011](https://standards.iteh.ai/catalog/standards/sist/a23cb1d1-c851-4814-af95-f942d1573233/iso-ts-13498-2011)



## iTeh STANDARD PREVIEW (standards.iteh.ai)

ISO/TS 13498:2011

<https://standards.iteh.ai/catalog/standards/sist/a23cb1d1-c851-4814-af95-f942d1573233/iso-ts-13498-2011>



### **COPYRIGHT PROTECTED DOCUMENT**

© ISO 2011

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Case postale 56 • CH-1211 Geneva 20  
Tel. + 41 22 749 01 11  
Fax + 41 22 749 09 47  
E-mail [copyright@iso.org](mailto:copyright@iso.org)  
Web [www.iso.org](http://www.iso.org)

Published in Switzerland

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

In other circumstances, particularly when there is an urgent market requirement for such documents, a technical committee may decide to publish other types of document:

- an ISO Publicly Available Specification (ISO/PAS) represents an agreement between technical experts in an ISO working group and is accepted for publication if it is approved by more than 50 % of the members of the parent committee casting a vote.
- an ISO Technical Specification (ISO/TS) represents an agreement between the members of a technical committee and is accepted for publication if it is approved by 2/3 of the members of the committee casting a vote.

<https://standards.iteh.ai/catalog/standards/sist/a23ch1d1-c851-4814-af05-642d1573233/iso-ts-13498-2011>

An ISO/PAS or ISO/TS is reviewed after three years in order to decide whether it will be confirmed for a further three years, revised to become an International Standard, or withdrawn. If the ISO/PAS or ISO/TS is confirmed, it is reviewed again after a further three years, at which time it must either be transformed into an International Standard or be withdrawn.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO/TS 13498 was prepared by Technical Committee ISO/TC 106, *Dentistry*, Subcommittee SC 8, *Dental implants*.

## Introduction

Most dental implant systems currently on the market employ a dental implant body that is inserted within the jaw bone, to which other components can be joined when constructing a prosthetic superstructure. The connection between these components and the implant body should be sufficiently rigid to resist masticatory loads, which have a significant torsional component. Implant systems therefore often incorporate features to restrict rotation at the connection. If this is insufficiently strong, then distortion/fracture of the linked components will occur. A standardised torsion test for the joint between the implant body and connecting part facilitates comparative evaluation.

## iTeh STANDARD PREVIEW (standards.iteh.ai)

[ISO/TS 13498:2011](https://standards.iteh.ai/catalog/standards/sist/a23cb1d1-c851-4814-af95-f942d1573233/iso-ts-13498-2011)

<https://standards.iteh.ai/catalog/standards/sist/a23cb1d1-c851-4814-af95-f942d1573233/iso-ts-13498-2011>

# Dentistry — Torsion test of implant body/connecting part joints of endosseous dental implant systems

## 1 Scope

This Technical Specification establishes a method to determine the torsional yield strength and maximum torque of the implant body/connecting part joints of endosseous dental implant systems. This test is most appropriate for evaluating new types of joints and connecting parts, as well as new materials.

This Technical Specification provides a protocol for torsional loading of an implant body/connecting part joint. It is not applicable for predicting the *in vivo* performance of an endosseous dental implant system and it is not derived from observations of clinical failure.

## 2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 1942, *Dentistry — Vocabulary*

ISO/TS 13498:2011

<https://standards.iteh.ai/catalog/standards/sist/a23cb1d1-c851-4814-af95-f942d1573233/iso-ts-13498-2011>

## 3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 1942 and the following apply.

### 3.1

#### torsional yield strength

$M_{\text{tors}}$

torque required to produce a rotation of 2° offset from the straight-line portion on the torque versus rotation angle curve

NOTE See Figure 3.

### 3.2

#### maximum torque

$M_{\text{max}}$

largest value of torque recorded on the torque versus rotation angle curve

NOTE See Figure 3.

## 4 Principle

The torsional yield strength and maximum torque of the implant body/connecting part interface are determined by clamping the implant body and connecting part to be tested in a testing device.

Testing shall be performed on finished devices or specimens that have an equivalent connecting part joint to the finished device (i.e. components that have undergone the same manufacturing process and sterilisation as

the device that is to be marketed). If the manufacturer intends the endosseous dental implant to be sterilised by the clinician prior to surgery, sterilisation shall be carried out as specified in the manufacturer's instructions for use before testing. However, if there is evidence that the specified sterilisation method has no significant effect on the properties of all the materials of the specimens being tested, sterilisation is not necessary prior to testing.

## 5 Test methods


### 5.1 Testing device

The test device shall have the following parts:

- specimen holders (the implant body and connecting part shall each be held at a maximum of 5 mm from the interface between them);
- torque transducer;
- torsional driving device, able to apply a torque no less than the anticipated maximum torque;
- torsional displacement transducer.

An example of a torsional testing device is illustrated in Figure 1.

The central long axes of the shafts of the torque transducer and torsional driving device shall be coincident.

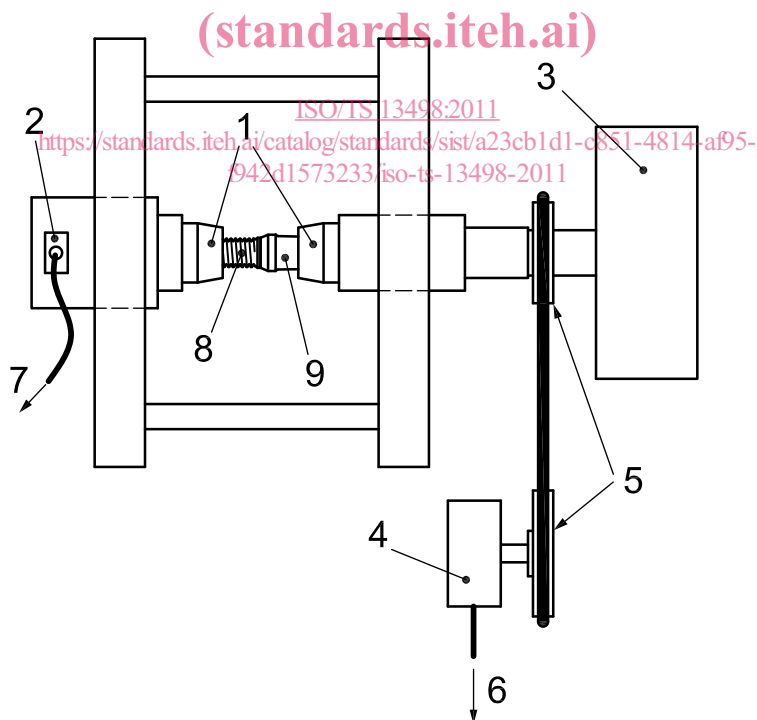

**Key**

- |                                     |                                    |
|-------------------------------------|------------------------------------|
| 1 specimen holder                   | 6 output to X-axis of X-Y recorder |
| 2 torque transducer                 | 7 output to Y-axis of X-Y recorder |
| 3 torsional driving device          | 8 implant body                     |
| 4 torsional displacement transducer | 9 connecting part                  |
| 5 pulley                            |                                    |


**Figure 1 — Example of a testing device**

## 5.2 Torque transducer

The torque transducer shall have a range not exceeding the quintuple of the anticipated minimum torsional yield strength. The maximum inaccuracy of the torque transducer shall be  $\pm 1\%$  of the maximum torque to be tested.

## 5.3 Preparation of test specimen

The connecting part shall be fixed on the implant body using the specified screw at tightening torques stated in the manufacturer's instructions for use. The ends of the implant body and connecting part shall be fixed in a rigid clamping device. These ends may be modified into shapes larger than the maximum diameter of implant body and/or connecting part and they should be easy to clamp with the holders. An example of a test specimen is illustrated in Figure 2.

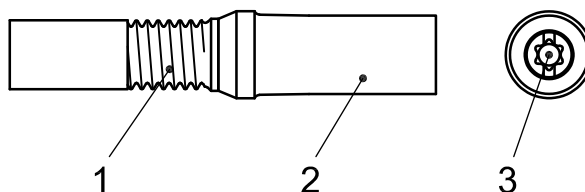

### Key

- 1 implant body
- 2 connecting part
- 3 connecting part screw

iTeh STANDARD PREVIEW  
(standards.iteh.ai)

Figure 2 — Schematic of a test specimen

ISO/TS 13498:2011

## 5.4 Test conditions

<https://standards.iteh.ai/catalog/standards/sist/a23cb1d1-c851-4814-af95-f942d1573233/iso-ts-13498-2011>

Carry out the test at room temperature ( $20 \pm 5$ ) °C in air.

## 5.5 Procedure


**5.5.1** The connecting part shall be fixed on the implant body using a specific screw at tightening torques stated in the manufacturer's instructions for use. Clamp the retaining portions of the implant body and connecting part of a test specimen into the specimen holders of the testing device. Apply torque continuously to the connecting part at a rate of between 1 and 10 degrees per minute and record the torque versus rotation angle curve. Measure the torsional yield strength and the maximum torque of at least six test specimens as described below.

**5.5.2** The torsional yield strength is determined by the 2° offset method<sup>[2]</sup> (see Figure 3) using the torque versus rotation angle curve produced as described in 5.5.1.


**5.5.3** On the torque versus rotation angle curve, locate a point, m, corresponding to 2° of rotation angle and draw a line, mB, parallel to a line, OA. Locate a point S, which is the intersection of mB with the torque versus rotation angle curve. Torque,  $M_{\text{tors}}$ , is defined as the torsional yield strength.

**5.5.4** The maximum torque,  $M_{\text{max}}$ , is determined by the largest value of torque on the torque versus rotation angle curve.

**NOTE** It is possible that a sag appears on the torque versus rotation angle curve depending on the testing configuration. In such cases, the torsional yield strength and the maximum torque are determined according to Figure 3 b).

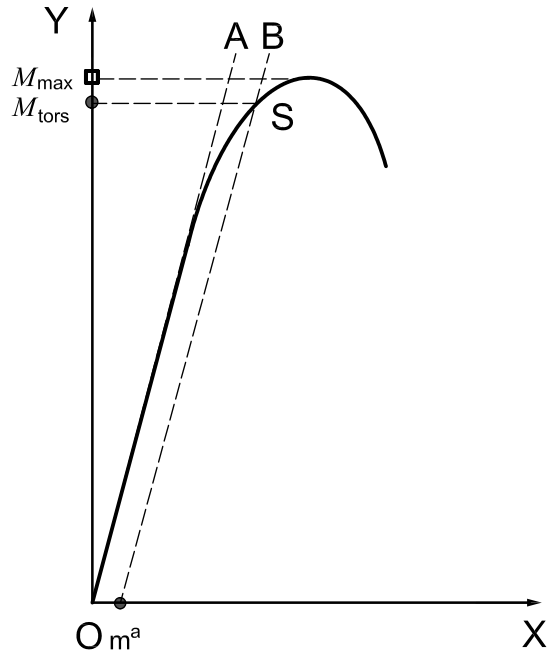

a) Without sag

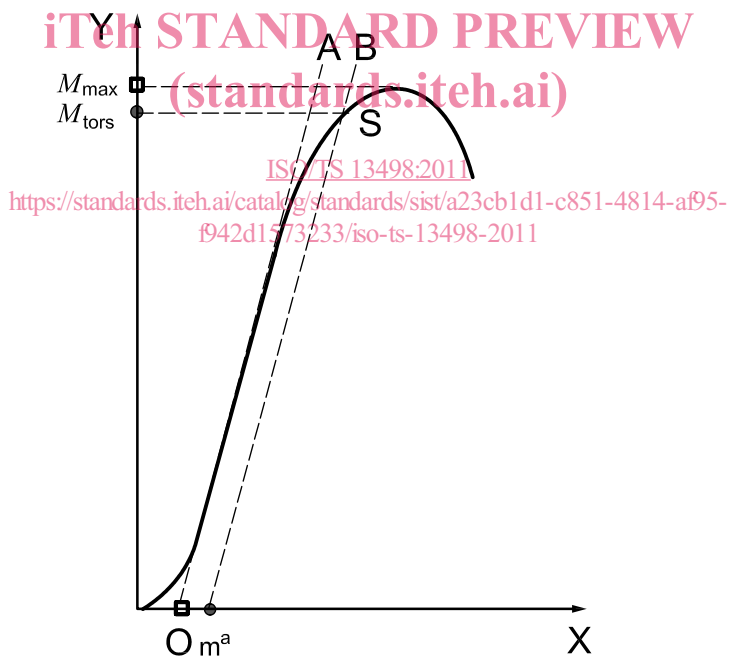

b) With sag

**Key**

- X rotation angle, in degrees (°)
- Y torque, in N·m
- O initial contact
- $M_{max}$  maximum torque
- $M_{tors}$  torsional yield strength
- <sup>a</sup> Rotation angle is 2°.

**Figure 3 — Method to determine torsional yield strength and maximum torque**



**5.5.5** Observe the deformed or fractured part of the implant body/connecting part joint under a low-magnification microscope.

## 5.6 Evaluation of torque test

Calculate the mean of the measured values of test specimens.

## 6 Test report

The test report shall include at least the following information:

- a) identification of the test specimens, including
  - type of connection (internal anti-rotation: taper-fit, notch-fit, hexagonal etc.; external anti-rotation: hexagonal etc.),
  - manufacturer(s), part numbers and lot numbers of the tested parts,
  - material(s) of the tested parts,
  - diameter and length of the implant body and connecting part;
- b) test method, including test condition, testing device, rotational rate, distance from the interface at which the components were held and a drawing of the test specimens;
- c) results obtained, namely **(standards.iteh.ai)**
  - torsional yield strength and maximum torque,  
ISO/TS 13498:2011
  - microscopic observation on deformed and fractured parts of the test specimens;  
<https://standards.iteh.ai/catalog/standards/sist/a23cb1d1-c851-4814-af95-b42d19752930/iso-ts-13498-2011>
- d) reference to this Technical Specification, i.e. ISO/TS 13498:2011.