

---

---

**Optics and optical instruments — Field  
procedures for testing geodetic and  
surveying instruments —**

**Part 4:  
Electro-optical distance meters (EDM  
measurements to reflectors)**

iTeh STANDARD PREVIEW  
(standards.iteh.ai)

*Optique et instruments d'optique — Méthodes d'essai sur site des  
instruments géodésiques et d'observation —*

*Partie 4: Télémètres électro-optiques (mesurages MED avec réflecteurs)*  
*ISO 17123-4:2012*

<https://standards.iteh.ai/catalog/standards/sist/751ecc9f-8466-4a47-8784-f623b3e6ba3e/iso-17123-4-2012>



## iTeh STANDARD PREVIEW (standards.iteh.ai)

ISO 17123-4:2012

<https://standards.iteh.ai/catalog/standards/sist/751ecc9f-8466-4a47-8784-f623b3e6ba3e/iso-17123-4-2012>



### **COPYRIGHT PROTECTED DOCUMENT**

© ISO 2012

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Case postale 56 • CH-1211 Geneva 20  
Tel. + 41 22 749 01 11  
Fax + 41 22 749 09 47  
E-mail [copyright@iso.org](mailto:copyright@iso.org)  
Web [www.iso.org](http://www.iso.org)

Published in Switzerland

# Contents

Page

Foreword .....	iv
Introduction .....	v
1 Scope .....	1
2 Normative references .....	1
3 Terms and definitions .....	2
4 General .....	2
4.1 Requirements .....	2
4.2 Procedure 1: Simplified test procedure .....	2
4.3 Procedure 2: Full test procedure (Type A evaluation of standard uncertainty) .....	2
5 Simplified test procedure .....	3
5.1 Configuration of the test field .....	3
5.2 Measurements .....	4
5.3 Calculation .....	4
5.4 Further investigations .....	4
6 Full test procedure .....	5
6.1 Configuration of the test line .....	5
6.2 Measurements .....	6
6.3 Calculation .....	7
6.4 Statistical tests .....	10
6.5 Combined standard uncertainty evaluation (Type A and Type B) .....	12
Annex A (informative) Example of the simplified test procedure .....	13
Annex B (informative) Example of the full test procedure .....	15
Annex C (informative) Example for the calculation of a combined uncertainty budget (Type A and Type B) .....	19
Bibliography .....	22

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 17123-4 was prepared by Technical Committee ISO/TC 172, *Optics and photonics*, Subcommittee SC 6, *Geodetic and surveying instruments*.

This second edition cancels and replaces the first edition (ISO 17123-4:2001), which has been technically revised.

ISO 17123 consists of the following parts, under the general title *Optics and optical instruments — Field procedures for testing geodetic and surveying instruments*:

- Part 1: Theory
- Part 2: Levels
- Part 3: Theodolites
- Part 4: Electro-optical distance meters (*EDM measurements to reflectors*)
- Part 5: Total stations
- Part 6: Rotating lasers
- Part 7: Optical plumbing instruments
- Part 8 : GNSS field measurement systems in real-time kinematic (RTK)

Annexes A, B and C of this part of ISO 17123 are for information only.

**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

[ISO 17123-4:2012](https://standards.iteh.ai/catalog/standards/sist/751ecc9f-8466-4a47-8784-162563c06a3c/iso-17123-4-2012)

<https://standards.iteh.ai/catalog/standards/sist/751ecc9f-8466-4a47-8784-162563c06a3c/iso-17123-4-2012>

## Introduction

This part of ISO 17123 specifies field procedures for adoption when determining and evaluating the uncertainty of measurement results obtained by geodetic instruments and their ancillary equipment, when used in building and surveying measuring tasks. Primarily, these tests are intended to be field verifications of suitability of a particular instrument for the immediate task. They are not proposed as tests for acceptance or performance evaluations that are more comprehensive in nature.

The definition and concept of uncertainty as a quantitative attribute to the final result of measurement were developed mainly in the last two decades, even though error analysis has long been a part of all measurement sciences. After several stages, the CIPM (Comité Internationale des Poids et Mesures) referred the task of developing a detailed guide to ISO. Under the responsibility of the ISO Technical Advisory Group on Metrology (TAG 4), and in conjunction with six worldwide metrology organizations, a guidance document on the expression of measurement uncertainty was compiled with the objective of providing rules for use within standardization, calibration, laboratory, accreditation and metrology services. ISO/IEC Guide 98-3 was first published as the *Guide to the Expression of Uncertainty in Measurement* (GUM) in 1995.

With the introduction of uncertainty in measurement in ISO 17123 (all parts), it is intended to finally provide a uniform, quantitative expression of measurement uncertainty in geodetic metrology with the aim of meeting the requirements of customers.

ISO 17123 (all parts) provides not only a means of evaluating the precision (experimental standard deviation) of an instrument, but also a tool for defining an uncertainty budget, which allows for the summation of all uncertainty components, whether they are random or systematic, to a representative measure of accuracy, i.e. the combined standard uncertainty.

ISO 17123 (all parts) therefore provides, for each instrument investigated by the procedures, a proposal for additional, typical influence quantities, which can be expected during practical use. The customer can estimate, for a specific application, the relevant standard uncertainty components in order to derive and state the uncertainty of the measuring result. [ISO 17123-4:2012](https://standards.iteh.ai/catalog/standards/sist/751ecc9f-8466-4a47-8784-f623b3e6ba3e/iso-17123-4-2012)

<https://standards.iteh.ai/catalog/standards/sist/751ecc9f-8466-4a47-8784-f623b3e6ba3e/iso-17123-4-2012>

**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

ISO 17123-4:2012

<https://standards.iteh.ai/catalog/standards/sist/751ecc9f-8466-4a47-8784-f623b3e6ba3e/iso-17123-4-2012>

# Optics and optical instruments — Field procedures for testing geodetic and surveying instruments —

## Part 4: Electro-optical distance meters (EDM measurements to reflectors)

### 1 Scope

This part of ISO 17123 specifies field procedures to be adopted when determining and evaluating the precision (repeatability) of electro-optical distance meters (EDM instruments) and their ancillary equipment when used in building and surveying measurements. This part of ISO 17123 is applicable to reflector-type EDM instruments only and is not designed to determine the precision of non-prism EDM types. Primarily, these tests are intended to be field verifications of the suitability of a particular instrument for the immediate task at hand and to satisfy the requirements of other standards. They are not proposed as tests for acceptance or performance evaluations that are more comprehensive in nature.

This part of ISO 17123 can be thought of as one of the first steps in the process of evaluating the uncertainty of a measurement (more specifically a measurand). The uncertainty of a result of a measurement is dependent on a number of parameters. Therefore we differentiate between different measures of accuracy and objectives in testing, like repeatability, reproducibility (e.g. between day repeatability), and of course a thorough assessment of all possible error sources, as prescribed by ISO/IEC Guide 98-3 and by ISO 17123-1.

These field procedures have been developed specifically for *in situ* applications without the need for special ancillary equipment and are purposefully designed to minimize atmospheric influences.

<https://standards.iteh.ai/catalog/standards/sist/751ecc9f-8466-4a47-8784-f623b3e6ba3e/iso-17123-4-2012>

### 2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 3534-1, *Statistics — Vocabulary and symbols — Part 1: General statistical terms and terms used in probability*

ISO 4463-1, *Measurement methods for building — Setting-out and measurement — Part 1: Planning and organization, measuring procedures, acceptance criteria*

ISO 7077, *Measuring methods for building — General principles and procedures for the verification of dimensional compliance*

ISO 7078, *Building construction — Procedures for setting out, measurement and surveying — Vocabulary and guidance notes*

ISO 9849, *Optics and optical instruments — Geodetic and surveying instruments — Vocabulary*

ISO 17123-1, *Optics and optical instruments — Field procedures for testing geodetic and surveying instruments — Part 1: Theory*

ISO/IEC Guide 98-3, *Uncertainty of measurement — Part 3: Guide to the expression of uncertainty in measurement (GUM:1995)*

ISO/IEC Guide 99, *International vocabulary of metrology — Basic and general concepts and associated terms (VIM)*

### 3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 4463-1, ISO 7077, ISO 7078, ISO 9849, ISO 17123-1, ISO/IEC Guide 98-3 and ISO/IEC Guide 99 apply.

### 4 General

#### 4.1 Requirements

Before commencing surveying, it is important that the operator investigates that the precision in use of the measuring equipment is appropriate to the intended measuring task.

The EDM instrument and its ancillary equipment shall be in known and acceptable states of permanent adjustment according to the methods specified in the manufacturer's handbook, and used with tripods, forced centring equipment and reflectors as recommended by the manufacturer.

The results of these tests are influenced by meteorological conditions. These conditions will include variations in air temperature and air pressure. Actual meteorological data shall be measured in order to derive atmospheric corrections, which shall be added to the raw distances. The particular conditions to be taken into account may vary, depending on the location where the tasks are to be undertaken. These conditions shall include variations in air temperature, wind speed, degree of cloudiness and visibility. Note should also be taken of the actual weather conditions at the time of measurement and the type of surface above which the measurements are made. The conditions chosen for the tests should match those expected when the intended measuring task is actually carried out (see ISO 7077 and ISO 7078).

This part of ISO 17123 describes two different field procedures as given in Clauses 5 and 6. The operator shall choose the procedure which is most relevant to the project's particular requirements.

#### 4.2 Procedure 1: Simplified test procedure

The simplified test procedure provides an estimate as to whether the precision of a given EDM equipment is within the specified permitted deviation according to ISO 4463-1.

The simplified test procedure is based on a limited number of measurements. Therefore, a significant standard deviation and consequently standard uncertainty cannot be obtained. If a more precise assessment of the EDM instrument under field conditions is required, it is recommended to adopt the more rigorous full test procedure as given in Clause 6.

This test procedure relies on having a test field with distances which are accepted as true values. If such a test field is not available, it is necessary to determine the unknown distances, using an EDM instrument of higher accuracy than that investigated in this test procedure. If no EDM with higher accuracy is available, the full test procedure has to be applied.

#### 4.3 Procedure 2: Full test procedure (Type A evaluation of standard uncertainty)

The full test procedure shall be adopted to determine the best achievable measure of precision of a particular EDM instrument and its ancillary equipment under field conditions, described by the operator.

The full test procedure is based on measurements of distances in all combinations on a test line without nominal values. The experimental standard deviation of a single distance measurement is determined from a least squares adjustment of the distances in all combinations. Scale errors of an EDM instrument cannot be detected by this procedure. But scale errors in general do not have any influence, neither on the experimental standard deviation,  $s$ , nor on the zero-point correction,  $\delta$ . In order to determine the stability of the scale, the measuring frequency of the EDM instrument can be checked by means of a frequency meter.



The test procedure given in Clause 6 is intended for determining the measure of precision in use of a particular EDM instrument. This measure of precision in use is expressed in terms of the experimental standard deviation,  $s$ , of a single measured distance, which is considered the type A standard uncertainty:

$$s = u_{\text{ISO-EDM}}$$

Further, this procedure implies:

- the measure of precision in use of EDM instruments by a single survey team with a single instrument and its ancillary equipment at a given time;
- the measure of precision in use of a single instrument over time;
- the measure of precision in use of each of several EDM instruments in order to enable a comparison of their respective achievable precisions to be obtained under similar field conditions.

Statistical tests should be applied to determine whether the experimental standard deviation,  $s$ , obtained belongs to the population of the instrumentation's theoretical standard deviation  $\sigma$ , whether two tested samples belong to the same population and whether the zero-point correction,  $\delta$ , is equal to zero or equal to a predetermined value,  $\delta_0$  (see 6.4).

## 5 Simplified test procedure

### 5.1 Configuration of the test field

The test field shall consist of one permanently marked instrument station and four permanently mounted reflectors at typical distances for the usual working range of the particular EDM instrument (e.g. from 20 m to 200 m). If permanent mounting of the reflectors is not possible, then the ground points of the reflector stations should be indelibly marked.

ISO 17123-4:2012

In order to set up the test field, each distance shall be measured and meteorologically corrected at least three times using a higher accurate EDM instrument (see Figure 1) to eventually obtain a mean value. For this purpose, air temperature and air pressure have to be measured individually at the instrument and the target point very thoroughly in order to determine the necessary corrections of the mean values [1 ppm for any deviation of 1 °C in temperature and/or for any deviation of 3 hPa (3 mbar) in air pressure].

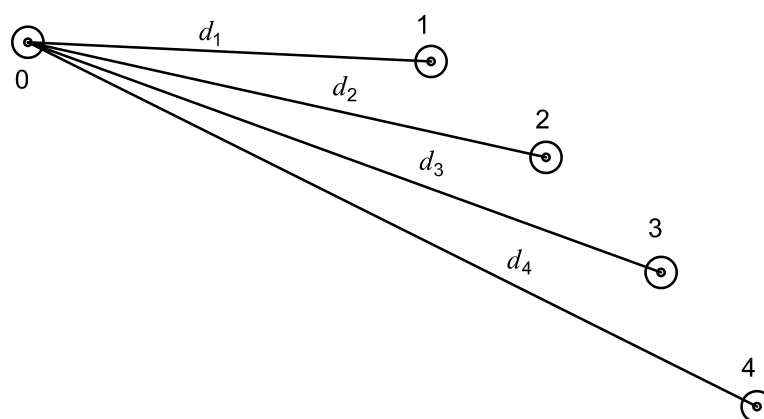


Figure 1 — Configuration of the test field for the simplified test procedure

The atmospherically corrected mean values of the four distances shall be considered to be true values:

$$\bar{x}_1 = d_1$$

$$\bar{x}_2 = d_2$$

$$\bar{x}_3 = d_3$$

$$\bar{x}_4 = d_4$$

**5.2 Measurements**

When setting up the EDM instrument, special care shall be taken when centring above the ground point.

Each distance shall be measured three times. Also, the air temperature and the air pressure shall be measured to derive the atmospheric corrections. The measured distances  $x_1, x_2, x_3, x_4$  are the mean values of the three measurements corrected for atmospheric influences.

**5.3 Calculation**

All differences  $\bar{x}_j = x_j$  shall be within the specified permitted deviation  $\pm p$  (according to ISO 4463-1) for the intended measuring task. If  $p$  is not given, all differences shall be  $|\bar{x}_j = x_j| \leq 2,5 \times s$ , where  $s$  is the standard uncertainty  $u_{\text{ISO-EDM}}$  of a single distance measurement, according to the full test procedure described in Clause 6.


If the differences  $|\bar{x}_j - x_j|$  are too large for the intended task, it is necessary to make further investigations in order to identify the main sources of errors.

**5.4 Further investigations**

If all differences  $\bar{x}_j = x_j$  have the same sign, then a systematic error is suspected. This can be an error of the zero-point correction or a scale error. If no source for the systematic error can be recognized, then it is recommended to carry out the full test procedure as given in Clause 6.

If a scale error is suspected, then the measuring frequency of the EDM instrument should be checked by means of a frequency meter, or the local service of the EDM manufacturer has to be contacted.

To check the zero-point correction,  $\delta$ , a temporary baseline (about 50 m) consisting of three points on a straight line with an in-line tolerance of 3 cm should be established (see Figure 2). Three tripods with forced centring shall constitute the baseline.



**Figure 2 — Temporary baseline to check the zero-point correction**

From the measured distances between the tripods, the zero-point correction is calculated

$$\delta = \overline{1,3} - \overline{1,2} - \overline{2,3} \tag{1}$$

where

- $\delta$  is the zero-point correction, and
- $\overline{1,3}$ ;  $\overline{1,2}$  and  $\overline{2,3}$  are the measured distances between the three tripods.

## 6 Full test procedure

### 6.1 Configuration of the test line

A test configuration between 300 m and 600 m long with seven points on a straight line shall be established. The total line can also have an appropriate length to the distance of the intended use of the EDM (for line setup, see Figure 3). The points shall be stable during the test measurements.

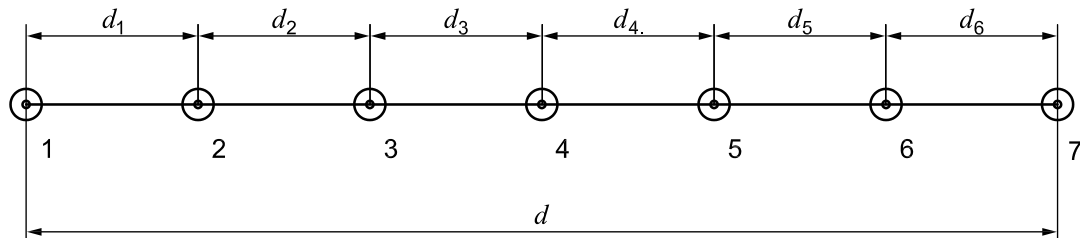


Figure 3 — Configuration of the test line for the full test procedure

#### A: Test line setup with 21 different distances

A good configuration of the test line will be achieved if the six distances  $d_1$  to  $d_6$  are selected in a way that all the 21 distances from the measurement combinations described in 6.2 are different.

The following procedure gives one way to derive the six distances between the seven points of the test line:

$d$  is the total length of the projected test line:

$$d_1 = \frac{d}{63}, \quad d_2 = 2d_1 \quad (2)$$

$$d_3 = 4d_1, \quad d_4 = 8d_1$$

$$d_5 = 16d_1, \quad d_6 = 32d_1$$

#### B: Test line setup for EDM instruments to include possible cyclic errors in measured data

In order to obtain representative values for the experimental standard uncertainty,  $u_{\text{ISO-EDM}}$ , and the zero-point correction,  $\delta$ , for EDMs with possible cyclic errors, the points of the test line shall be selected in such a way that the parts of the measured distances determined by phase measurements with the fine frequency are evenly distributed over the unit length (measuring scale) of the EDM instrument.

A good configuration will be achieved if the six distances between the seven points of the test line are derived by the following procedure:

$$\beta_0 = \frac{d - 6,5\lambda}{15} \quad (3)$$

where

$d$  is the total length of the projected test line;

$\lambda$  is the wavelength of the EDM instrument (derived from the EDM modulation frequency);

$\lambda/2$  is the unit length (measuring scale) of the EDM instrument.

and

$$\beta = \mu \times \lambda / 2 \tag{4}$$

Select an integer number  $\mu$  in such a way that  $\beta$  approaches  $\beta_0$  as close as possible,

with

$$\gamma = \frac{\lambda}{72} \tag{5}$$

the six distances of the test line and the whole length,  $d$ , are calculated:

$$d_1 = \lambda + \beta + 3\gamma \tag{6a}$$

$$d_2 = \lambda + 3\beta + 7\gamma \tag{6b}$$

$$d_3 = \lambda + 5\beta + 11\gamma \tag{6c}$$

$$d_4 = \lambda + 4\beta + 9\gamma \tag{6e}$$

$$d_5 = \lambda + 2\beta + 5\gamma \tag{6f}$$

$$d_6 = \lambda + \gamma \tag{6g}$$

$$d = 6\lambda + 15\beta + 36\gamma \tag{6h}$$

**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

<https://standards.iteh.ai/catalog/standards/sist/751ecc9f-8466-4a47-8784-f623b3e6ba3e/iso-17123-4-2012>

## 6.2 Measurements

All possible 21 distances between the seven points (see Figure 4) shall be measured on the same day. The forced centring interchange should be used to eliminate centring errors. All distances should be measured with a good return signal. The measurement of the distances should only be started when the visibility is good and a low insolation is to be expected. The air temperature and pressure should often be measured to ensure that reliable atmospheric corrections can be derived.