



Designation: E1495 – 02 (Reapproved 2007)

Standard Guide for Acousto-Ultrasonic Assessment of Composites, Laminates, and Bonded Joints¹

This standard is issued under the fixed designation E1495; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This guide explains the rationale and basic technology for the acousto-ultrasonic (AU) method. Guidelines are given for nondestructive evaluation (NDE) of flaws and physical characteristics that influence the mechanical properties and relative strength of composite structures (for example, filament-wound pressure vessels), adhesive bonds (for example, joints between metal plates), and interlaminar and fiber/matrix bonds in man-made composites and natural composites (for example, wood products).

1.2 This guide covers technical details and rules that must be observed to ensure reliable and reproducible quantitative AU assessments of laminates, composites, and bonded structures. The underlying principles, prototype apparatus, instrumentation, standardization, examination methods, and data analysis for such assessments are covered. Limitations of the AU method and guidelines for taking advantage of its capabilities are cited.

1.3 The objective of AU is to assess subtle flaws and associated strength variations in composite structures and bonded joints. Discontinuities such as large voids, disbands, or extended lack of contact at interfaces can be assessed by other NDE methods such as conventional ultrasonics.

1.4 Additional information may be found in the publications cited in the list of references at the end of this guide. The referenced works provide background on research, applications, and various aspects of signal acquisition, processing, and interpretation.

1.5 The values stated in SI units are to be regarded as the standard. The values given in parentheses are for information only.

1.6 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

¹ This guide is under the jurisdiction of ASTM Committee E07 on Nondestructive Testing and is the direct responsibility of Subcommittee E07.04 on Acoustic Emission Method.

Current edition approved July 1, 2007. Published July 2007. Originally approved in 1992. Last previous edition approved in 2002 as E1495 - 02. DOI: 10.1520/E1495-02R07.

2. Referenced Documents

2.1 *ASTM Standards*:²

E543 Specification for Agencies Performing Nondestructive Testing

E1316 Terminology for Nondestructive Examinations

2.2 *ASNT Standard*:³

ANSI/ASNT CP-189 Standard for Qualification and Certification of Nondestructive Testing Personnel

SNT-TC-1A Recommended Practice for Personnel Qualifications and Certification in Nondestructive Testing

2.3 *AIA Document*:⁴

NAS-410 Certification and Qualification of Nondestructive Testing Personnel

3. Terminology

3.1 *Definitions*:

3.1.1 *acousto-ultrasonics (AU)*—a nondestructive examination method that uses induced stress waves to detect and assess the diffuse defect states, damage conditions, and variations of mechanical properties of an examination structure. The AU method combines aspects of acoustic emission (AE) signal analysis with ultrasonic materials characterization methods (Terminology E1316).

3.1.2 Additional related definitions may be found in Terminology E1316.

3.2 *Definitions of Terms Specific to This Standard*:

3.2.1 *stress wave factor (SWF)*—a generic measure of the relative energy loss (attenuation) or propagation efficiency of stress waves generated by the AU method. There are many ways to define and calculate the SWF. Several of these are described in Section 11 of this guide.

4. Summary of Guide

4.1 *General*—Two probes are attached to a sample in a send-receive configuration. One (a pulsed sending probe) is

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

³ Available from American Society for Nondestructive Testing (ASNT), P.O. Box 28518, 1711 Arlington Ln., Columbus, OH 43228-0518, <http://www.asnt.org>.

⁴ Available from Aerospace Industries Association of America, Inc. (AIA), 1000 Wilson Blvd., Suite 1700, Arlington, VA 22209-3928, <http://www.aia-aerospace.org>.

optimized for wave generation, while the other (a receiving probe) is optimized for signal sensing. The probes are attached to the sample surface at normal incidence. The usual, and often most practical, configuration has piezoelectric probes, a sender and receiver, on the same side of the examination part (1).⁵ Measurements are performed by allowing ultrasonic stress waves to interact with a volume of material between the probes. The waves are modified by the material microstructure and morphology (2).

4.2 *Principle*—The AU method measures the relative efficiency of stress wave propagation in a material. The dominant attribute measured is stress wave attenuation. Lower attenuation, a high SWF value, means better stress wave energy transmission for many composites and, therefore, better transmission and redistribution of dynamic strain energy. More efficient strain energy transfer and strain redistribution during loading or impact corresponds to increased strength and fracture resistance in composite structures and adhesive bonds. A lower SWF usually indicates regions in which strain energy is likely to concentrate and result in crack growth and fracture (3).

4.3 *Structure Configuration Effects*—In monolithic plates and homogeneous composite slabs, the SWF will exhibit signal attenuation effects due to variations in microstructure, morphology, porosity, cure state, microcrack populations, etc. (4). A lower SWF typically corresponds to regions of higher attenuation. In laminated structures or bonded joints, however, interfaces and bondlines can produce either lower or higher SWF values, depending on the bond quality (5). Delaminated regions can produce higher SWF values because more energy is reflected or channeled to the receiving probe.

4.4 *In-Plane Measurements*—Offsetting probes enables the collection of stress wave reverberations that have traveled in-plane from sender to receiver. It is therefore possible to measure in-plane, mechanical property variations in principal load directions in fiber-reinforced laminates or adhesively bonded joints (that is, properties such as interlaminar shear strength and adhesive bond strength).

4.5 *Signal Collection Criterion*—With the AU method, instead of singling out specific echoes, all of the multiple reverberations, including signals from internal reflectors and scatterers, are collected and analyzed together. Even with pulse-echo or through-transmission configurations, all stress wave reflections and reverberations in a local volume of material are collected and evaluated, as in backscatter, forward-scatter, and diffuse field analysis.

4.6 *Wavelength Criterion*—In composite panels or bonded plates, the sender should produce wavelengths that are comparable to or less than the panel or plate thickness. Suitable wavelengths are those passed by the examination piece at frequencies equal to or greater than the sending probe center frequencies.

5. Significance and Use

5.1 *General*—Conventional ultrasonics should be considered first for the detection of overt flaws such as delaminations

⁵ The boldface numbers in parentheses refer to the list of references at the end of this guide.

in composites. Thereafter, AU should be considered for composites that are proved to be free of major flaws or discontinuities. The AU method is intended almost exclusively for assessing the collective effects of dispersed defects and subcritical flaw populations. These are material aberrations that influence AU measurements and also underlie mechanical property variations, dynamic load response, and impact and fracture resistance.

5.2 *Specific Advantages*—The AU method can be used to evaluate composite laminate and bond quality using access to only one surface as, for example, the exterior surface of pressure vessels. It is unnecessary to utilize angle beam fixtures because the method can always be applied with probes at normal incidence. The method can be applied using dry coupling with elastomer pads attached to the probes, and there is no need to immerse the examination object in water.

5.3 *General Applications*—The AU method was devised to assess diffuse discontinuity populations and any associated changes of the mechanical properties of composites and composite-like materials. The AU method has been used to evaluate fiber-reinforced composites (6), composite laminates (7), filament-wound pressure vessels (8), adhesive bonds (9), paper and wood products (10), and cable and rope (11). The method has been shown to be particularly practical for assessing the strength of adhesively bonded joints. It has also been shown to be useful for assessing microporosity (12), microcracking (13), hydrothermal aging (14), and damage produced by impacts (15) and fatigue (16).

6. Basis of Application

6.1 Personnel Qualification

6.1.1 If specified in the contractual agreement, personnel performing examinations to this standard shall be qualified in accordance with a nationally recognized NDT personnel qualification practice or standard such as **ANSI/ASNT CP-189**, **SNT-TC-1A**, **NAS-410**, or a similar document and certified by the employer or certifying agency, as applicable. The practice or standard used and its applicable revision shall be identified in the contractual agreement between the using parties.

6.2 Qualification of Nondestructive Agencies

6.2.1 If specified in the contractual agreement, NDT agencies shall be qualified and evaluated as described in Practice **E543**. The applicable edition of Practice **E543** shall be specified in the contractual agreement.

6.3 Proper application of the AU method requires the involvement of an NDE specialist to plan and guide the examination procedure. Knowledge of the principles of ultrasonic examination is required. Personnel applying AU should be experienced practitioners of conventional ultrasonic and acoustic emission examination and associated methods for signal acquisition, processing, and interpretation.

6.4 Particular emphasis should be placed on personnel having proficiency in computer signal processing and the use of digital methods for time and frequency domain signal analysis. Familiarity with ultrasonic spectrum analysis using digital Fourier transforms is mandatory. Spectral distribution, multiple regression, and pattern recognition analyses and adaptive learning procedures are important.

6.5 Application of the AU method also requires proficiency in developing and designing reference standards. The development of reference standards is needed for each type of material and configuration to be examined. Because AU measurements are relative and comparative, experimental examinations confirmed by destructive testing are needed to avoid ambiguities in the interpretation of results.

7. Limitations

7.1 *General*—The AU method possesses the limitations common to all ultrasonic methods that attempt to measure either absolute or relative attenuation. When instrument settings and probe configurations are optimized for AU, they are unsuitable for conventional ultrasonic flaw detection.

7.2 *Signal Reproducibility Factors*—The AU results may be affected adversely by the following factors: (1) improper selection of type and amount of couplant, (2) couplant thickness variations and bubbles, (3) specimen surface roughness and texture, (4) probe misalignment and insufficient pressure, (5) probe resonances and insufficient damping, and (6) insufficient instrument bandwidth.

8. Standardization

8.1 *Self-Standardization*—The sender and receiver probes can be used to verify each other. Deficiencies in the instrumentation and probe response become evident by comparing the results with the standard waveforms established previously for a reference item. Commercial ultrasonic probes and AE sensors respond to deformation (stress) waves in a complex fashion that involves both normal and in-plane displacements of the examination sample surface. Although it is possible to standardize such probes in an absolute sense, even sensors of the same design and specification should be treated as unique and definitely noninterchangeable.

8.2 *Stress Wave Factor Normalization*—Regardless of how the SWF is defined, it is practical to normalize it relative to

some standard value, for example, the maximum value found for the optimum condition of a representative material sample or structure. This is appropriate where many nominally identical articles will be examined.

8.3 *Reference Standards*—Normalization of the SWF is the first step toward establishing a reference standard. The second step is to fabricate a set of samples exhibiting the full range of expected material conditions and flaw states. One of these samples should represent the optimum condition of the material. This procedure should be followed by the development of benchmark structures that can be used as comparative standards.

9. System Configuration

9.1 *Standard Configuration*—Four possible AU probe configurations are shown in Fig. 1. With the probes on the same side of a panel, examination proceeds by holding the probes in a fixture and moving them as a unit to cover the examined area. For zero offset between probes, the configuration reduces to either the pulse-echo or through-transmission mode, as shown in Fig. 1 (b) and (d) respectively. The prototype apparatus depicted in Fig. 2 illustrates the essential features of a standard configuration.

9.2 *Probes*—Two classes of piezoelectric probes are appropriate: (1) resonant and non-resonant AE sensors, and (2) damped broadband ultrasonic probes. Resonant AE sensors have more sensitivity, but the signals transmitted by the test piece may be of sufficient strength such that sensitivity is not a problem. One reason for avoiding resonant sensors is that they have ringdown characteristics that may be difficult to separate from the multiple reflections transmitted by the examination sample.

9.2.1 *Probe Bandwidth*—Non-resonant AE sensors have a flatter frequency response curve than resonant sensors. This response characteristic should be exploited in AU because it would render a truer signal over a wider bandwidth. Another

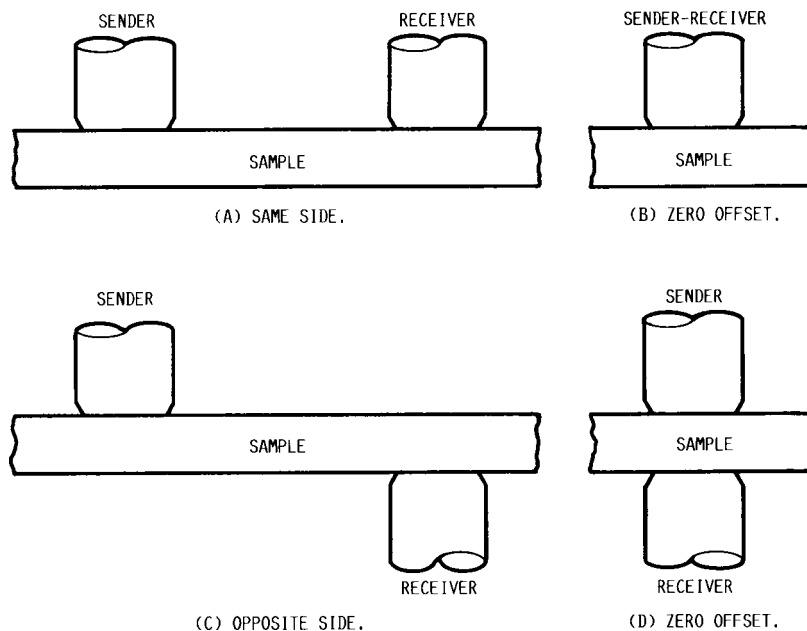


FIG. 1 Four Possible AU Probe Configurations

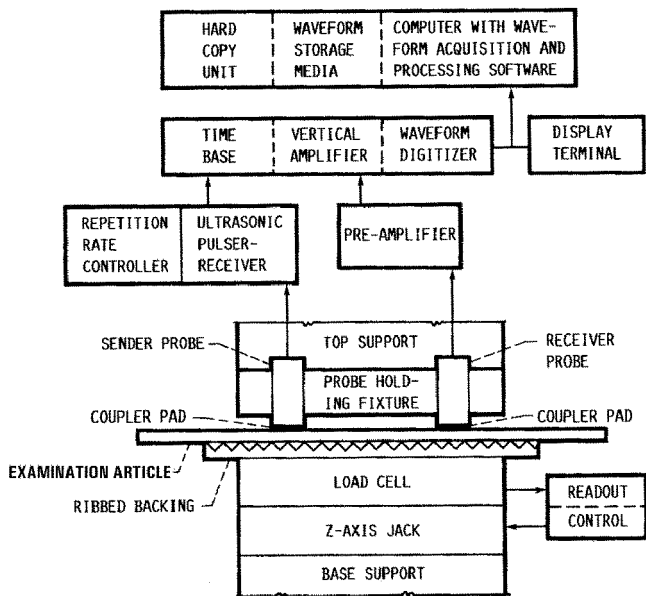


FIG. 2 Diagram of Apparatus and Instrumentation Used for Laboratory Application of AU

approach is to use the bandwidth response of damped broadband ultrasonic probes. Good results can be obtained with broadband ultrasonic probes working as both senders and receivers. For many fiber-reinforced composites, broadband probe pairs with center frequencies ranging from 0.5 to 5 MHz prove useful, for example, send-recv pairs of 2.25 MHz damped probes. Broadband commercial piezoelectric probes will produce satisfactory AU results for many composite structures.

9.2.2 *Probe Combinations*—Combinations of damped broadband ultrasonic and AE sensors can be used. The choice depends on the nature of the material being examined. The material may require the use of a broadband ultrasonic sender and a resonant AE sensor as receiver. A broadband sender would cover frequencies potentially passed by the examination sample, while the receiving sensor would be tuned to a particular frequency determined to be the most appropriate for assessing a particular property.

9.2.3 *Probe Facing*—To improve coupling, it is useful to machine the epoxy face or wearplate of the probes so that the contact area is reduced to a fraction of 1 cm.² To reduce the area of contact, it also helps to bond waveguides to the faces of the probes. Waveguides should consist of truncated solid cones with their wide ends bonded to probe faces.

9.2.4 *Reverberation Effects*—Reverberations in faceplates and facing attachments can mimic probe ringdown. The reverberations can be quite strong if the acoustic impedances between layers (wearplate, facing, and examination materials) are significantly mismatched. The effect will appear in waveforms as additional ringdown and in spectra as spurious interference peaks. Since these effects do not represent the examination sample, care should be taken to avoid or eliminate them during signal analysis.

9.2.5 *Probe Fixturing*—The probes shown in Fig. 2 are held firmly in a support fixture so that a predetermined spacing is

maintained. The fixture is designed to avert crosstalk between probes. It must be rigid enough to assure that the probes can be pressed firmly, as a unit, against the examination piece to optimize coupling pressure.

9.2.6 *Probe Spacing*—Probe spacing is determined by the following factors: (1) wave attenuation within the examination sample, (2) probe bandwidth and sensitivity, (3) sample thickness and shape, (4) diameter of the probes, and (5) spatial resolution required in the scan images. Because the objective of AU is not the generation of high-resolution images of minute flaws, probe spacing may be quite large, typically several centimetres from probe centerline to centerline. The objective should be to interrogate a representative volume of material for a given probe spacing.

9.2.7 *Probe Alignment*—The AU method should be accomplished with probes at normal incidence because the method is particularly sensitive to probe alignment and associated coupling variations. There is no need for oblique angle probes. In conventional ultrasonics, the chief reason for oblique incidence is to produce shear waves. Shear waves will arise naturally with the AU approach due to beam spread and mode conversions of reflected waves.

9.3 *Coupling Methods*—When a fluid medium is used for coupling probes to a surface, a gel type is preferred. A fluid couplant should (1) provide good acoustic coupling over the desired frequency range, (2) be chemically inert, (3) be easy to remove, (4) be consistent from batch to batch, and (5) maintain consistent properties during the period and at the temperatures used.

9.3.1 *Couplant Application*—Particular attention should be paid to the application of fluid couplant to probes. Control should be exercised over the following factors: (1) amount of couplant applied, (2) avoidance of air bubbles, (3) assurance of a thin and uniform film, and (4) avoidance of excess couplant. The amount of couplant should not be such that it overflows at the edge of the probe face, thereby absorbing energy and altering results.

9.3.2 *Coupling Pressure*—Laboratory experiments have shown that an optimum coupling pressure exists. When the pressure applied to the probes is small, the received signal will also be small. As the pressure is increased, a definite increase in signal strength will occur until the pressure is optimal for the probe-couplant-material combination. Any further increase in pressure will have no significant effect on the signals.

9.3.3 *Dry Coupling*—The need for dry, soft coupling occurs in instances in which it is necessary to either deal with rough surfaces or avoid the infusion of fluid into porous materials. Efficient coupling can be achieved with elastomer pads bonded to the probe face. When pressed against the examination surface, the elastomer will conform to any surface roughness or texture providing good coupling.

9.3.4 *Example*—For the laboratory prototype apparatus depicted in Fig. 2, the force applied was roughly 12 N (2.7 lb) at a pressure of 120 000 Pa (18 psi) per probe over the area of the silicon rubber pads. The uncompressed elastomer pad thickness was approximately 1 mm, and the contact area was approximately 0.2 cm². The pads did not cover the entire probe