
**Anaesthetic and respiratory
equipment — Conical connectors —
Part 1:
Cones and sockets**

*Matériel d'anesthésie et de réanimation respiratoire — Raccords
coniques —*

iTeh STANDARD PREVIEW
Partie 1: Raccords mâles et femelles
(standards.iteh.ai)

ISO 5356-1:2015

<https://standards.iteh.ai/catalog/standards/sist/4120333f-4c7d-43d2-9457-3e3a63f85876/iso-5356-1-2015>



iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 5356-1:2015

<https://standards.iteh.ai/catalog/standards/sist/4120333f-4c7d-43d2-9457-3e3a63f85876/iso-5356-1-2015>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2015

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

	Page
Foreword	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Dimensional requirements	1
3.1 General requirements	1
3.2 Additional requirements	3
4 22 mm latching sockets	4
Annex A (normative) Plug and ring test gauges for cones and sockets made of materials other than metal	5
Annex B (normative) Test for security of engagement of 22 mm latching sockets to cones	7
Annex C (normative) Test for leakage from 22 mm latching sockets	8
Annex D (normative) Drop procedure for 22 mm latching sockets	9
Annex E (informative) Plug and ring test gauges for cones and sockets made of metal	10
Annex F (informative) Suggested apparatus and methods for testing the security of engagement of 22 mm latching sockets	12
Bibliography	17

iTeh STANDARD PREVIEW

(standards.iteh.ai)

[ISO 5356-1:2015](https://standards.iteh.ai/catalog/standards/sist/4120333f-4c7d-43d2-9457-3e3a63f85876/iso-5356-1-2015)

<https://standards.iteh.ai/catalog/standards/sist/4120333f-4c7d-43d2-9457-3e3a63f85876/iso-5356-1-2015>

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT) see the following URL: [Foreword - Supplementary information \(standards.iteh.ai\)](http://Foreword - Supplementary information (standards.iteh.ai))

The committee responsible for this document is ISO/TC 121, *Anaesthetic and respiratory equipment*, Subcommittee SC 1, *Breathing attachments and anaesthetic machines*.

This fourth edition cancels and replaces the third edition (ISO 5356-1:2004), which has been technically revised with the following changes:

- harmonizing the terminology used in the text with the title of this part of ISO 5356;
- deleting the definition of 22 mm latching connector because the content is covered by the text of this part of ISO 5356;
- including 11,5 mm cones and sockets;
- adding the minimum internal diameter for the 30 mm cone and changing the minimum internal diameter of the 8,5 mm cone from 6,0 mm to 6,25 mm;
- deleting the requirements on reuse of 22 mm latching sockets and cones because this is covered by the standards for the specific medical devices and accessories;
- making the recess and the shoulder for the 22 mm cone conditional;
- correcting the dimension D for the plug and ring test gauges for 8,5 mm cones and sockets made of materials other than metal in [Annex A](#) of this part of ISO 5356;
- restructuring the document for clarity.

ISO 5356 consists of the following parts, under the general title *Anaesthetic and respiratory equipment — Conical connectors*:

- *Part 1: Cones and sockets*
- *Part 2: Screw-threaded weight-bearing connectors*

Introduction

In clinical practice, several breathing attachments used in anaesthetic and respiratory equipment may have to be joined together to provide a suitable breathing system. Items of medical equipment, such as a humidifier or a spirometer, are often incorporated into the breathing system which might also be connected to an anaesthetic gas scavenging system. Connections for these purposes are usually cone and socket joints, and a lack of standardization of these connections has given rise to problems of interchangeability when connecting equipment made by different manufacturers. This part of ISO 5356 specifies the requirements and dimensions for cones and sockets used in anaesthetic and respiratory equipment.

An important consideration is that conical connections need to be secure but nevertheless disconnectable by the operator. The use of cones and sockets meeting the requirements of this part of ISO 5356 will not necessarily prevent them being disconnected accidentally. To minimize the risk of 22 mm connectors being accidentally disconnected, latching sockets can be used.

[Annex A](#) includes a figure and a table detailing plug and ring test gauges that are used to check cones and sockets made of materials other than metal. [Annex B](#), [Annex C](#), and [Annex D](#) provide test methods for latching sockets, [Annex E](#) includes a figure and table detailing plug and ring test gauges that can be used to check metal cones and sockets, and [Annex F](#) contains recommendations for testing the security of latching sockets.

[Figure 1](#), detailing the dimensions and tolerances of cones and sockets, has been prepared in accordance with ISO 3040.

In this document, the following print types are used:

- requirements, compliance with which can be verified, and definitions: roman type;
- notes and examples: smaller roman type;
- test methods: *italic type*.

ITIH STANDARD PREVIEW

(standards.iteh.ai)

ISO 5356-1:2015

<https://standards.iteh.ai/catalog/standards/sist/4120333f-4c7d-43d2-9457-3e3a63f85876/iso-5356-1-2015>

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 5356-1:2015

<https://standards.iteh.ai/catalog/standards/sist/4120333f-4c7d-43d2-9457-3e3a63f85876/iso-5356-1-2015>

Anaesthetic and respiratory equipment — Conical connectors —

Part 1: Cones and sockets

1 Scope

This part of ISO 5356 specifies dimensional and gauging requirements for cones and sockets intended for connecting anaesthetic and respiratory equipment, e.g. in breathing systems, anaesthetic gas scavenging systems, and vaporizers. The cones and sockets are therefore not regarded as devices in their own right.

This part of ISO 5356 gives requirements for the following cones and sockets:

- 8,5 mm and 11,5 mm sizes intended for use in neonatal and paediatric breathing systems;
- 15 mm and 22 mm sizes intended for general use in breathing systems;
- 22 mm latching sockets (including performance requirements);
- 23 mm size intended for use with vaporizers, but not for use in breathing systems;
- 30 mm size intended for the connection of a breathing system to an anaesthetic gas scavenging system.

This part of ISO 5356 does not specify the medical devices and accessories on which these cones and sockets are to be provided.

Requirements for the application of cones and sockets are not included in this part of ISO 5356, but are or will be given in the relevant International Standards for specific medical devices and accessories.

NOTE Requirements for screw-threaded weight-bearing connectors are specified in ISO 5356-2.

2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 5367:2014, *Anaesthetic and respiratory equipment — Breathing sets and connectors*

3 Dimensional requirements

3.1 General requirements

3.1.1 Cones and sockets made of metal shall comply with [Figure 1](#) and the dimensions given in [Table 1](#) as appropriate.


Check compliance by functional testing.

NOTE [Annex E](#) includes a figure and table detailing plug and ring test gauges that can be used to check metal cones and sockets.

3.1.2 Cones and sockets made of non-metallic materials shall comply with [Figure 1](#) and the dimensions given in [Table 1](#) except that the dimensions A and B and ratio F may vary from those given in [Table 1](#).

Check compliance by engaging the cone or socket in the appropriate plug or ring test gauge according to [Figure A.1](#) and [Table A.1](#), by applying an axial force of $(35 \pm 3,5)$ N for 8,5 mm, 11,5 mm, and 15 mm cones or sockets and (50 ± 5) N for 22 mm and 30 mm cones or sockets while simultaneously rotating the cone or socket $(20 \pm 5)^\circ$. Its leading edge shall lie between the minimum and maximum diameter steps of the gauge. The cones or sockets and gauges shall be maintained at a temperature of $(20 \pm 3)^\circ\text{C}$ during the test.

NOTE Because cones or sockets made from plastics materials (for example polyamide, polyacetal, polycarbonate, polysulfone) can vary greatly in their physical characteristics, it is not considered practicable to specify dimensions A , B , and ratio F ; for this reason, gauging requirements have been included. It is also considered impracticable to generalize on matters such as cold flow and thermal instability, as well as possible changes in physical characteristics, contact with solvents, etc.

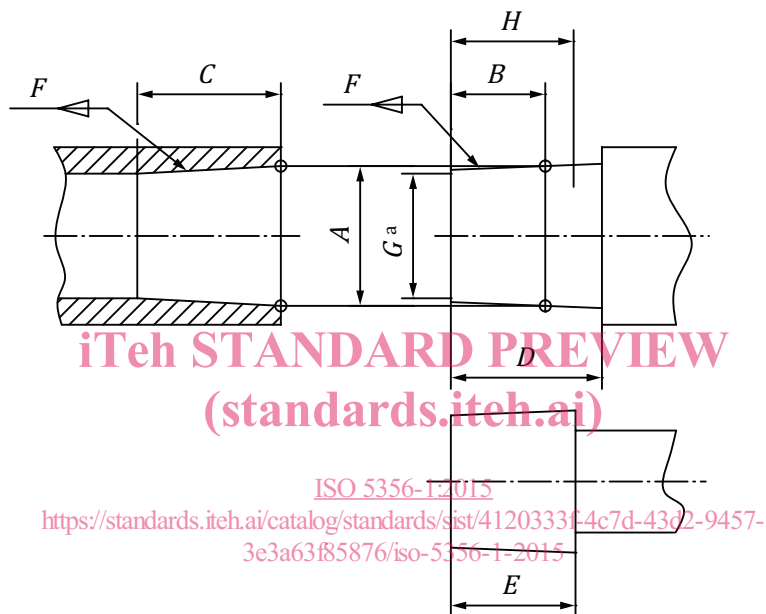

^a For the 8,5 mm cone and the 30 mm cone, dimension G over the minimum length, H , as specified in [Table 1](#).

NOTE The radius on the entrance to the socket and on the leading edge of the cone is not intended to be less than 0,5 mm and not more than 0,8 mm.

Figure 1 — Interconnecting details of cones and sockets

Table 1 — Dimensions of cones and sockets (see Figure 1)

Dimensions in millimetres

Connector size	A	B	Taper length C	Clearance to shoulder (if present) D	Length to taper E	Taper ratio F	Minimum internal diameter of cone G	Minimum length of internal diameter of the cone (G) H
8,5	8,45 ± 0,04	6	≥6,4	≥8,9	≥8	1:19	6,25	6,0
11,5	11,50 ± 0,04	10	≥13,5	≥16	≥15	1:40	a	a
15	15,47 ± 0,04	10	≥16	≥16	≥14,5	1:40	a	a
22	22,37 ± 0,04	15	≥21	See Figure 3	See Figure 3	1:40	a	a
23	23,175 ± 0,02	13	≥18	≥18	≥15	1:36	a	a
30	30,9 ± 0,05	14	≥18	≥18	≥14	1:20	27,0	12,0

a Not specified.


3.2 Additional requirements

3.2.1 22 mm cones designed to connect to a breathing tube complying with ISO 5367:2014, 5.3.2.2, or a latching socket (see Clause 4) shall incorporate a recess, the dimensions of which are given in Figure 2.

Check compliance by functional testing.

ISO 5356-1:2015
<https://standards.iteh.ai/catalog/standards/sis/120333f4c7d-43d2-9457-3e3a63f85876/iso-5356-1-2015>

Dimensions in millimetres

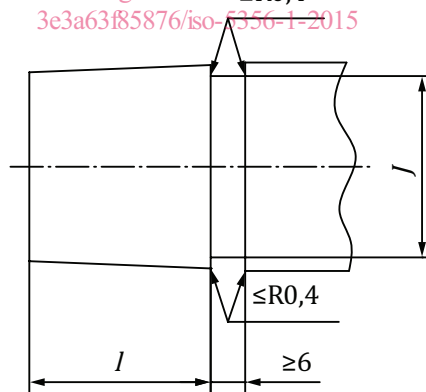

Key

l taper length: 19,5^{+0,5}₀

J diameter of recess: 20^{+0,5}₀

Figure 2 — Details of recess for 22 mm cones

3.2.2 22 mm cones, designed to connect to a face mask shall incorporate a means to prevent over insertion (e.g. shoulder) and comply with the dimensions given in Figure 3.

Check compliance by functional testing.

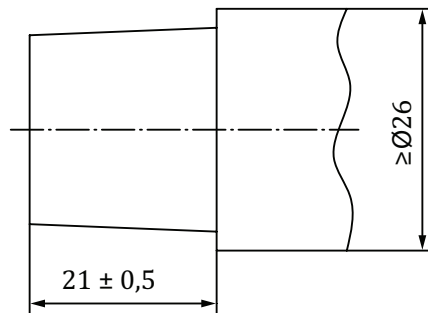


Figure 3 — Dimensions of 22 mm cones designed to connect to a face mask

4 22 mm latching sockets

4.1 22 mm latching sockets shall be designed to engage with the recess of the 22 mm cone as specified in [Figure 2](#).

Check compliance by visual inspection.

4.2 Engaged latching cones and sockets shall not become disconnected when subjected to an axial separation force of (50 ± 5) N for 10 s.

Check compliance by the test method given in [Annex B](#).

4.3 Engaged latching cones and sockets shall not leak by more than 5 ml/min (corrected to 20 °C and 101,3 kPa) when subjected to an internal pressure of $(8 \pm 0,5)$ kPa.

Check compliance by the test method given in [Annex C](#).


4.4 Engaged latching cones and sockets shall meet the requirements of [4.2](#) and [4.3](#) after being dropped from a height of 1 m.

Check compliance by the test method given in [Annex D](#).

Annex A (normative)

Plug and ring test gauges for cones and sockets made of materials other than metal

Figure A.1 and Table A.1 give details of plug and ring gauges for use in checking cones and sockets made of materials other than metals.

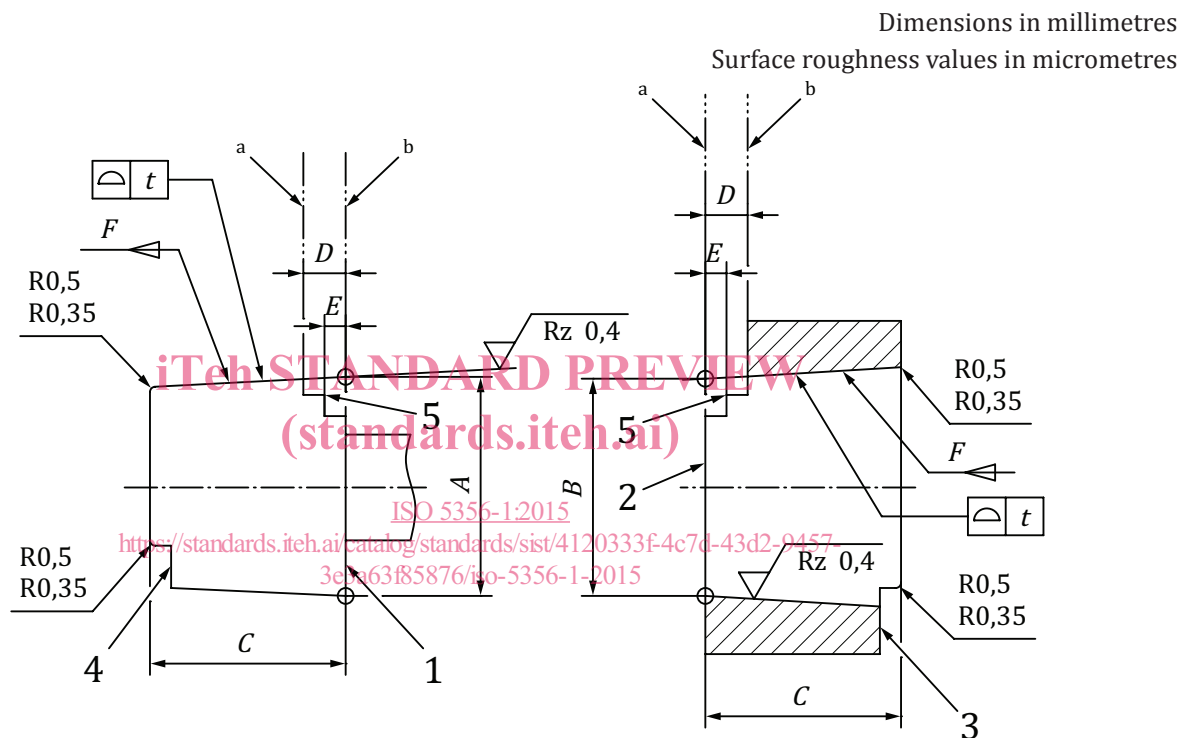

Key

- 1 face A
- 2 face B
- 3 step to check mating gauges ground flush to face A
- 4 step to check mating gauges ground flush to face B
- 5 basic steps
- a Position min.
- b Position max.

NOTE 1 Basic and mating gauge steps are optional.

NOTE 2 Test gauges are usually made of metal.

Figure A.1 — Plug and ring test gauges for cones and sockets made of materials other than metal